

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
 Data File : PL069236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 15:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:47:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.571	8247995	26705689	19.940	26.302 #
28)	SA Decachlor...	10.407	11.496	11236971	21716445	19.553	22.382
Target Compounds							
4)	MA Heptachlor	6.154f	0.000	850652	0	1.448	N.D. #
6)	B beta-BHC	6.154	0.000	850652	0	3.018	N.D. #
8)	B Heptachlo...	0.000	8.040	0	395121	N.D.	0.342 #
10)	B gamma-Chl...	0.000	8.303	0	122430	N.D.	0.107 #
11)	B alpha-Chl...	0.000	8.398	0	37720	N.D.	0.033 #
14)	MA Endrin	8.082f	0.000	431015	0	0.894	N.D. #
15)	B Endosulfa...	0.000	9.219f	0	1045070	N.D.	1.139 #
21)	B Endrin ke...	0.000	10.096f	0	434842	N.D.	0.427 #
25)	Chlordane-3	0.000	8.303	0	122430	N.D.	0.749 #
26)	Chlordane-4	0.000	8.398	0	37720	N.D.	0.190 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
Data File : PL069236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 15:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:47:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

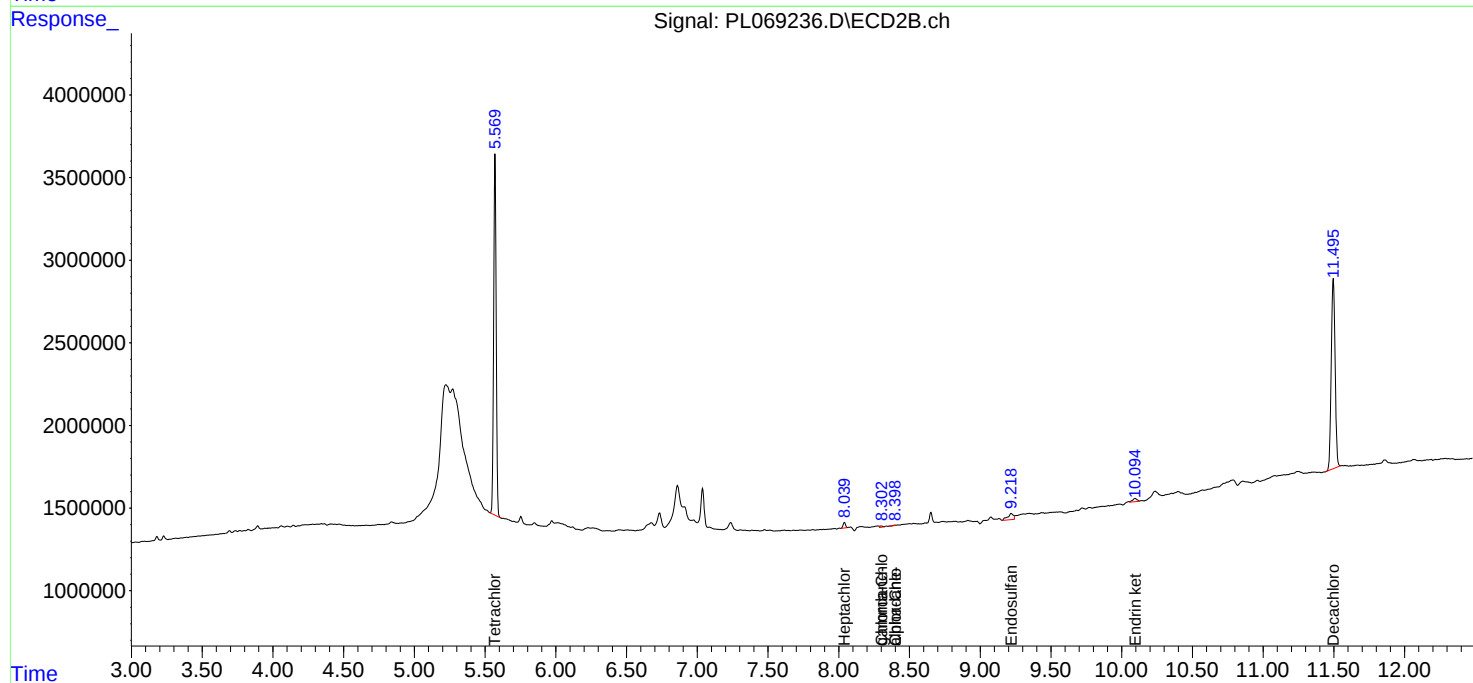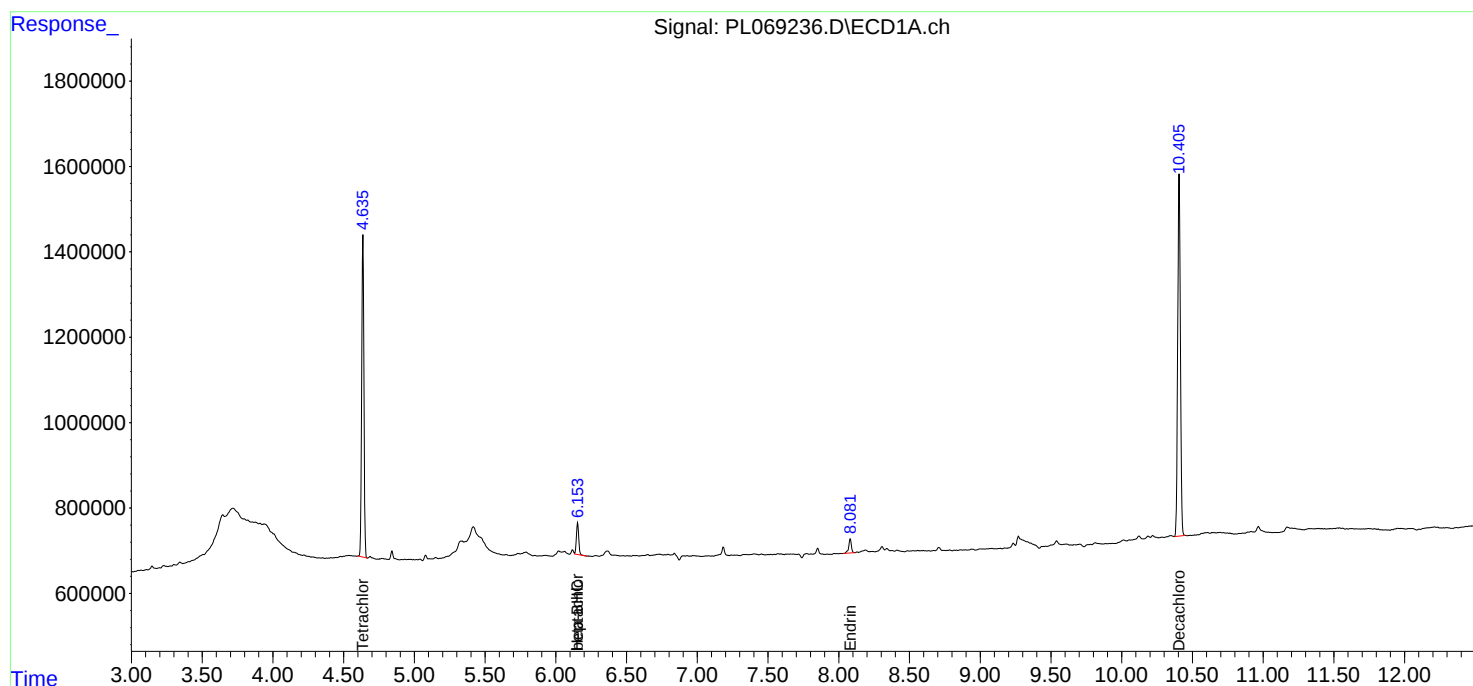


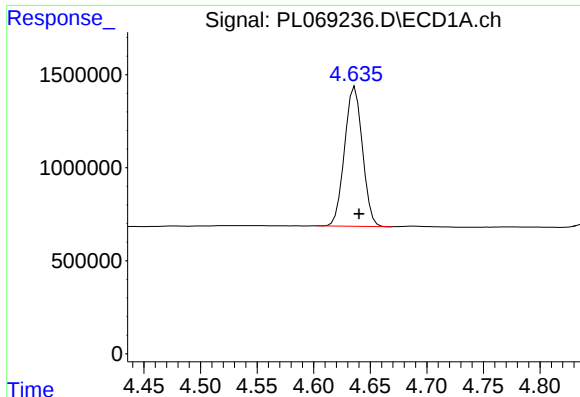

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.003 min
Response: 8247995
Conc: 19.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

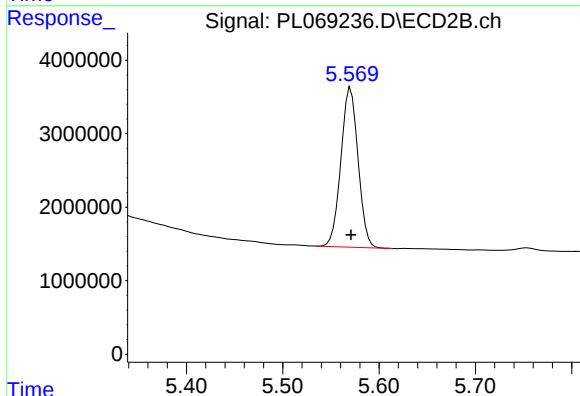


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 26705689
Conc: 26.30 ng/ml

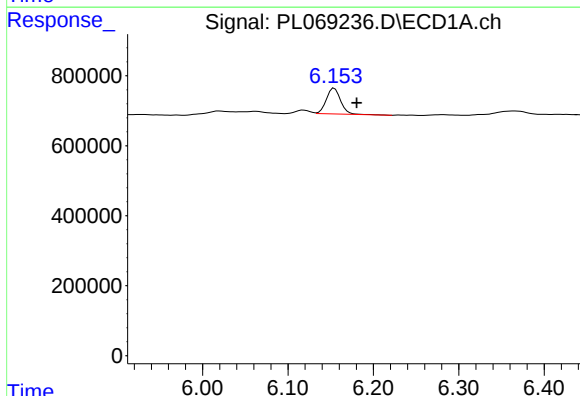


#4 Heptachlor

R.T.: 6.154 min
Delta R.T.: -0.026 min
Response: 850652
Conc: 1.45 ng/ml

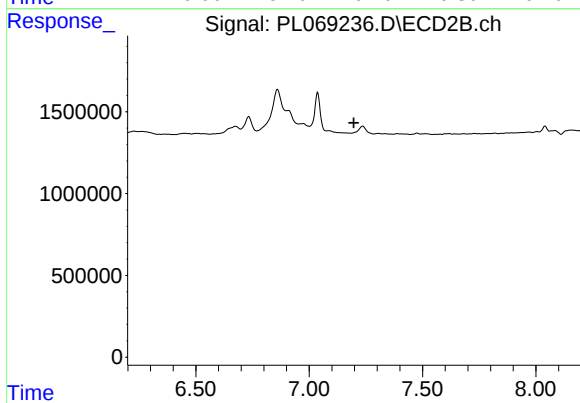

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.197 min
Response: 0
Conc: N.D.

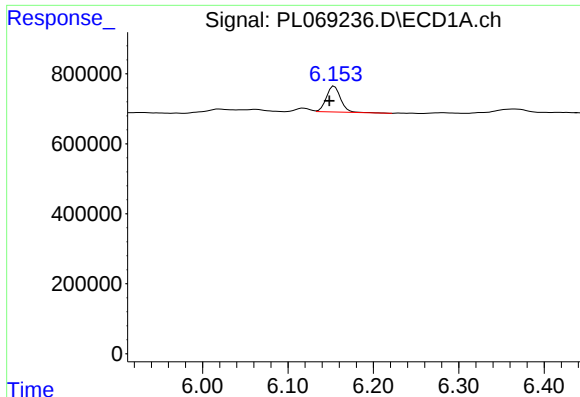

#6 beta-BHC


R.T.: 6.154 min
Delta R.T.: 0.006 min
Response: 850652
Conc: 3.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

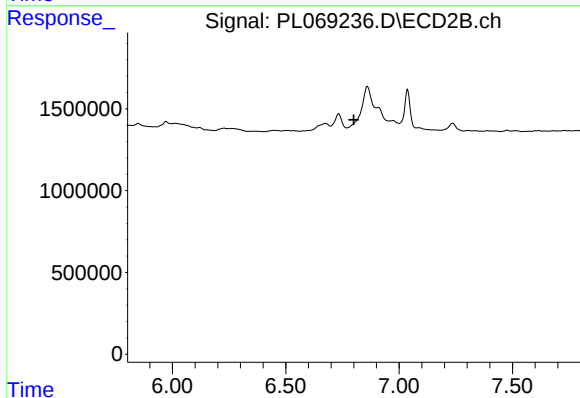


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

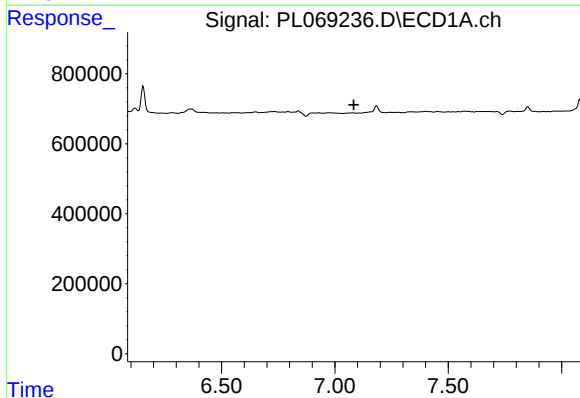


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

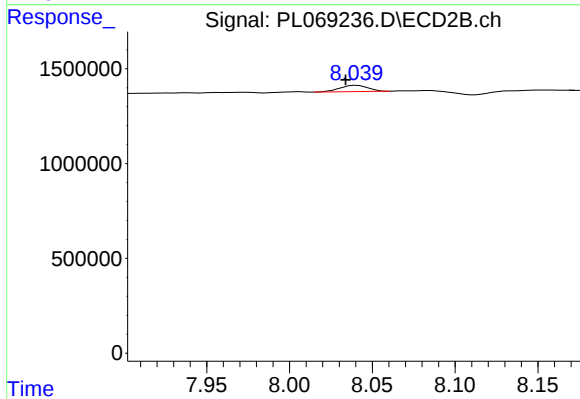

#8 Heptachlor epoxide


R.T.: 8.040 min
Delta R.T.: 0.006 min
Response: 395121
Conc: 0.34 ng/ml

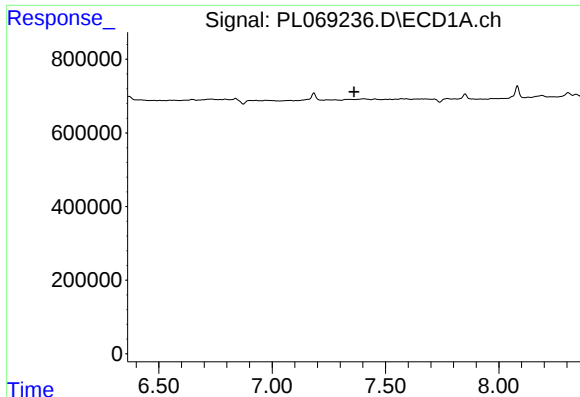

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

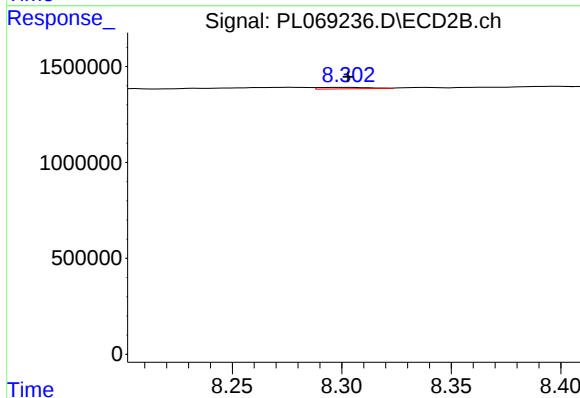


#10 gamma-Chlordane

R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 122430
Conc: 0.11 ng/ml

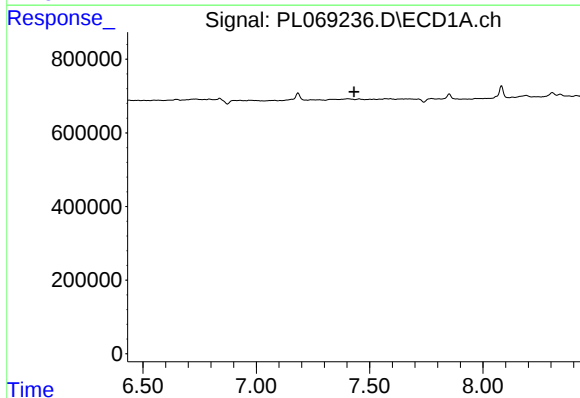


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

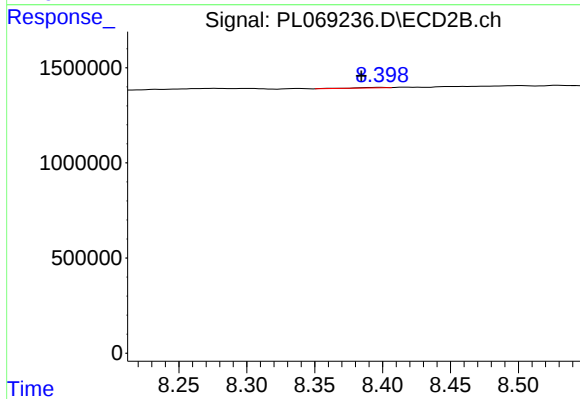

#11 alpha-Chlordane


R.T.: 8.398 min
Delta R.T.: 0.014 min
Response: 37720
Conc: 0.03 ng/ml

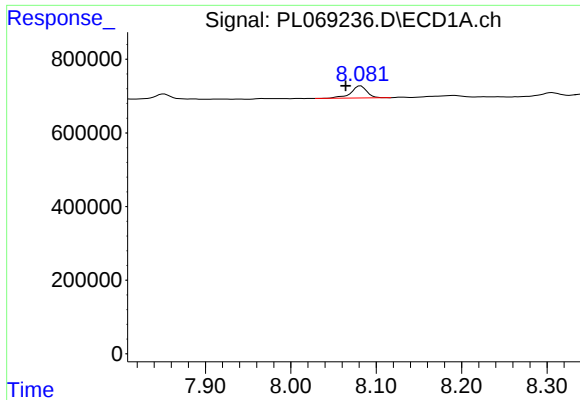

#14 Endrin


R.T.: 8.082 min
Delta R.T.: 0.018 min
Response: 431015
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

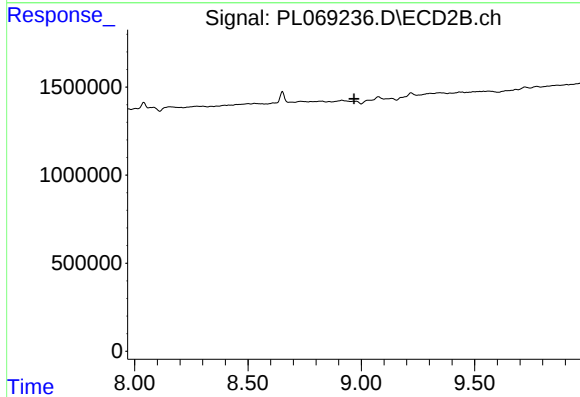


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

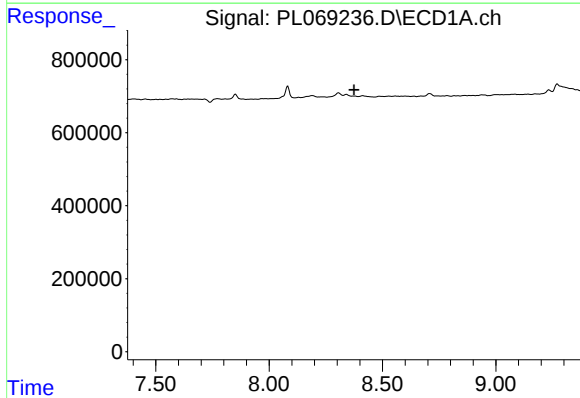


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

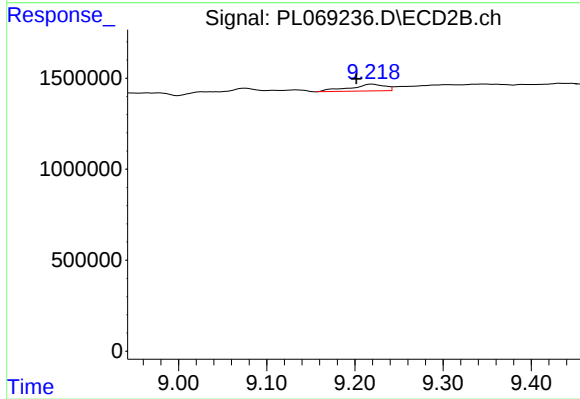

#15 Endosulfan II


R.T.: 9.219 min
Delta R.T.: 0.018 min
Response: 1045070
Conc: 1.14 ng/ml

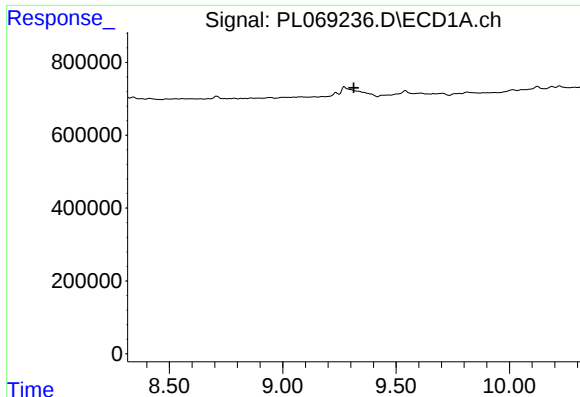

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

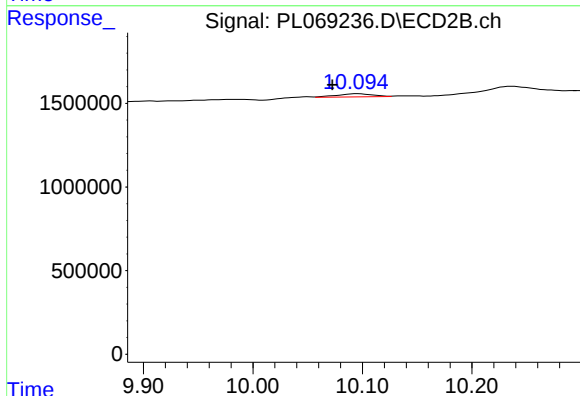


#21 Endrin ketone

R.T.: 10.096 min
Delta R.T.: 0.023 min
Response: 434842
Conc: 0.43 ng/ml

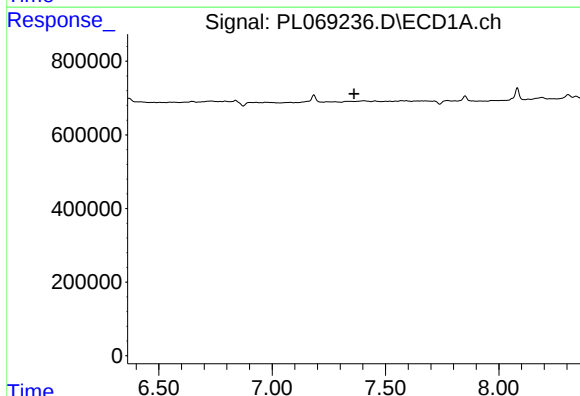


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

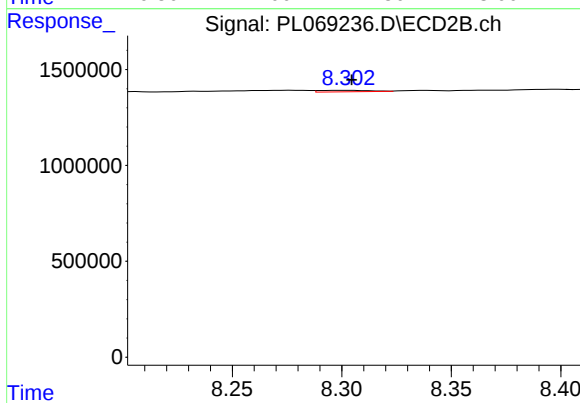

#25 Chlordane-3


R.T.: 8.303 min
Delta R.T.: -0.001 min
Response: 122430
Conc: 0.75 ng/ml

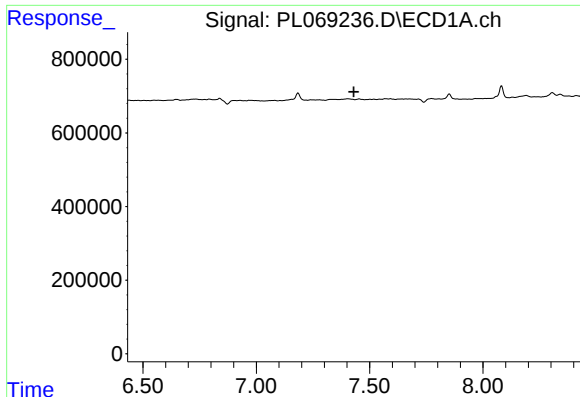

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

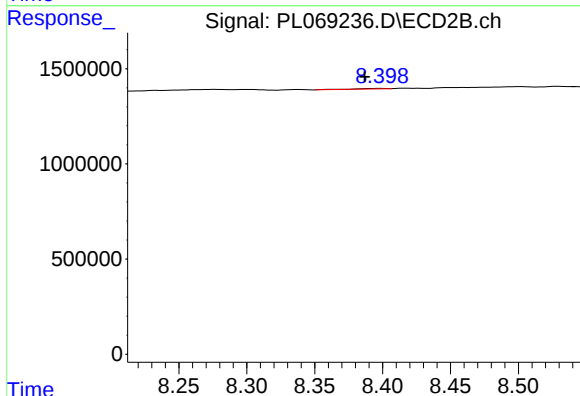


#26 Chlordane-4

R.T.: 8.398 min
Delta R.T.: 0.011 min
Response: 37720
Conc: 0.19 ng/ml

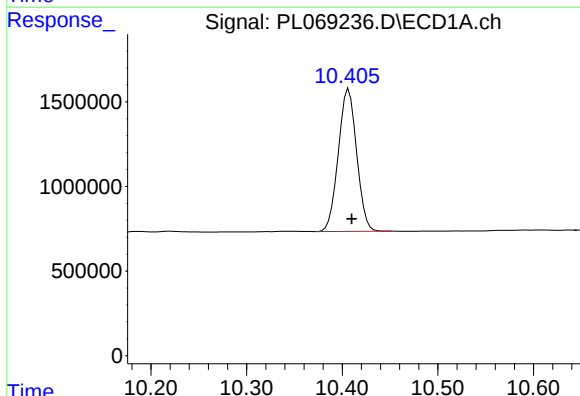

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.003 min
Response: 11236971
Conc: 19.55 ng/ml

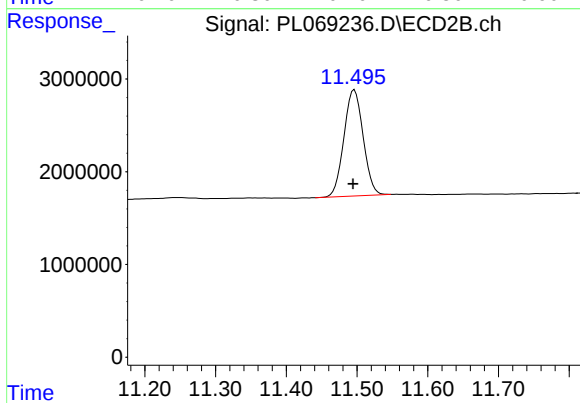

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.002 min
Response: 21716445
Conc: 22.38 ng/ml