

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
 Data File : PL069230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 12:26
 Operator : AR\AJ
 Sample : M3428-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-01-COMP

Manual Integrations
 APPROVED

mohammad
 8/20/2021 8:28:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:36:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.570	7443205	22738170	17.994	22.395
28)	SA Decachlor...	10.406	11.495	9325967	19111768	16.228	19.698
Target Compounds							
12)	B 4,4'-DDE	7.637	8.570	191263	419850	0.396m	0.397
17)	MA 4,4'-DDT	8.482	9.429	147100	315020	0.303m	0.333

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
Data File : PL069230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 12:26
Operator : AR\AJ
Sample : M3428-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-01-COMP


Manual Integrations
APPROVED

mohammad
8/20/2021 8:28:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:36:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

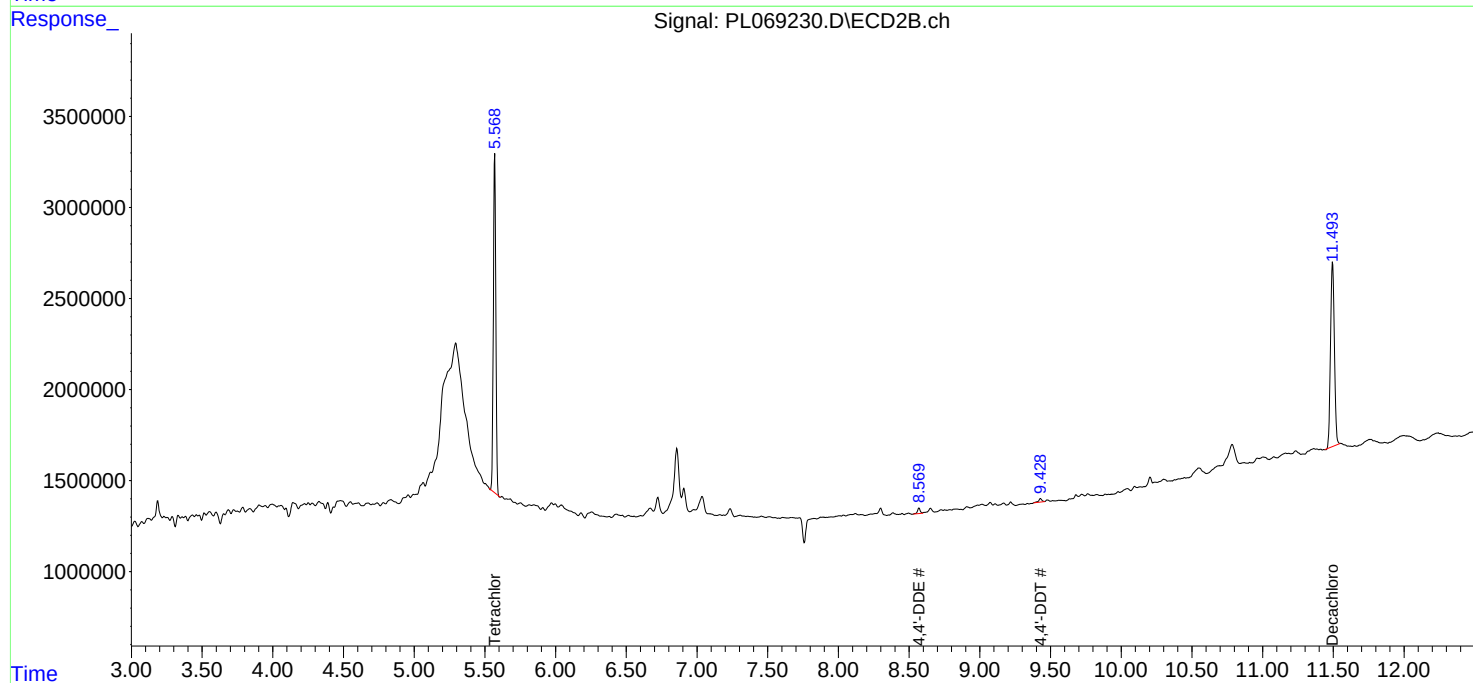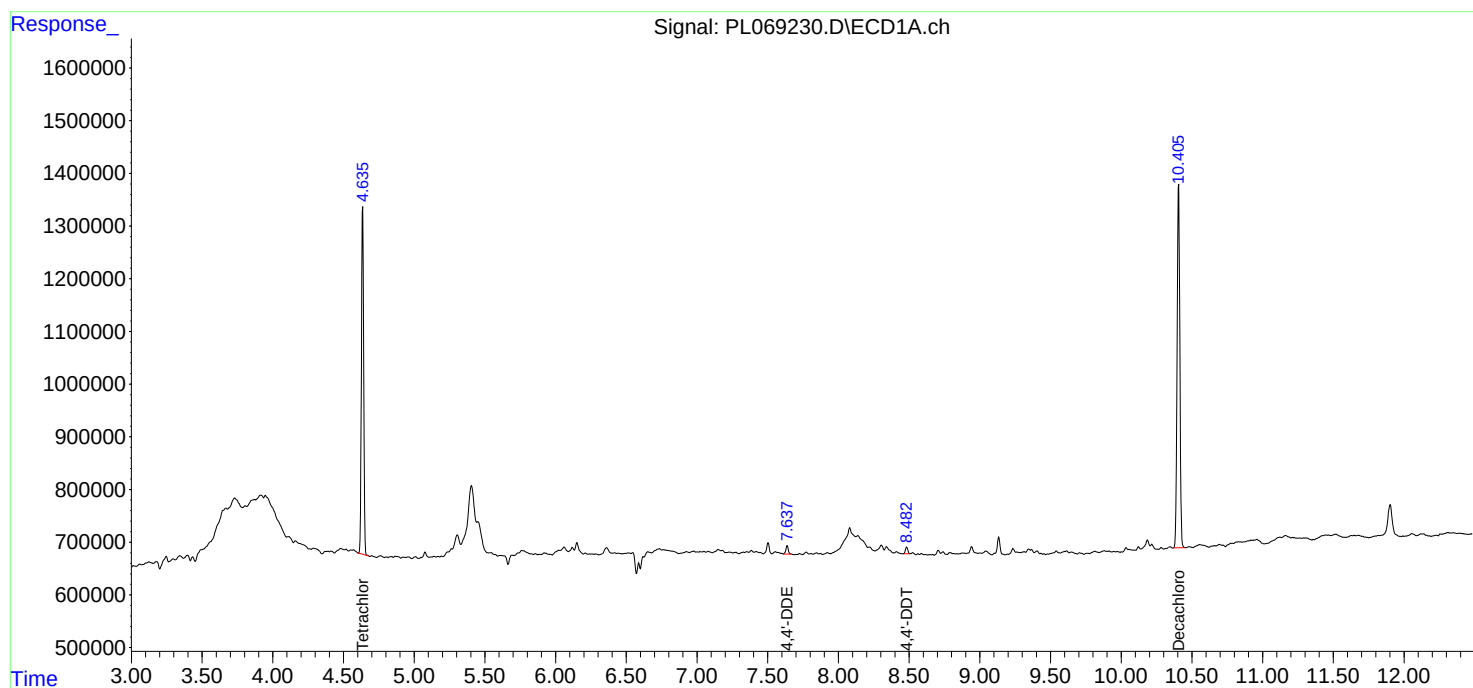

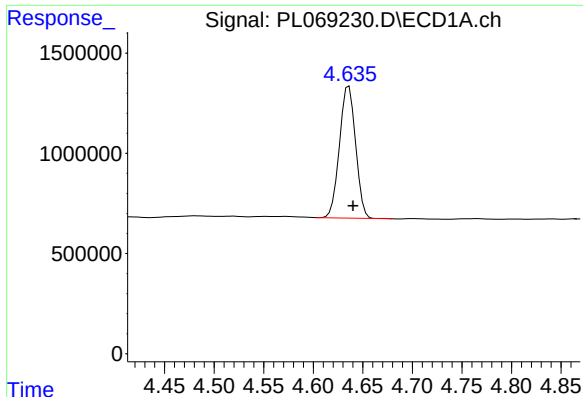


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 7443205
Conc: 17.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-COMP


Manual Integrations
APPROVED

mohammad
8/20/2021 8:28:21 AM

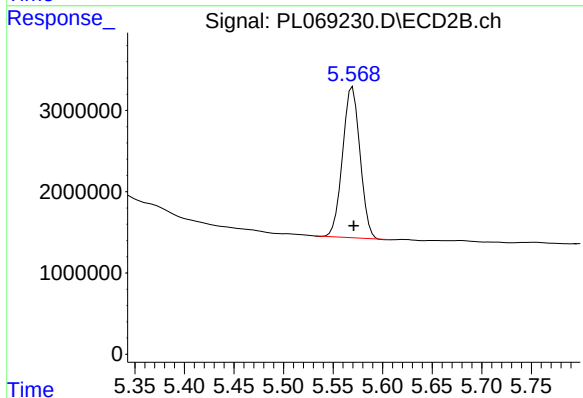


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 22738170
Conc: 22.39 ng/ml

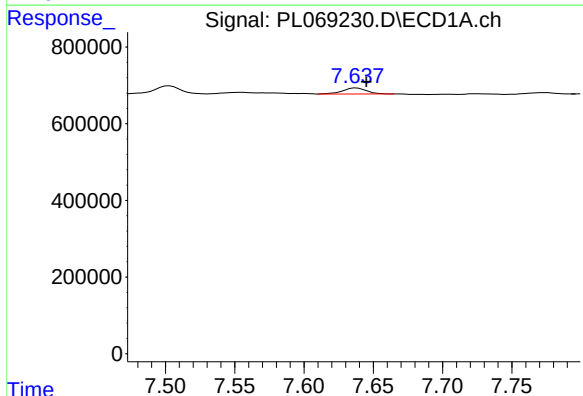


#12 4,4'-DDE

R.T.: 7.637 min
Delta R.T.: -0.008 min
Response: 191263
Conc: 0.40 ng/ml m

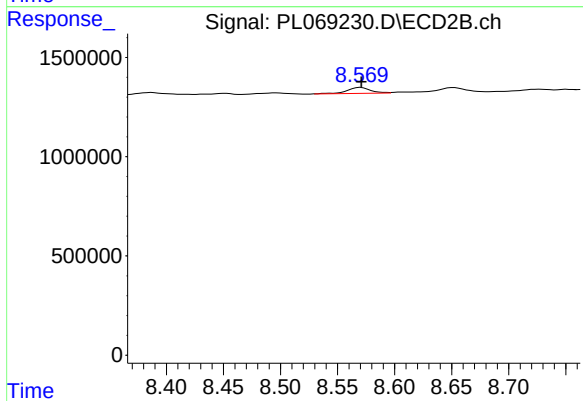

#12 4,4'-DDE

R.T.: 8.570 min
Delta R.T.: 0.000 min
Response: 419850
Conc: 0.40 ng/ml

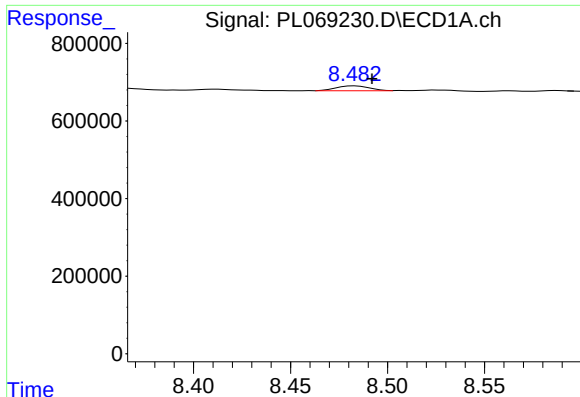


#17 4,4'-DDT

R.T.: 8.482 min
Delta R.T.: -0.010 min
Response: 147100
Conc: 0.30 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-01-COMP


Manual Integrations
APPROVED

mohammad
8/20/2021 8:28:21 AM

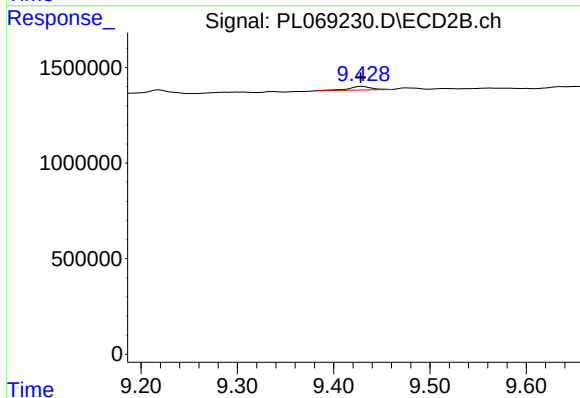


#17 4,4'-DDT

R.T.: 9.429 min
Delta R.T.: 0.001 min
Response: 315020
Conc: 0.33 ng/ml

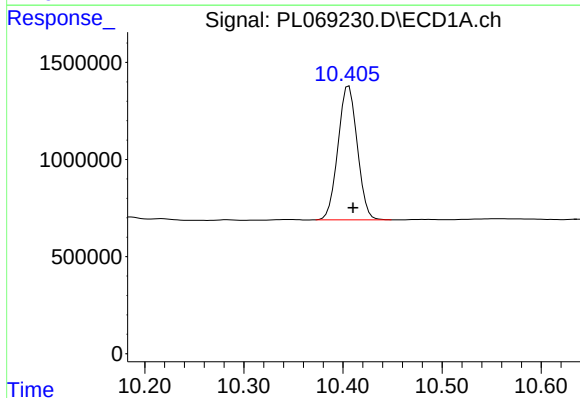

#28 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: -0.004 min
Response: 9325967
Conc: 16.23 ng/ml

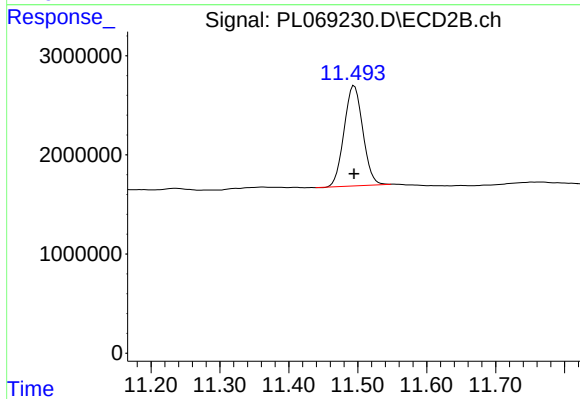

#28 Decachlorobiphenyl

R.T.: 11.495 min
Delta R.T.: 0.000 min
Response: 19111768
Conc: 19.70 ng/ml