

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081922\
 Data File : PL077216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 17:05
 Operator : AR\AJ
 Sample : N4234-01RE
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANTRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 23:06:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.420	2.634	12803893	22351872	13.058	7.808m#
2) SA Decachlor...	8.909	7.737	5981513	30584795	7.923	13.586 #
Target Compounds						
12) B 4,4'-DDE	6.085	5.065	3977928	16284240	4.559m	5.644

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081922\
Data File : PL077216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 17:05
Operator : AR\AJ
Sample : N4234-01RE
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 23:06:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

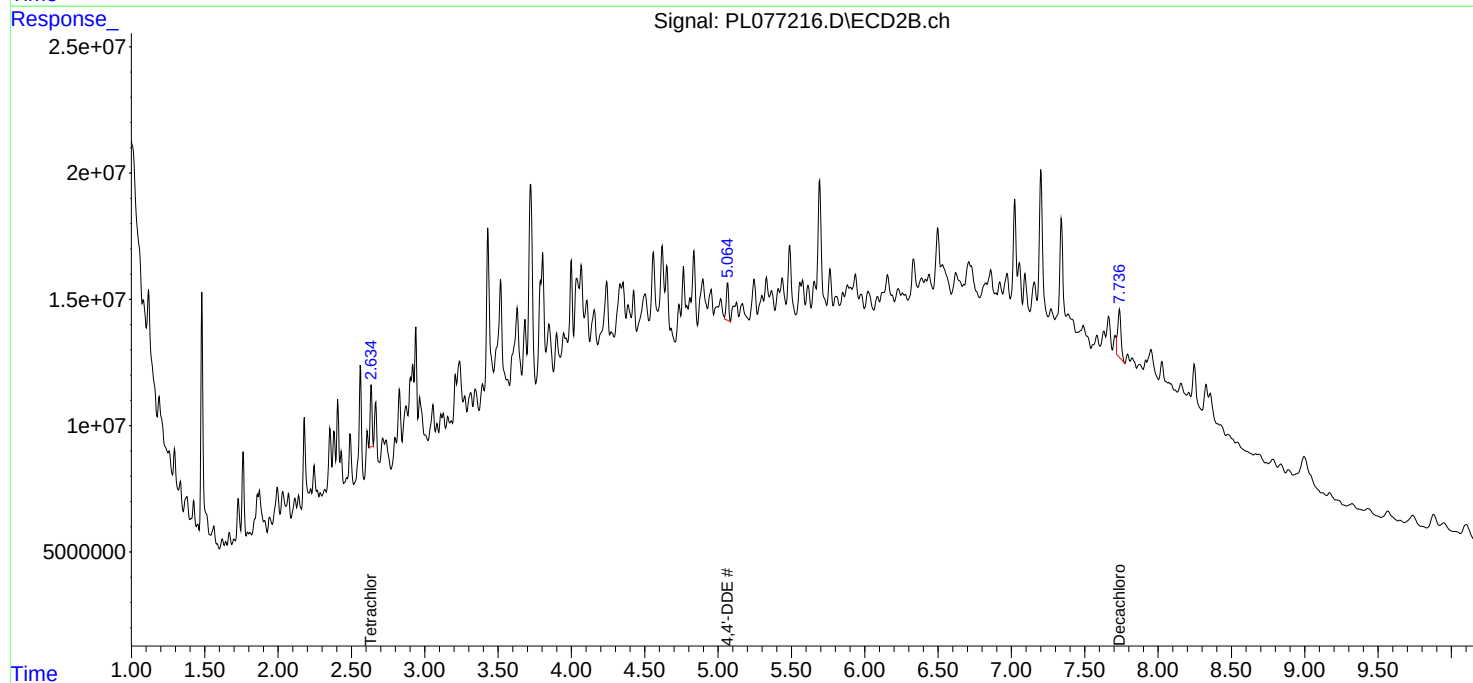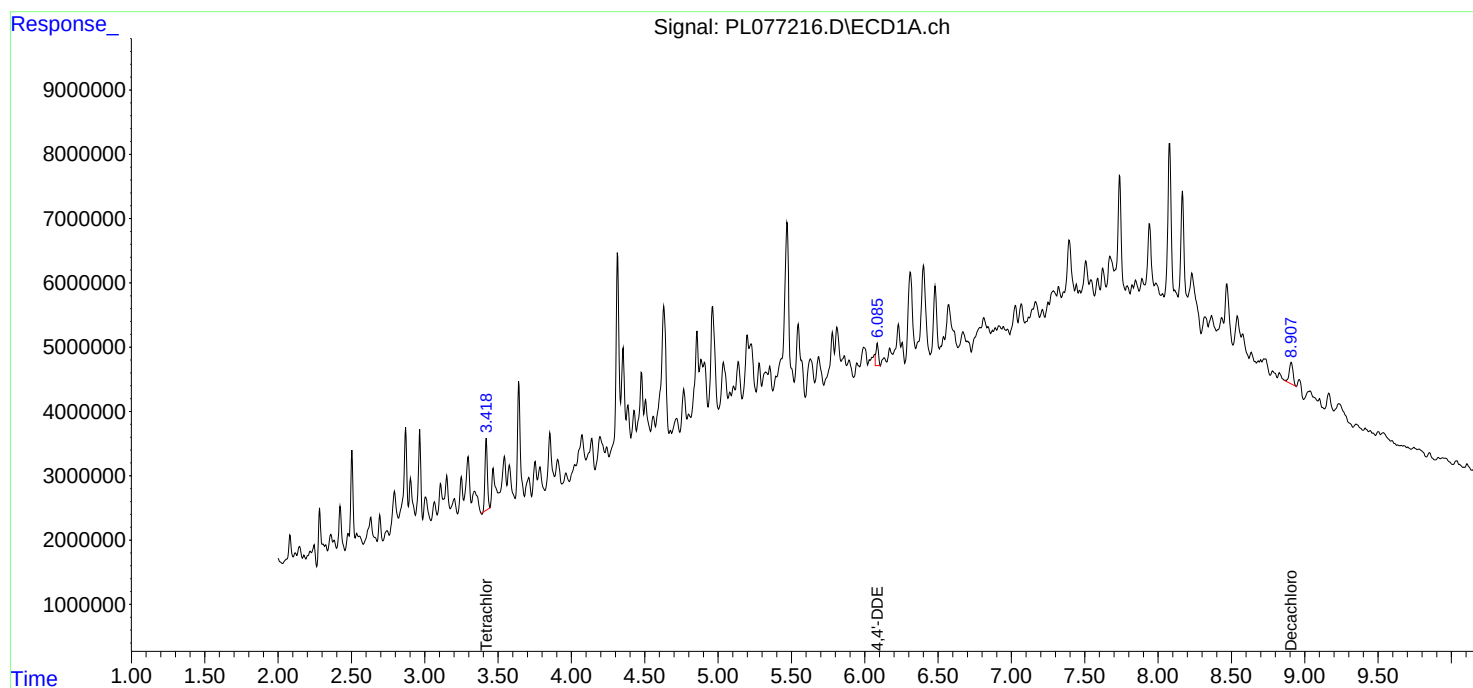

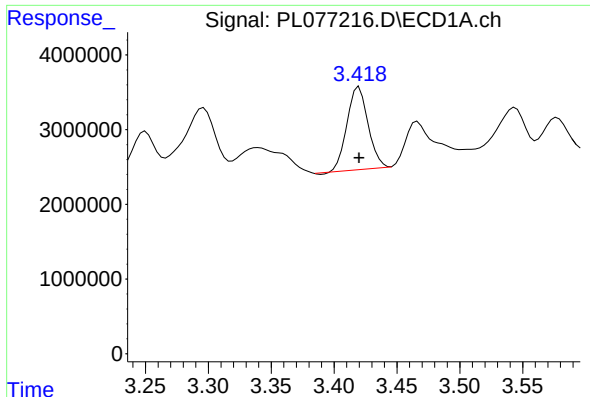


#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 12803893
Conc: 13.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

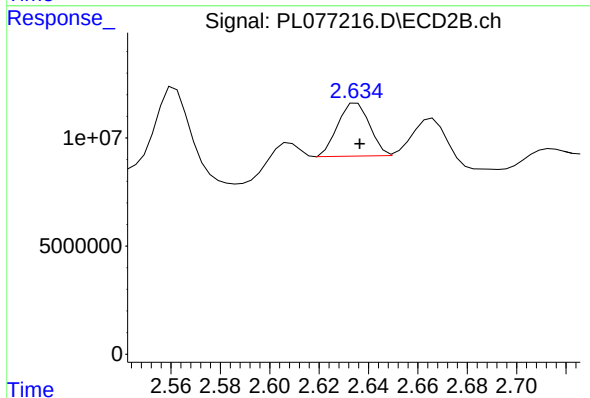


#1 Tetrachloro-m-xylene

R.T.: 2.634 min
Delta R.T.: -0.002 min
Response: 22351872
Conc: 7.81 ng/ml m

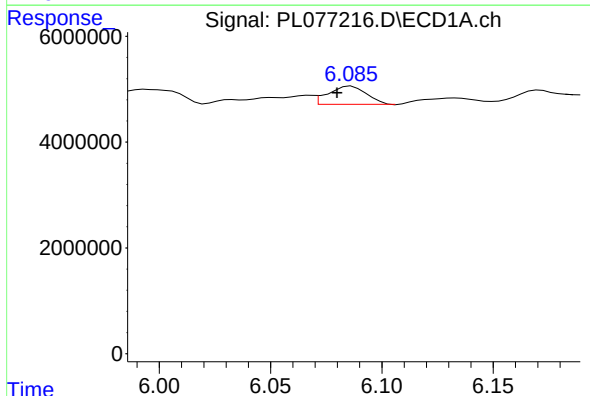


#12 4,4'-DDE

R.T.: 6.085 min
Delta R.T.: 0.005 min
Response: 3977928
Conc: 4.56 ng/ml m

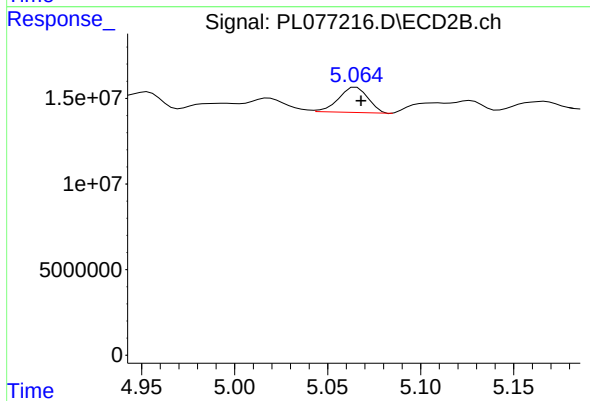

#12 4,4'-DDE

R.T.: 5.065 min
Delta R.T.: -0.002 min
Response: 16284240
Conc: 5.64 ng/ml

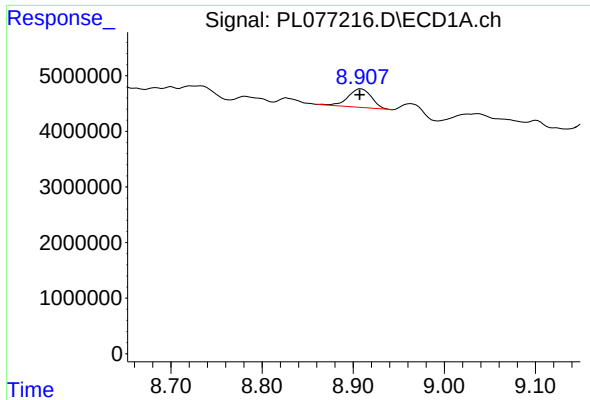


#28 Decachlorobiphenyl

R.T.: 8.909 min
Delta R.T.: 0.002 min
Response: 5981513
Conc: 7.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANTRE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

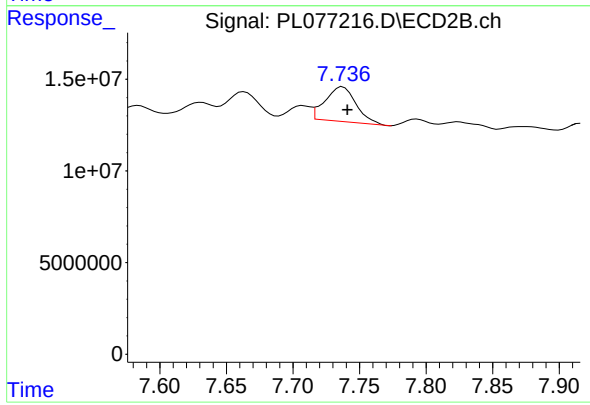

#28 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: -0.003 min
Response: 30584795
Conc: 13.59 ng/ml