

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081922\
 Data File : PL077218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2022 17:33
 Operator : AR\AJ
 Sample : N4236-01RE
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENTRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/19/2022
 Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 23:07:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.417	2.637	10143670	25647674	10.345m	8.960m
2) SA Decachlor...	8.916	7.731	6497506	7809634	8.607m	3.469m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081922\
Data File : PL077218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2022 17:33
Operator : AR\AJ
Sample : N4236-01RE
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 23:07:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

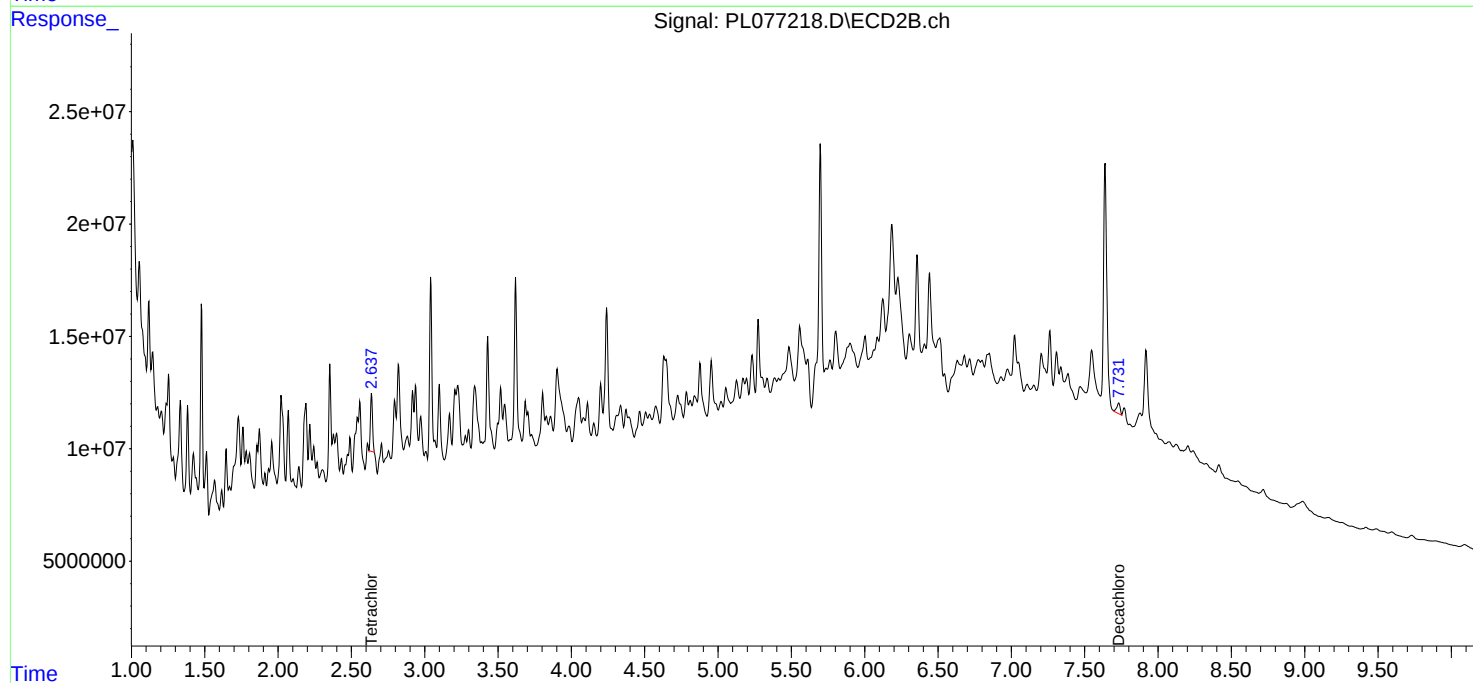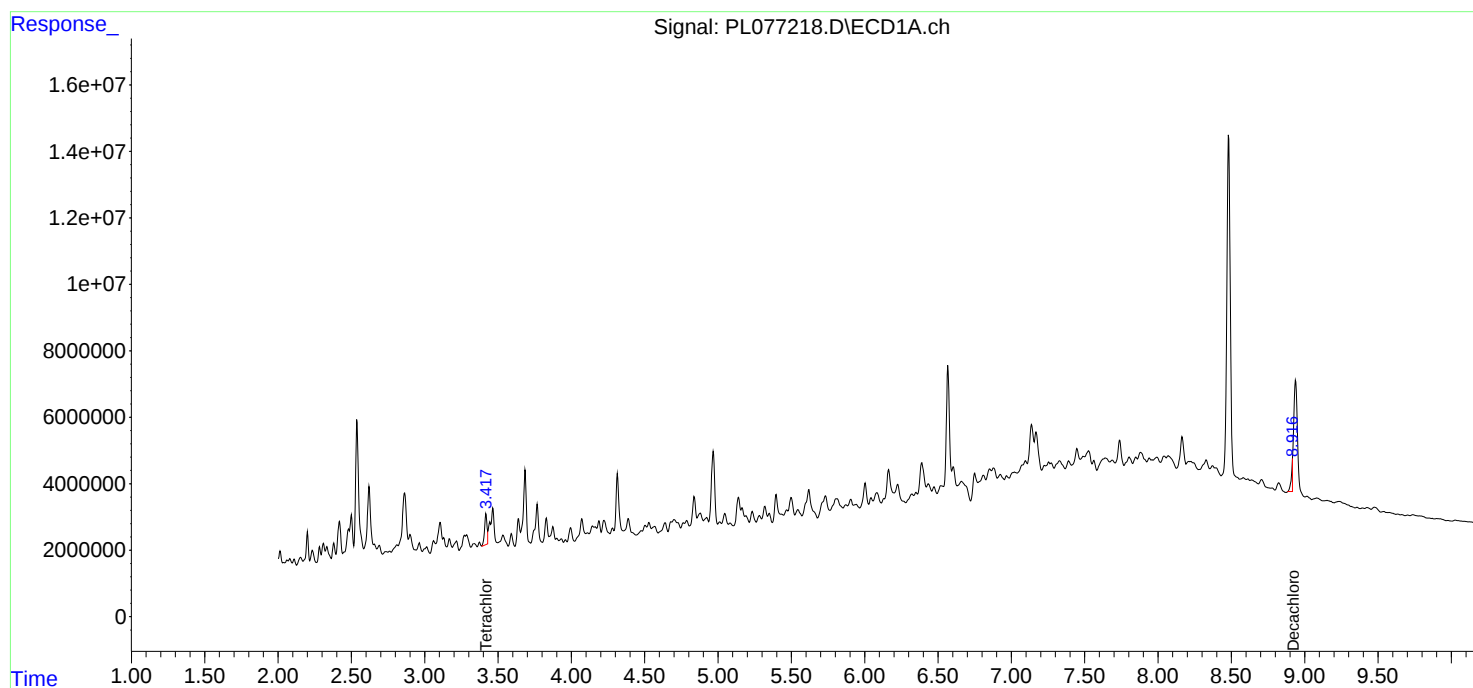

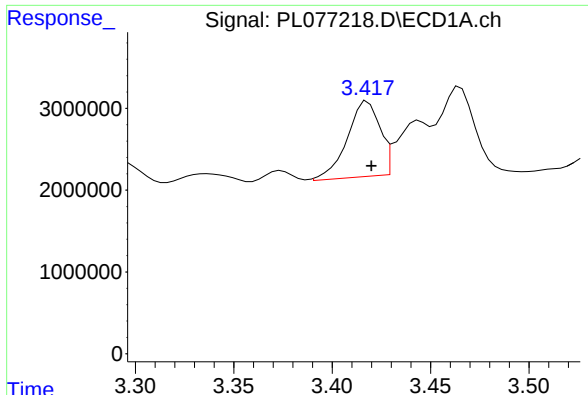


#1 Tetrachloro-m-xylene

R.T.: 3.417 min
Delta R.T.: -0.003 min
Response: 10143670
Conc: 10.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/19/2022
Supervised By :Ankita Jodhani 08/19/2022

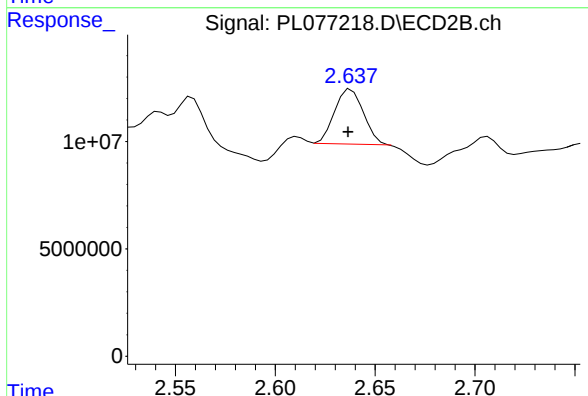


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: 0.000 min
Response: 25647674
Conc: 8.96 ng/ml m

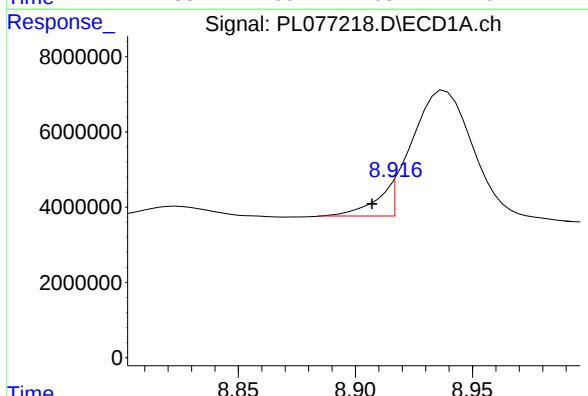

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: 0.009 min
Response: 6497506
Conc: 8.61 ng/ml m

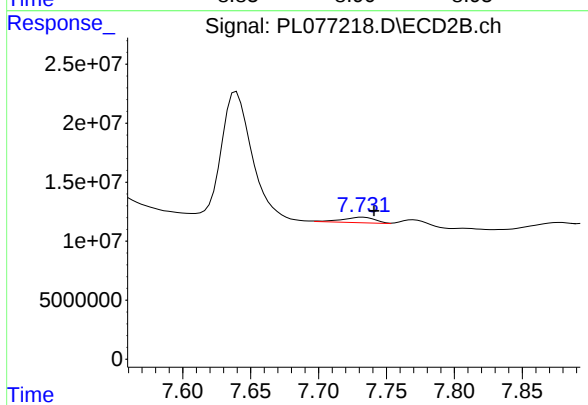

#28 Decachlorobiphenyl

R.T.: 7.731 min
Delta R.T.: -0.010 min
Response: 7809634
Conc: 3.47 ng/ml m