

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081925\
 Data File : PL096906.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 19:03
 Operator : AR\AJ
 Sample : Q2892-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 1-FLOOR-NORTH-EAST-CORNER-BACK-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:39:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.825	86551319	91995855	27.211	19.255 #
28)	SA Decachlor...	9.003	7.986	42552721	77478950	17.844	17.859
Target Compounds							
8)	B Heptachlo...	5.667	0.000	15604900	0	4.046	N.D. #
9)	A Endosulfan I	0.000	5.185f	0	10044812	N.D.	1.816 #
12)	B 4,4'-DDE	6.158	5.299	11817334	17061873	3.680	3.094
13)	MA Dieldrin	0.000	5.428	0	12619362	N.D.	2.137 #
14)	MA Endrin	0.000	5.712	0	6240166	N.D.	1.154 #
15)	B Endosulfa...	6.784f	6.027f	6792750	7846143	2.121	1.528 #
17)	MA 4,4'-DDT	6.981	6.103	10679763	20287003	3.724	4.011
18)	B Endrin al...	0.000	6.169	0	13640868	N.D.	3.753 #
27)	Chlordane-5	0.000	6.027f	0	7846143	N.D.	30.756 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081925\
Data File : PL096906.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2025 19:03
Operator : AR\AJ
Sample : Q2892-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-NORTH-EAST-CORNER-BACK-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:39:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

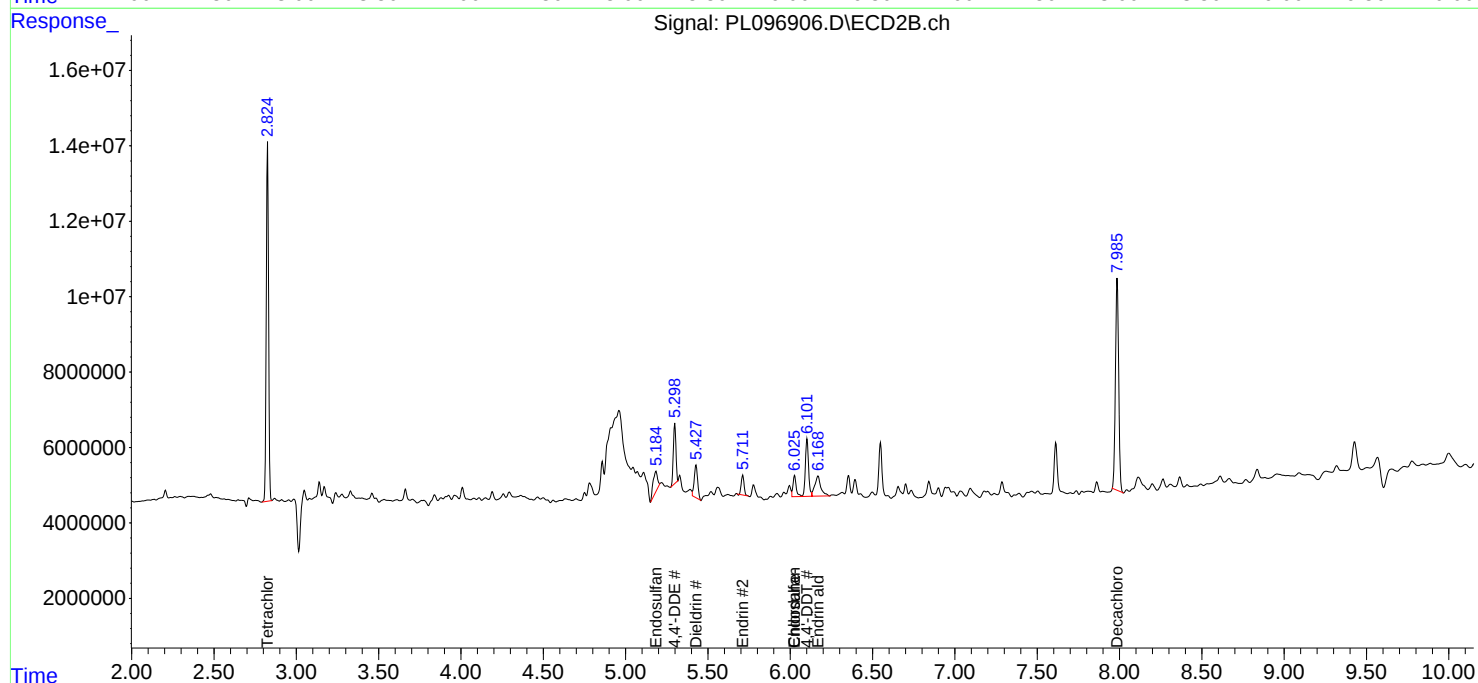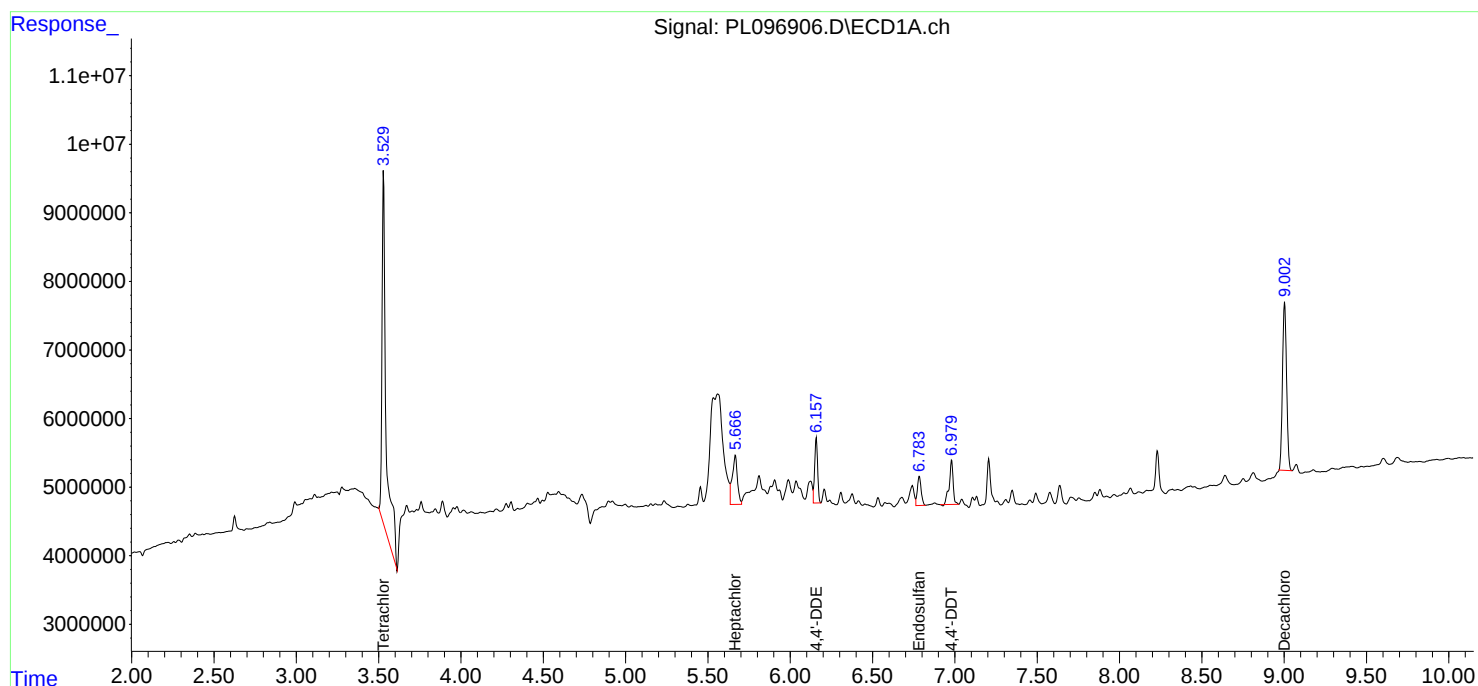


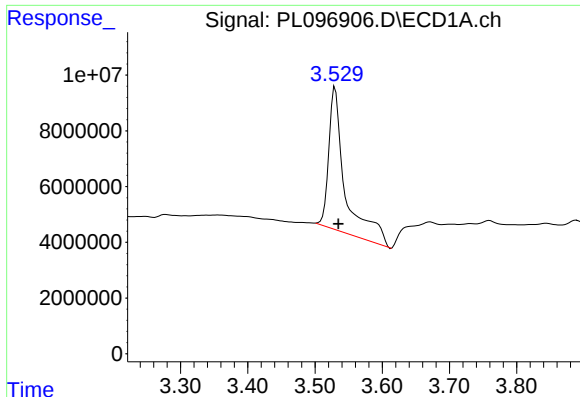

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: -0.005 min
Response: 86551319
Conc: 27.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-NORTH-EAST-CORNER-BACK-A

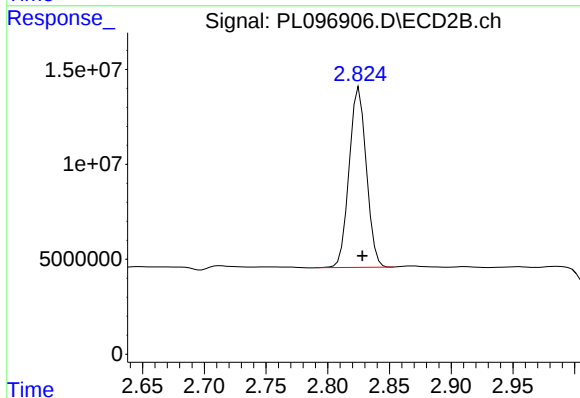


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.002 min
Response: 91995855
Conc: 19.25 ng/ml

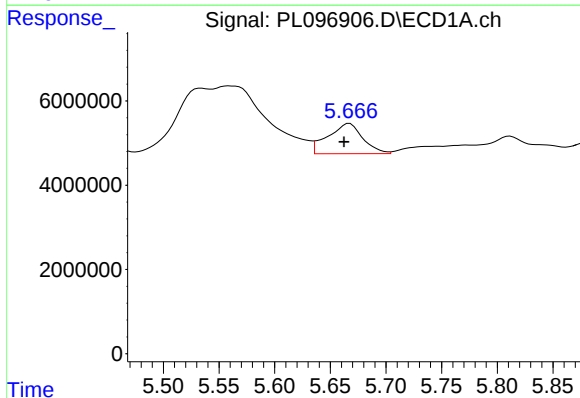


#8 Heptachlor epoxide

R.T.: 5.667 min
Delta R.T.: 0.005 min
Response: 15604900
Conc: 4.05 ng/ml

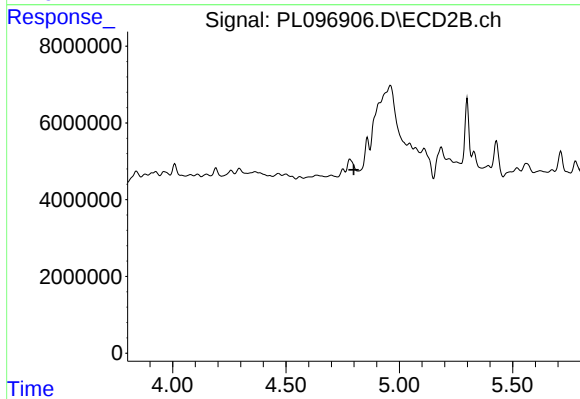

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.799 min
Response: 0
Conc: N.D.

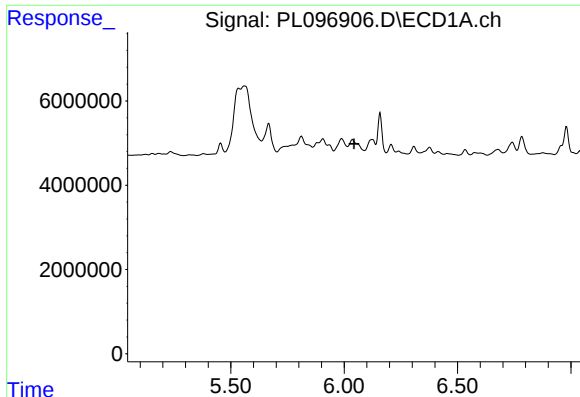

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.044 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-NORTH-EAST-CORNER-BACK-A

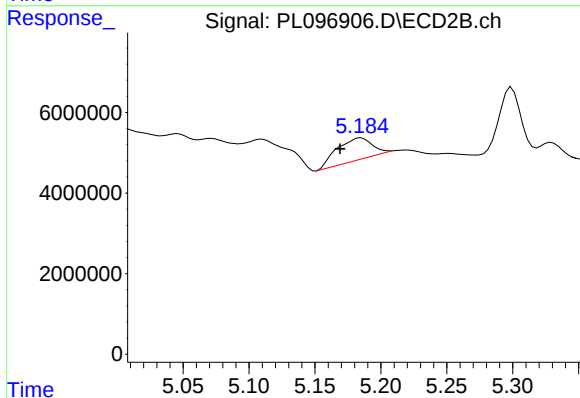


#9 Endosulfan I

R.T.: 5.185 min
Delta R.T.: 0.016 min
Response: 10044812
Conc: 1.82 ng/ml

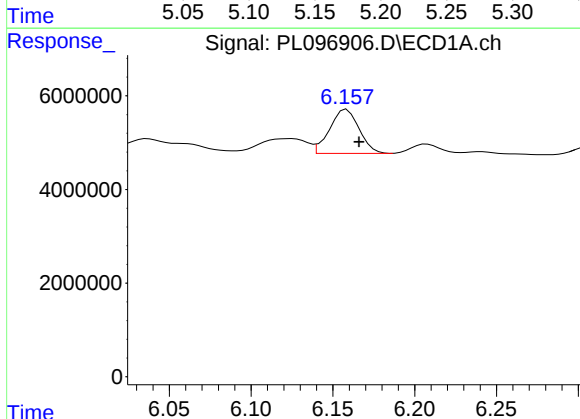


#12 4,4'-DDE

R.T.: 6.158 min
Delta R.T.: -0.008 min
Response: 11817334
Conc: 3.68 ng/ml

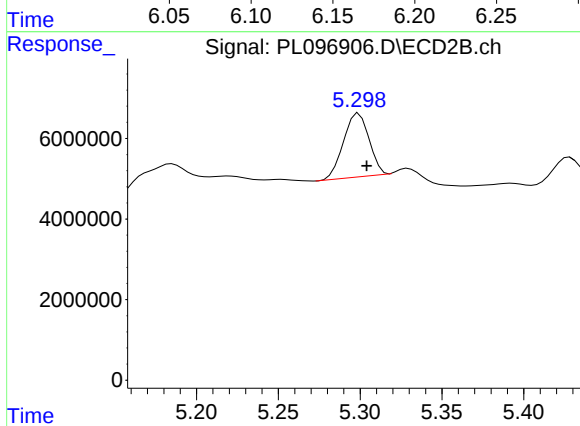

#12 4,4'-DDE


R.T.: 5.299 min
Delta R.T.: -0.005 min
Response: 17061873
Conc: 3.09 ng/ml

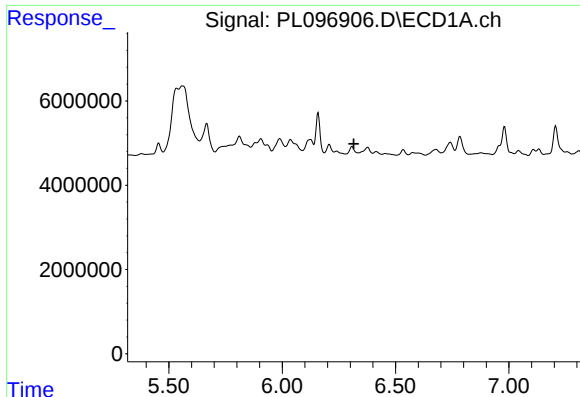

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-NORTH-EAST-CORNER-BACK-A

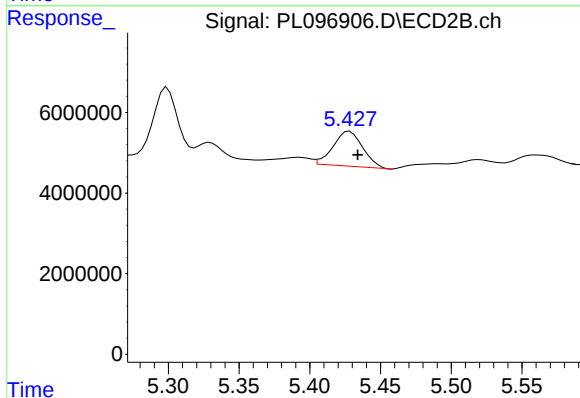


#13 Dieldrin

R.T.: 5.428 min
Delta R.T.: -0.006 min
Response: 12619362
Conc: 2.14 ng/ml

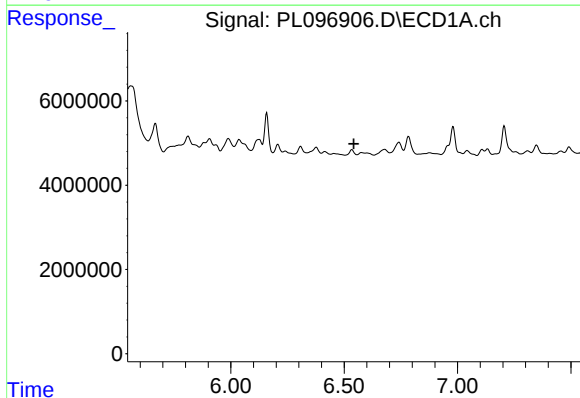


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.542 min
Response: 0
Conc: N.D.

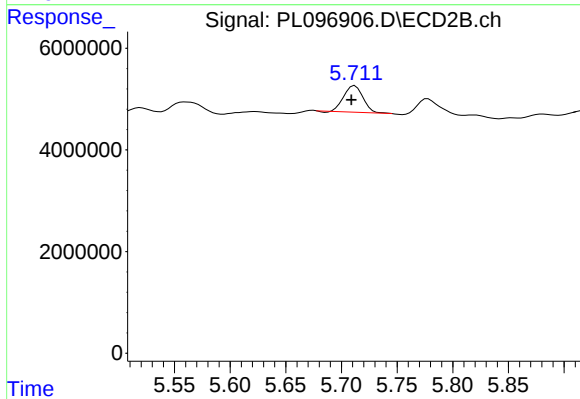

#14 Endrin

R.T.: 5.712 min
Delta R.T.: 0.003 min
Response: 6240166
Conc: 1.15 ng/ml

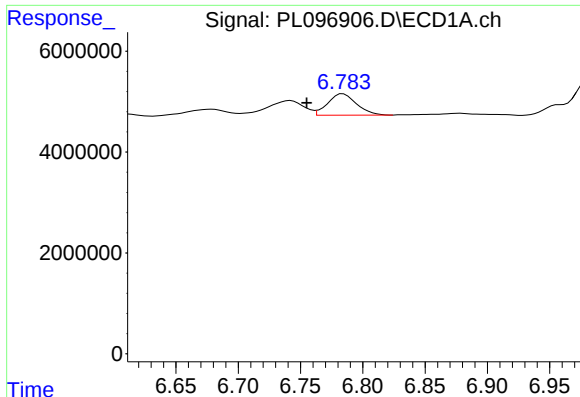

#15 Endosulfan II


R.T.: 6.784 min
Delta R.T.: 0.029 min
Response: 6792750
Conc: 2.12 ng/ml

Instrument :

ECD_L


ClientSampleId :

1-FLOOR-NORTH-EAST-CORNER-BACK-A

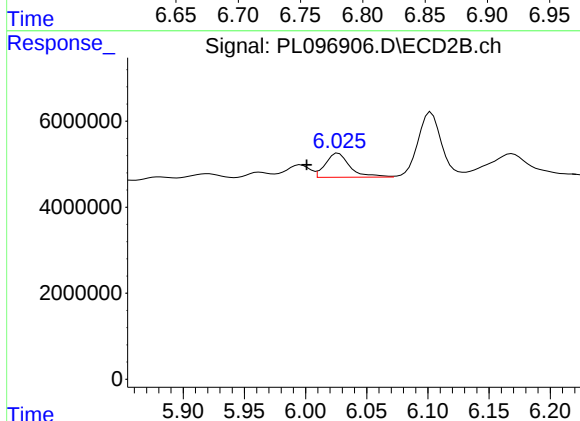


#15 Endosulfan II

R.T.: 6.027 min
Delta R.T.: 0.026 min
Response: 7846143
Conc: 1.53 ng/ml

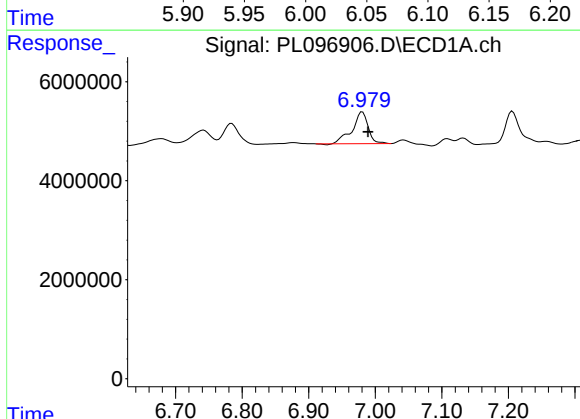


#17 4,4'-DDT

R.T.: 6.981 min
Delta R.T.: -0.009 min
Response: 10679763
Conc: 3.72 ng/ml

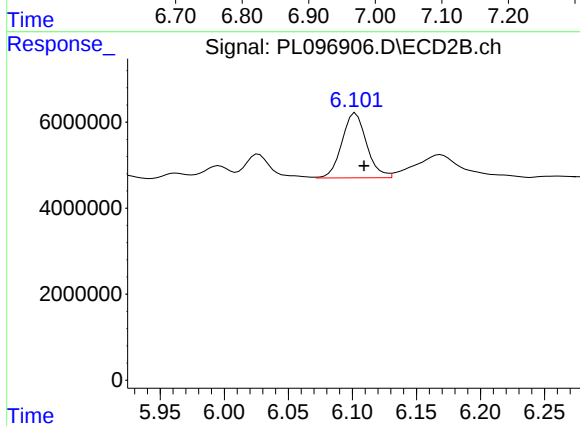

#17 4,4'-DDT


R.T.: 6.103 min
Delta R.T.: -0.006 min
Response: 20287003
Conc: 4.01 ng/ml

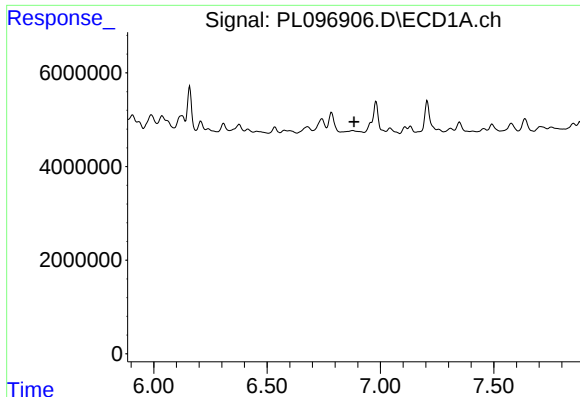

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-NORTH-EAST-CORNER-BACK-A

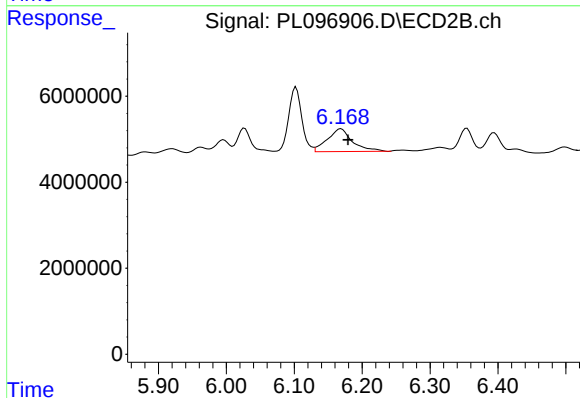


#18 Endrin aldehyde

R.T.: 6.169 min
Delta R.T.: -0.010 min
Response: 13640868
Conc: 3.75 ng/ml

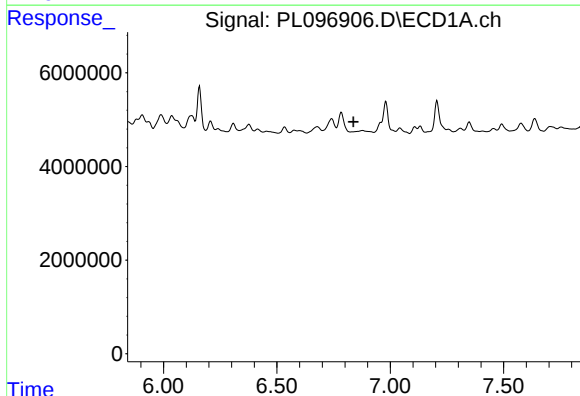


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.838 min
Response: 0
Conc: N.D.

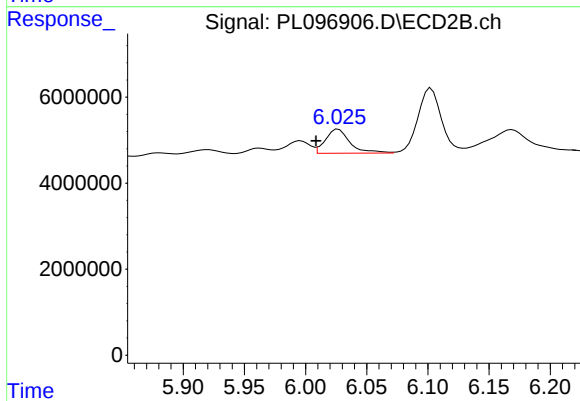

#27 Chlordane-5


R.T.: 6.027 min
Delta R.T.: 0.018 min
Response: 7846143
Conc: 30.76 ng/ml

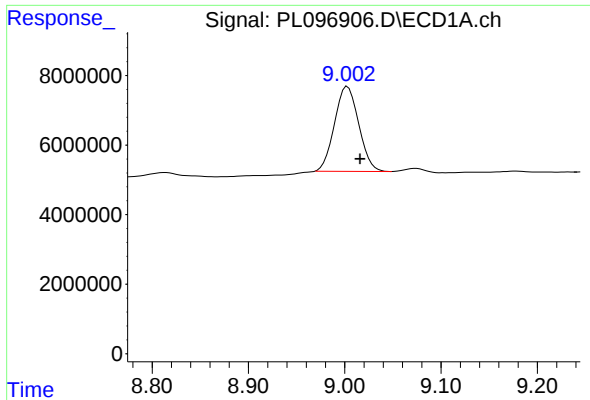

#28 Decachlorobiphenyl

R.T.: 9.003 min
Delta R.T.: -0.013 min
Response: 42552721
Conc: 17.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
1-FLOOR-NORTH-EAST-CORNER-BACK-A

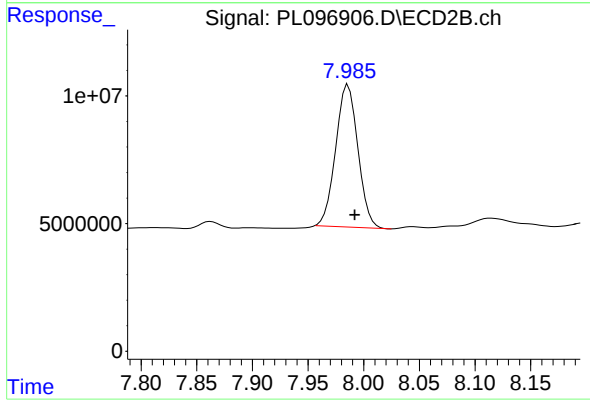

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 77478950
Conc: 17.86 ng/ml