

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081925\
 Data File : PL096900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2025 17:42
 Operator : AR\AJ
 Sample : Q2683-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DSN003

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/20/2025
 Supervised By : mohammad ahmed 08/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 01:38:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.530	2.825	52017419	98136279	16.354m	20.540m#
28) SA Decachlor...	9.002	7.986	43977674	64653189	18.442m	14.903
Target Compounds						
13) MA Dieldrin	6.306	5.443	19089824	27269135	5.144	4.617

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081925\
Data File : PL096900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2025 17:42
Operator : AR\AJ
Sample : Q2683-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DSN003


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/20/2025
Supervised By : mohammad ahmed 08/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 01:38:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

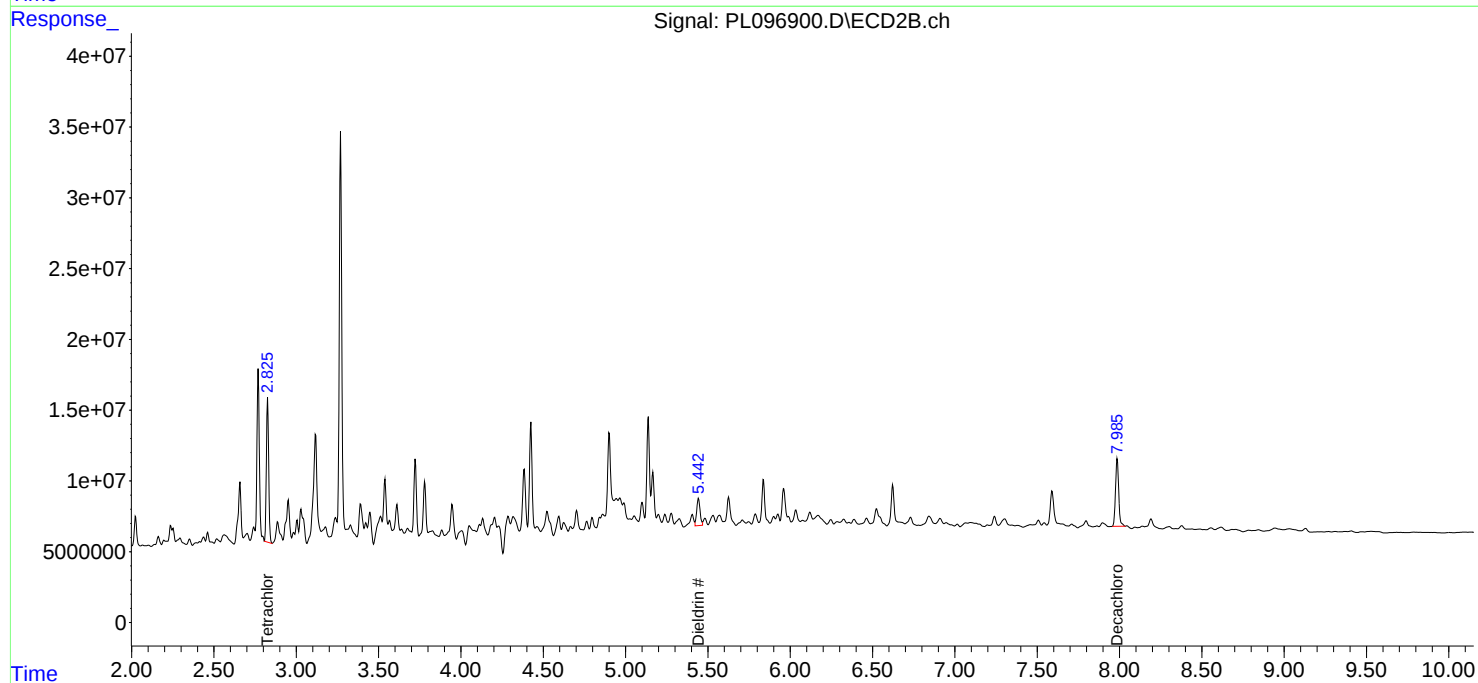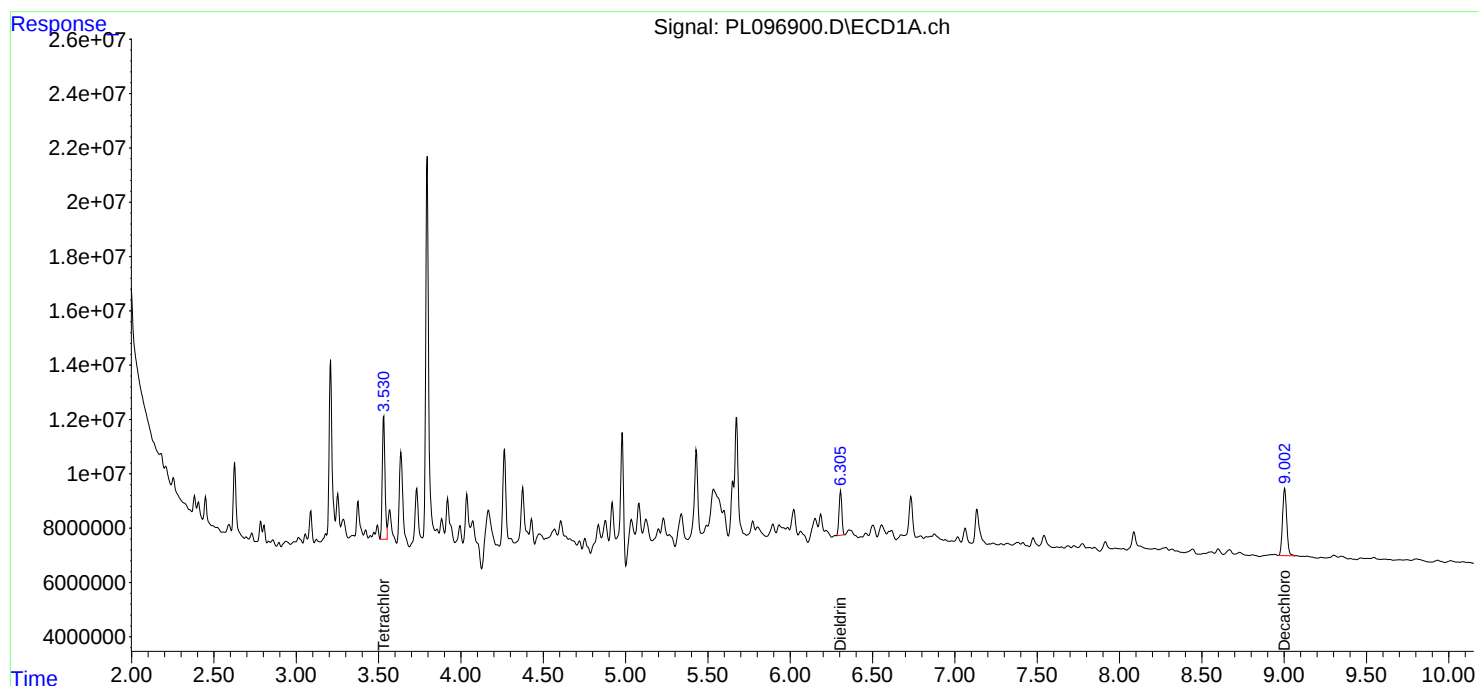

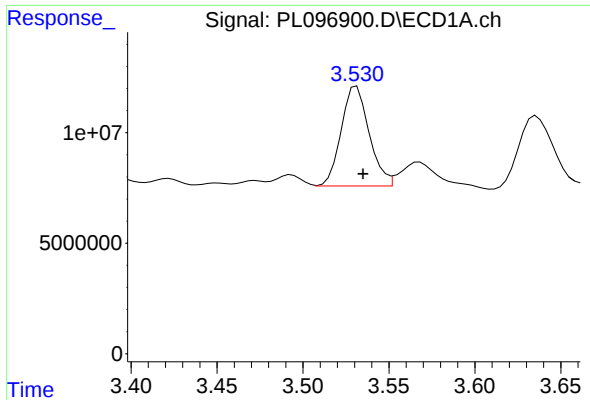


#1 Tetrachloro-m-xylene

R.T.: 3.530 min
Delta R.T.: -0.005 min
Response: 52017419
Conc: 16.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
DSN003


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/20/2025
Supervised By :mohammad ahmed 08/21/2025

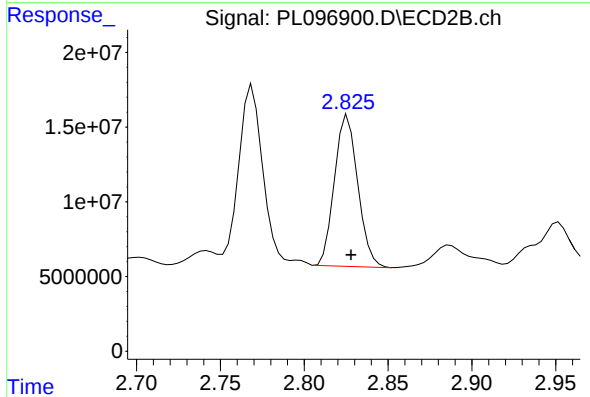


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.003 min
Response: 98136279
Conc: 20.54 ng/ml m

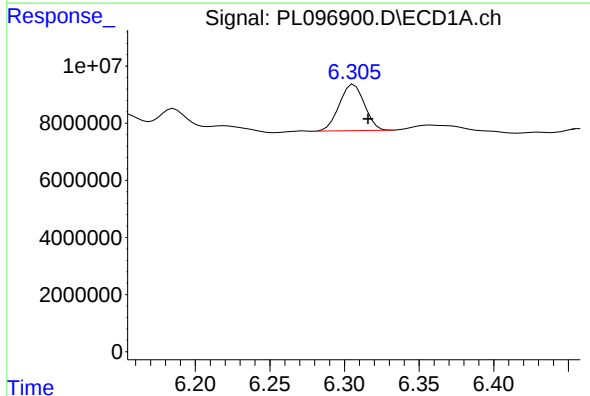


#13 Dieldrin

R.T.: 6.306 min
Delta R.T.: -0.009 min
Response: 19089824
Conc: 5.14 ng/ml

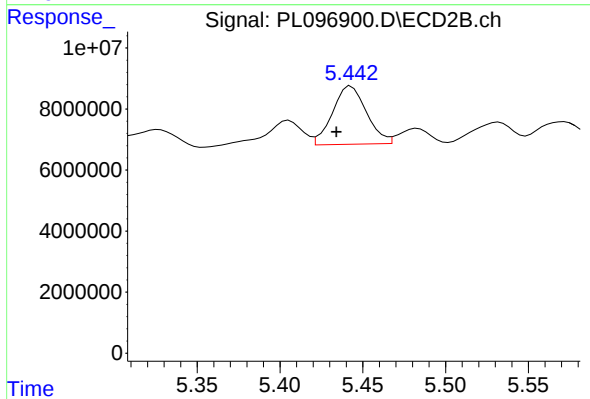

#13 Dieldrin

R.T.: 5.443 min
Delta R.T.: 0.009 min
Response: 27269135
Conc: 4.62 ng/ml

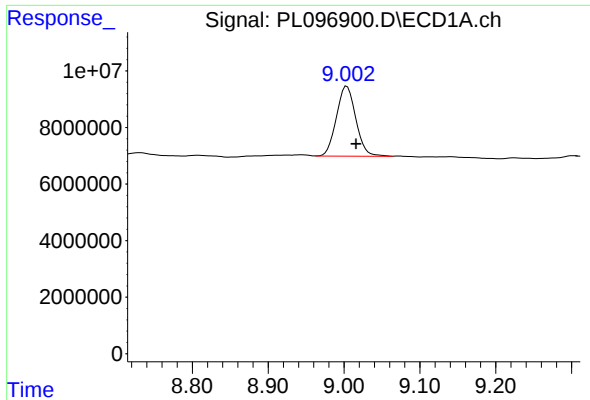


#28 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: -0.013 min
Response: 43977674
Conc: 18.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
DSN003

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/20/2025
Supervised By :mohammad ahmed 08/21/2025

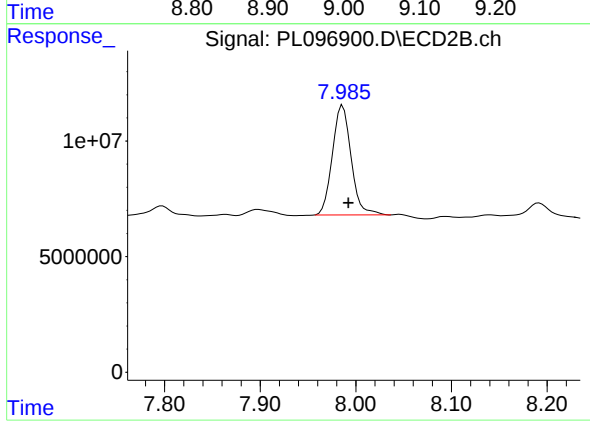

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 64653189
Conc: 14.90 ng/ml