

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082018\
 Data File : PL039314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2018 11:56
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:16:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	4.920f	0.000	1414352	0	0.148	N.D. #
14) MA	Endrin	5.796	0.000	14457869	0	1.615	N.D. #
17) MA	4,4'-DDT	6.167	0.000	56520869	0	7.456	N.D. #
18) B	Endrin al...	6.167f	0.000	56520869	0	8.340	N.D. #
20) A	Methoxychlor	6.635f	0.000	22150376	0	5.413	N.D. #
24)	Chlordane-2	4.674	0.000	4785614	0	13.689	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082018\
Data File : PL039314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2018 11:56
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:16:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

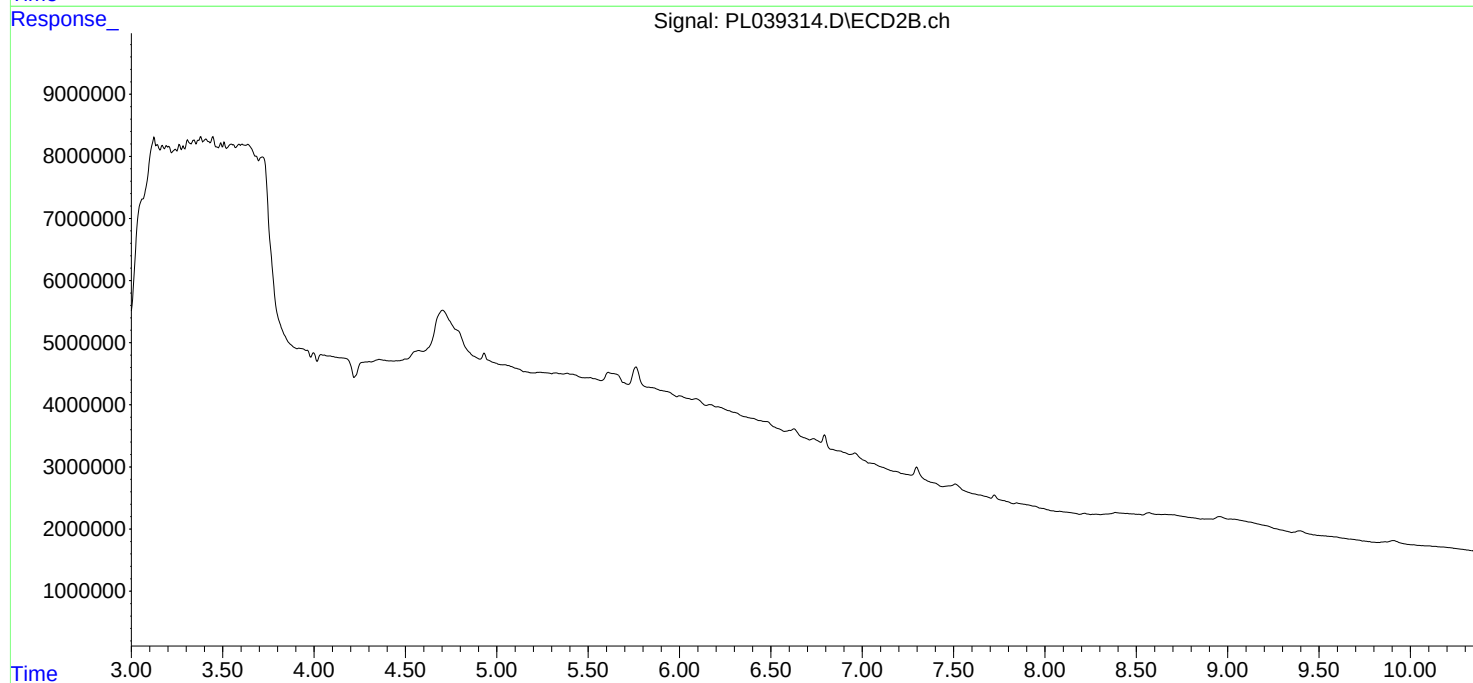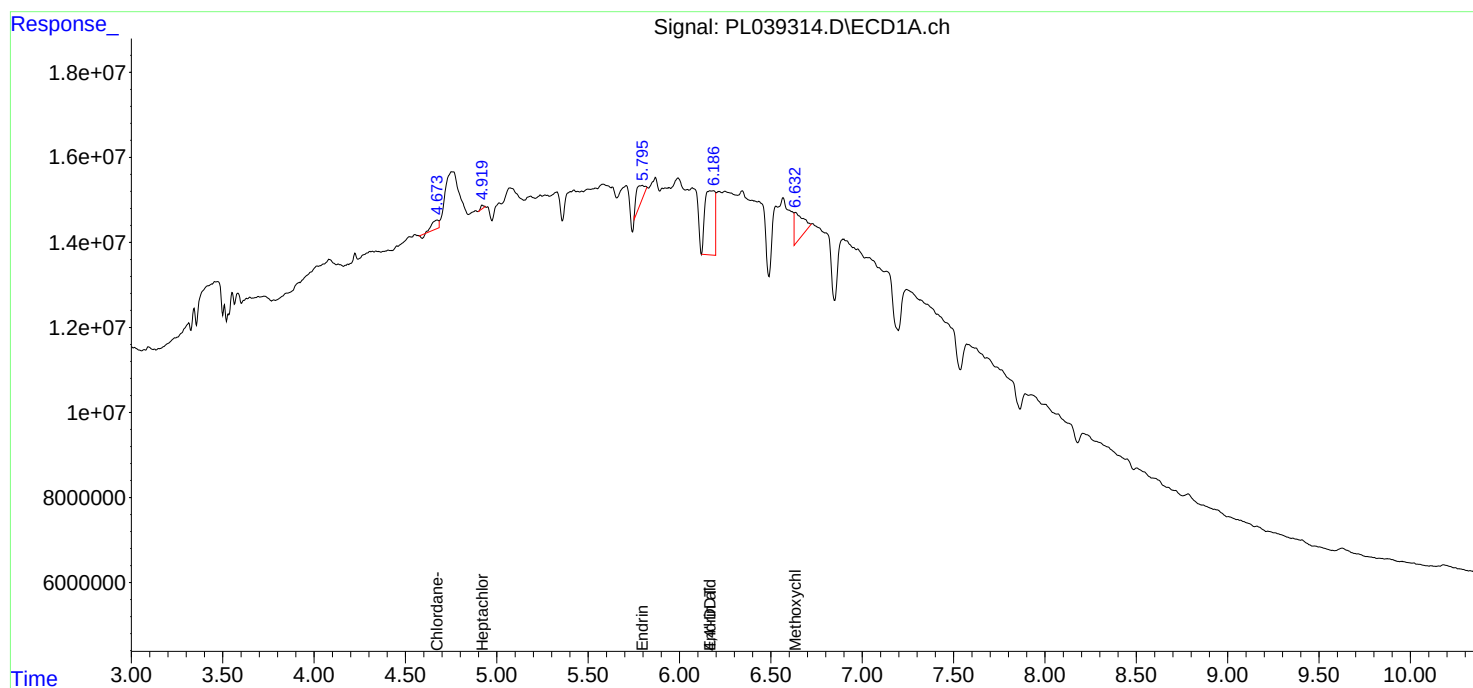


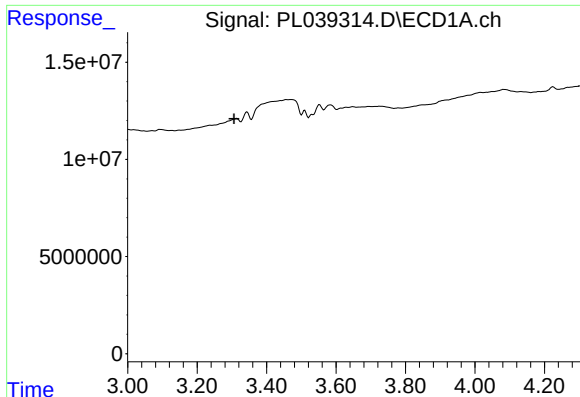

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.306 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

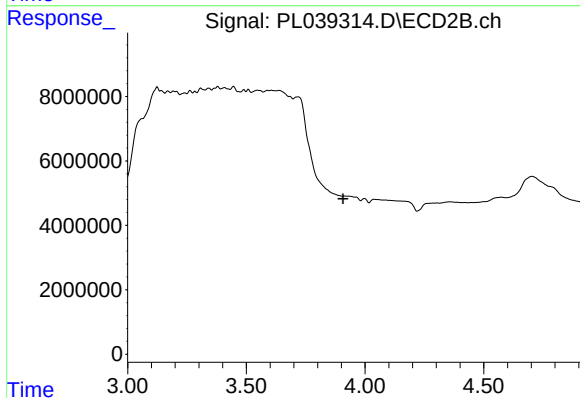


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.907 min
Response: 0
Conc: N.D.

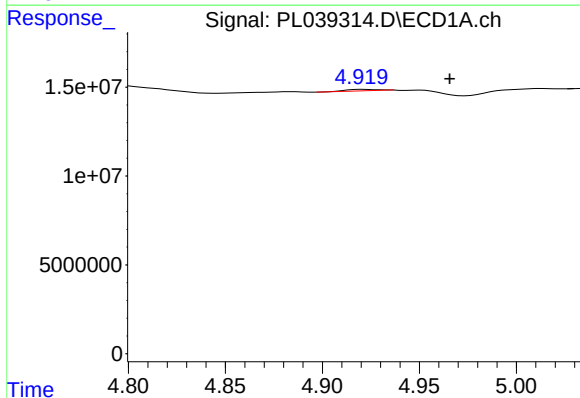


#8 Heptachlor epoxide

R.T.: 4.920 min
Delta R.T.: -0.045 min
Response: 1414352
Conc: 0.15 ng/ml

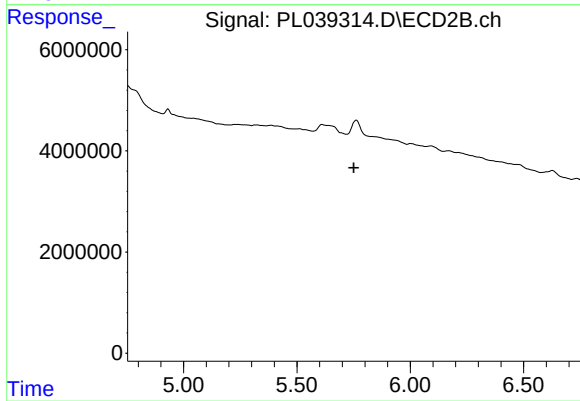

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.751 min
Response: 0
Conc: N.D.

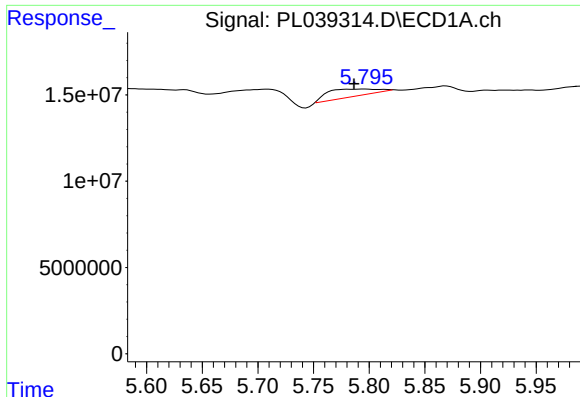

#14 Endrin


R.T.: 5.796 min
Delta R.T.: 0.010 min
Response: 14457869
Conc: 1.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

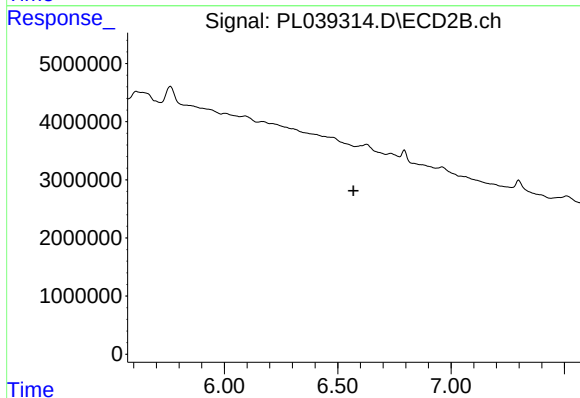


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

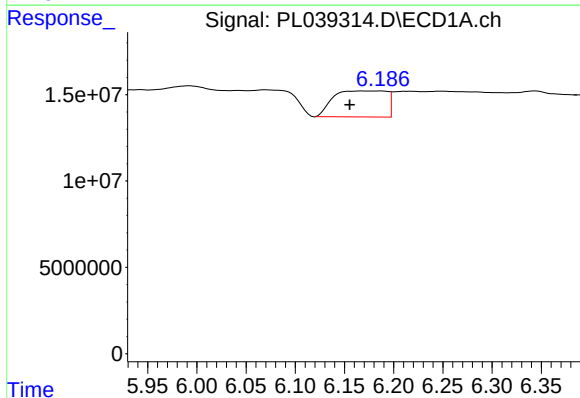


#17 4,4'-DDT

R.T.: 6.167 min
Delta R.T.: 0.011 min
Response: 56520869
Conc: 7.46 ng/ml

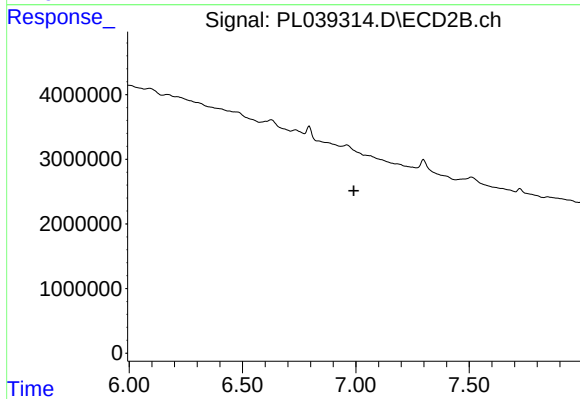

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

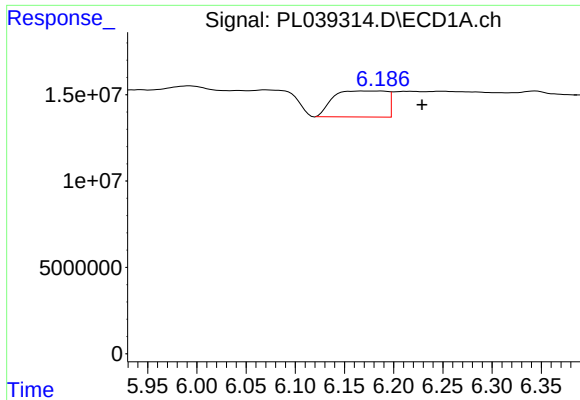

#18 Endrin aldehyde


R.T.: 6.167 min
Delta R.T.: -0.062 min
Response: 56520869
Conc: 8.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

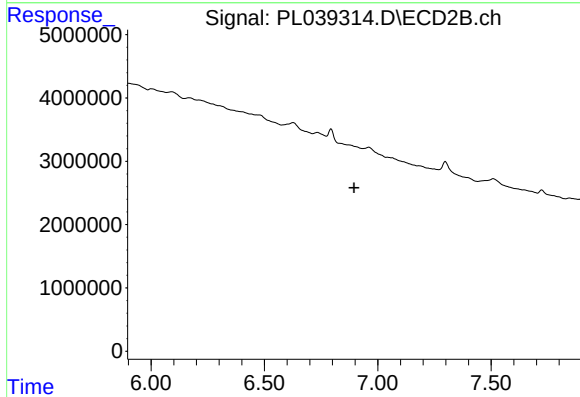


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

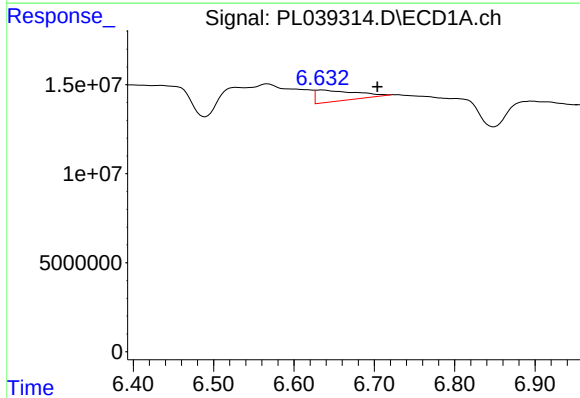


#20 Methoxychlor

R.T.: 6.635 min
Delta R.T.: -0.069 min
Response: 22150376
Conc: 5.41 ng/ml

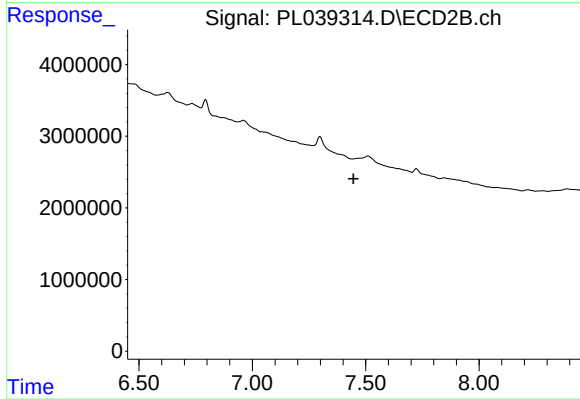

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

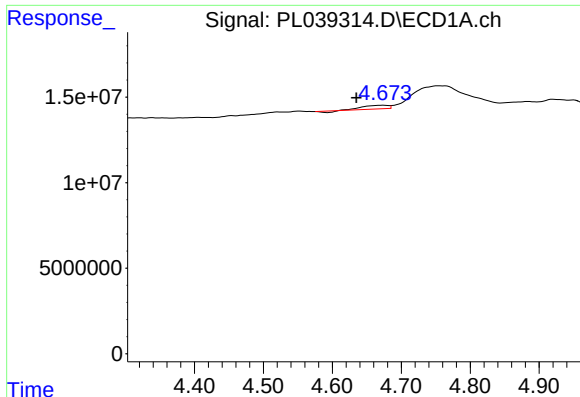

#24 Chlordane-2


R.T.: 4.674 min
Delta R.T.: 0.040 min
Response: 4785614
Conc: 13.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

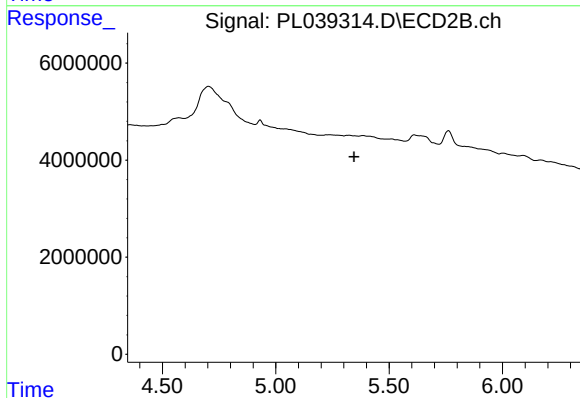


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

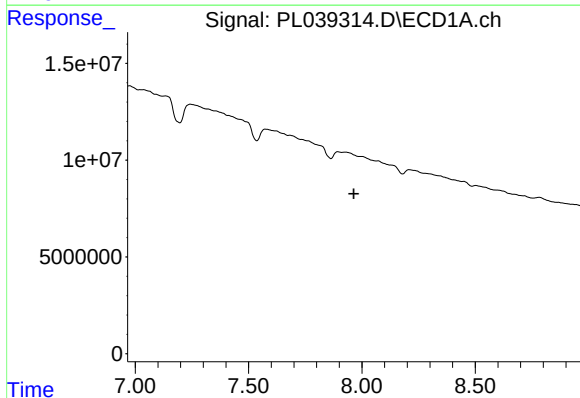

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.964 min
Response: 0
Conc: N.D.

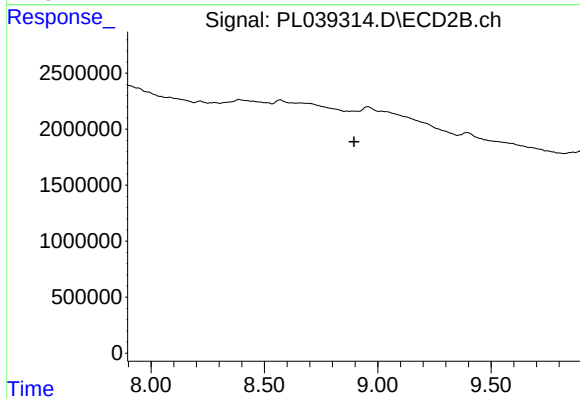

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.896 min
Response: 0
Conc: N.D.