

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082018\
 Data File : PL039330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2018 17:22
 Operator : AJ\SJ
 Sample : J4538-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:22:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	83788673	37122829	11.986	13.847
28)	SA Decachlor...	7.959	8.892	72361567	28642351	10.303	12.343
Target Compounds							
2)	A alpha-BHC	3.692f	0.000	15078056	0	1.276	N.D. #
6)	B beta-BHC	4.215f	0.000	12144810	0	2.614	N.D. #
8)	B Heptachlo...	4.917f	0.000	1945048	0	0.204	N.D. #
23)	Chlordane-1	4.077	0.000	20972843	0	66.247	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082018\
Data File : PL039330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2018 17:22
Operator : AJ\SJ
Sample : J4538-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:22:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

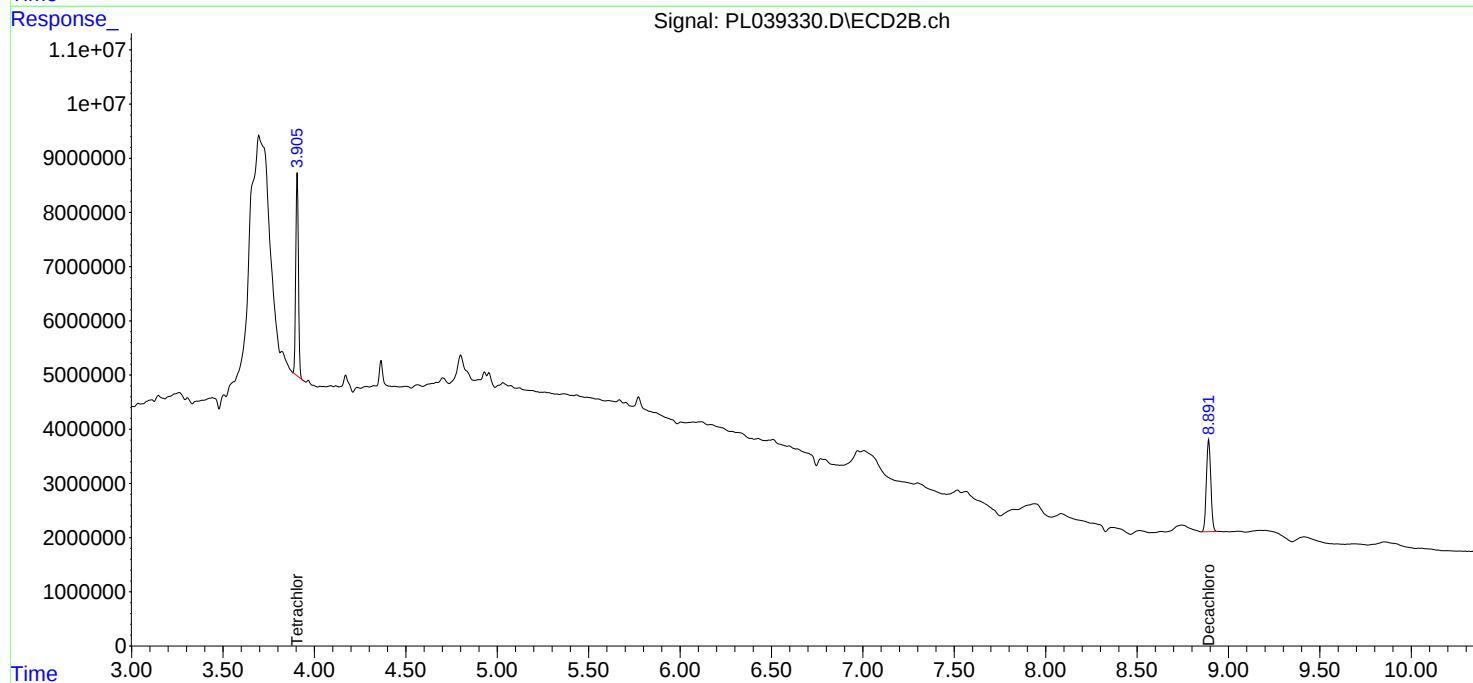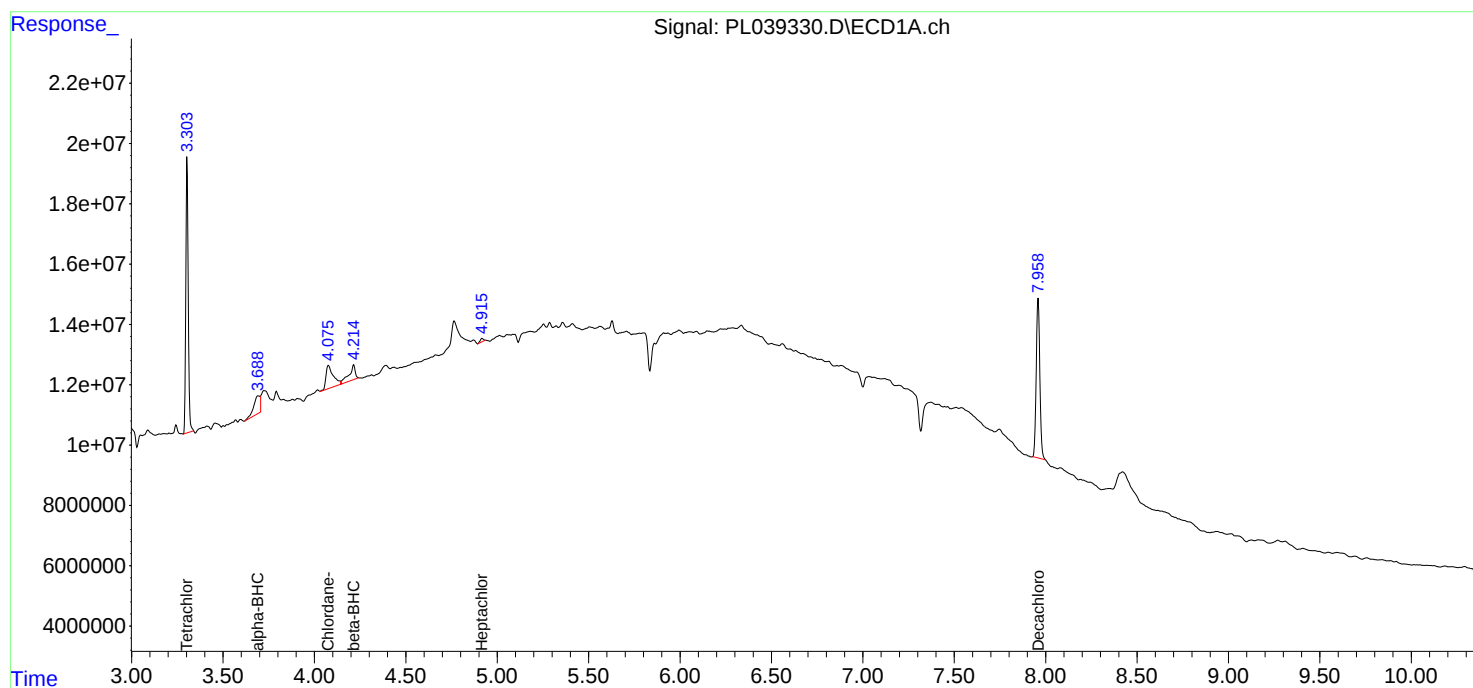


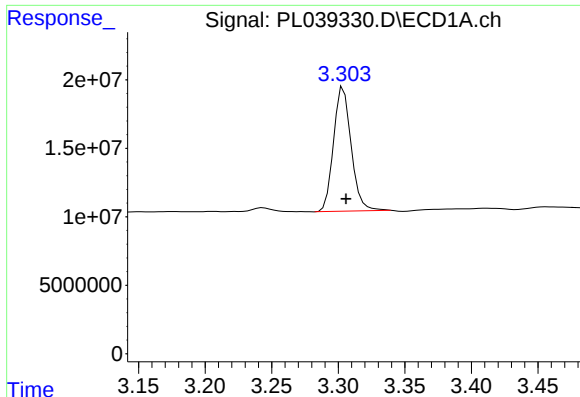

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 83788673
Conc: 11.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

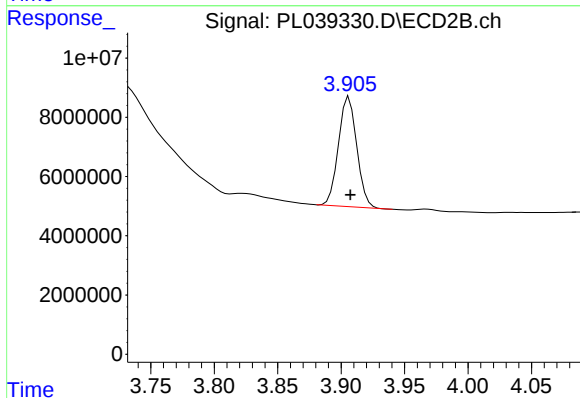


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 37122829
Conc: 13.85 ng/ml

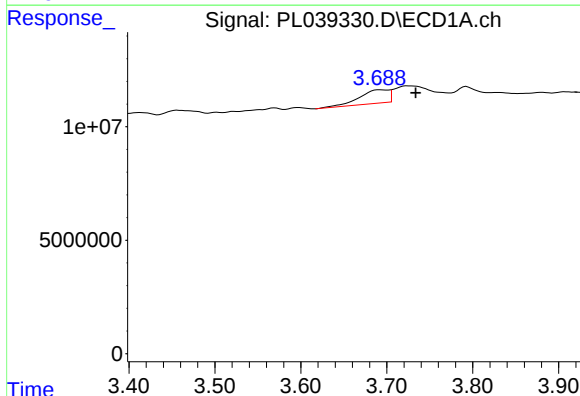


#2 alpha-BHC

R.T.: 3.692 min
Delta R.T.: -0.042 min
Response: 15078056
Conc: 1.28 ng/ml

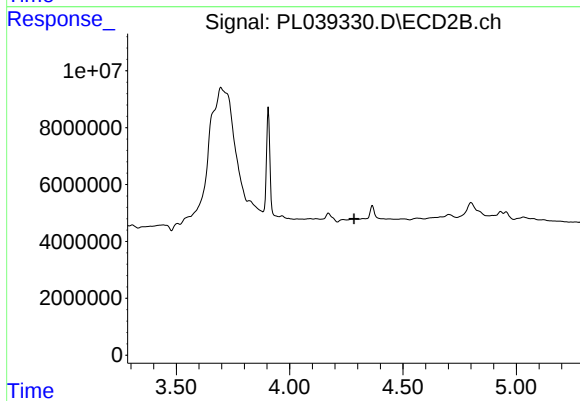

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.285 min
Response: 0
Conc: N.D.

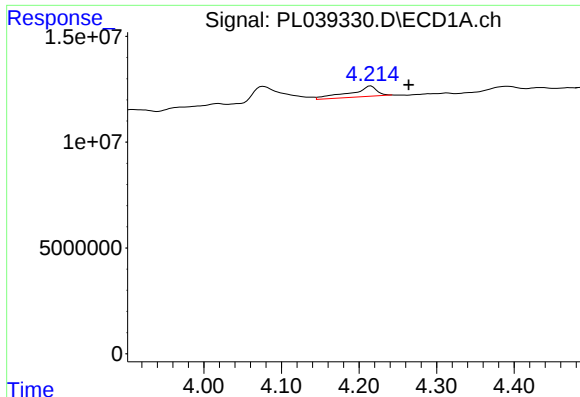

#6 beta-BHC


R.T.: 4.215 min
Delta R.T.: -0.049 min
Response: 12144810
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

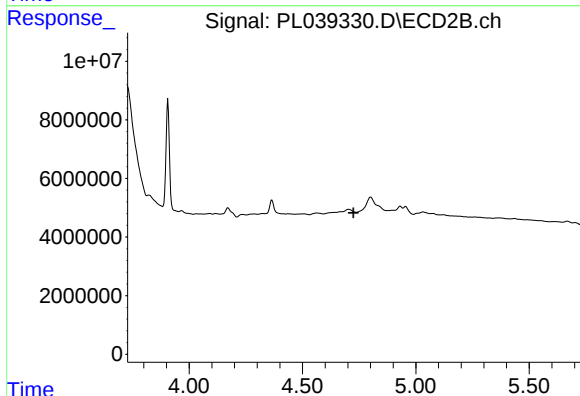


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

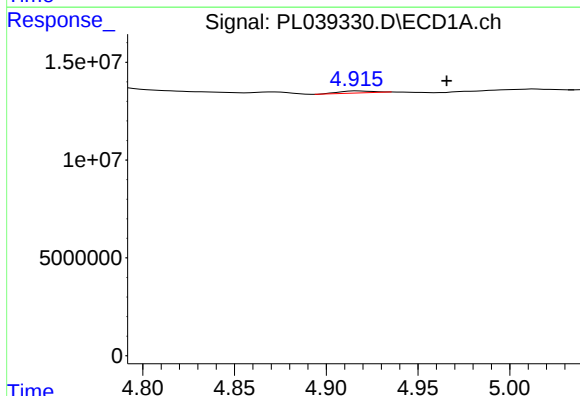


#8 Heptachlor epoxide

R.T.: 4.917 min
Delta R.T.: -0.049 min
Response: 1945048
Conc: 0.20 ng/ml

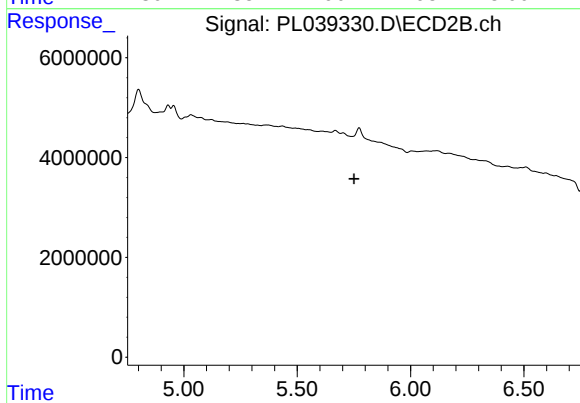

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

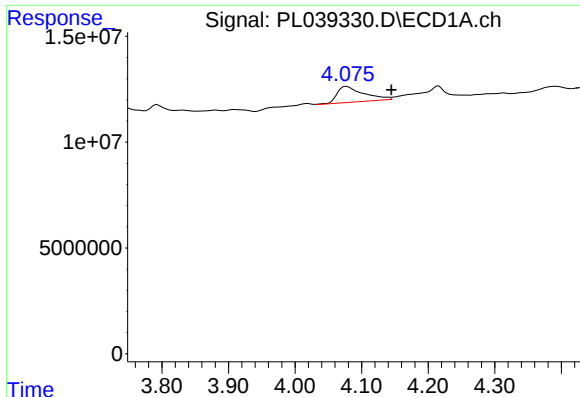

#23 Chlordane-1


R.T.: 4.077 min
Delta R.T.: -0.068 min
Response: 20972843
Conc: 66.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

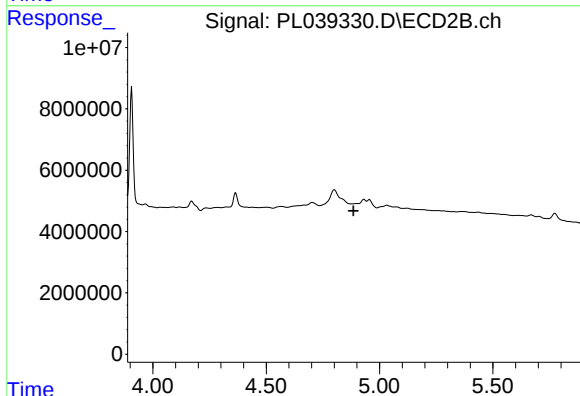


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

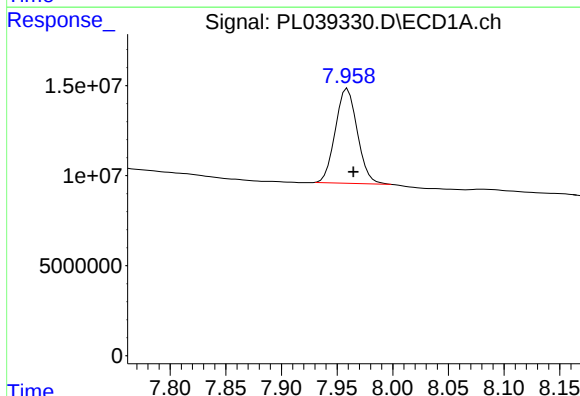

#28 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.005 min
Response: 72361567
Conc: 10.30 ng/ml

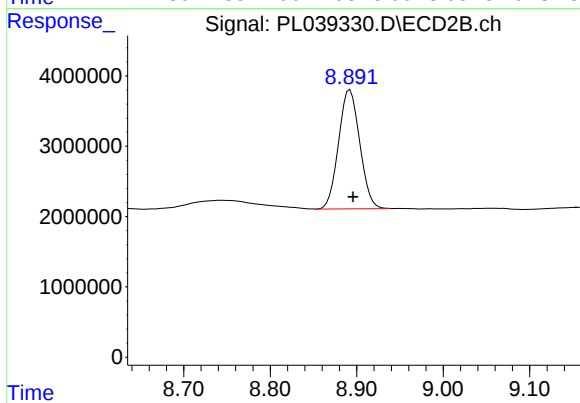

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.003 min
Response: 28642351
Conc: 12.34 ng/ml