

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082018\
 Data File : PL039339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2018 19:30
 Operator : AJ\SJ
 Sample : J4277-05 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:25:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	0.000	10473623	0	1.498	N.D. #
28)	SA Decachlor...	7.959	0.000	9584273	0	1.365	N.D. #
Target Compounds							
5)	MB Aldrin	4.521	0.000	2450751	0	0.245	N.D. #
6)	B beta-BHC	4.215f	0.000	17289951	0	3.722	N.D. #
8)	B Heptachlo...	4.927f	0.000	2606036	0	0.273	N.D. #
9)	A Endosulfan I	5.318	0.000	14842409	0	1.695	N.D. #
10)	B gamma-Chl...	5.131f	0.000	1351666	0	0.137	N.D. #
23)	Chlordane-1	4.152	0.000	13185880	0	41.650	N.D. #
24)	Chlordane-2	4.616	0.000	5870538	0	16.793	N.D. #
25)	Chlordane-3	5.131	0.000	1351666	0	1.237	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082018\
Data File : PL039339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2018 19:30
Operator : AJ\SJ
Sample : J4277-05 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:25:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

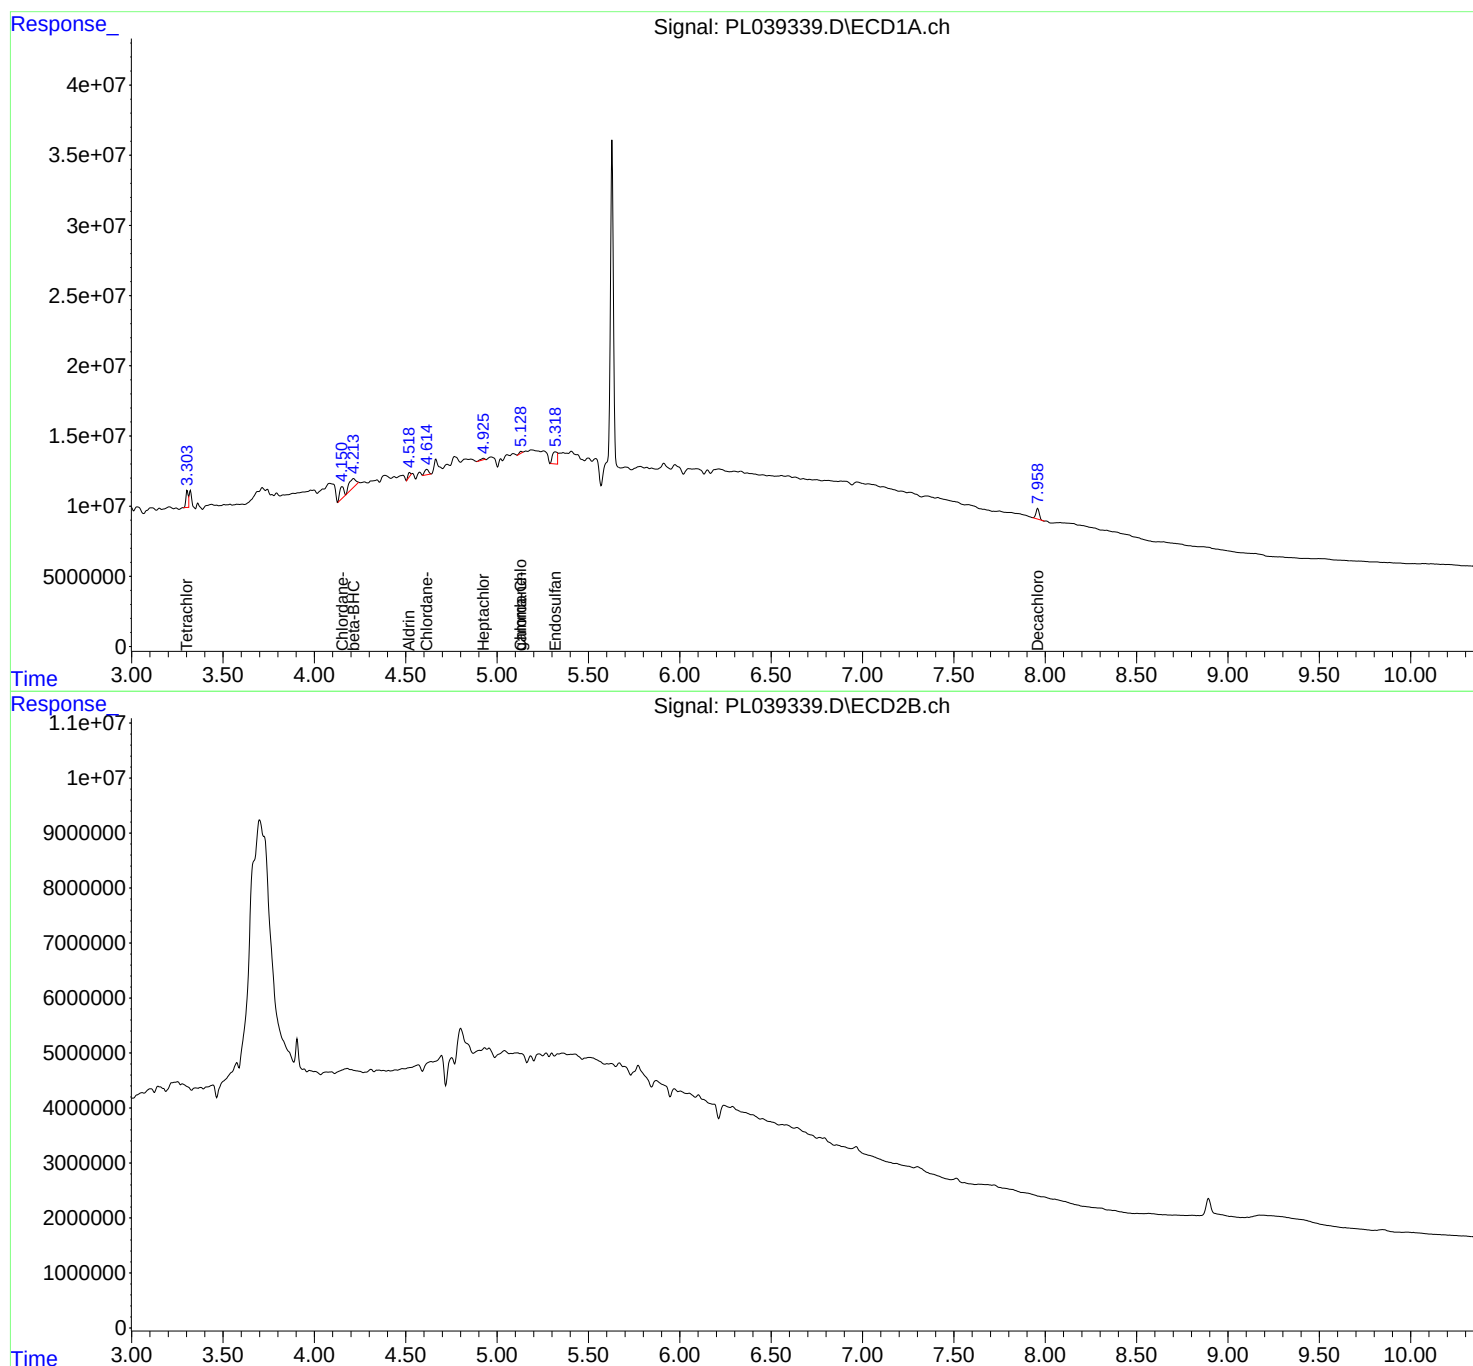


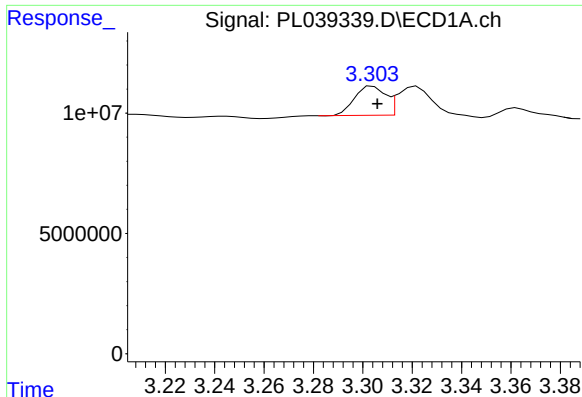

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 10473623
Conc: 1.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

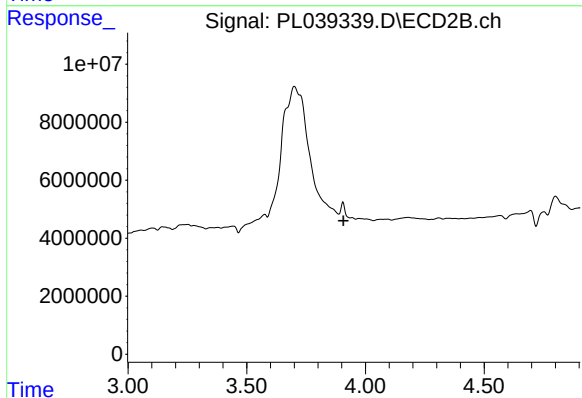


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.907 min
Response: 0
Conc: N.D.

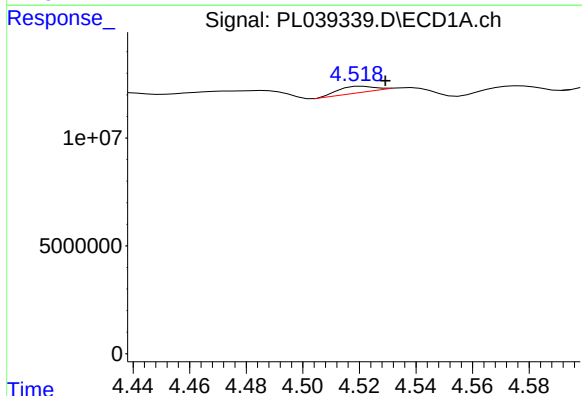


#5 Aldrin

R.T.: 4.521 min
Delta R.T.: -0.008 min
Response: 2450751
Conc: 0.24 ng/ml

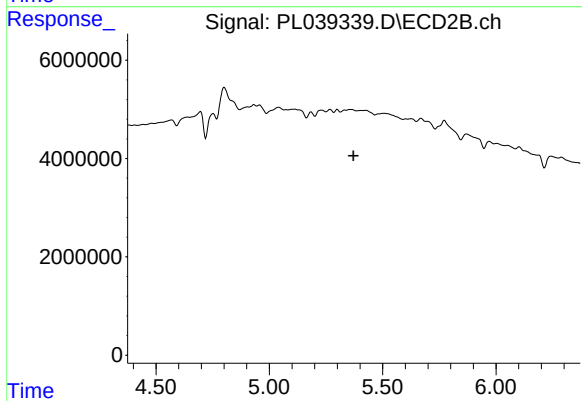

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.372 min
Response: 0
Conc: N.D.

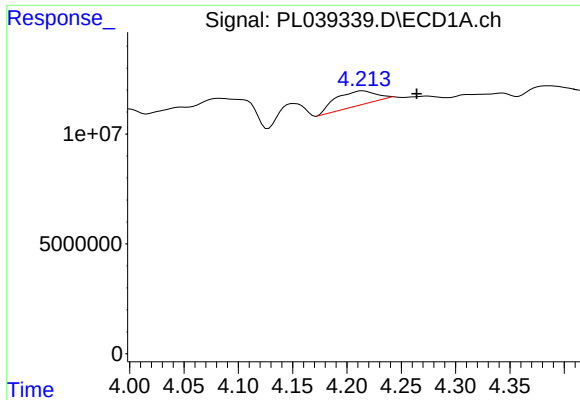

#6 beta-BHC


R.T.: 4.215 min
Delta R.T.: -0.049 min
Response: 17289951
Conc: 3.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

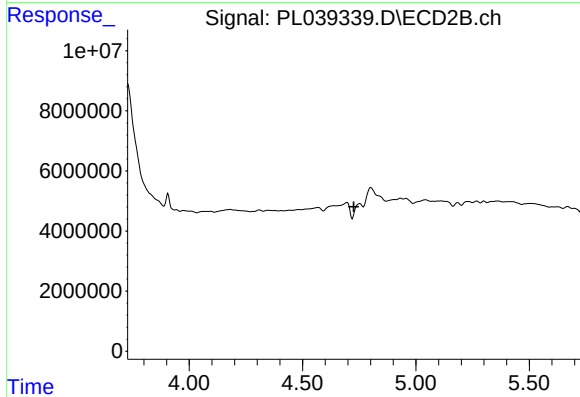


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

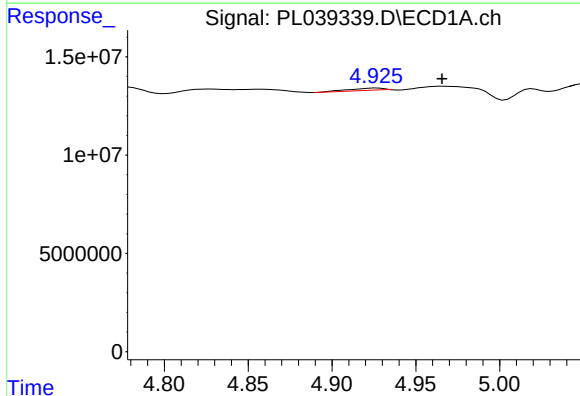


#8 Heptachlor epoxide

R.T.: 4.927 min
Delta R.T.: -0.039 min
Response: 2606036
Conc: 0.27 ng/ml

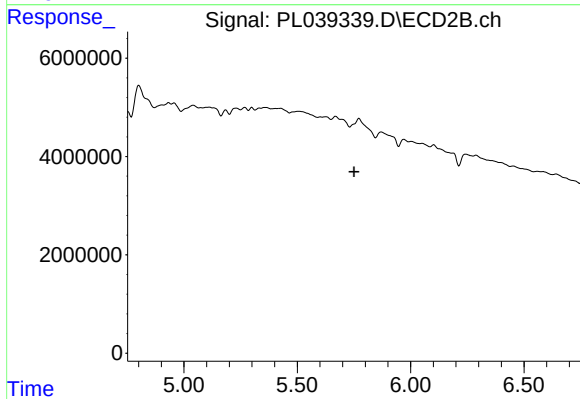

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

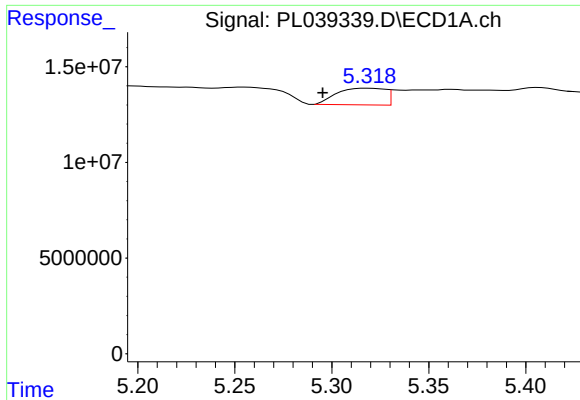

#9 Endosulfan I


R.T.: 5.318 min
Delta R.T.: 0.023 min
Response: 14842409
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

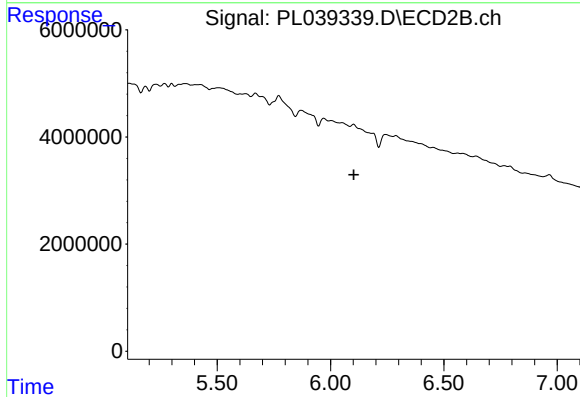


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

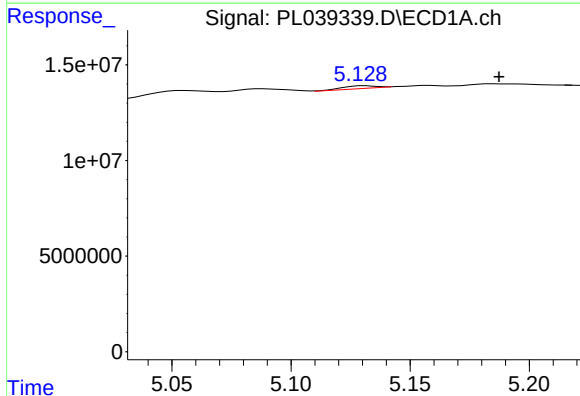


#10 gamma-Chlordane

R.T.: 5.131 min
Delta R.T.: -0.056 min
Response: 1351666
Conc: 0.14 ng/ml

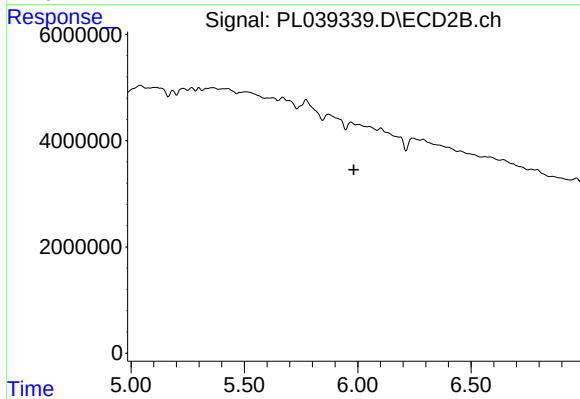

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

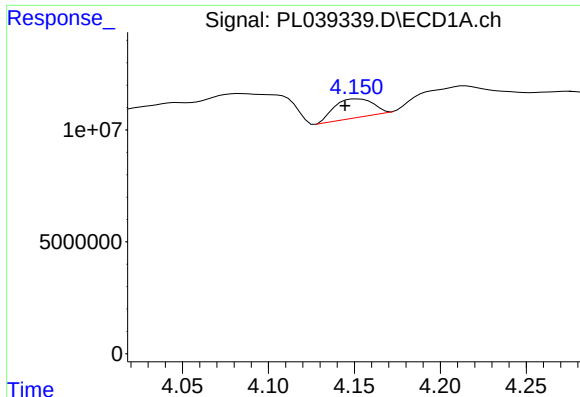

#23 Chlordane-1


R.T.: 4.152 min
Delta R.T.: 0.007 min
Response: 13185880
Conc: 41.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

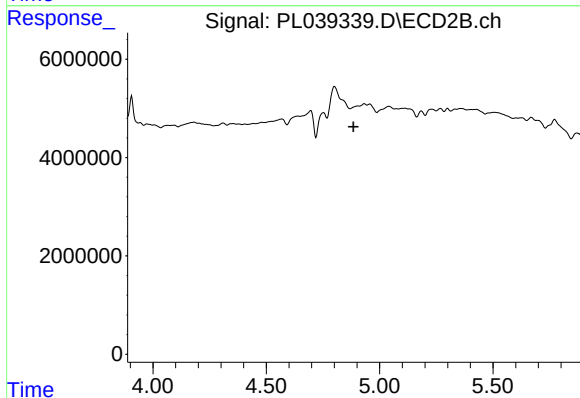


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

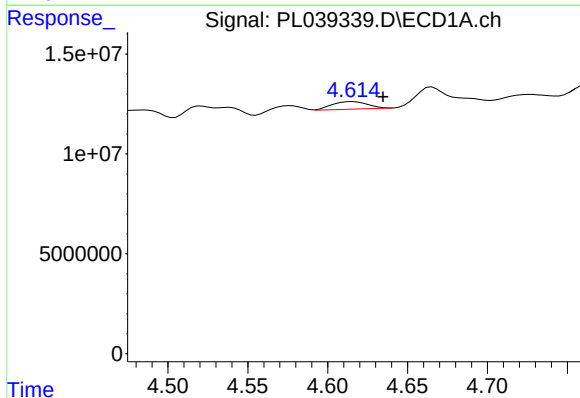


#24 Chlordane-2

R.T.: 4.616 min
Delta R.T.: -0.019 min
Response: 5870538
Conc: 16.79 ng/ml

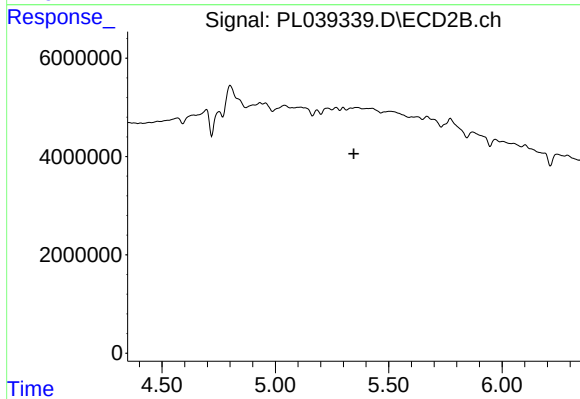

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

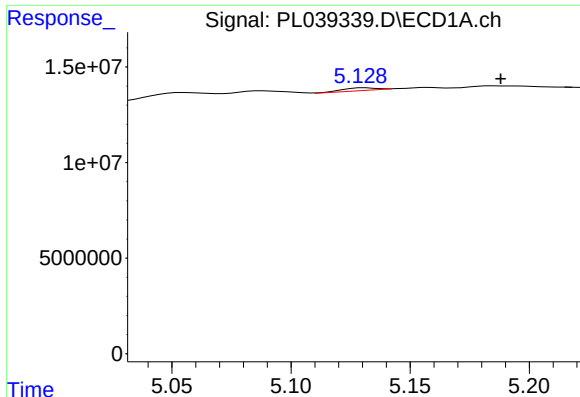

#25 Chlordane-3


R.T.: 5.131 min
Delta R.T.: -0.057 min
Response: 1351666
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

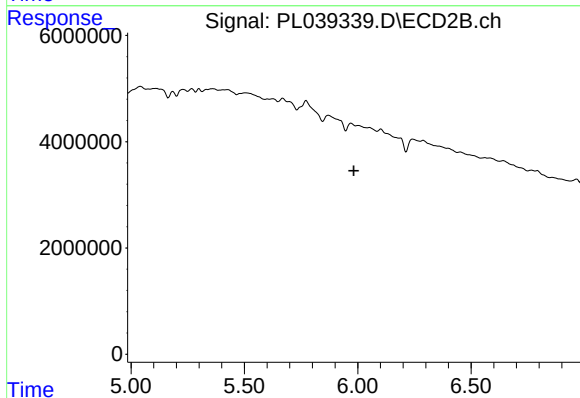


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

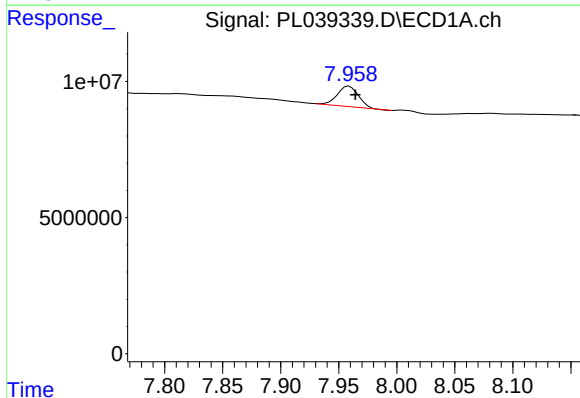

#28 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.005 min
Response: 9584273
Conc: 1.36 ng/ml

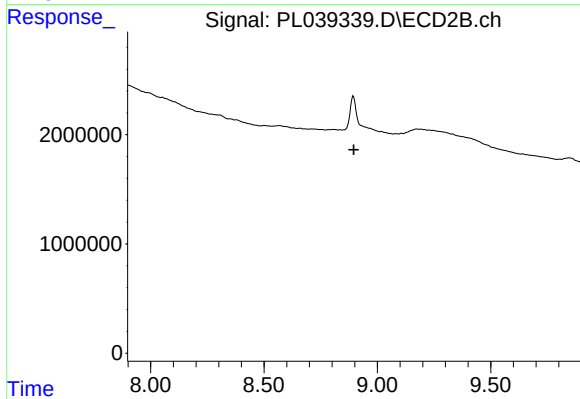

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.896 min
Response: 0
Conc: N.D.