

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
 Data File : PL051647.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 16:04
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 20 17:48:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	174.2E6	44634663	20.351	20.429
28)	SA Decachlor...	7.972	8.951	234.0E6	57551126	19.277	18.907
Target Compounds							
5)	MB Aldrin	4.564f	0.000	2492162	0	0.172	N.D. #
6)	B beta-BHC	0.000	4.804f	0	4284676	N.D.	2.940 #
8)	B Heptachlo...	0.000	5.801	0	6430648	N.D.	1.905 #
10)	B gamma-Chl...	5.192	0.000	5575450	0	0.373	N.D. #
11)	B alpha-Chl...	5.257	0.000	2392401	0	0.165	N.D. #
15)	B Endosulfa...	0.000	6.836	0	5313716	N.D.	1.612 #
16)	A 4,4'-DDD	5.947f	0.000	6633767	0	0.542	N.D. #
25)	Chlordane-3	5.192	0.000	5575450	0	4.294	N.D. #
26)	Chlordane-4	5.257	0.000	2392401	0	1.962	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
Data File : PL051647.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 16:04
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 20 17:48:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

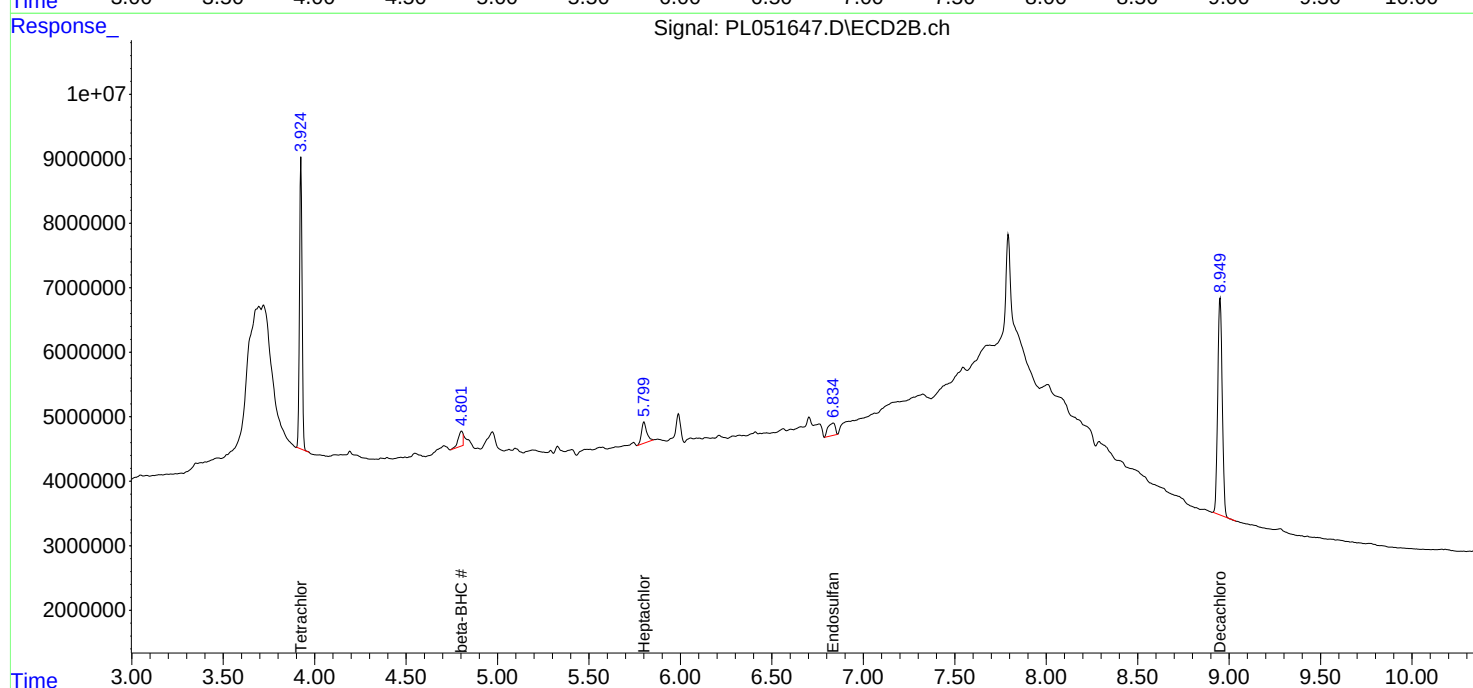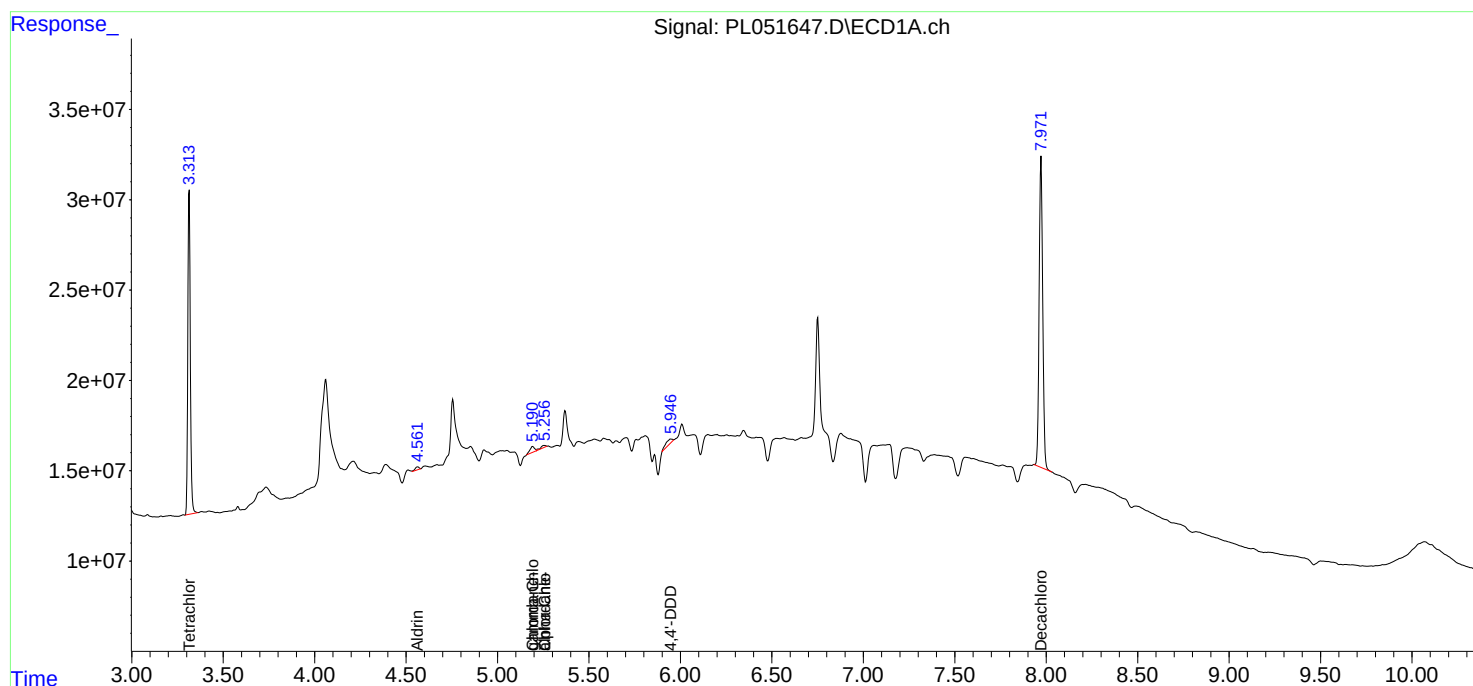


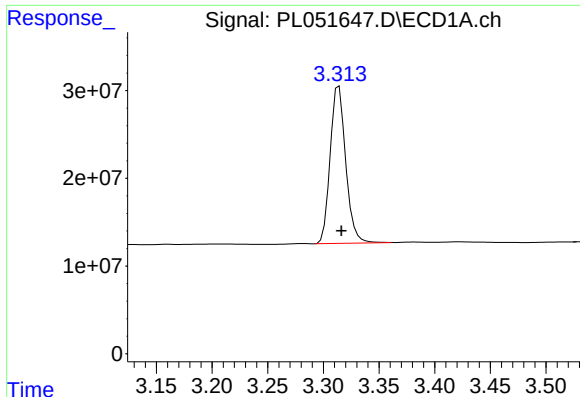

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 174178765
Conc: 20.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

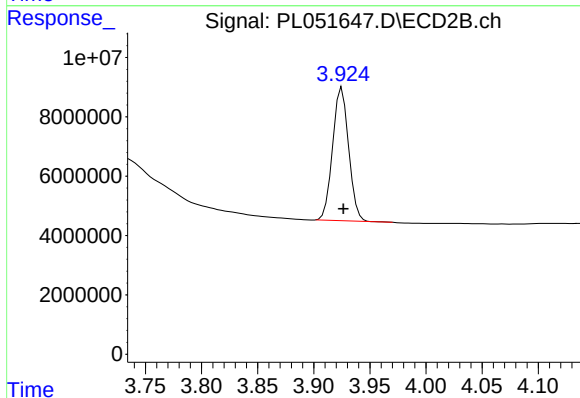


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.001 min
Response: 44634663
Conc: 20.43 ng/ml

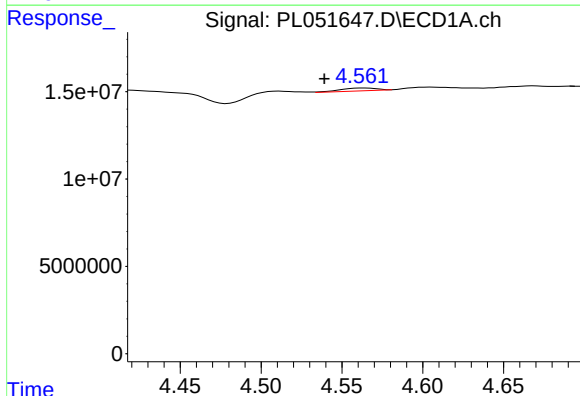


#5 Aldrin

R.T.: 4.564 min
Delta R.T.: 0.024 min
Response: 2492162
Conc: 0.17 ng/ml

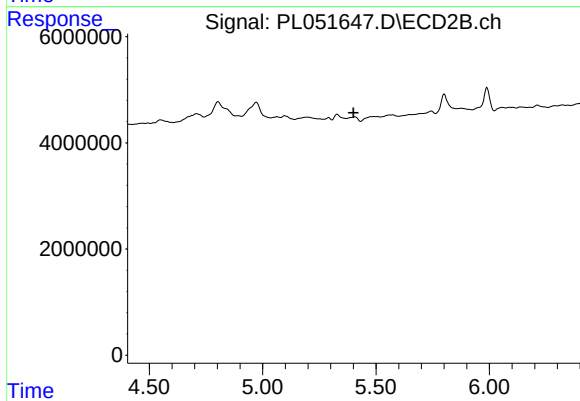

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.401 min
Response: 0
Conc: N.D.

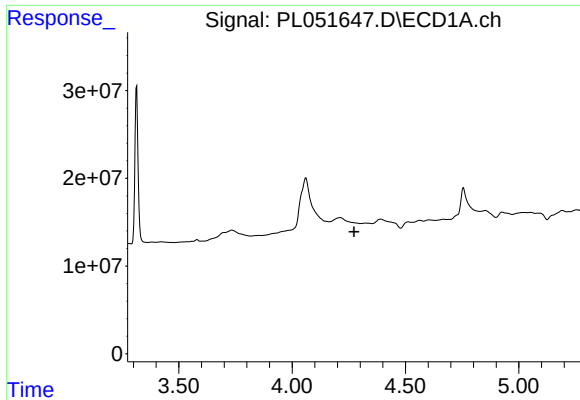

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

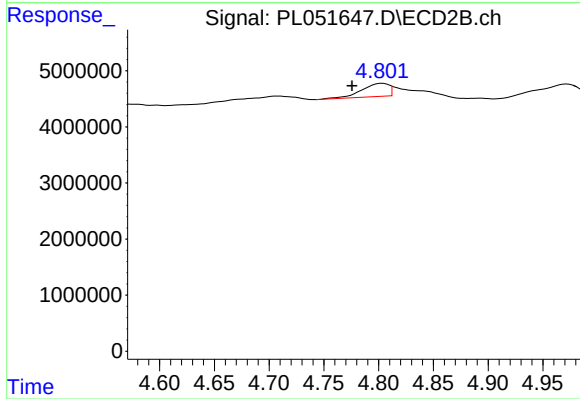


#6 beta-BHC

R.T.: 4.804 min
Delta R.T.: 0.028 min
Response: 4284676
Conc: 2.94 ng/ml

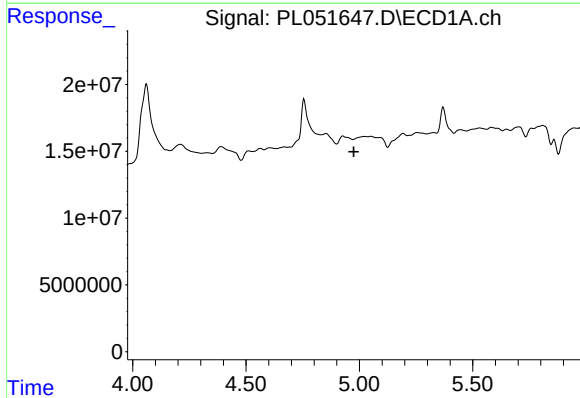


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

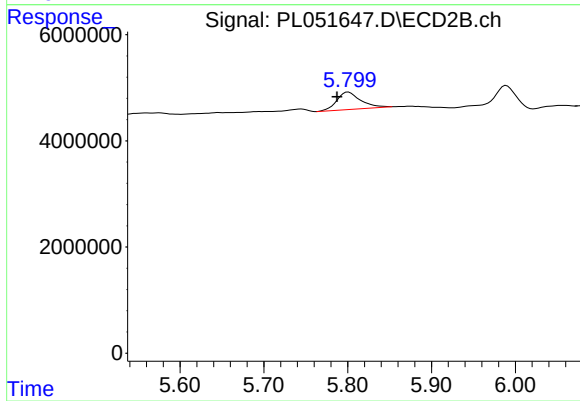

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.014 min
Response: 6430648
Conc: 1.91 ng/ml

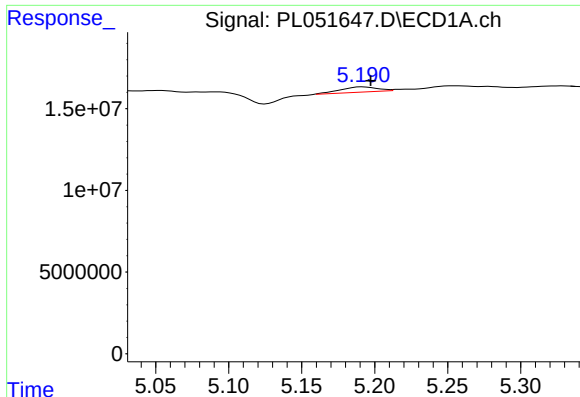

#10 gamma-Chlordane


R.T.: 5.192 min
Delta R.T.: -0.005 min
Response: 5575450
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

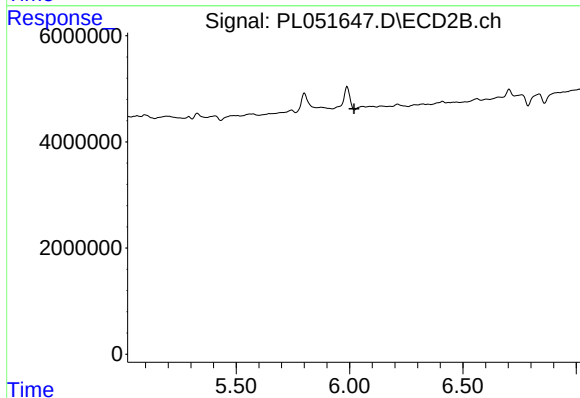


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.020 min
Response: 0
Conc: N.D.

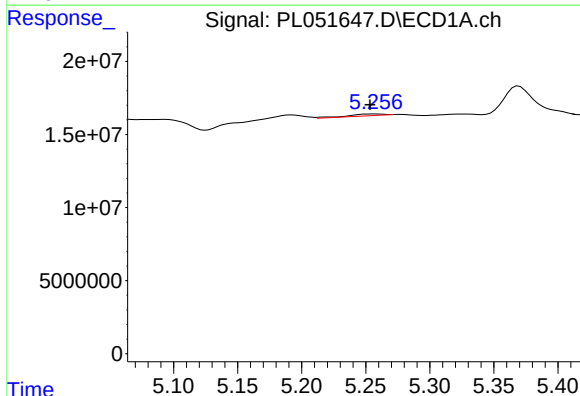


#11 alpha-Chlordane

R.T.: 5.257 min
Delta R.T.: 0.003 min
Response: 2392401
Conc: 0.17 ng/ml

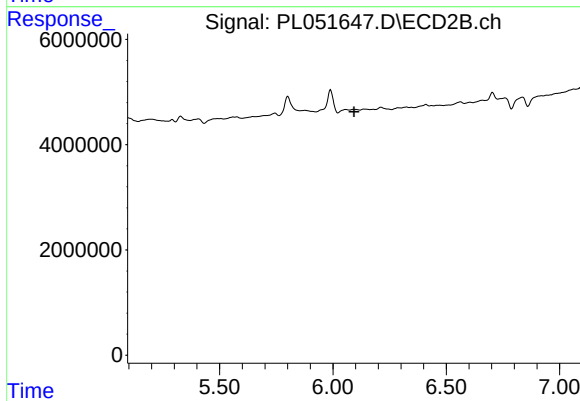

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

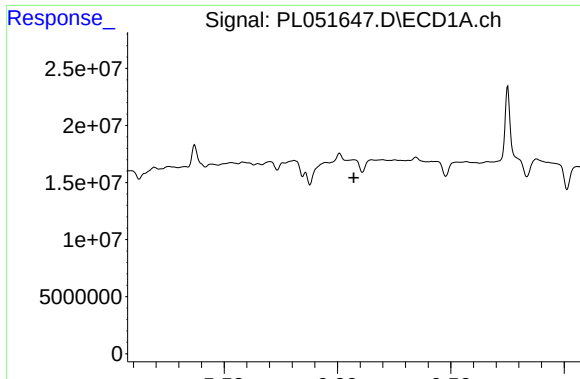

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

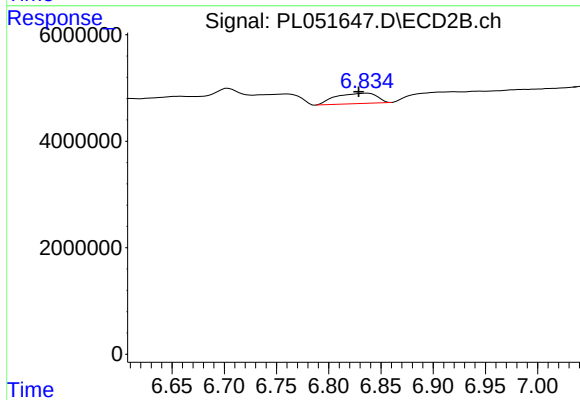


#15 Endosulfan II

R.T.: 6.836 min
Delta R.T.: 0.008 min
Response: 5313716
Conc: 1.61 ng/ml

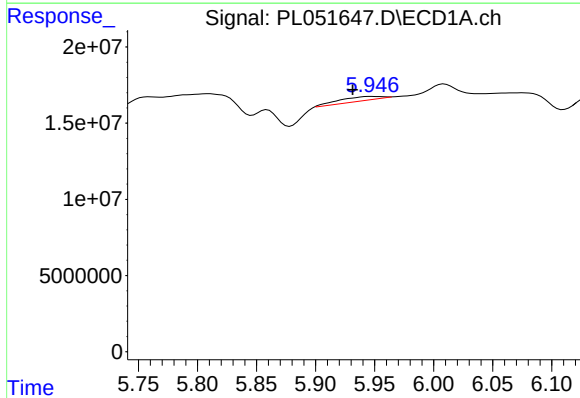


#16 4,4'-DDD

R.T.: 5.947 min
Delta R.T.: 0.016 min
Response: 6633767
Conc: 0.54 ng/ml

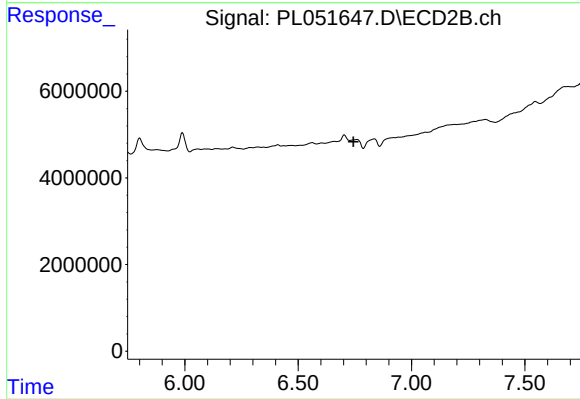

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.744 min
Response: 0
Conc: N.D.

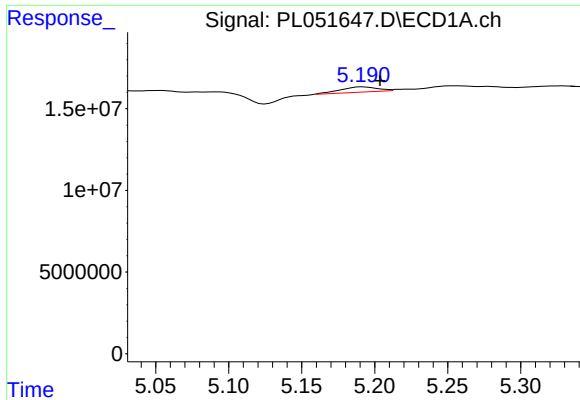

#25 Chlordane-3


R.T.: 5.192 min
Delta R.T.: -0.012 min
Response: 5575450
Conc: 4.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

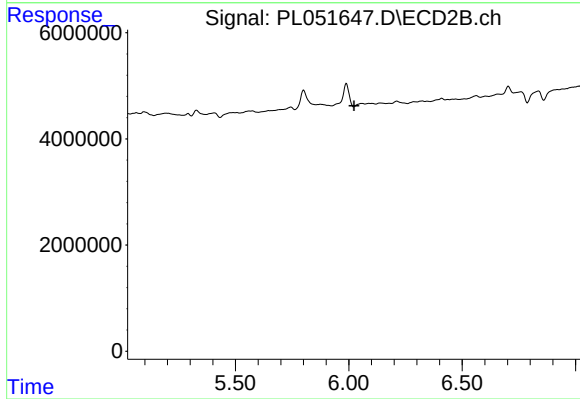


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

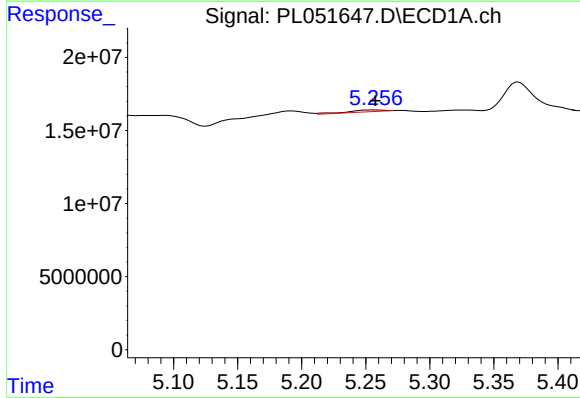


#26 Chlordane-4

R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 2392401
Conc: 1.96 ng/ml

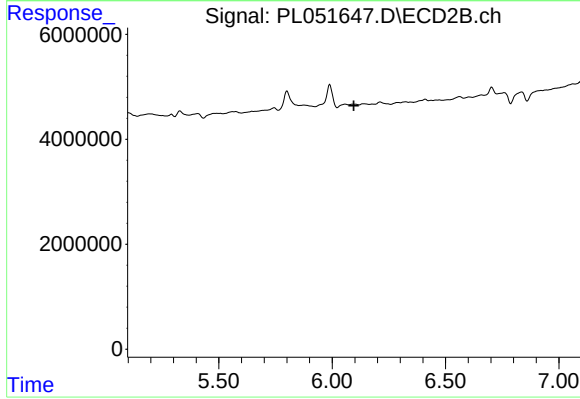

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

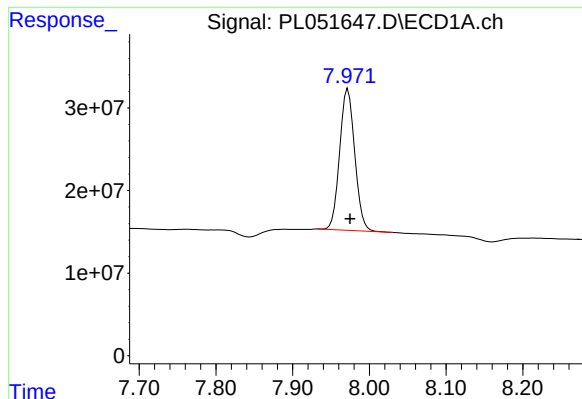

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.003 min
Response: 233982930
Conc: 19.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

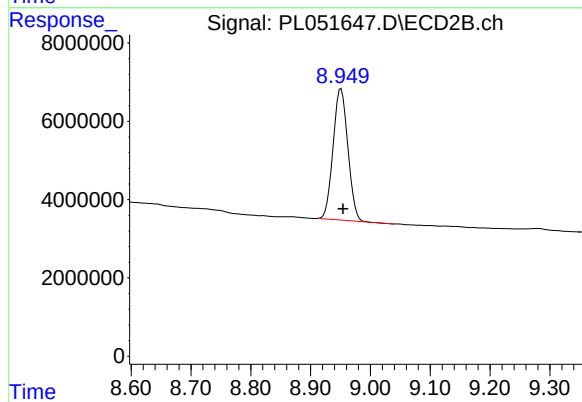

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.003 min
Response: 57551126
Conc: 18.91 ng/ml