

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
 Data File : PL051675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 23:31
 Operator : SG\AJ
 Sample : K4403-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:32:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	128.4E6	33029292	14.999	15.118
28)	SA Decachlor...	7.972	8.952	126.1E6	40633994	10.390	13.349 #
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	5957490	N.D.	4.088 #
10)	B gamma-Chl...	5.196	0.000	7384777	0	0.495	N.D. #
13)	MA Dieldrin	5.542	0.000	23341176	0	1.535	N.D. #
14)	MA Endrin	5.800	0.000	7636772	0	0.524	N.D. #
16)	A 4,4'-DDD	0.000	6.745	0	5817162	N.D.	2.149 #
17)	MA 4,4'-DDT	6.158	0.000	31508798	0	2.471	N.D. #
18)	B Endrin al...	6.250	0.000	13955827	0	1.200	N.D. #
19)	B Endosulfa...	6.439	0.000	22927514	0	1.762	N.D. #
20)	A Methoxychlor	6.687f	0.000	66147861	0	9.757	N.D. #
21)	B Endrin ke...	6.955f	0.000	13155372	0	0.930	N.D. #
25)	Chlordane-3	5.196	0.000	7384777	0	5.688	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
Data File : PL051675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 23:31
Operator : SG\AJ
Sample : K4403-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:32:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

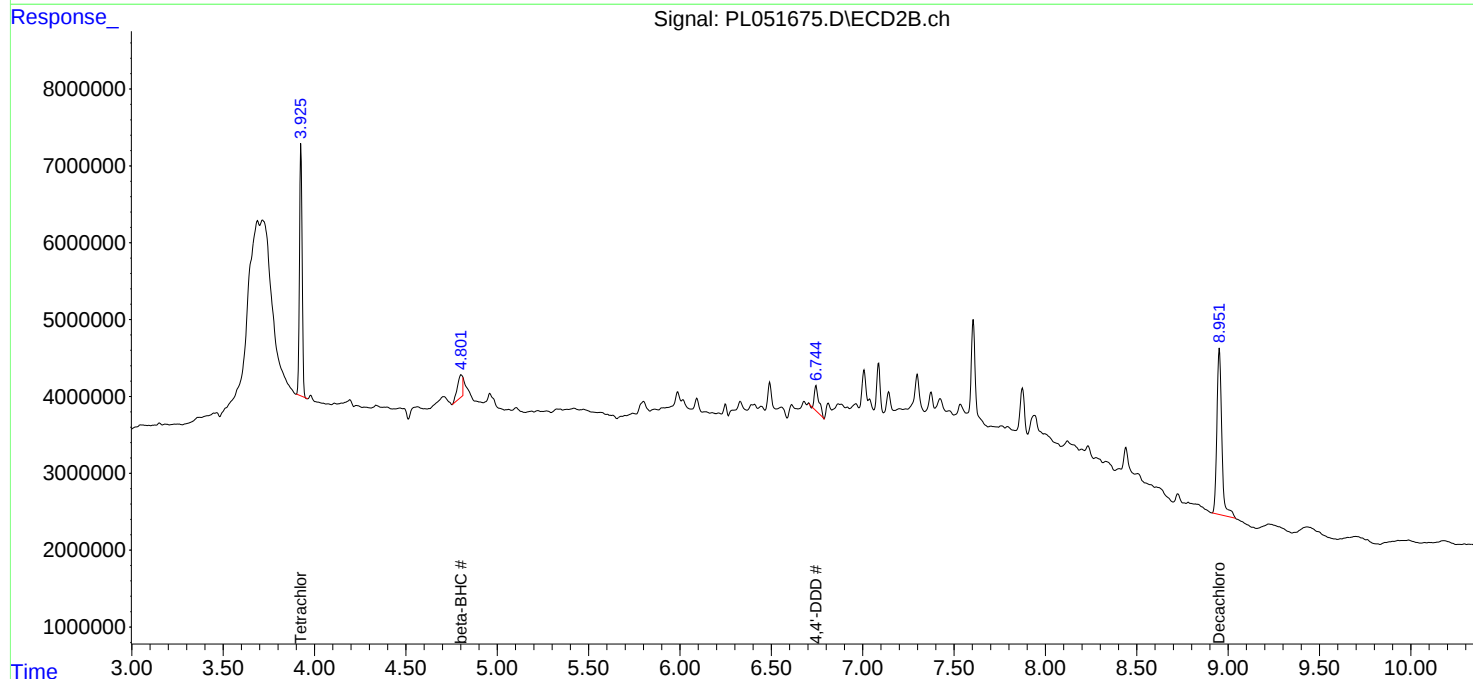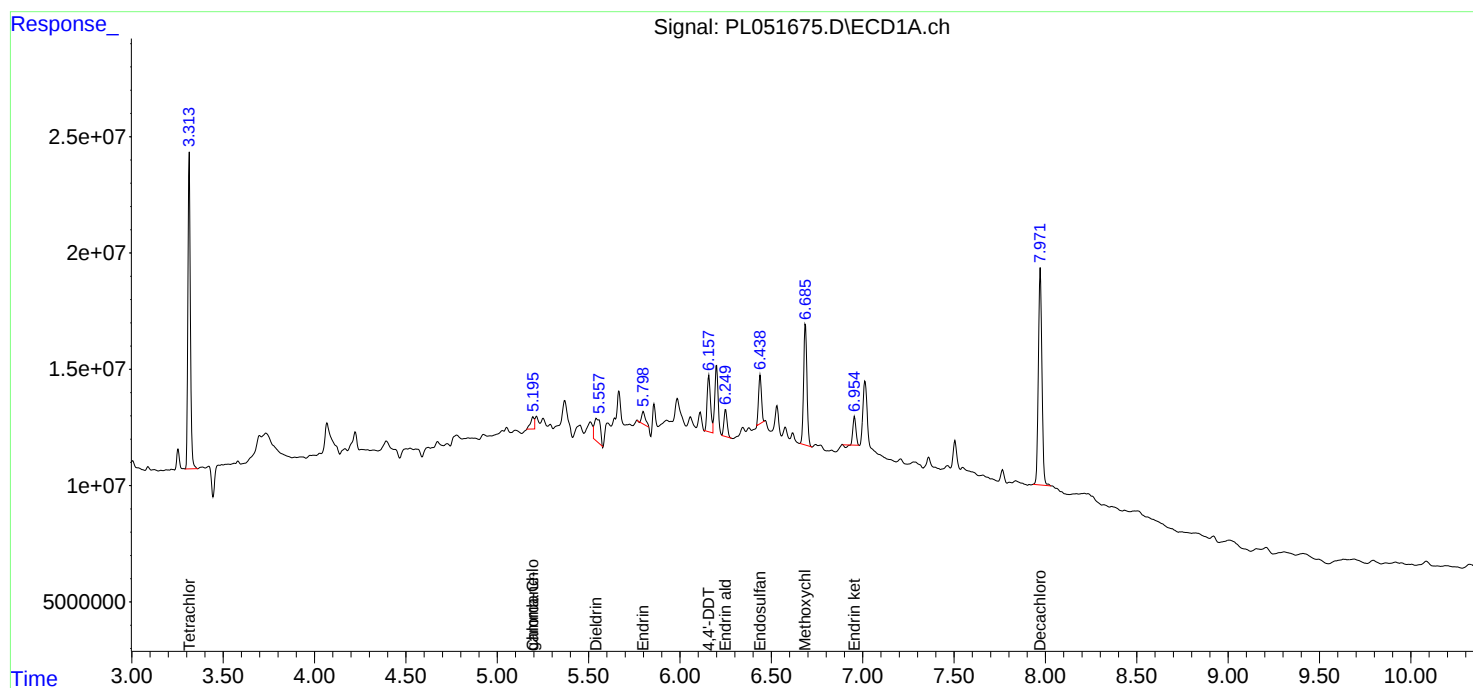


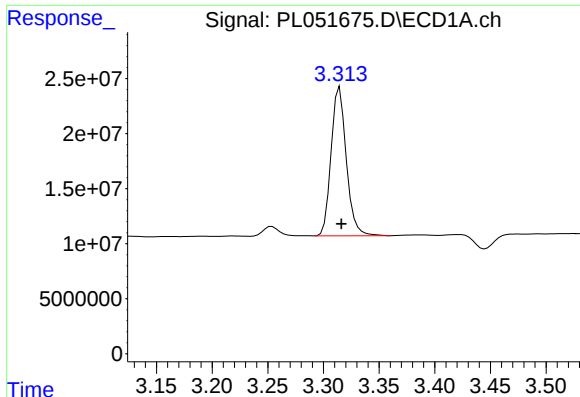

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.001 min
Response: 128369478
Conc: 15.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

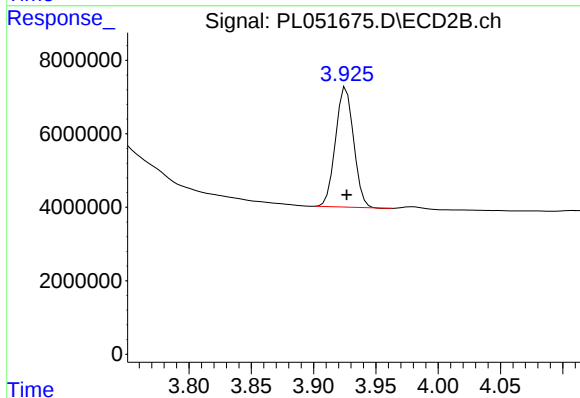


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 33029292
Conc: 15.12 ng/ml

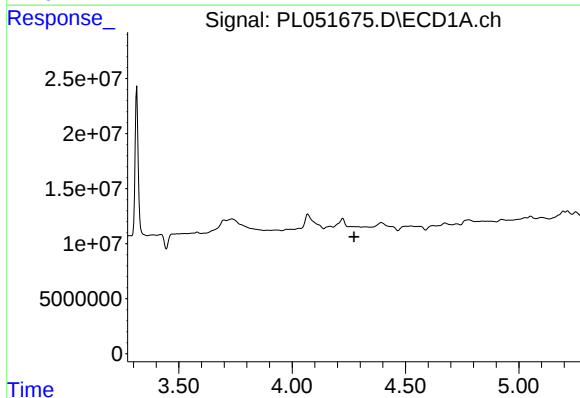


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

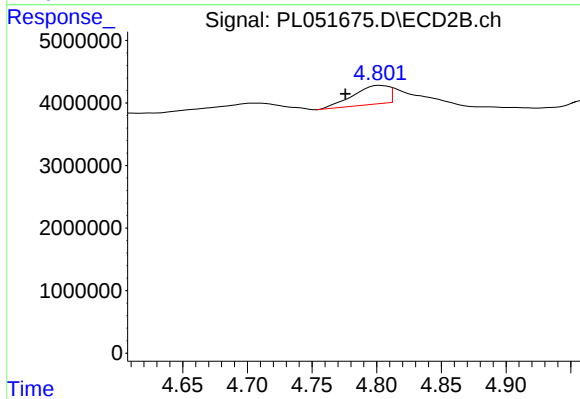

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.027 min
Response: 5957490
Conc: 4.09 ng/ml

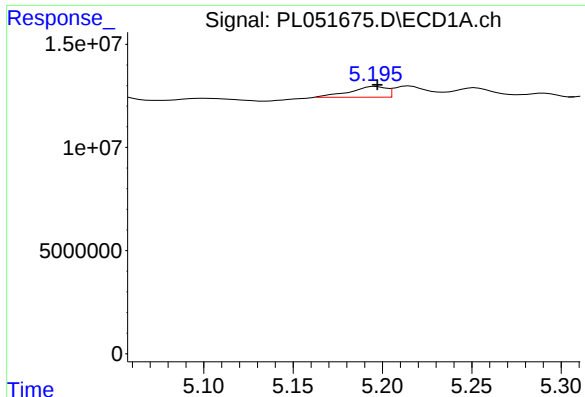

#10 gamma-Chlordane


R.T.: 5.196 min
Delta R.T.: -0.001 min
Response: 7384777
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

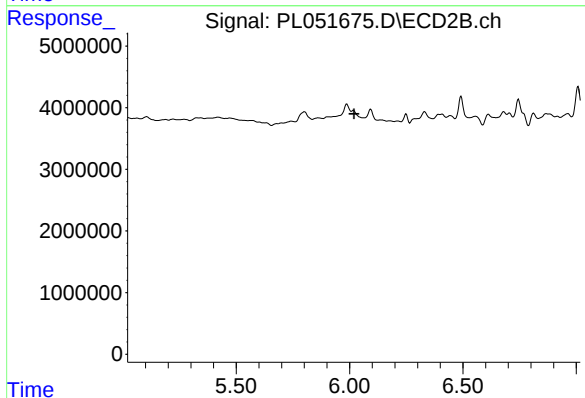


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.020 min
Response: 0
Conc: N.D.

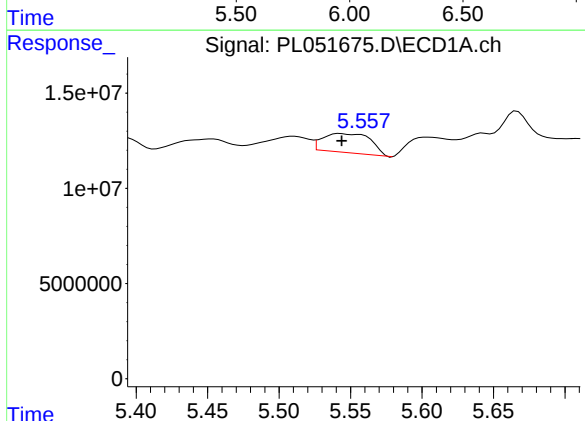


#13 Dieldrin

R.T.: 5.542 min
Delta R.T.: -0.002 min
Response: 23341176
Conc: 1.54 ng/ml

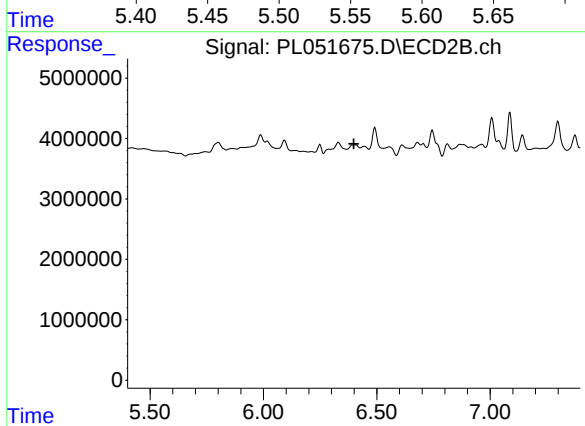

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

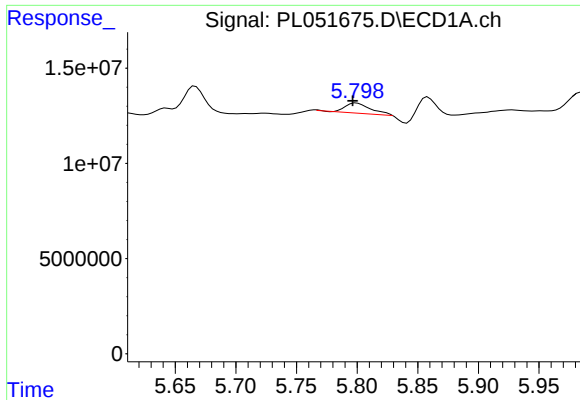

#14 Endrin


R.T.: 5.800 min
Delta R.T.: 0.003 min
Response: 7636772
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

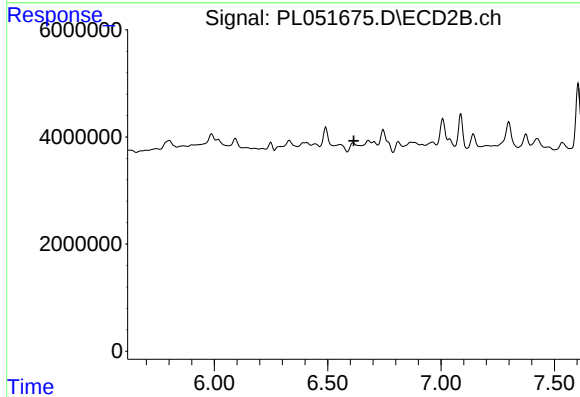


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.616 min
Response: 0
Conc: N.D.

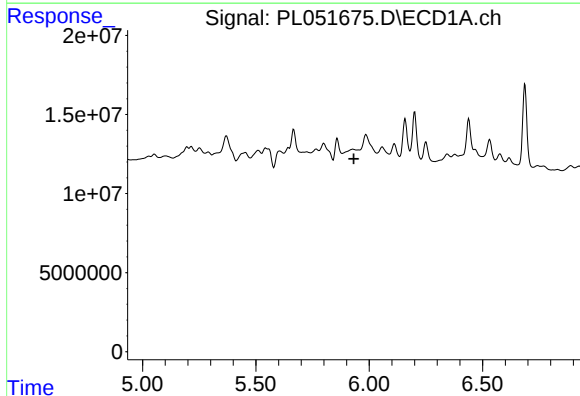


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.931 min
Response: 0
Conc: N.D.

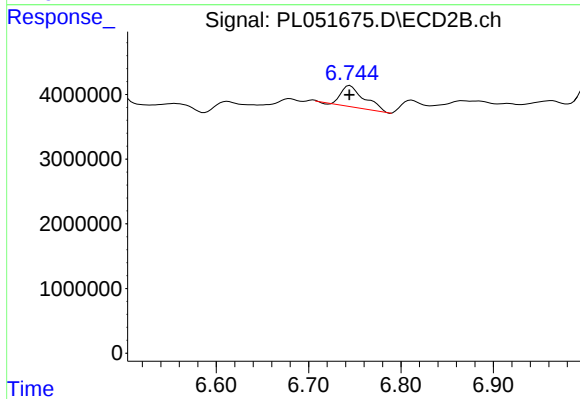

#16 4,4'-DDD


R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 5817162
Conc: 2.15 ng/ml

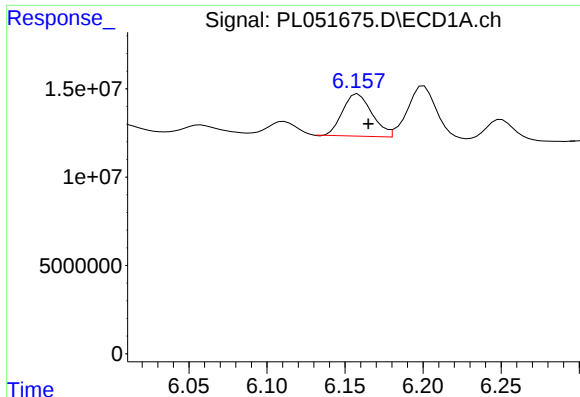

#17 4,4'-DDT


R.T.: 6.158 min
Delta R.T.: -0.006 min
Response: 31508798
Conc: 2.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

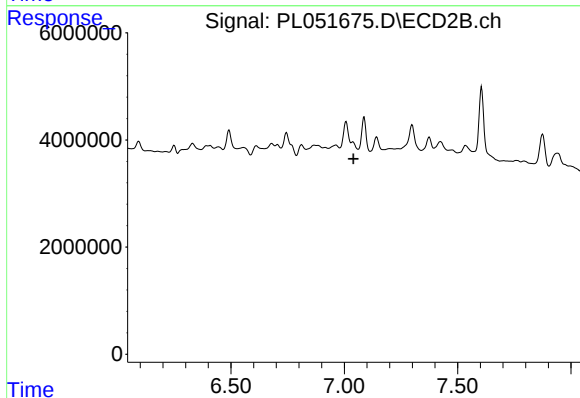


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.041 min
Response: 0
Conc: N.D.

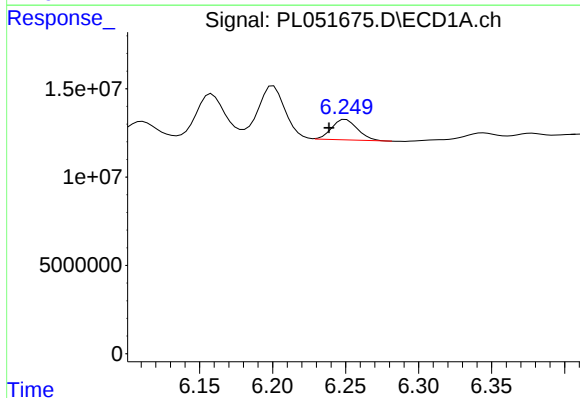


#18 Endrin aldehyde

R.T.: 6.250 min
Delta R.T.: 0.011 min
Response: 13955827
Conc: 1.20 ng/ml

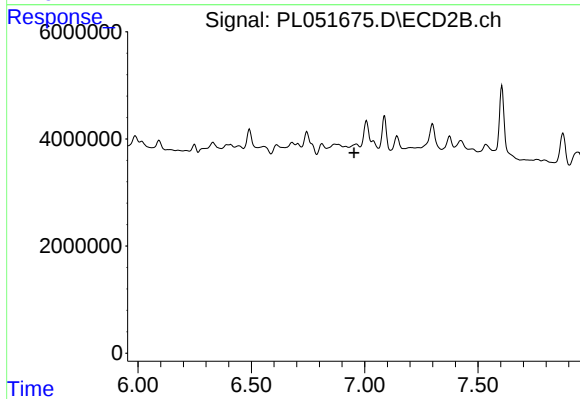

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.953 min
Response: 0
Conc: N.D.

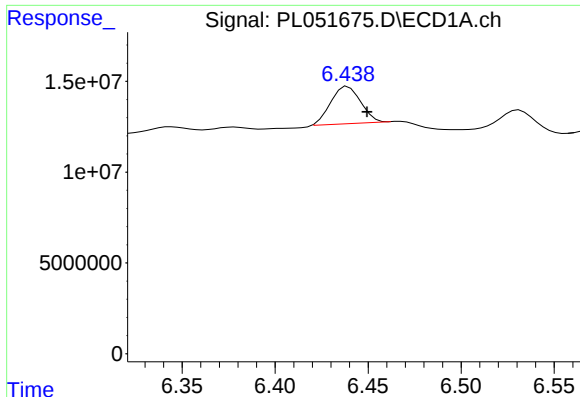

#19 Endosulfan Sulfate


R.T.: 6.439 min
Delta R.T.: -0.010 min
Response: 22927514
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

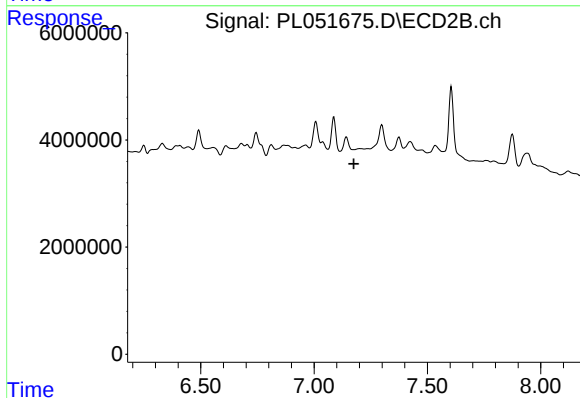


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.176 min
Response: 0
Conc: N.D.

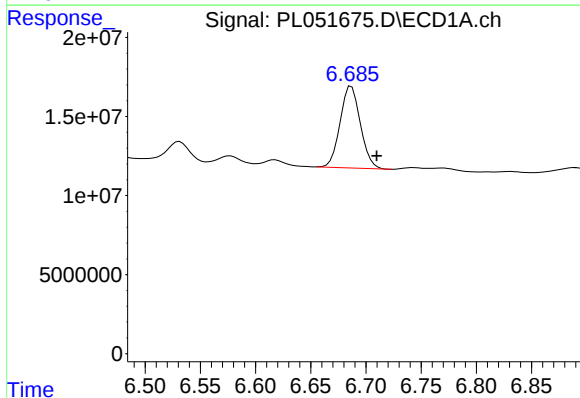


#20 Methoxychlor

R.T.: 6.687 min
Delta R.T.: -0.023 min
Response: 66147861
Conc: 9.76 ng/ml

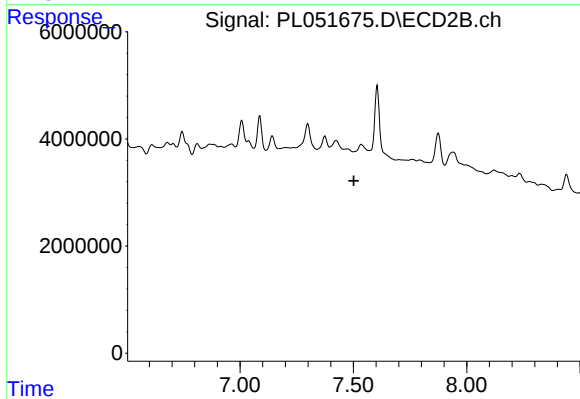

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.502 min
Response: 0
Conc: N.D.

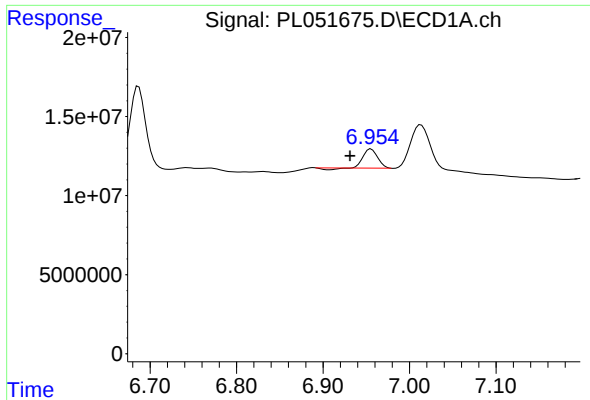

#21 Endrin ketone


R.T.: 6.955 min
Delta R.T.: 0.024 min
Response: 13155372
Conc: 0.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

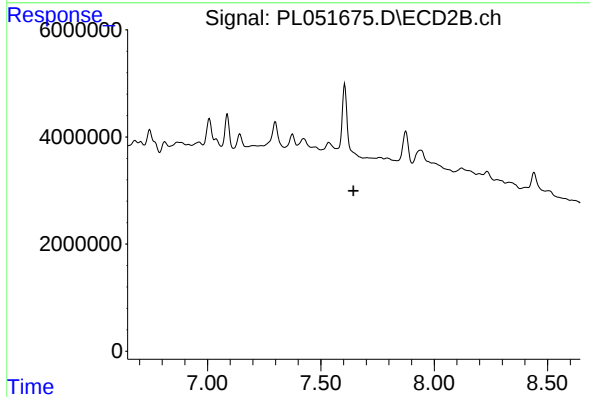


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.644 min
Response: 0
Conc: N.D.

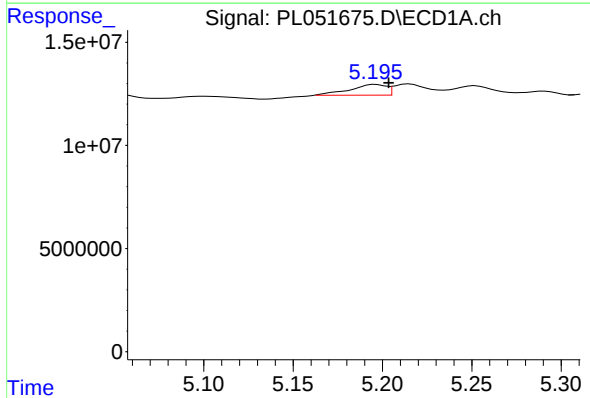


#25 Chlordane-3

R.T.: 5.196 min
Delta R.T.: -0.007 min
Response: 7384777
Conc: 5.69 ng/ml

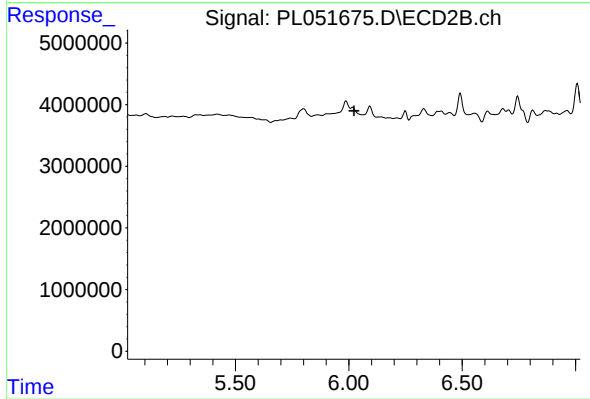

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

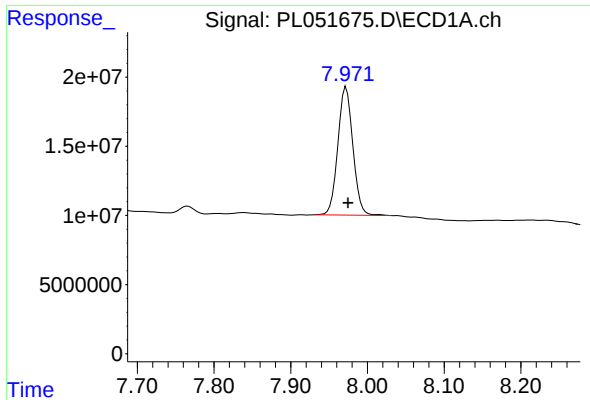

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.002 min
Response: 126115563
Conc: 10.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

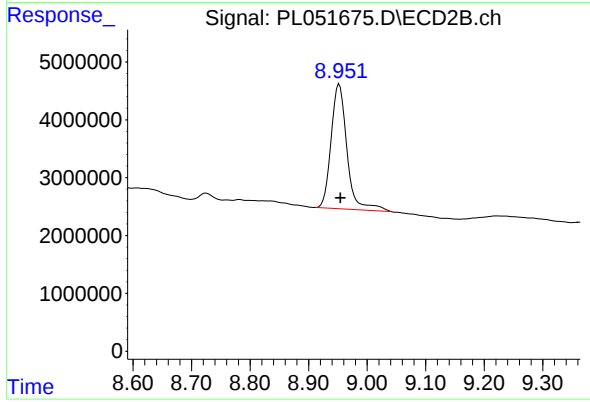

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 40633994
Conc: 13.35 ng/ml