

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
 Data File : PL051679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2019 00:28
 Operator : SG\AJ
 Sample : K4408-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:33:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.925	165.6E6	42344813	19.352	19.381
28)	SA Decachlor...	7.973	8.952	136.1E6	36740645	11.209	12.070
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	3780846	N.D.	2.594 #
8)	B Heptachlo...	0.000	5.800	0	8686863	N.D.	2.574 #
9)	A Endosulfan I	5.332f	0.000	7402137	0	0.551	N.D. #
13)	MA Dieldrin	5.543	0.000	8087119	0	0.532	N.D. #
15)	B Endosulfa...	0.000	6.838	0	12749453	N.D.	3.868 #
16)	A 4,4'-DDD	5.933	0.000	4979759	0	0.407	N.D. #
18)	B Endrin al...	0.000	6.972f	0	12304064	N.D.	4.354 #
24)	Chlordane-2	4.674f	0.000	9642848	0	23.593	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
Data File : PL051679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2019 00:28
Operator : SG\AJ
Sample : K4408-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:33:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

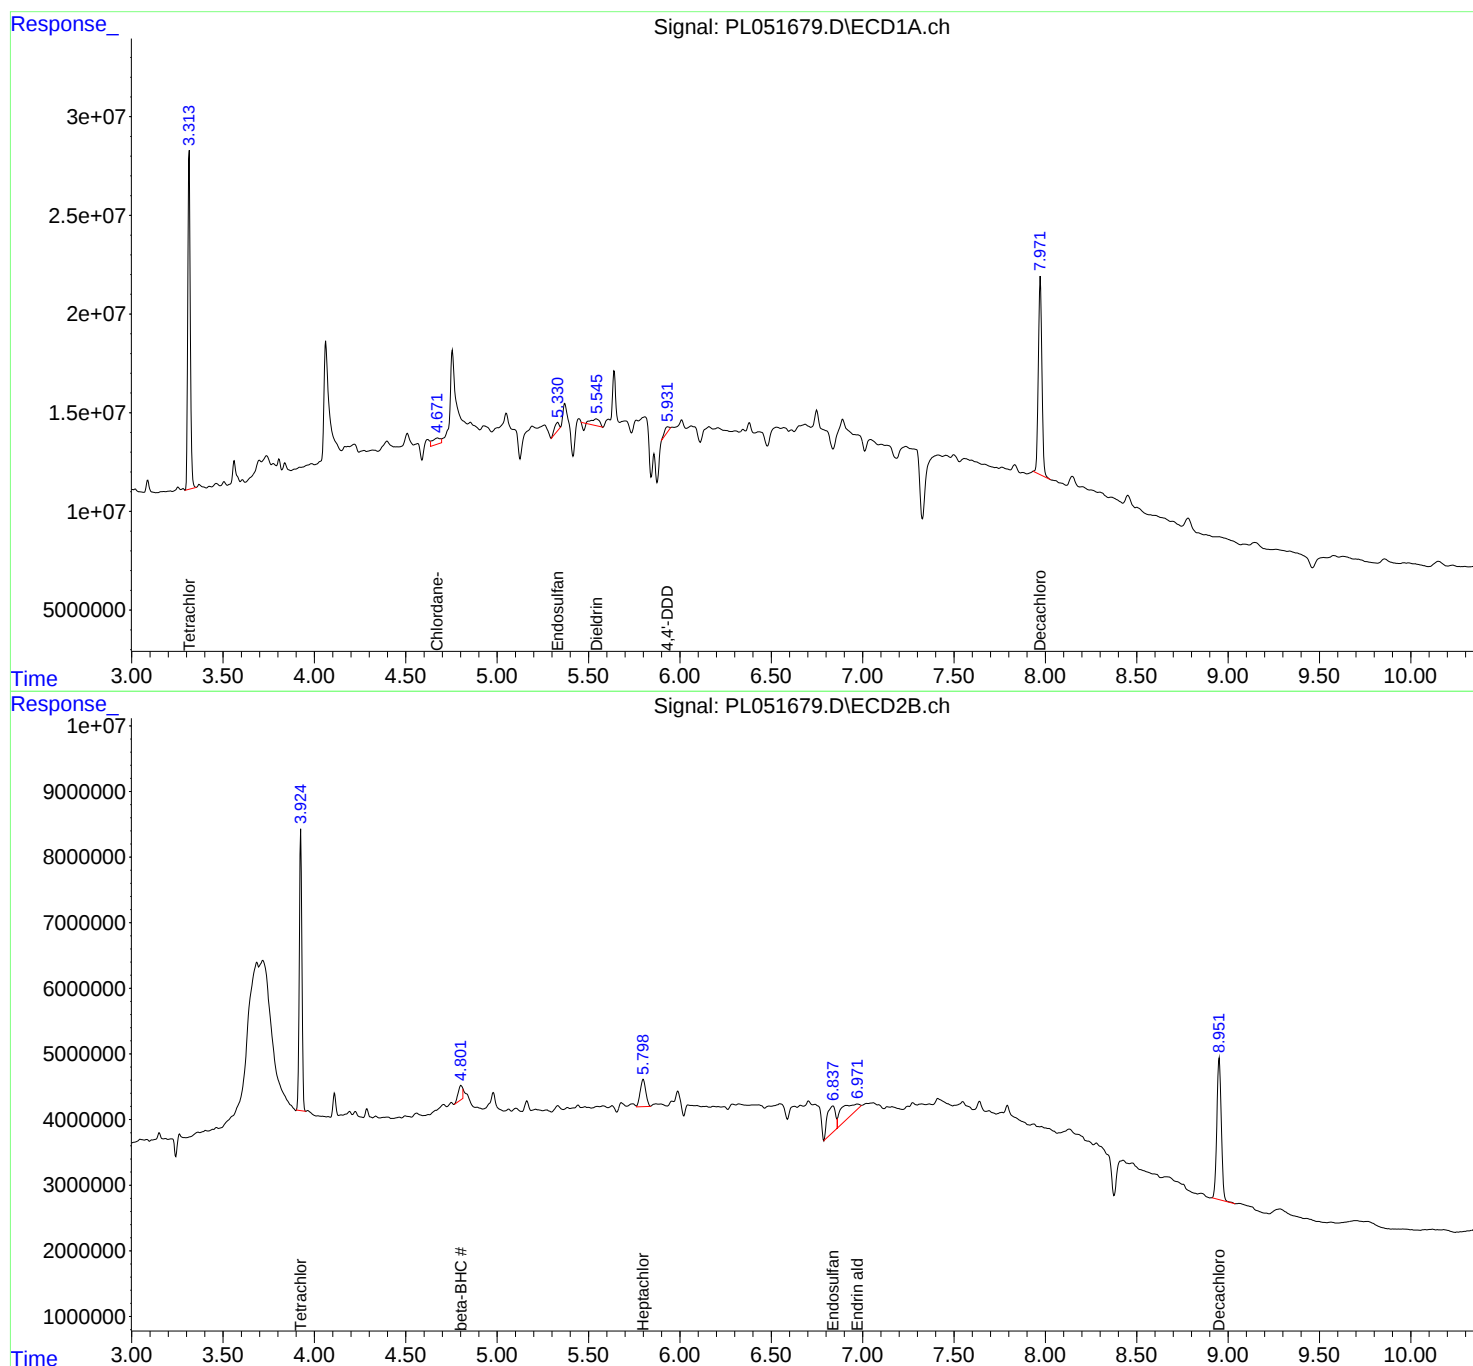


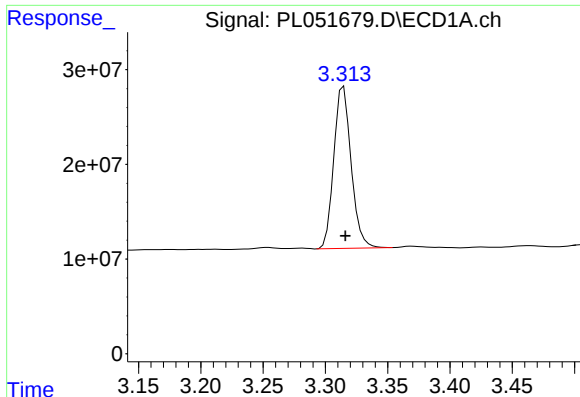

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.001 min
Response: 165624616
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

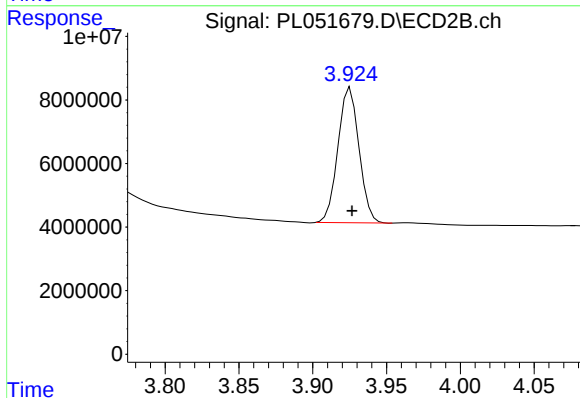


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.001 min
Response: 42344813
Conc: 19.38 ng/ml

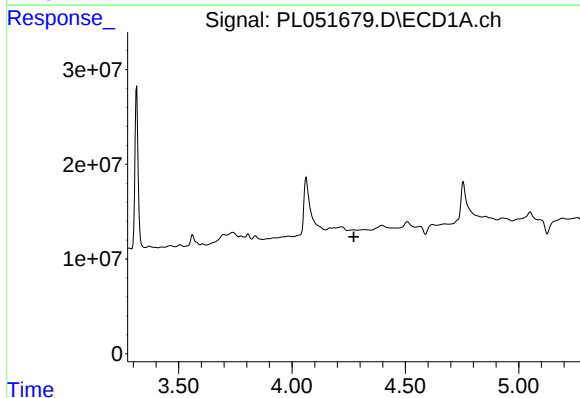


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.273 min
Response: 0
Conc: N.D.

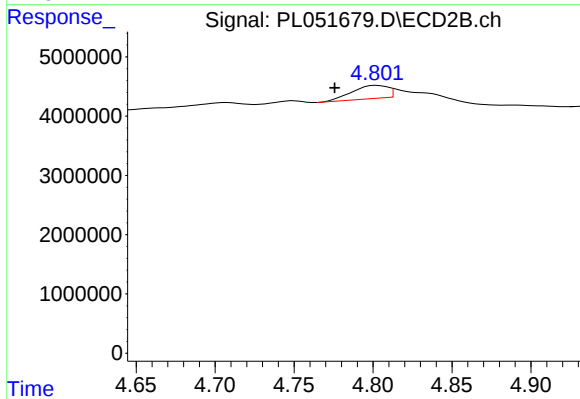

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 3780846
Conc: 2.59 ng/ml

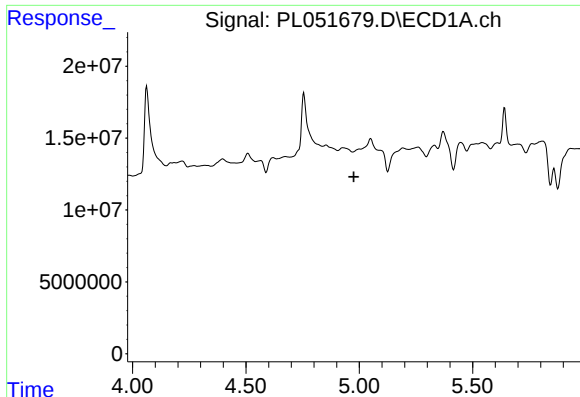

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

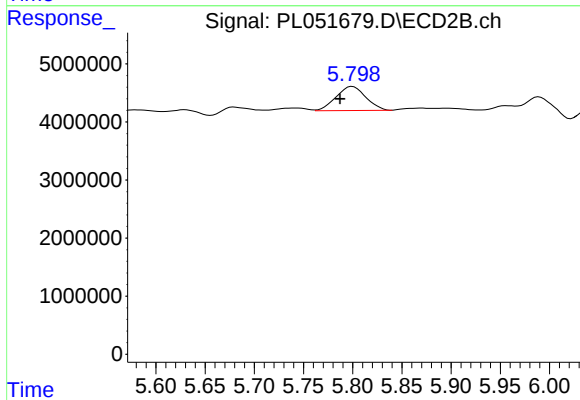


#8 Heptachlor epoxide

R.T.: 5.800 min
Delta R.T.: 0.013 min
Response: 8686863
Conc: 2.57 ng/ml

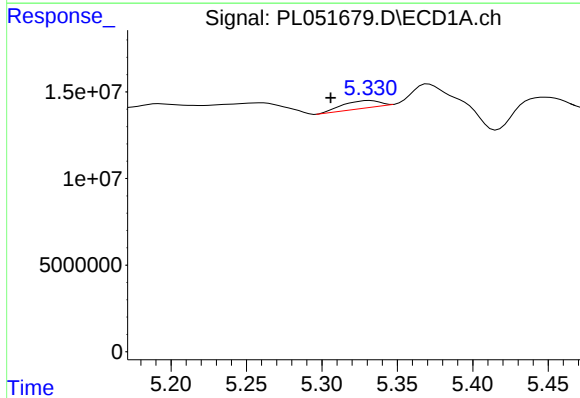


#9 Endosulfan I

R.T.: 5.332 min
Delta R.T.: 0.026 min
Response: 7402137
Conc: 0.55 ng/ml

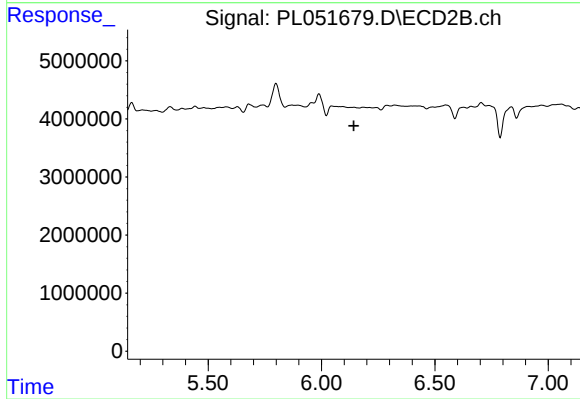

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

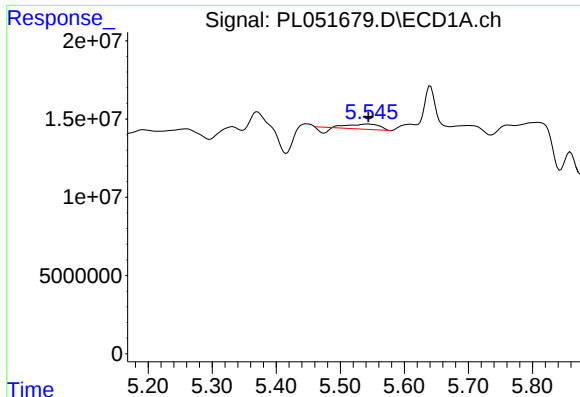

#13 Dieldrin


R.T.: 5.543 min
Delta R.T.: 0.000 min
Response: 8087119
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

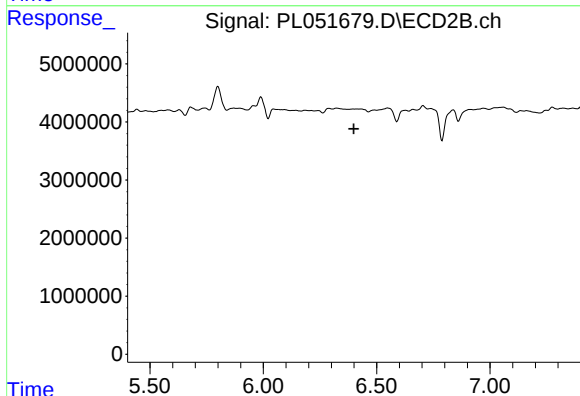


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

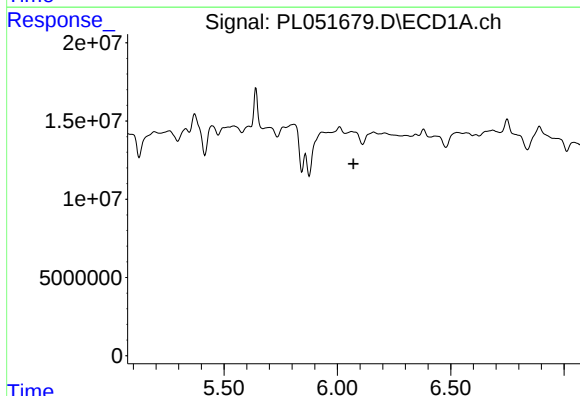


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

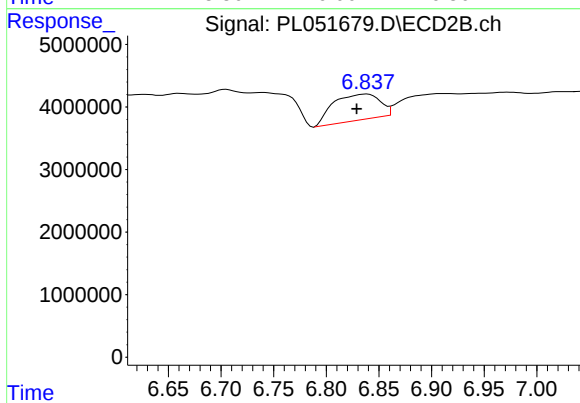

#15 Endosulfan II


R.T.: 6.838 min
Delta R.T.: 0.010 min
Response: 12749453
Conc: 3.87 ng/ml

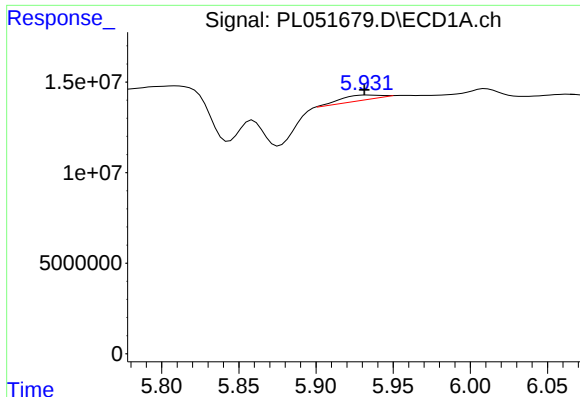

#16 4,4'-DDD


R.T.: 5.933 min
Delta R.T.: 0.002 min
Response: 4979759
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

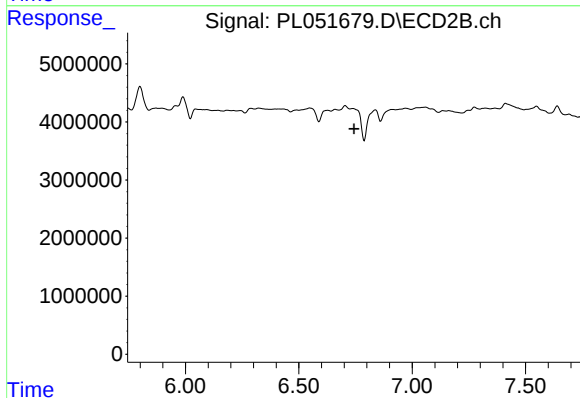


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.744 min
Response: 0
Conc: N.D.

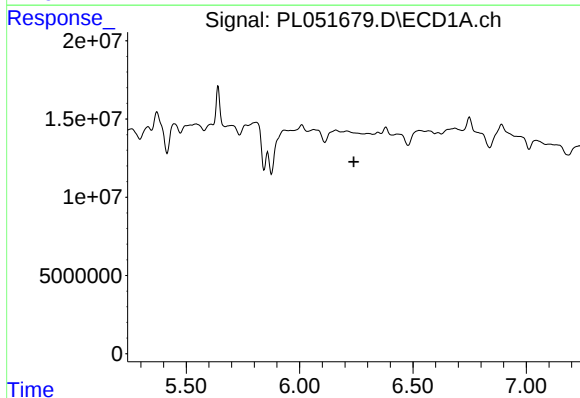


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

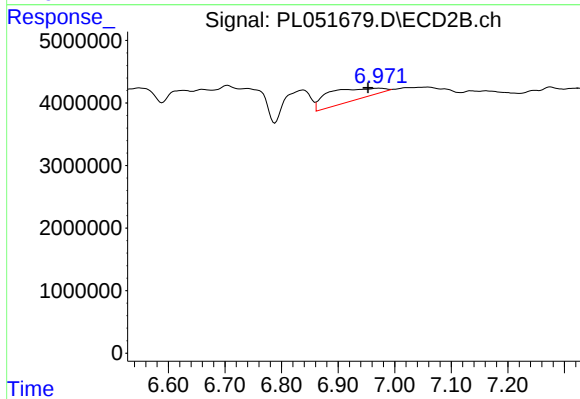

#18 Endrin aldehyde


R.T.: 6.972 min
Delta R.T.: 0.019 min
Response: 12304064
Conc: 4.35 ng/ml

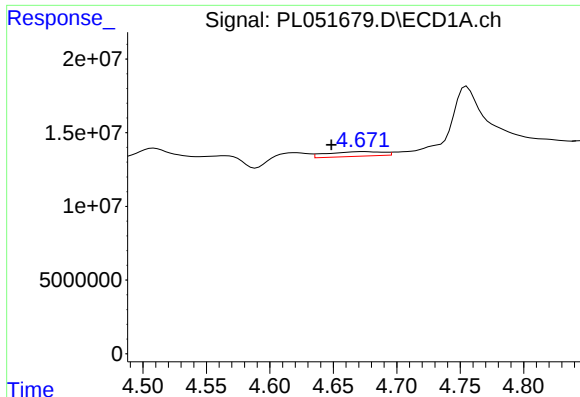

#24 Chlordane-2


R.T.: 4.674 min
Delta R.T.: 0.026 min
Response: 9642848
Conc: 23.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

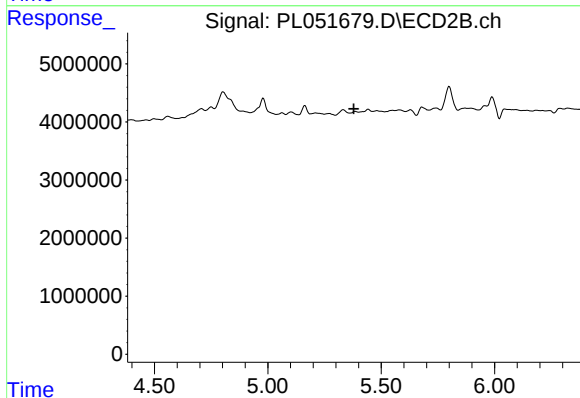


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.380 min
Response: 0
Conc: N.D.

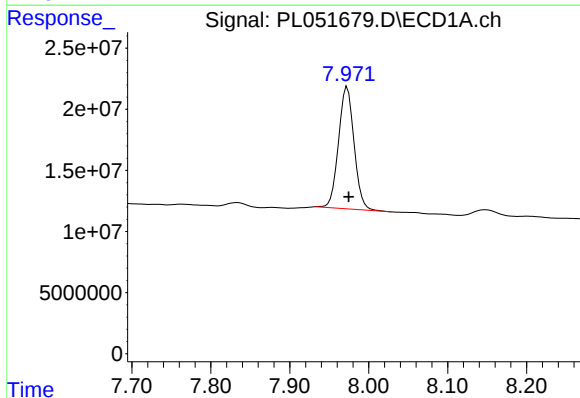

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 136058754
Conc: 11.21 ng/ml

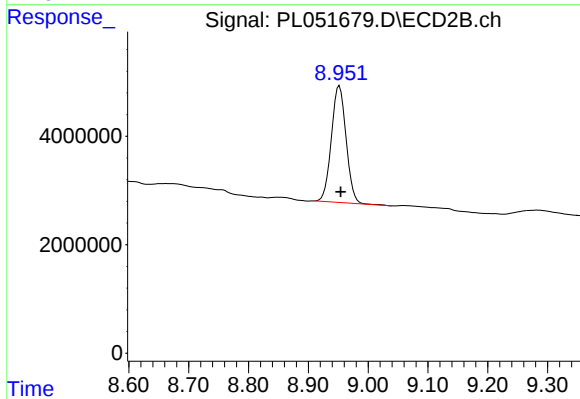

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 36740645
Conc: 12.07 ng/ml