

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
 Data File : PL051624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 08:48
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 08:51:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	3.738	0.000	12315168	0	0.850	N.D. #
6) B	beta-BHC	0.000	4.802f	0	6277449	N.D.	4.307 #
10) B	gamma-Chl...	5.193	5.991f	6013693	4015681	0.403	1.100 #
11) B	alpha-Chl...	5.254	0.000	5139386	0	0.355	N.D. #
25)	Chlordane-3	5.193	0.000	6013693	0	4.632	N.D. #
26)	Chlordane-4	5.254	0.000	5139386	0	4.215	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
Data File : PL051624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 08:48
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 08:51:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

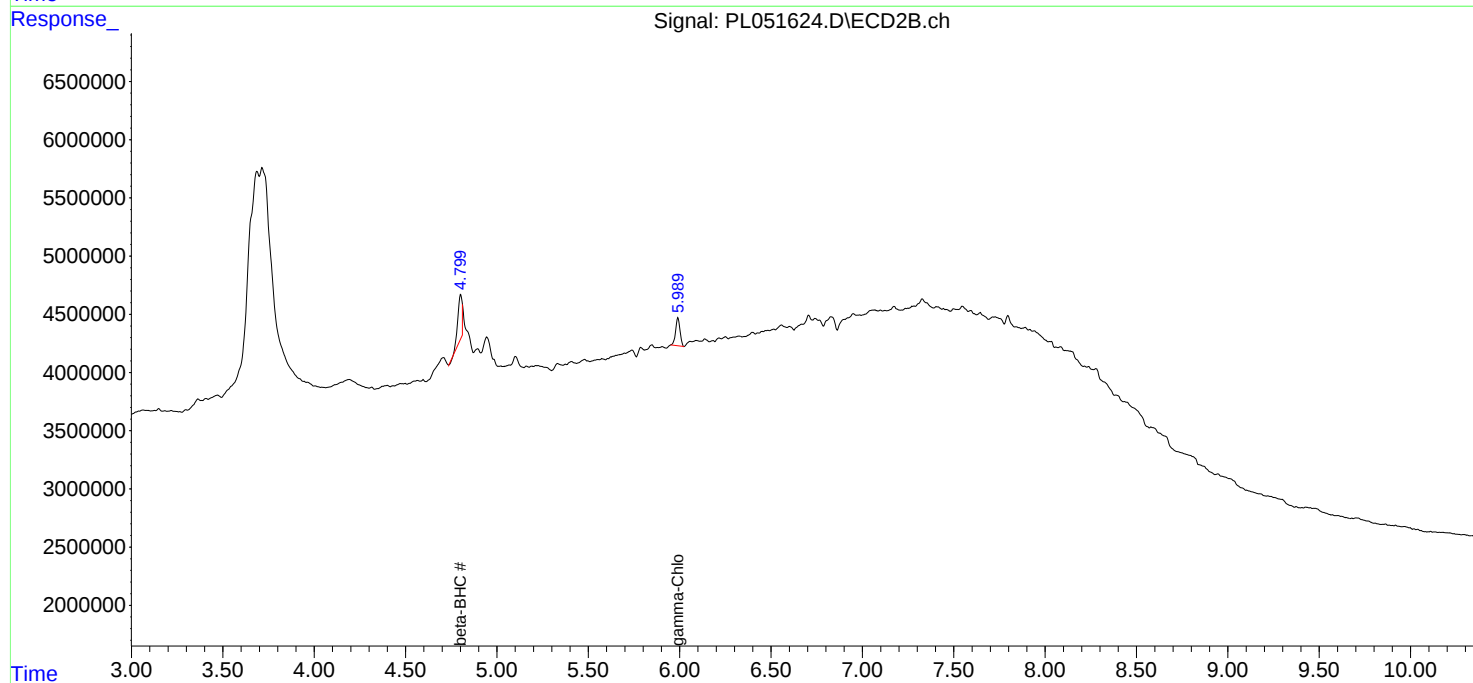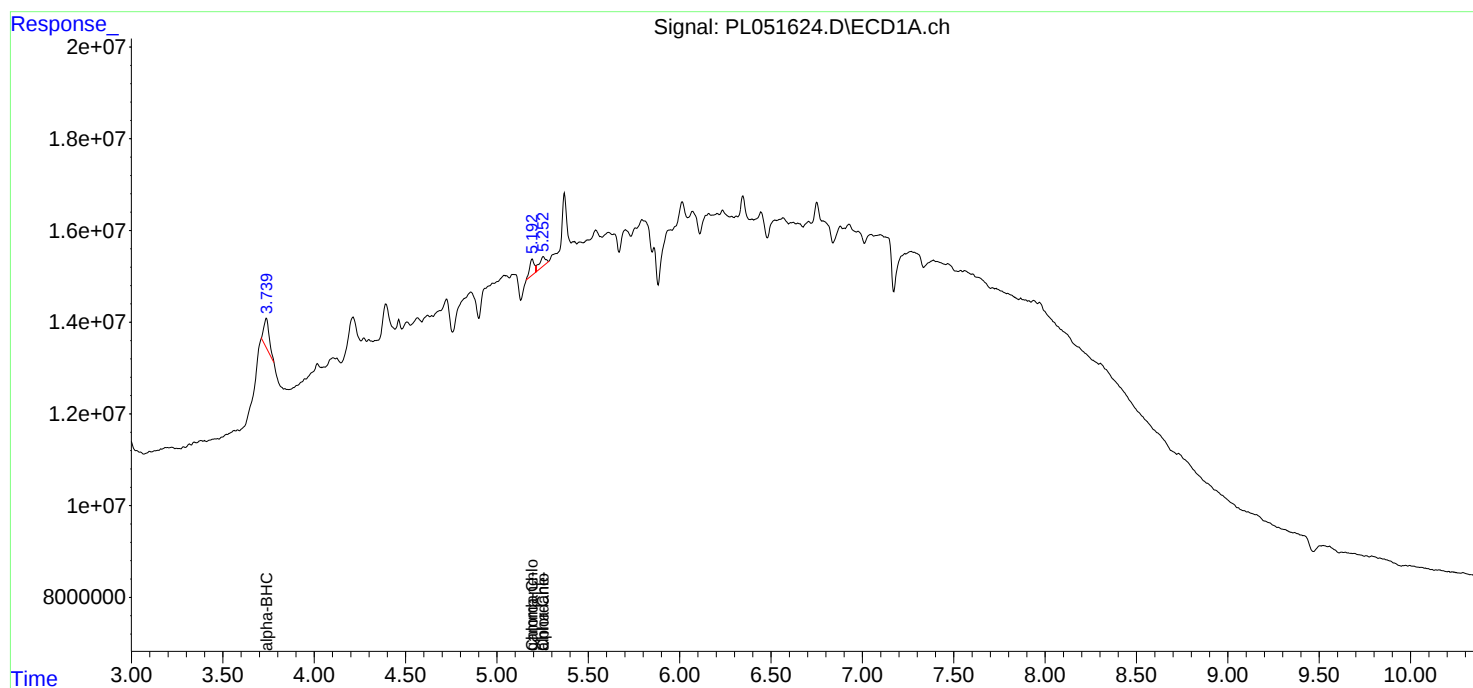


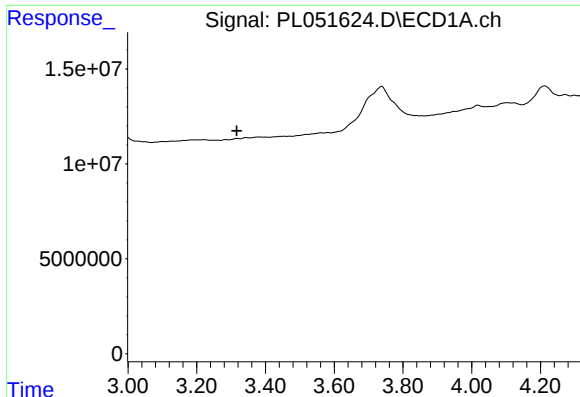

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

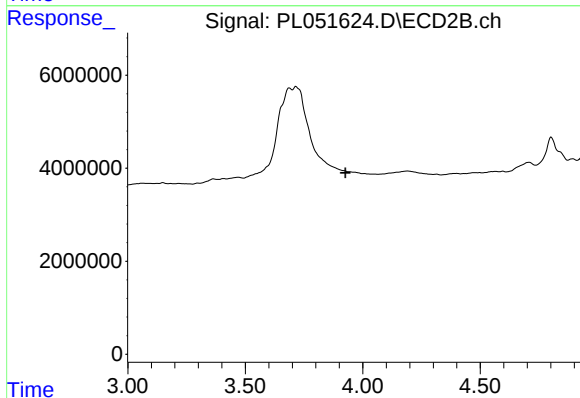


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.927 min
Response: 0
Conc: N.D.

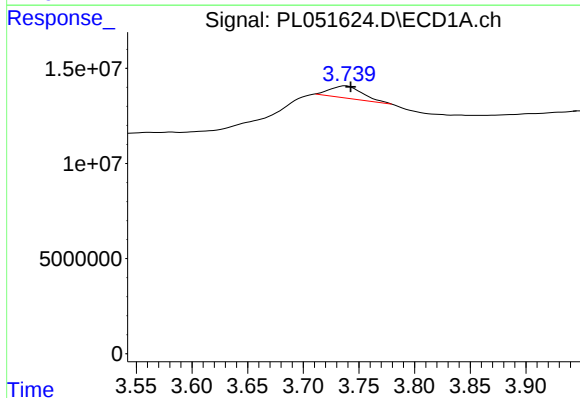


#2 alpha-BHC

R.T.: 3.738 min
Delta R.T.: -0.004 min
Response: 12315168
Conc: 0.85 ng/ml

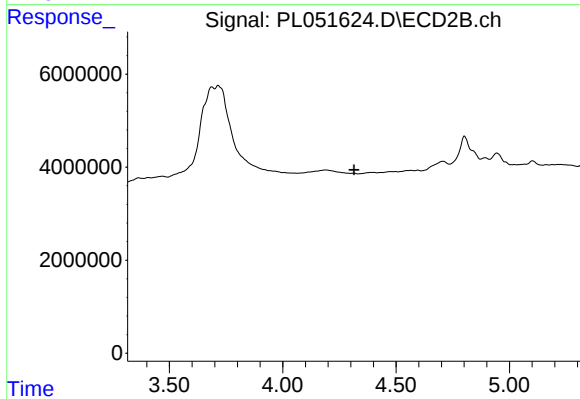

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.315 min
Response: 0
Conc: N.D.

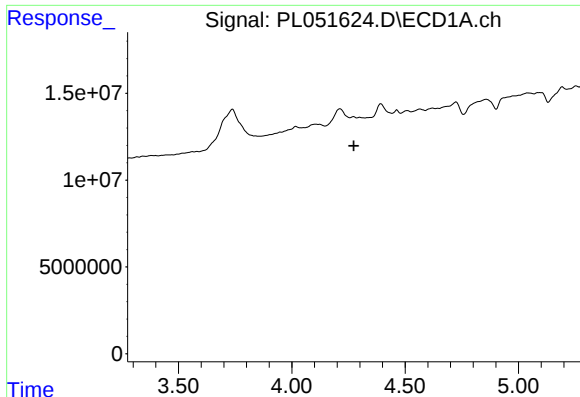

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.273 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

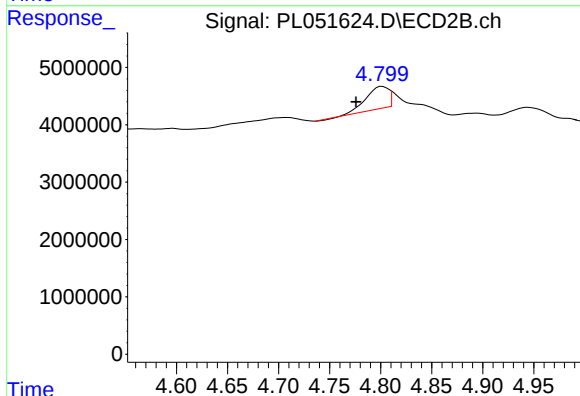


#6 beta-BHC

R.T.: 4.802 min
Delta R.T.: 0.026 min
Response: 6277449
Conc: 4.31 ng/ml

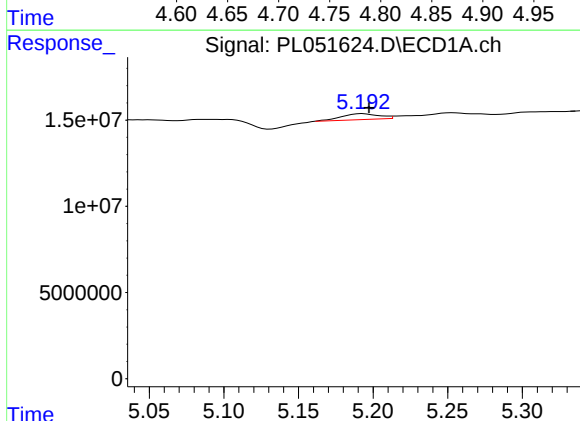


#10 gamma-Chlordane

R.T.: 5.193 min
Delta R.T.: -0.004 min
Response: 6013693
Conc: 0.40 ng/ml

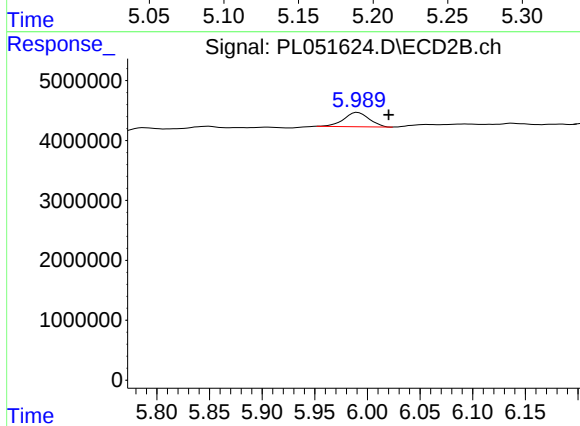

#10 gamma-Chlordane


R.T.: 5.991 min
Delta R.T.: -0.029 min
Response: 4015681
Conc: 1.10 ng/ml

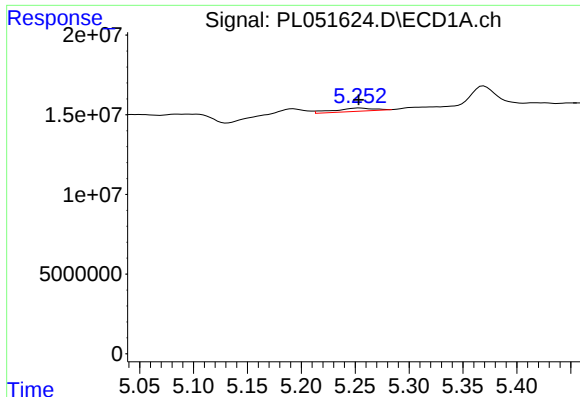

#11 alpha-Chlordane


R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 5139386
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

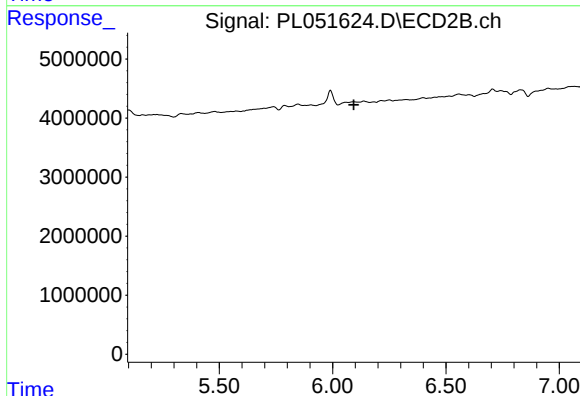


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

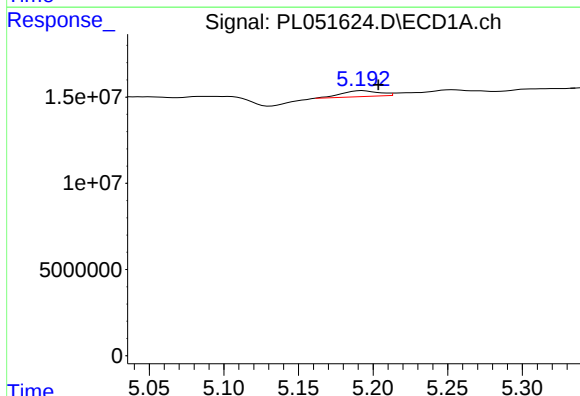


#25 Chlordane-3

R.T.: 5.193 min
Delta R.T.: -0.011 min
Response: 6013693
Conc: 4.63 ng/ml

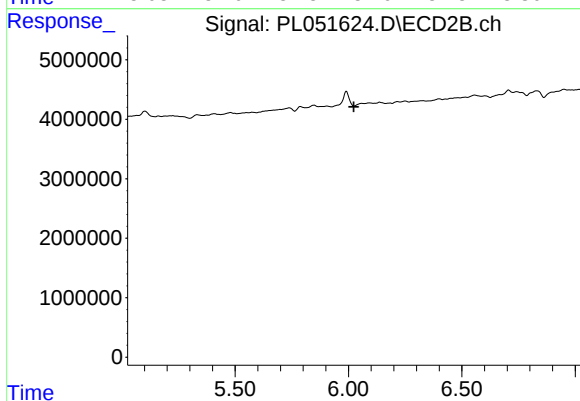

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

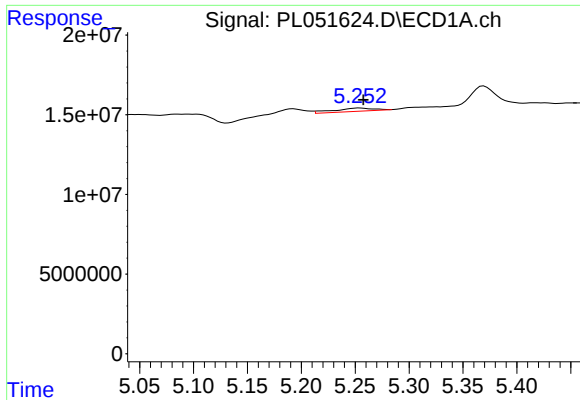

#26 Chlordane-4


R.T.: 5.254 min
Delta R.T.: -0.003 min
Response: 5139386
Conc: 4.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

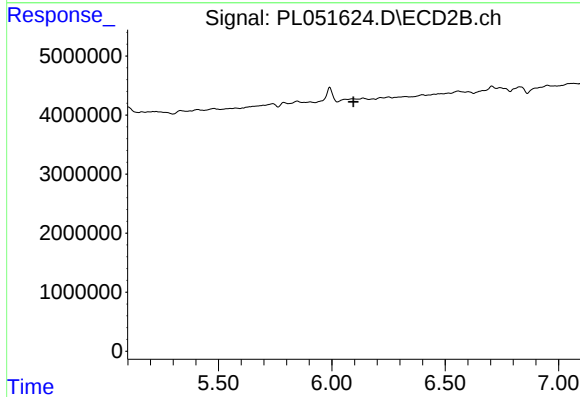


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

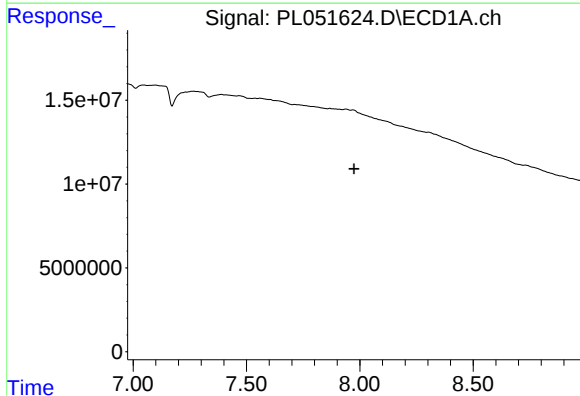

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.975 min
Response: 0
Conc: N.D.

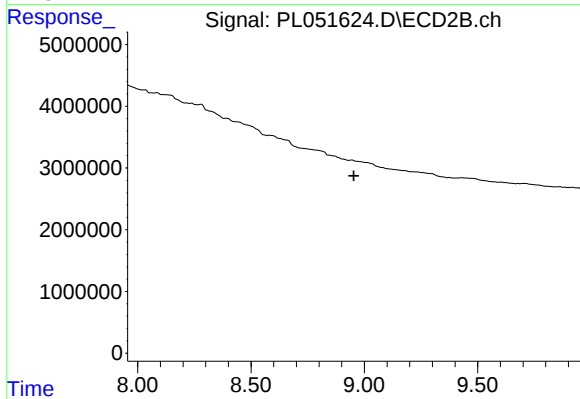

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.954 min
Response: 0
Conc: N.D.