

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
 Data File : PL051676.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 23:45
 Operator : SG\AJ
 Sample : K4403-10
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T1-G-(0-2.5)

Manual Integrations
 APPROVED

Ankita
 8/23/2019 2:20:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:32:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.926	120.7E6	30853214	14.101	14.122
28)	SA Decachlor...	7.973	8.953	120.5E6	34103802	9.925	11.204
Target Compounds							
12)	B 4,4'-DDE	5.418	6.248	4452086	1875650	0.325m	0.533m#
14)	MA Endrin	5.798	6.608	14280862	2892633	0.979m	0.956m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
Data File : PL051676.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 23:45
Operator : SG\AJ
Sample : K4403-10
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
T1-G-(0-2.5)


Manual Integrations
APPROVED

Ankita
8/23/2019 2:20:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:32:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

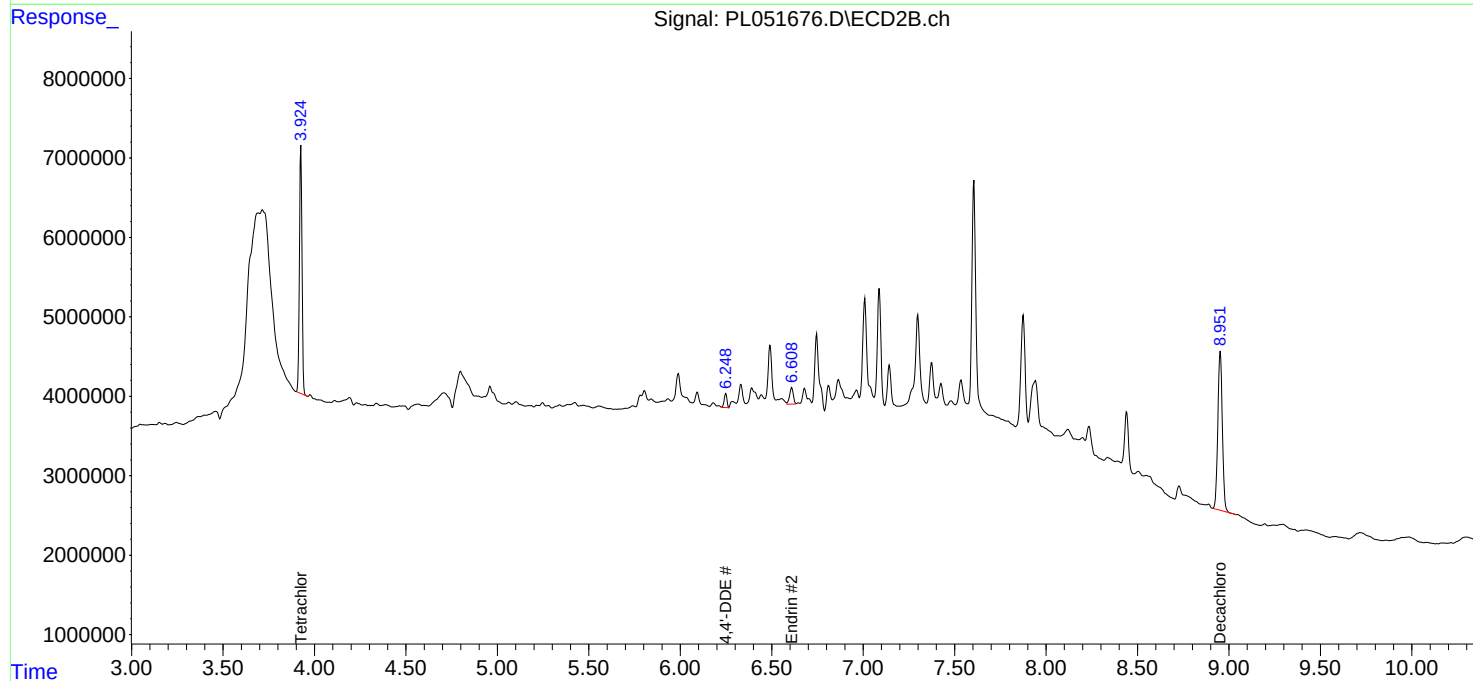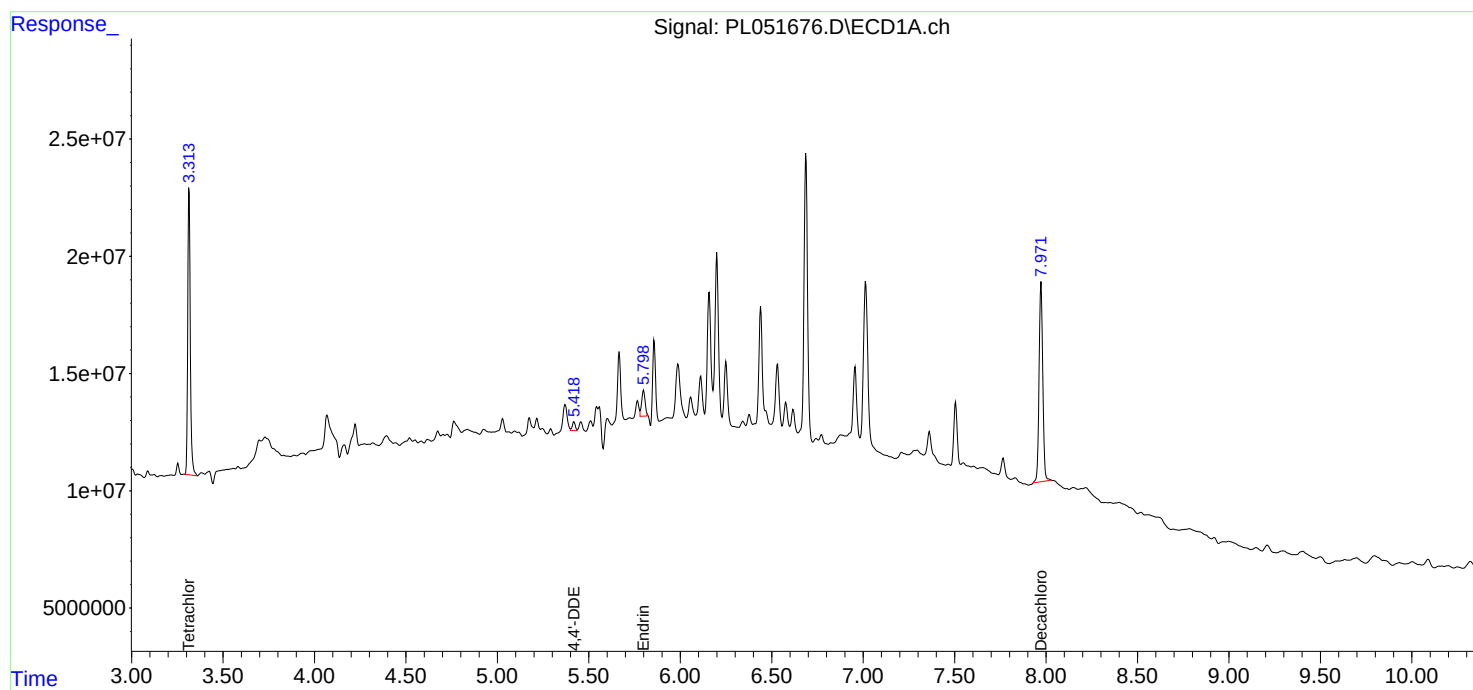

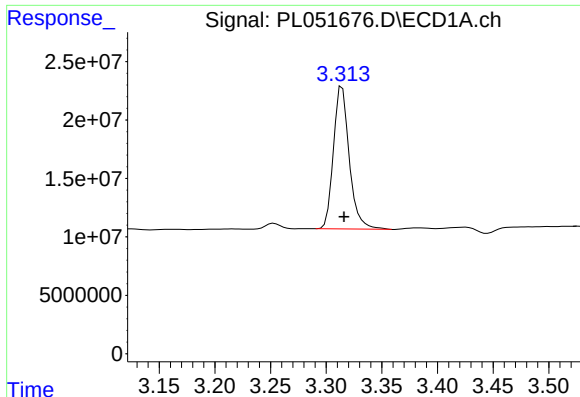


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 120683901
Conc: 14.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
T1-G-(0-2.5)


Manual Integrations
APPROVED

Ankita
8/23/2019 2:20:07 PM

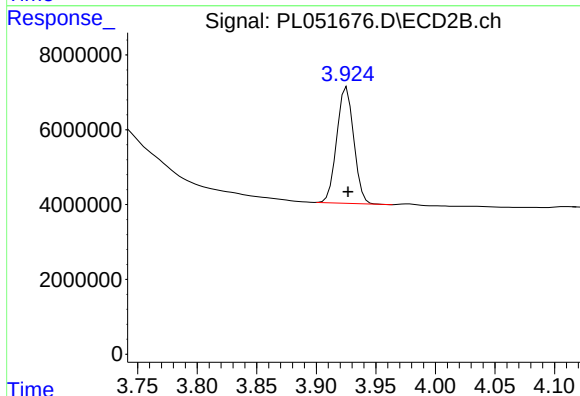


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.001 min
Response: 30853214
Conc: 14.12 ng/ml

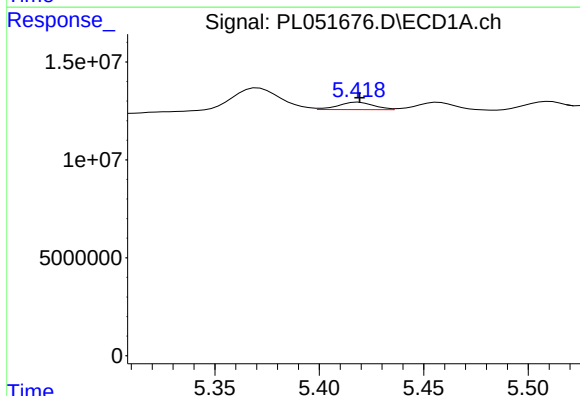


#12 4,4'-DDE

R.T.: 5.418 min
Delta R.T.: -0.002 min
Response: 4452086
Conc: 0.33 ng/ml m

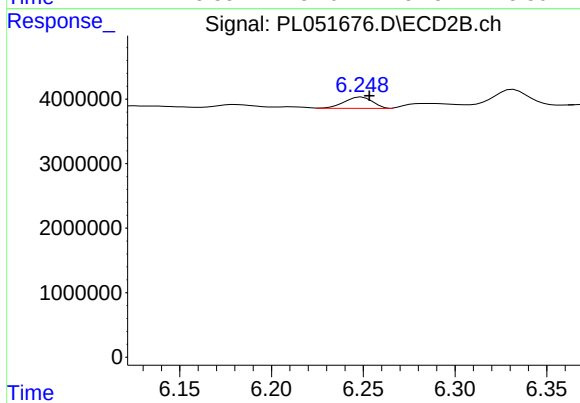

#12 4,4'-DDE

R.T.: 6.248 min
Delta R.T.: -0.005 min
Response: 1875650
Conc: 0.53 ng/ml m

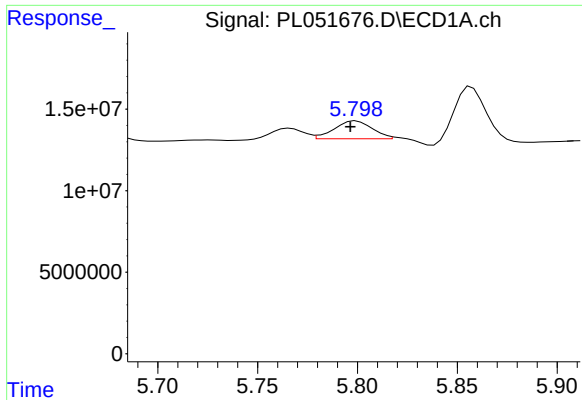


#14 Endrin

R.T.: 5.798 min
Delta R.T.: 0.002 min
Response: 14280862
Conc: 0.98 ng/ml m

Instrument :
ECD_L
ClientSampleId :
T1-G-(0-2.5)


Manual Integrations
APPROVED

Ankita
8/23/2019 2:20:07 PM

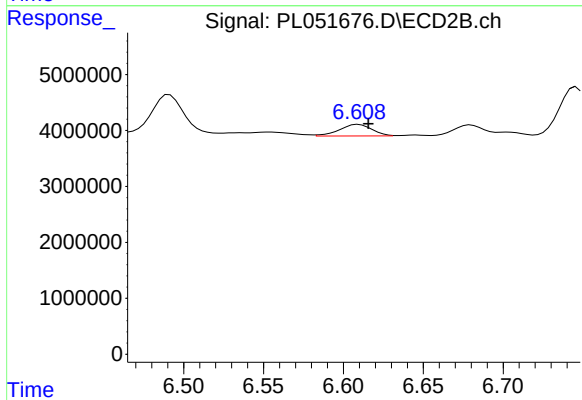


#14 Endrin

R.T.: 6.608 min
Delta R.T.: -0.008 min
Response: 2892633
Conc: 0.96 ng/ml m

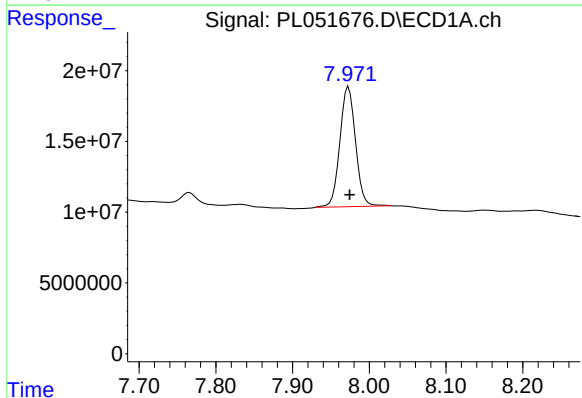

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 120472623
Conc: 9.93 ng/ml

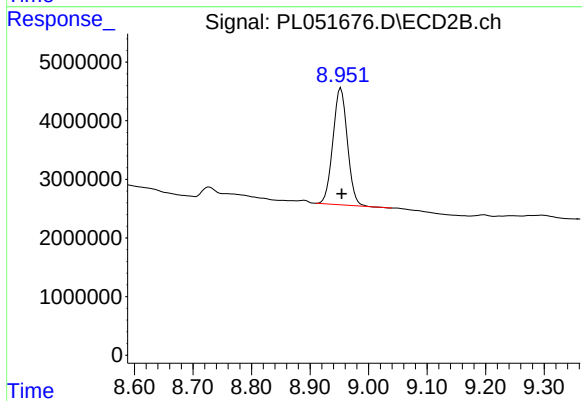

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.002 min
Response: 34103802
Conc: 11.20 ng/ml