

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
 Data File : PL051677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2019 23:59
 Operator : SG\AJ
 Sample : K4403-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T1-I-(0-2.5)

Manual Integrations
 APPROVED

Ankita
 8/23/2019 2:19:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 01:32:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 19 18:03:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.925	119.8E6	31220163	13.997	14.290
28)	SA Decachlor...	7.972	8.952	125.8E6	32925369	10.362	10.817
Target Compounds							
11)	B alpha-Chl...	5.248	6.092	5553182	2309131	0.384m	0.669m#
14)	MA Endrin	5.798	6.609	22586887	3920498	1.549m	1.296m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082019\
Data File : PL051677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2019 23:59
Operator : SG\AJ
Sample : K4403-13
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
T1-I-(0-2.5)


Manual Integrations
APPROVED

Ankita
8/23/2019 2:19:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 01:32:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081919.M
Quant Title : GC Extractables
QLast Update : Mon Aug 19 18:03:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

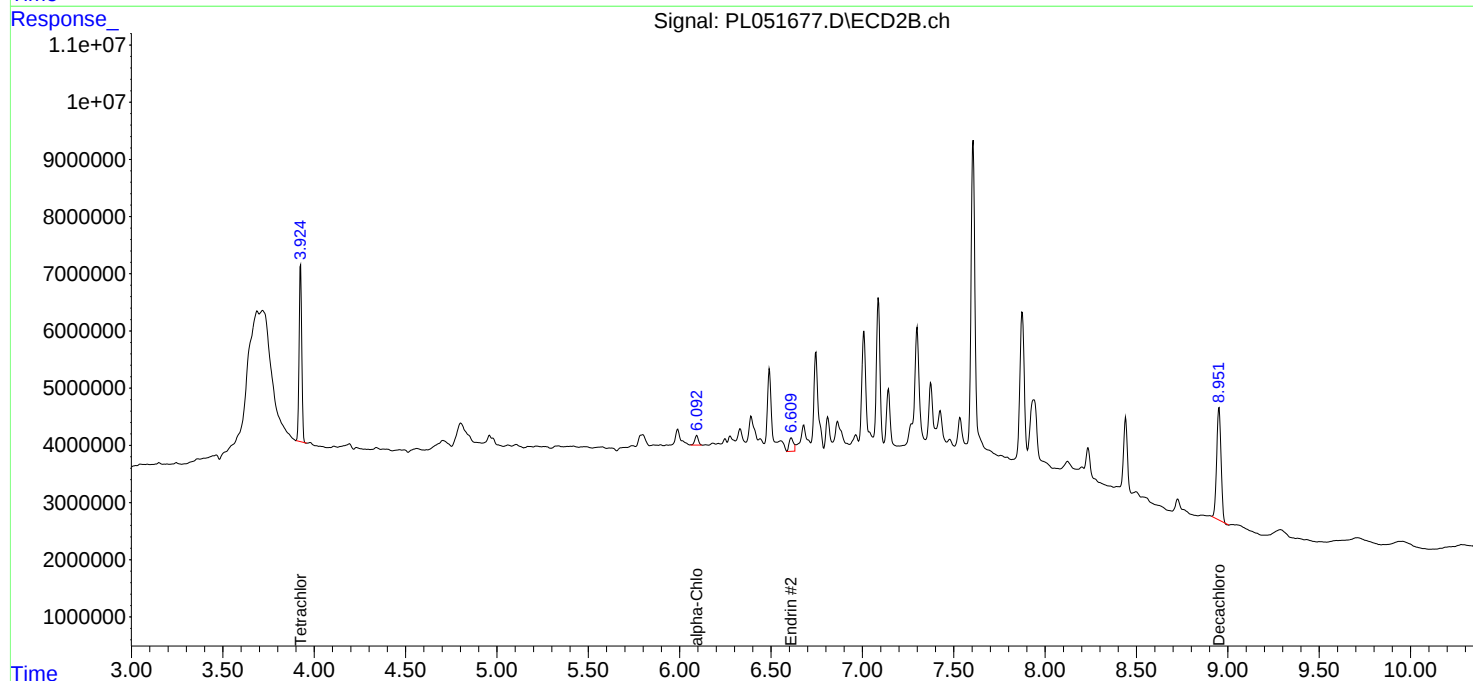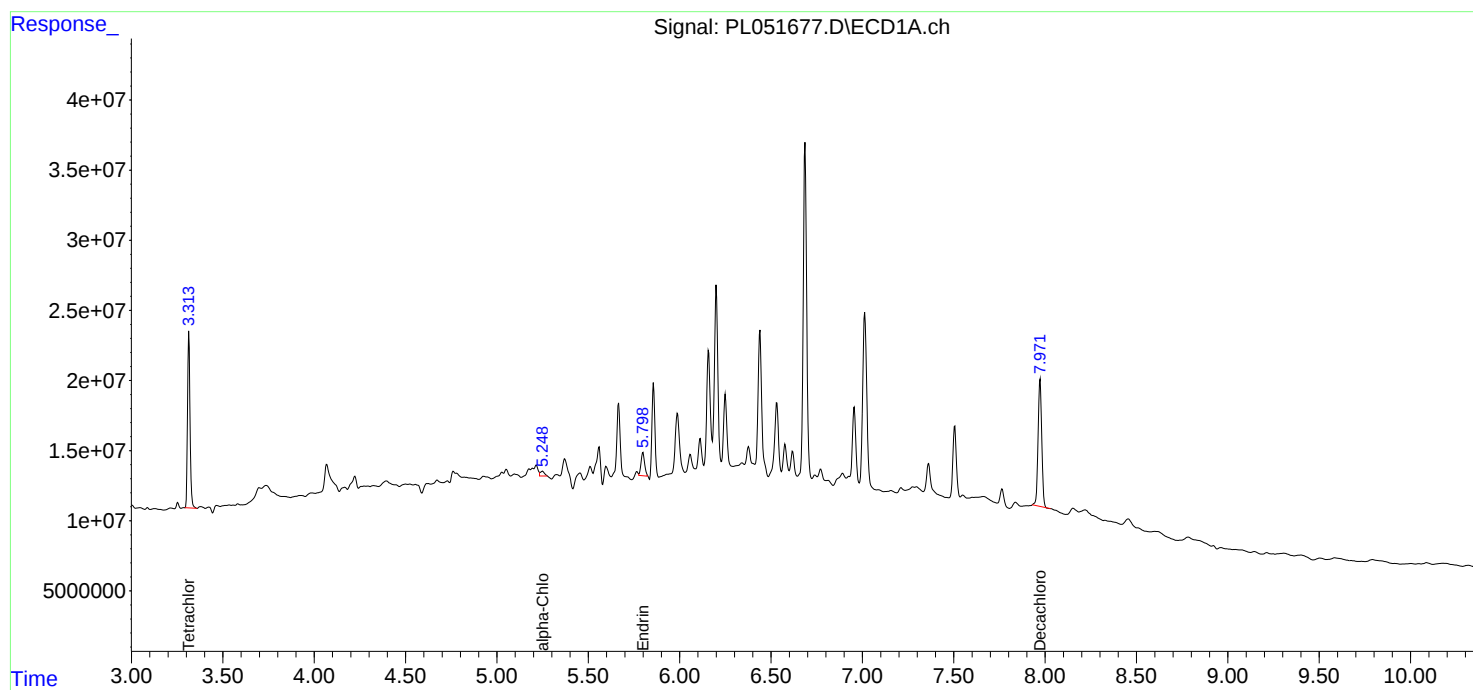

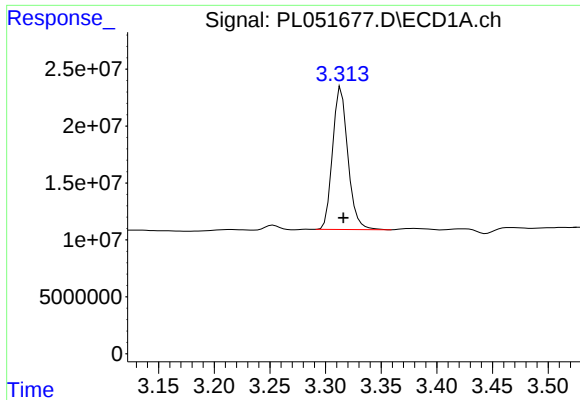


#1 Tetrachloro-m-xylene

R.T.: 3.314 min
Delta R.T.: -0.002 min
Response: 119792233
Conc: 14.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
T1-I-(0-2.5)


Manual Integrations
APPROVED

Ankita
8/23/2019 2:19:01 PM

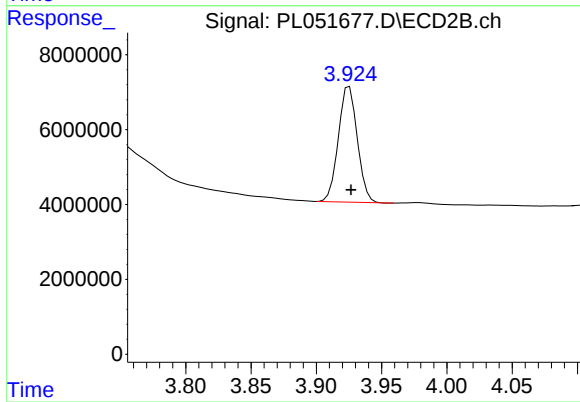


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.001 min
Response: 31220163
Conc: 14.29 ng/ml

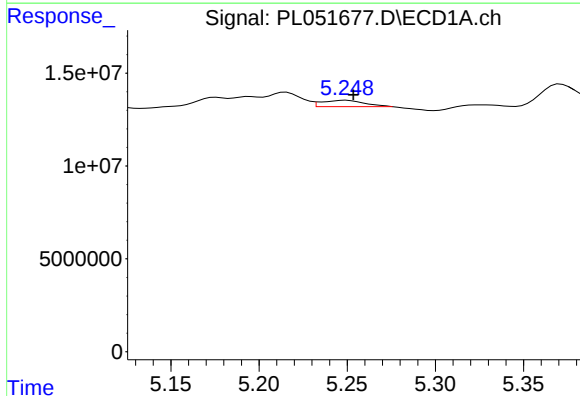


#11 alpha-Chlordane

R.T.: 5.248 min
Delta R.T.: -0.005 min
Response: 5553182
Conc: 0.38 ng/ml m

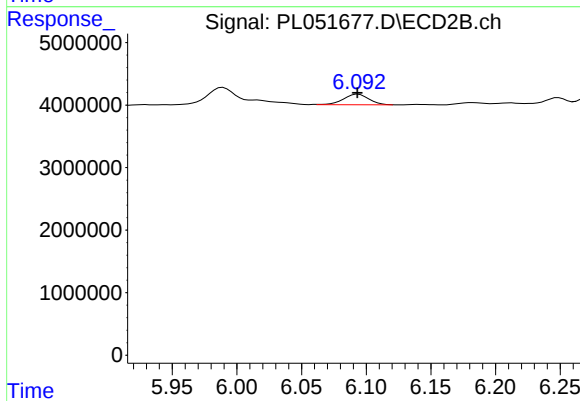

#11 alpha-Chlordane

R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 2309131
Conc: 0.67 ng/ml m

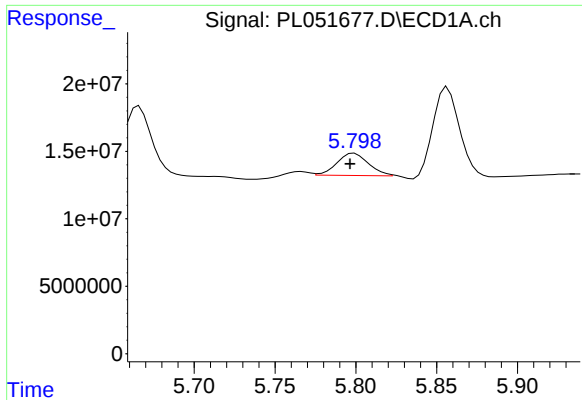


#14 Endrin

R.T.: 5.798 min
Delta R.T.: 0.001 min
Response: 22586887
Conc: 1.55 ng/ml m

Instrument :
ECD_L
ClientSampleId :
T1-I-(0-2.5)


Manual Integrations
APPROVED

Ankita
8/23/2019 2:19:01 PM

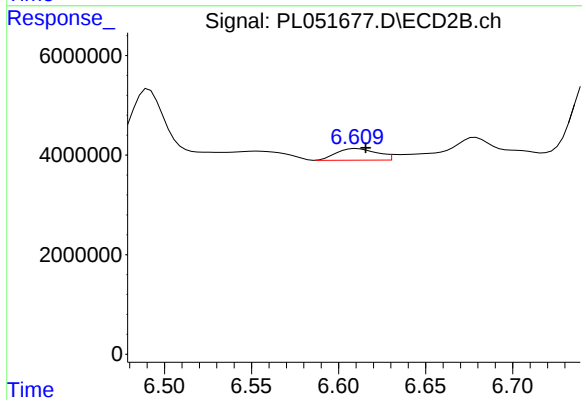


#14 Endrin

R.T.: 6.609 min
Delta R.T.: -0.007 min
Response: 3920498
Conc: 1.30 ng/ml m

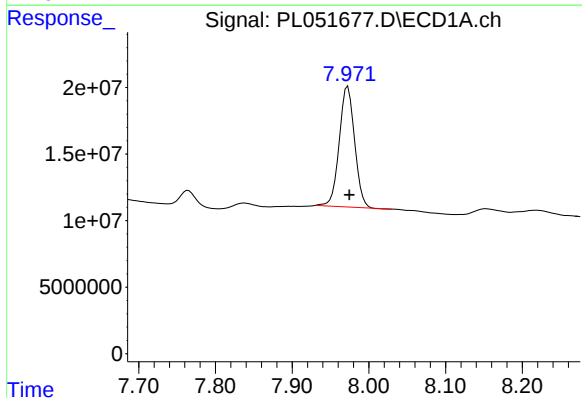

#28 Decachlorobiphenyl

R.T.: 7.972 min
Delta R.T.: -0.002 min
Response: 125770816
Conc: 10.36 ng/ml

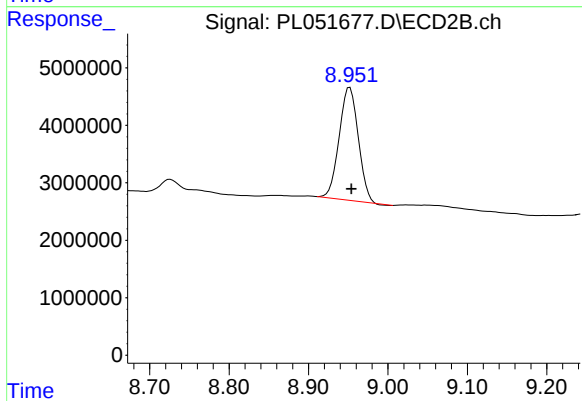

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.002 min
Response: 32925369
Conc: 10.82 ng/ml