

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
 Data File : PL096921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 15:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 06:37:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.825	68735701	100.2E6	17.429	17.773
28)	SA Decachlor...	9.002	7.985	56495954	90361068	19.082	18.842
Target Compounds							
15)	B Endosulfa...	6.734	0.000	13597794	0	3.087	N.D. #
18)	B Endrin al...	0.000	6.168	0	21849768	N.D.	0.786 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
Data File : PL096921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 15:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 06:37:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

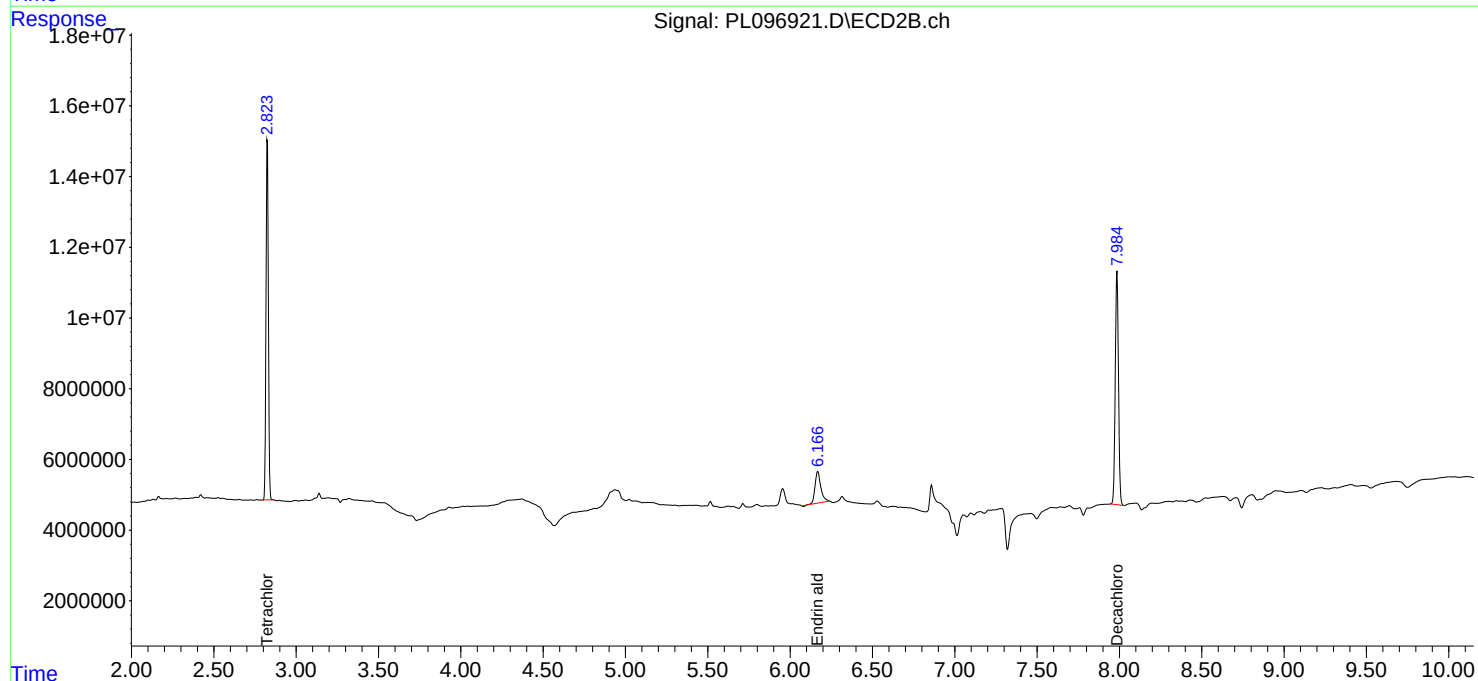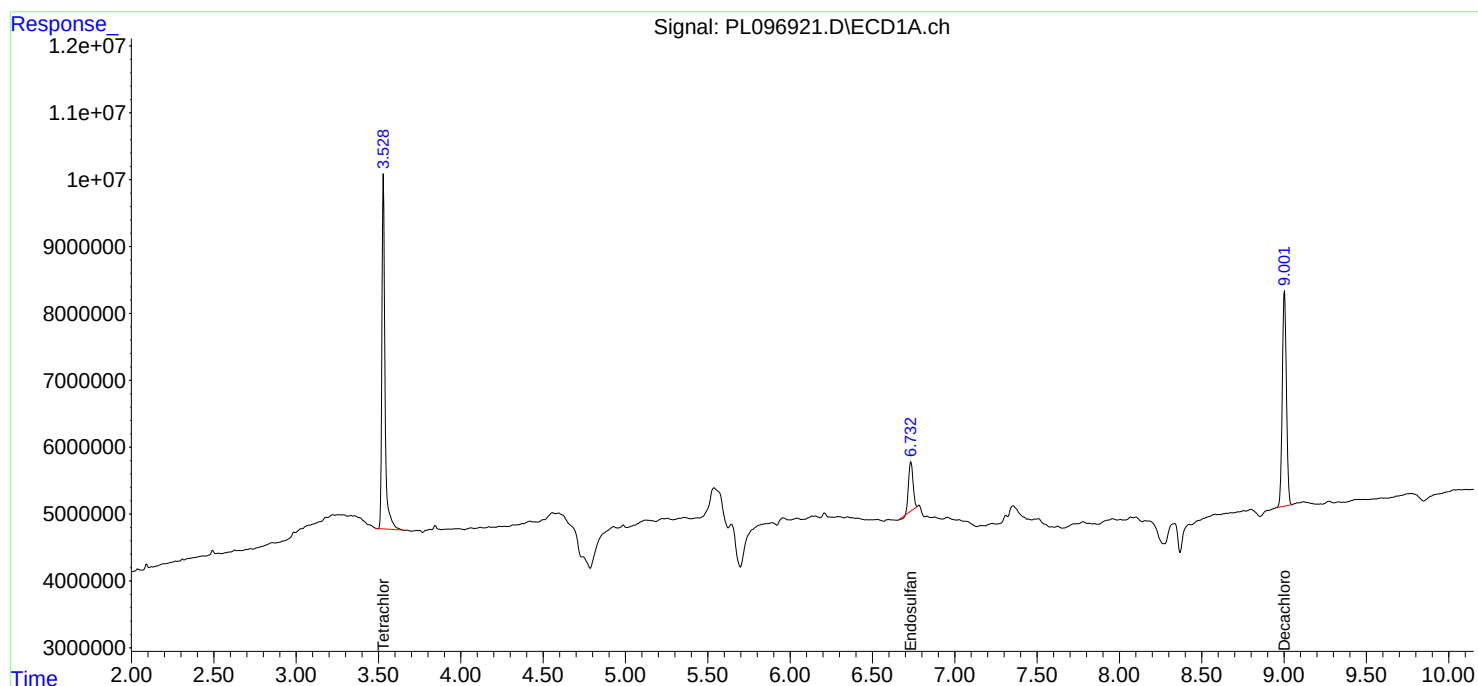


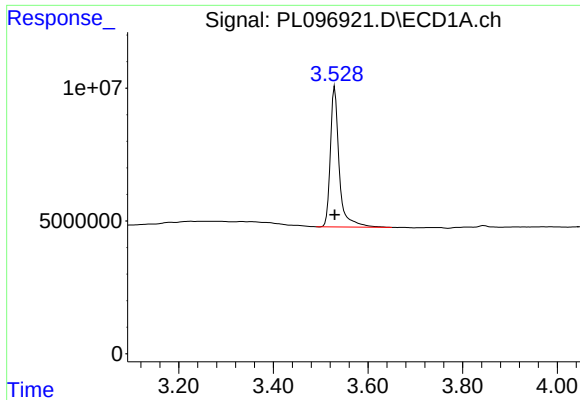

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 68735701
Conc: 17.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

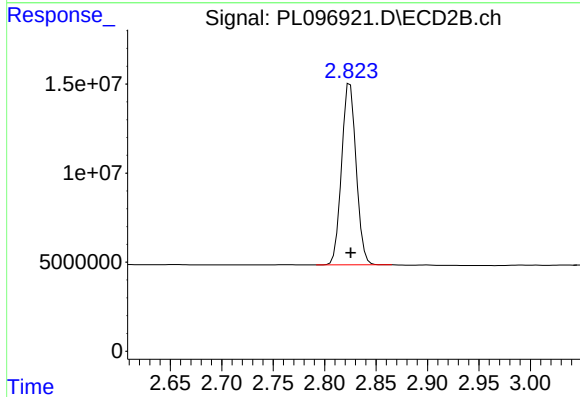


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: 0.000 min
Response: 100178595
Conc: 17.77 ng/ml

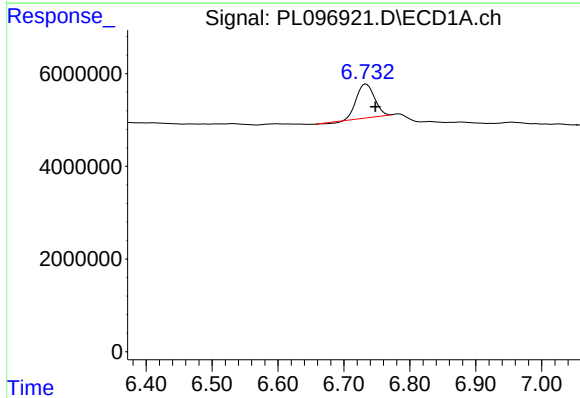


#15 Endosulfan II

R.T.: 6.734 min
Delta R.T.: -0.014 min
Response: 13597794
Conc: 3.09 ng/ml

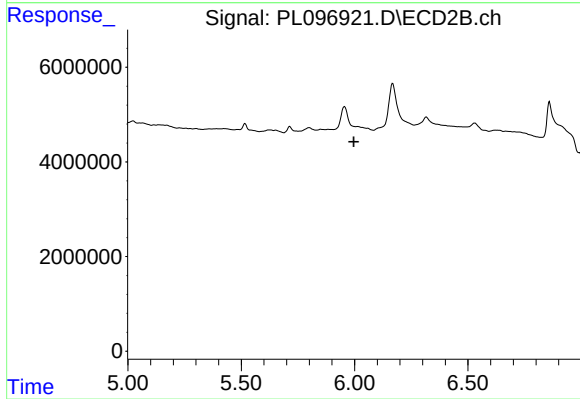

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

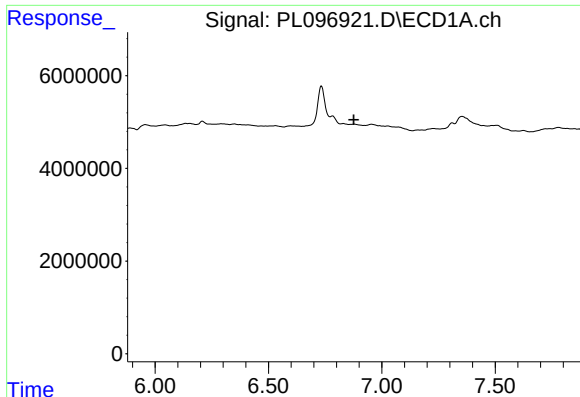

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.876 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

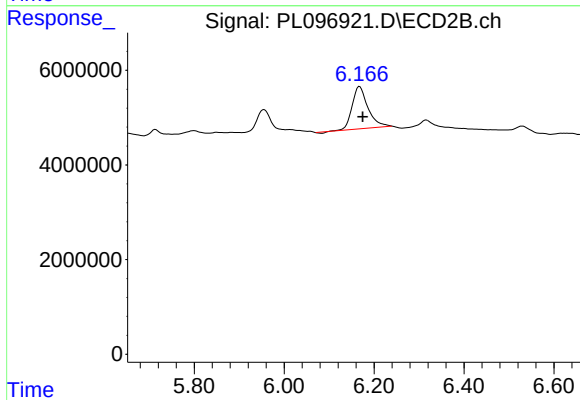


#18 Endrin aldehyde

R.T.: 6.168 min
Delta R.T.: -0.007 min
Response: 21849768
Conc: 0.79 ng/ml

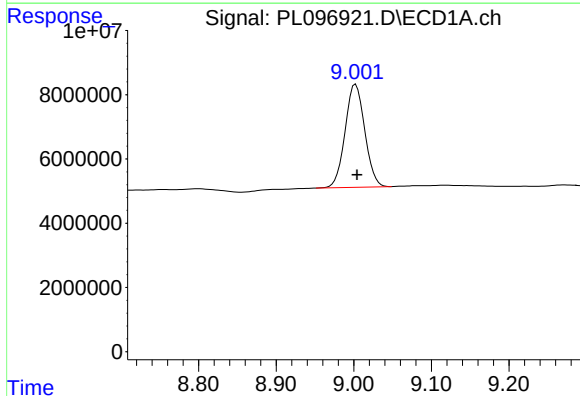

#28 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: -0.001 min
Response: 56495954
Conc: 19.08 ng/ml

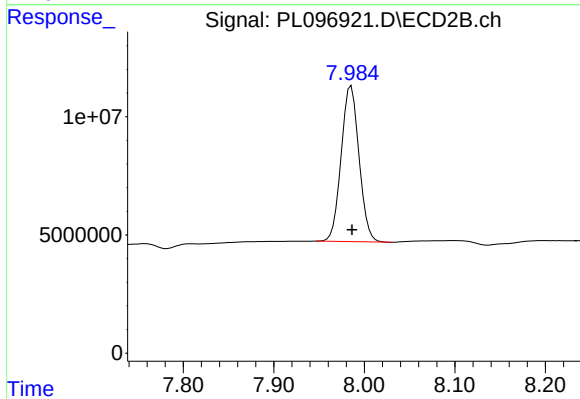

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.001 min
Response: 90361068
Conc: 18.84 ng/ml