

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
 Data File : PL096929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 17:33
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:51:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 04:50:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	2.823	284.1E6	546.7E6	101.646	104.520
28)	SA Decachlor...	9.003	7.986	207.6E6	348.4E6	99.389	101.972
Target Compounds							
23)	Chlordane-1	4.683	3.834	175.8E6	206.5E6	1020.424	1030.695
24)	Chlordane-2	5.206	4.413	182.0E6	232.7E6	988.829	1004.769
25)	Chlordane-3	5.909	5.046	674.9E6	699.7E6	1039.502	1081.984
26)	Chlordane-4	5.993	5.109	839.5E6	614.3E6	1031.694	1063.931
27)	Chlordane-5	6.830	6.004	139.9E6	244.2E6	1027.405	1050.727



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
Data File : PL096929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 17:33
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:51:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 04:50:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

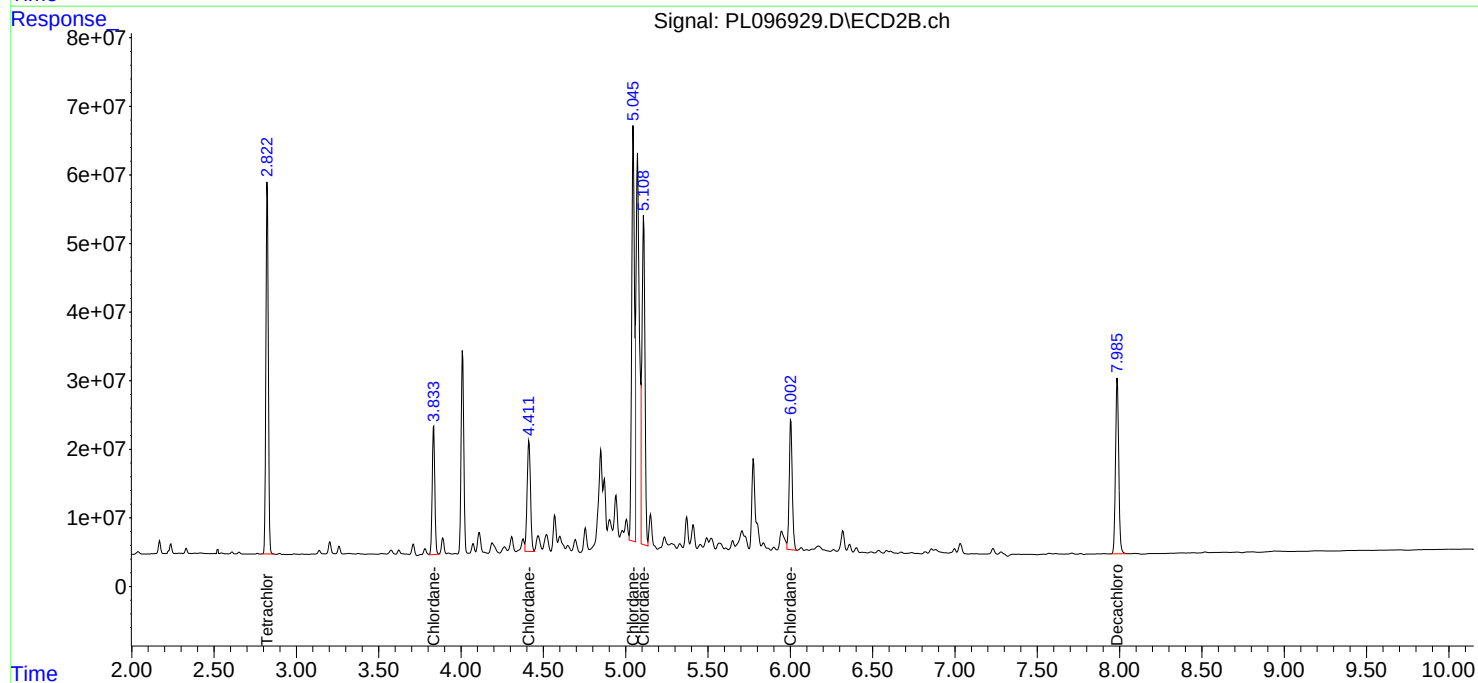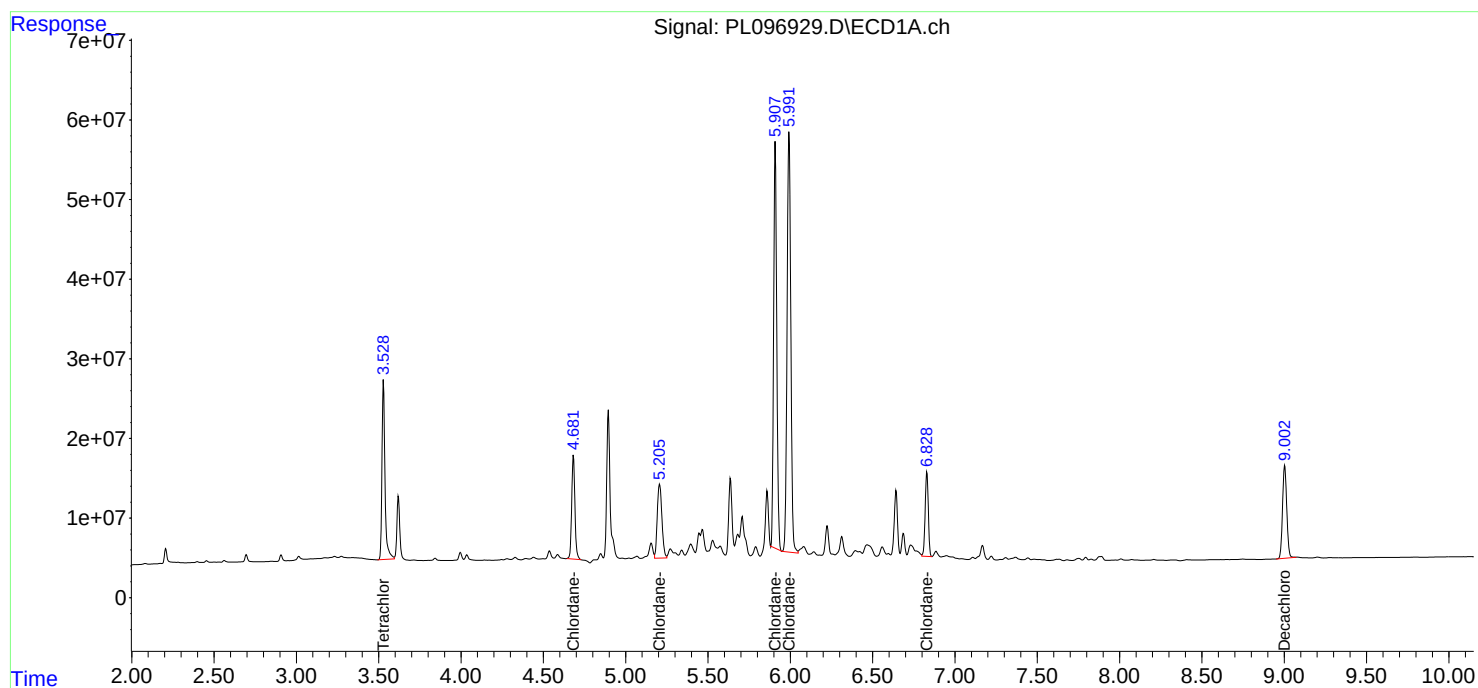


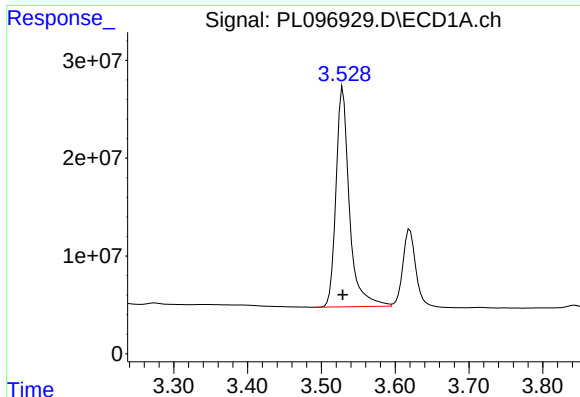

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 284139653
Conc: 101.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

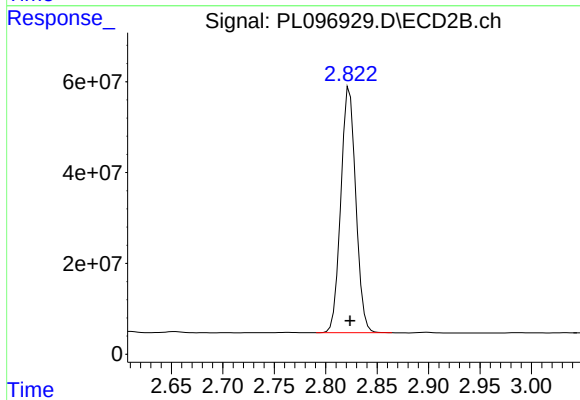


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 546732452
Conc: 104.52 ng/ml

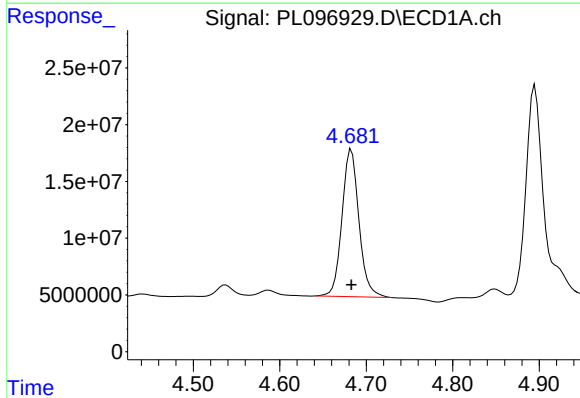


#23 Chlordane-1

R.T.: 4.683 min
Delta R.T.: 0.000 min
Response: 175765150
Conc: 1020.42 ng/ml

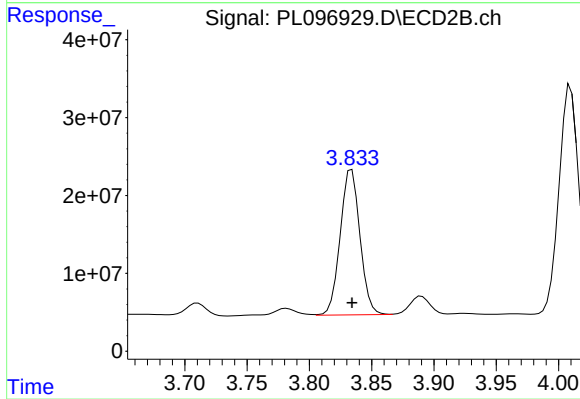

#23 Chlordane-1


R.T.: 3.834 min
Delta R.T.: 0.000 min
Response: 206495891
Conc: 1030.69 ng/ml

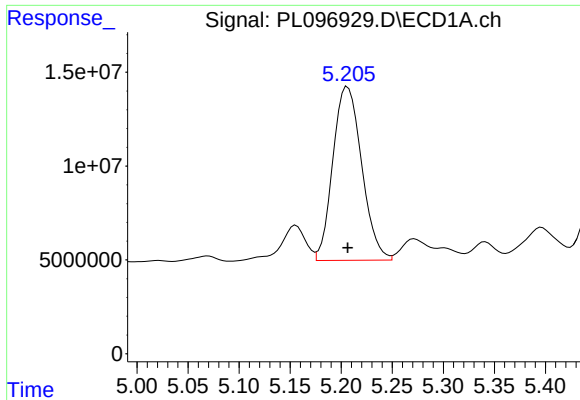

#24 Chlordane-2


R.T.: 5.206 min
Delta R.T.: 0.000 min
Response: 181968192
Conc: 988.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

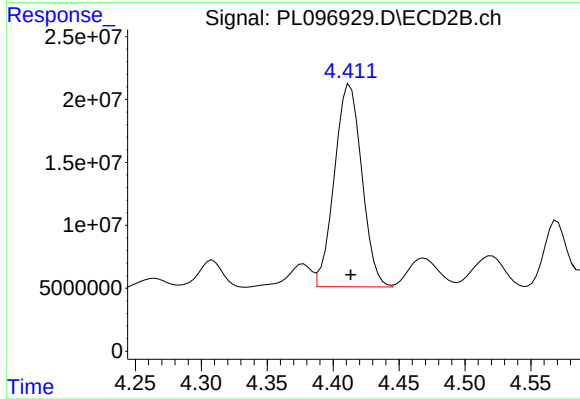


#24 Chlordane-2

R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 232673079
Conc: 1004.77 ng/ml

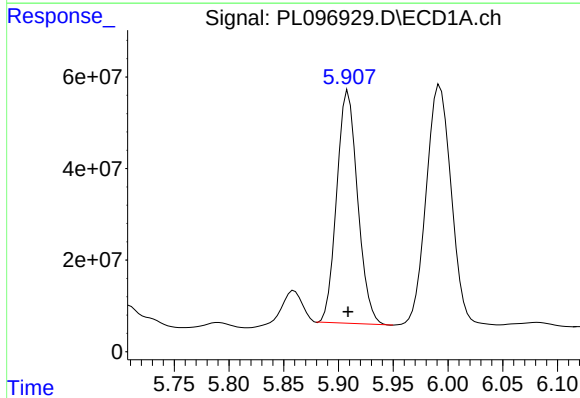


#25 Chlordane-3

R.T.: 5.909 min
Delta R.T.: 0.000 min
Response: 674871866
Conc: 1039.50 ng/ml

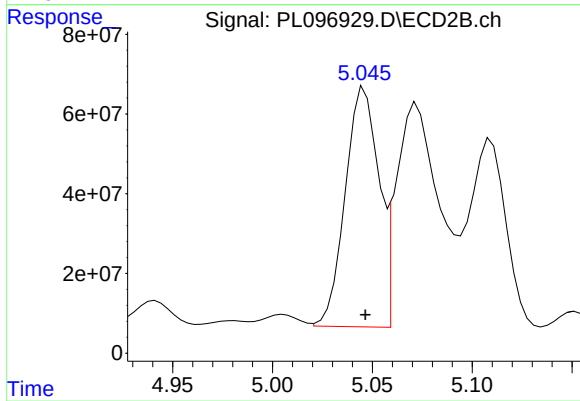

#25 Chlordane-3


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 699671030
Conc: 1081.98 ng/ml

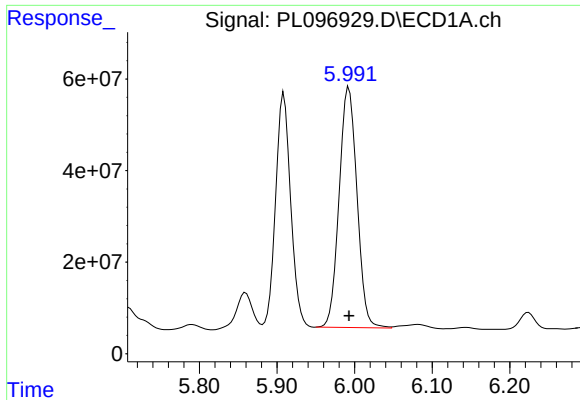

#26 Chlordane-4


R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 839515388
Conc: 1031.69 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

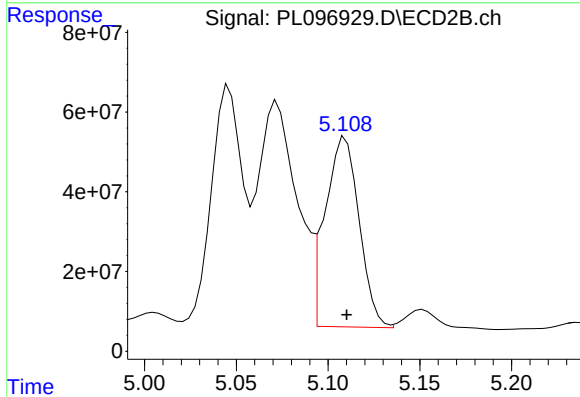


#26 Chlordane-4

R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 614258718
Conc: 1063.93 ng/ml

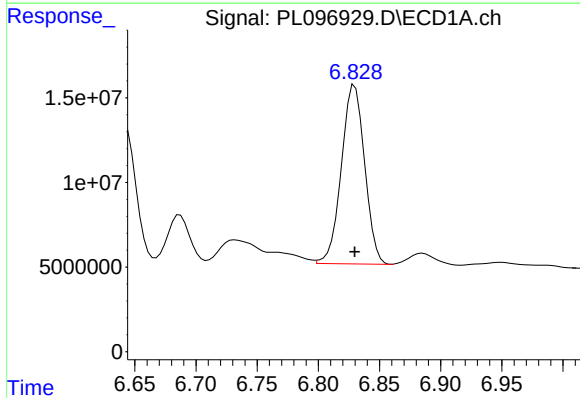


#27 Chlordane-5

R.T.: 6.830 min
Delta R.T.: 0.000 min
Response: 139937986
Conc: 1027.40 ng/ml

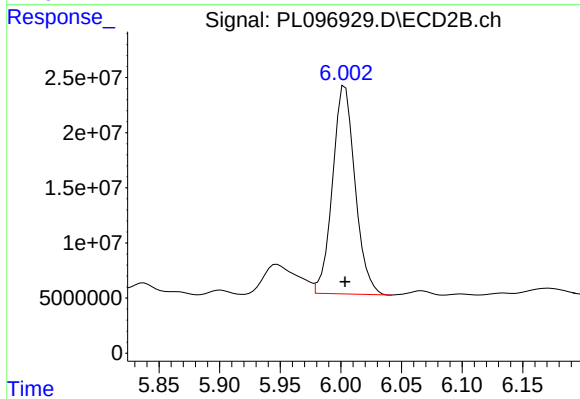

#27 Chlordane-5


R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 244229853
Conc: 1050.73 ng/ml

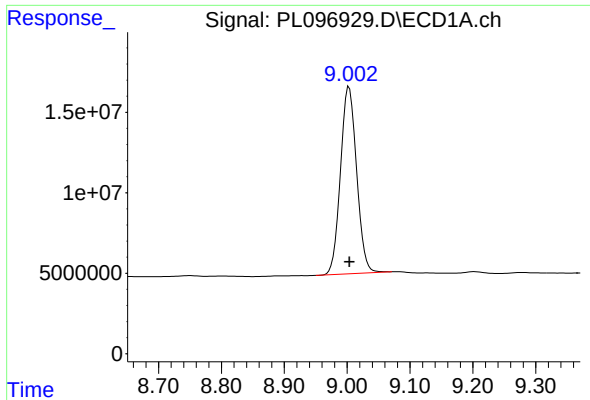

#28 Decachlorobiphenyl

R.T.: 9.003 min
Delta R.T.: 0.000 min
Response: 207649060
Conc: 99.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

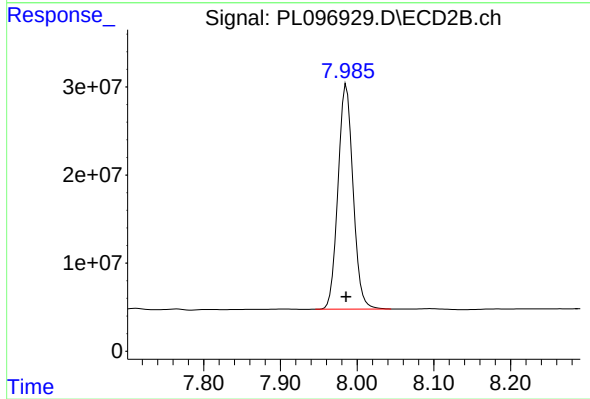

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: 0.000 min
Response: 348439590
Conc: 101.97 ng/ml