

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
 Data File : PL096931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 18:01
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:51:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 04:50:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	2.824	139.8E6	261.5E6	50.000	50.000
28)	SA Decachlor...	9.003	7.986	104.5E6	170.9E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.683	3.834	86123564	100.2E6	500.000	500.000
24)	Chlordane-2	5.206	4.413	92011980	115.8E6	500.000	500.000
25)	Chlordane-3	5.909	5.046	324.6E6	323.3E6	500.000	500.000
26)	Chlordane-4	5.993	5.110	406.9E6	288.7E6	500.000	500.000
27)	Chlordane-5	6.830	6.004	68102649	116.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
Data File : PL096931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 18:01
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:51:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 04:50:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

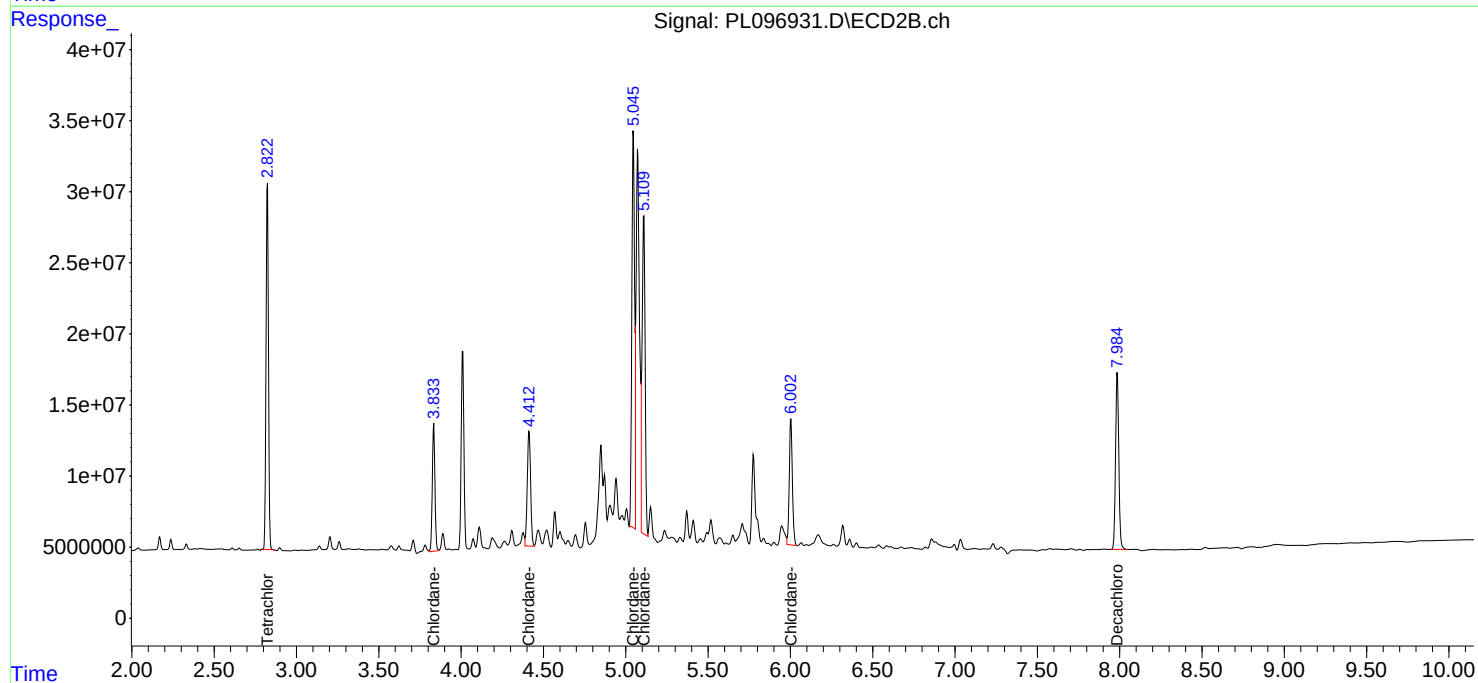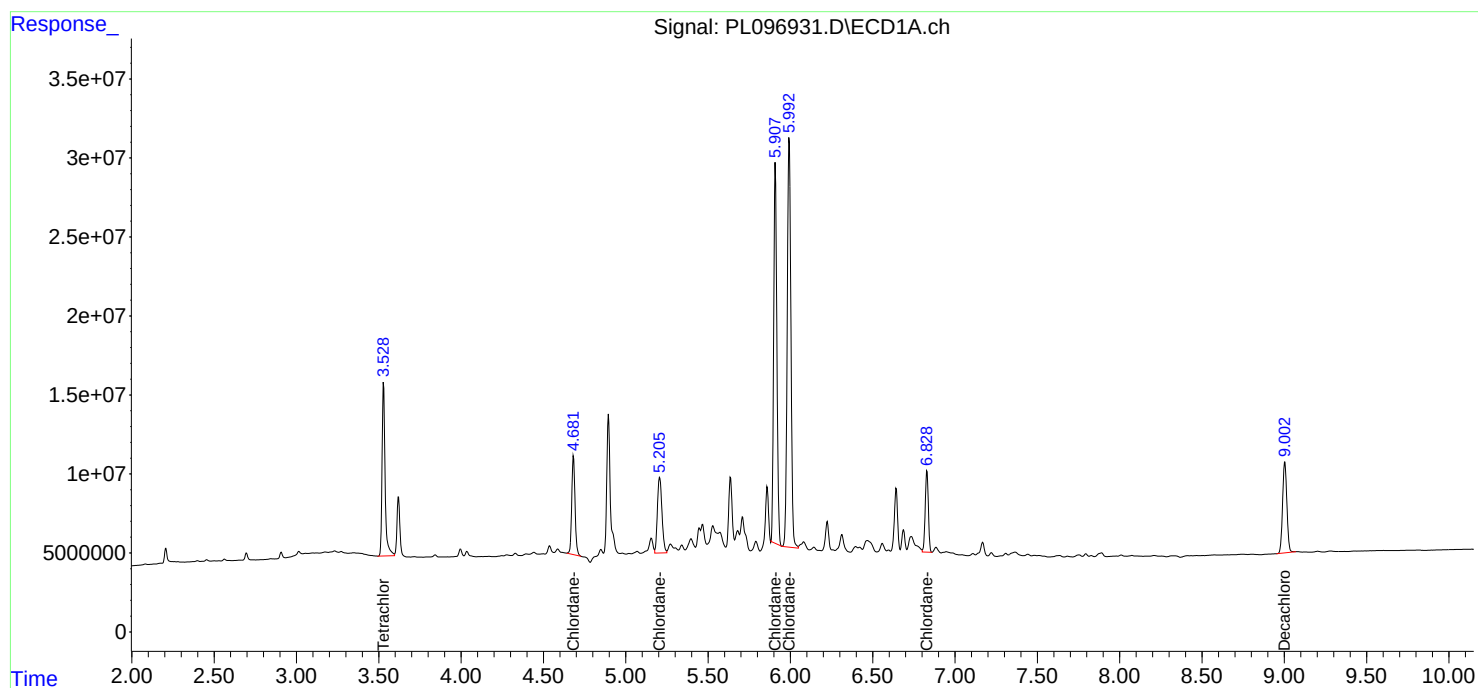


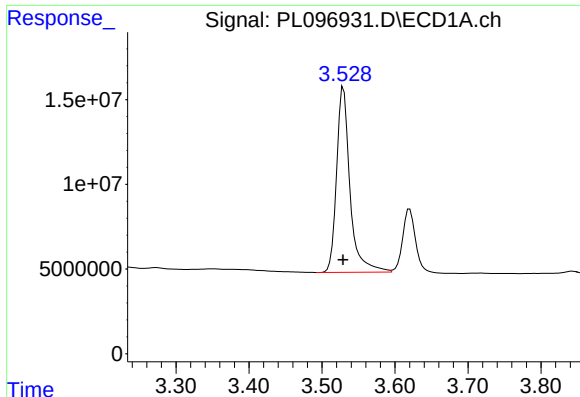

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 139768993
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

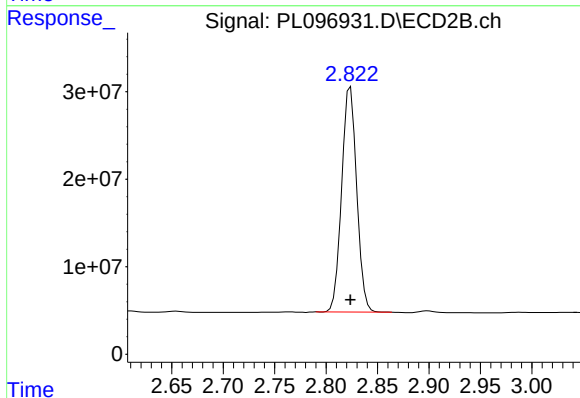


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 261544464
Conc: 50.00 ng/ml

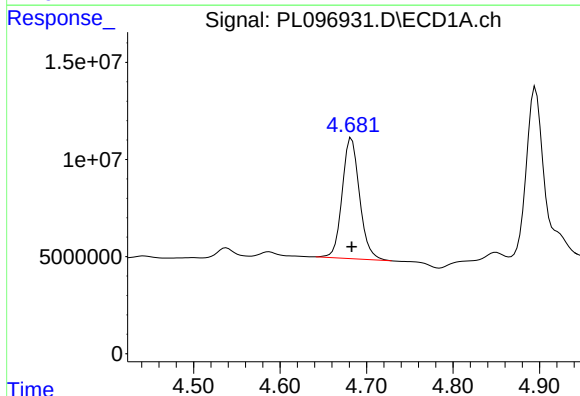


#23 Chlordane-1

R.T.: 4.683 min
Delta R.T.: 0.000 min
Response: 86123564
Conc: 500.00 ng/ml

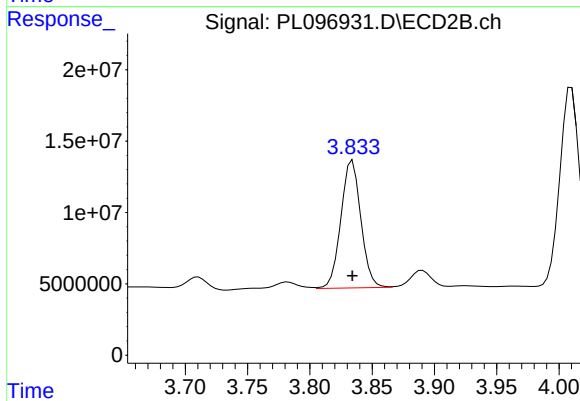

#23 Chlordane-1


R.T.: 3.834 min
Delta R.T.: 0.000 min
Response: 100173171
Conc: 500.00 ng/ml

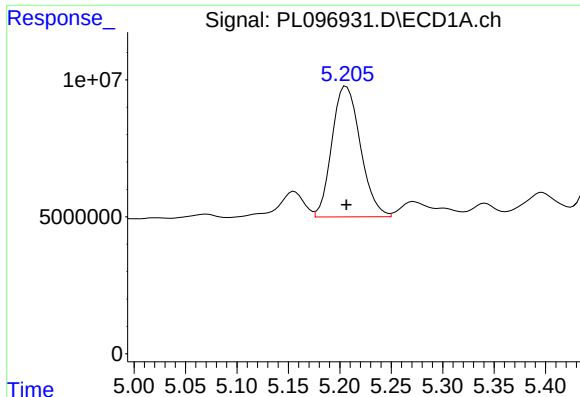

#24 Chlordane-2


R.T.: 5.206 min
Delta R.T.: 0.000 min
Response: 92011980
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

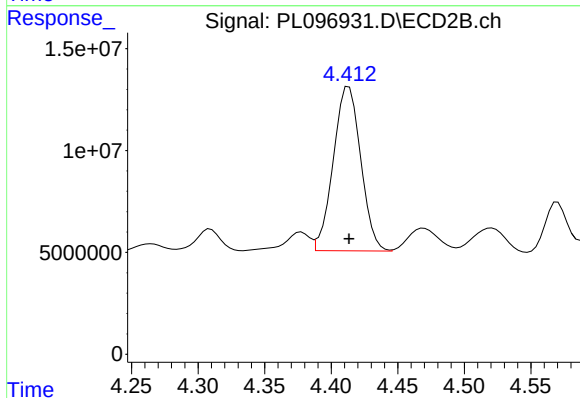


#24 Chlordane-2

R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 115784356
Conc: 500.00 ng/ml

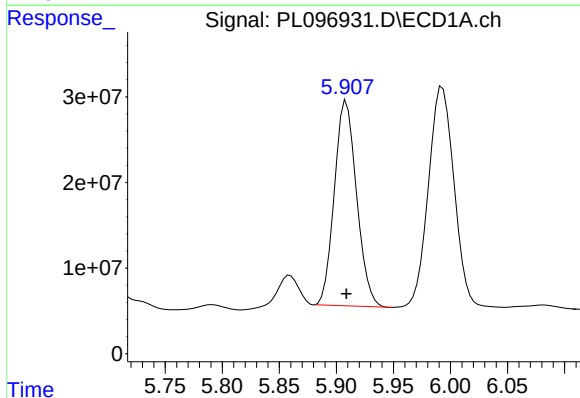


#25 Chlordane-3

R.T.: 5.909 min
Delta R.T.: 0.000 min
Response: 324613017
Conc: 500.00 ng/ml

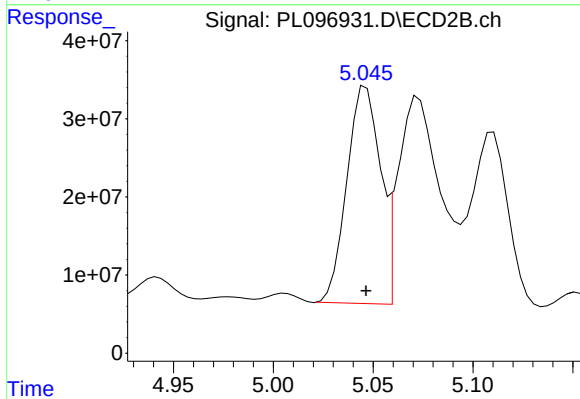

#25 Chlordane-3


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 323327674
Conc: 500.00 ng/ml

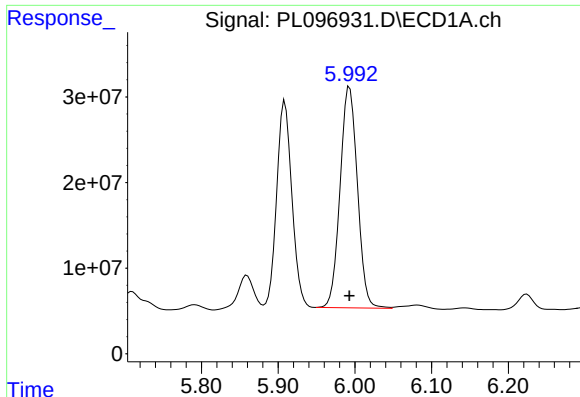

#26 Chlordane-4


R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 406862654
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

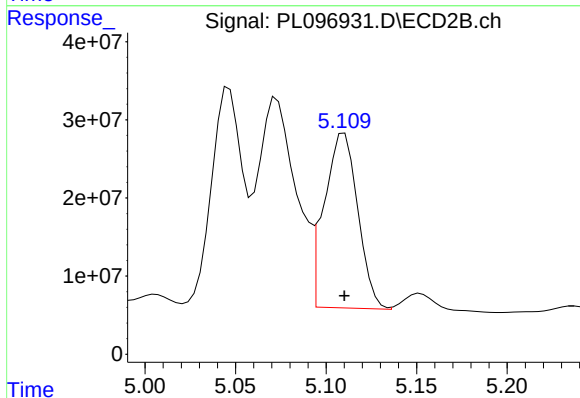


#26 Chlordane-4

R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 288674266
Conc: 500.00 ng/ml

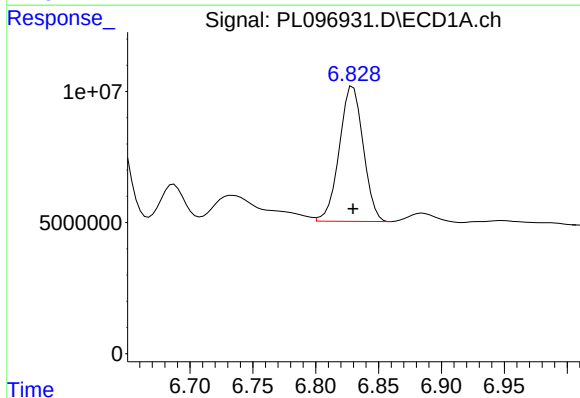


#27 Chlordane-5

R.T.: 6.830 min
Delta R.T.: 0.000 min
Response: 68102649
Conc: 500.00 ng/ml

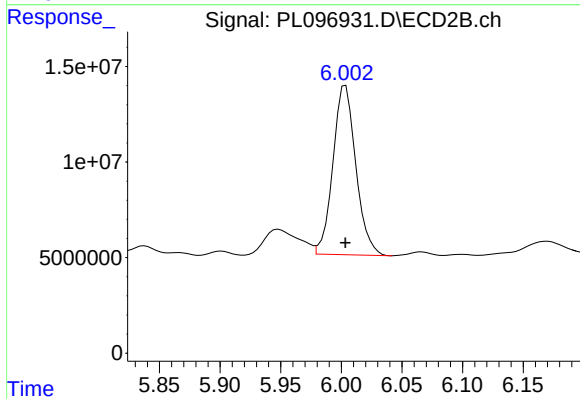

#27 Chlordane-5


R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 116219503
Conc: 500.00 ng/ml

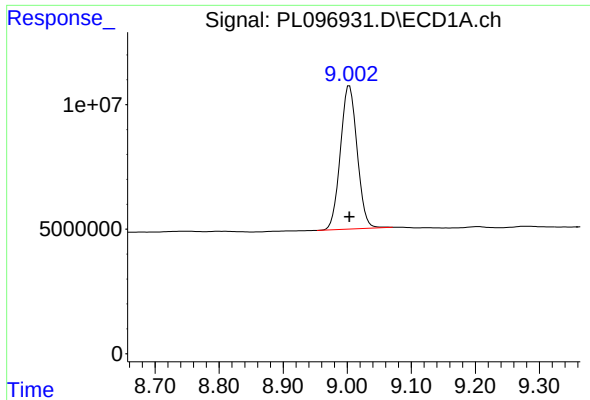

#28 Decachlorobiphenyl

R.T.: 9.003 min
Delta R.T.: 0.000 min
Response: 104462435
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

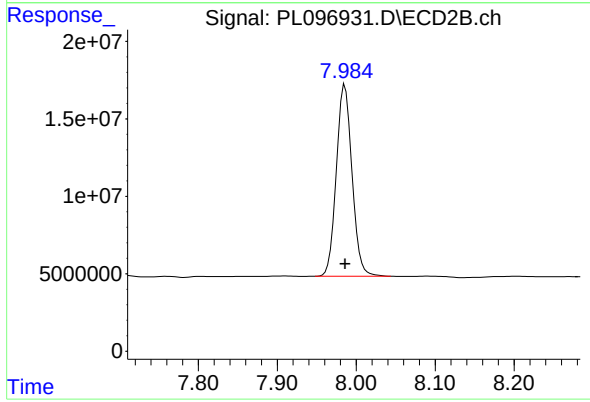

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: 0.000 min
Response: 170850213
Conc: 50.00 ng/ml