

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
 Data File : PL096932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 18:14
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:51:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 04:50:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	2.824	66121051	122.1E6	23.654	23.350
28)	SA Decachlor...	9.004	7.986	51261554	85996027	24.536	25.167
Target Compounds							
23)	Chlordane-1	4.682	3.834	41579296	46642943	241.393	232.812
24)	Chlordane-2	5.205	4.414	45984109	57204534	249.881	247.030
25)	Chlordane-3	5.909	5.047	150.6E6	149.8E6	231.900	231.601
26)	Chlordane-4	5.993	5.110	189.8E6	134.4E6	233.237	232.803
27)	Chlordane-5	6.830	6.004	32406098	54987817	237.921	236.569



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
Data File : PL096932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 18:14
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:51:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 04:50:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

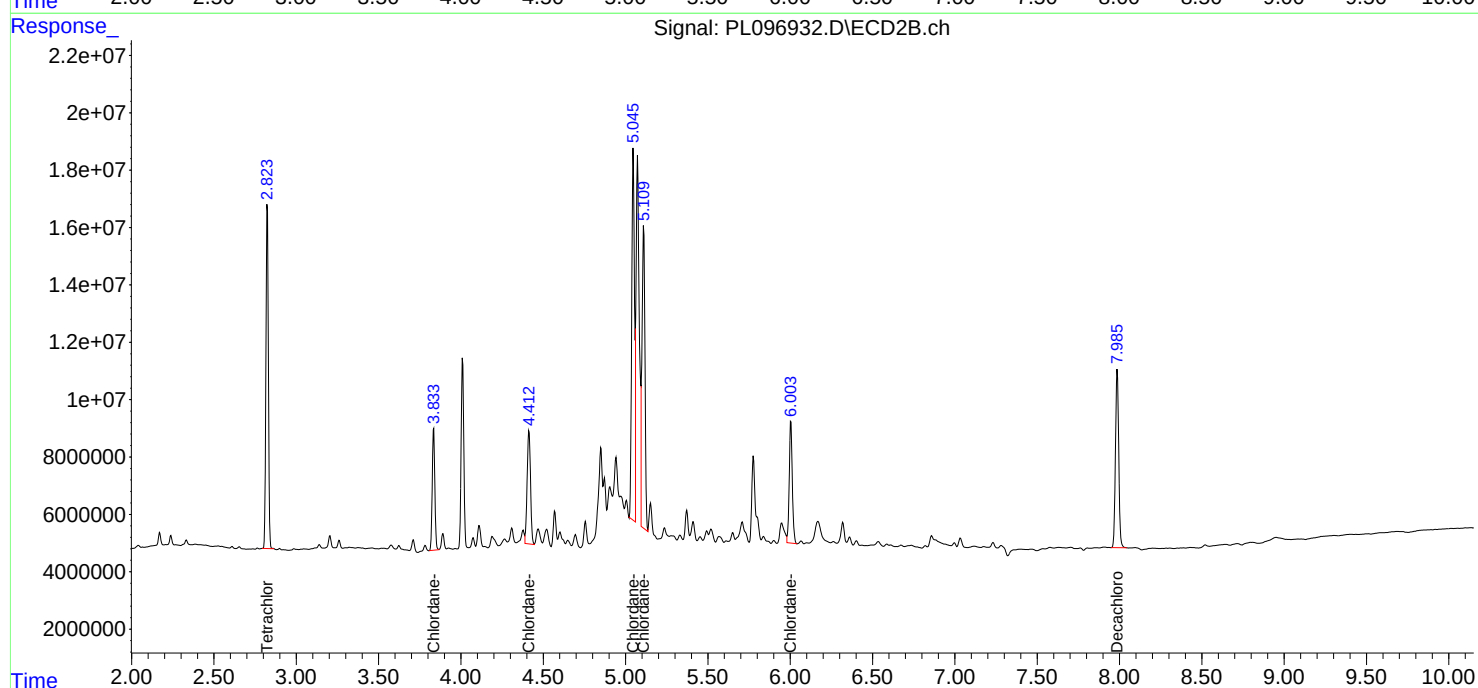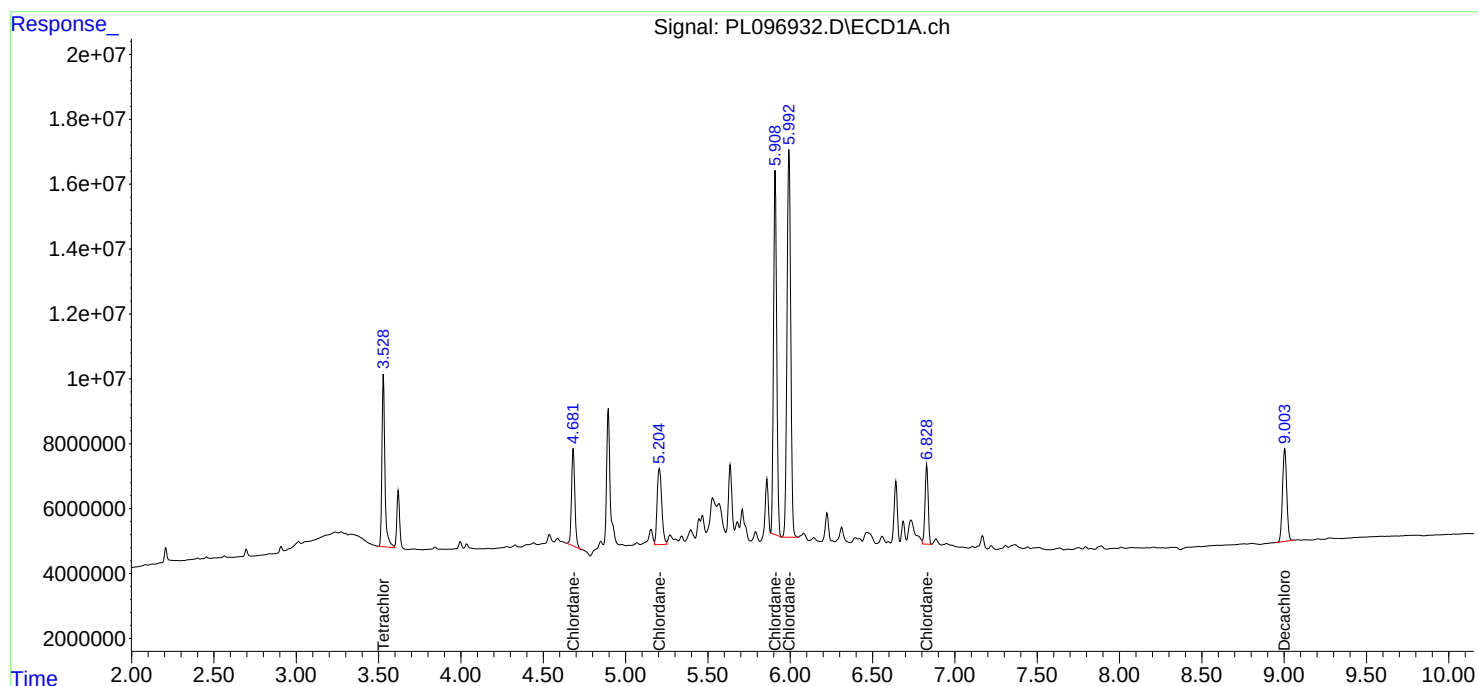


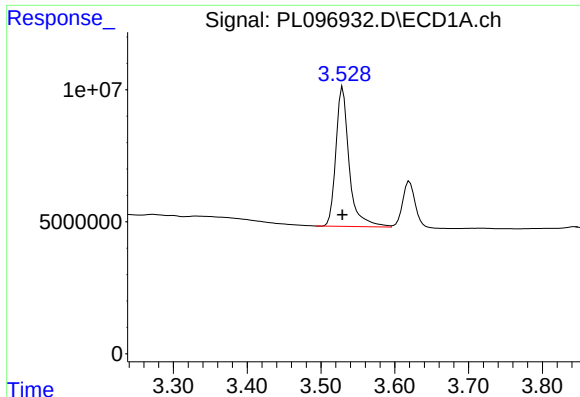

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 66121051
Conc: 23.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

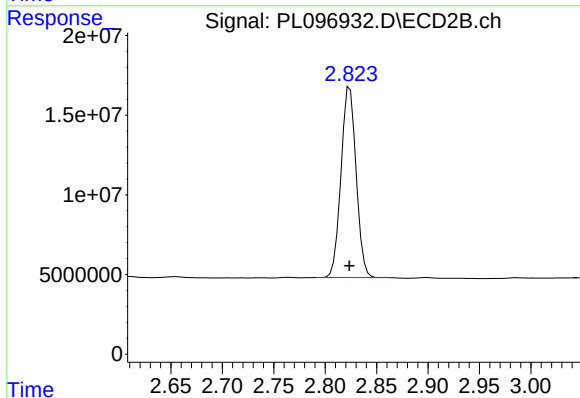


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 122142431
Conc: 23.35 ng/ml

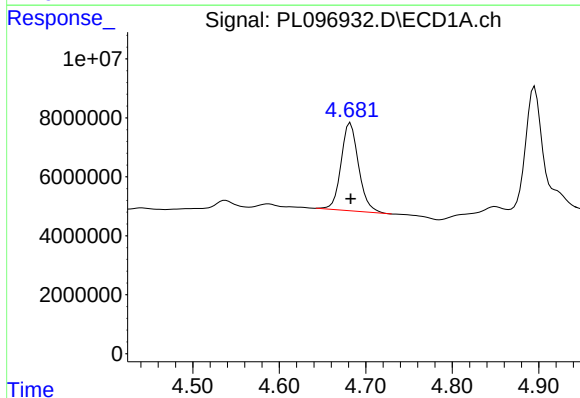


#23 Chlordane-1

R.T.: 4.682 min
Delta R.T.: 0.000 min
Response: 41579296
Conc: 241.39 ng/ml

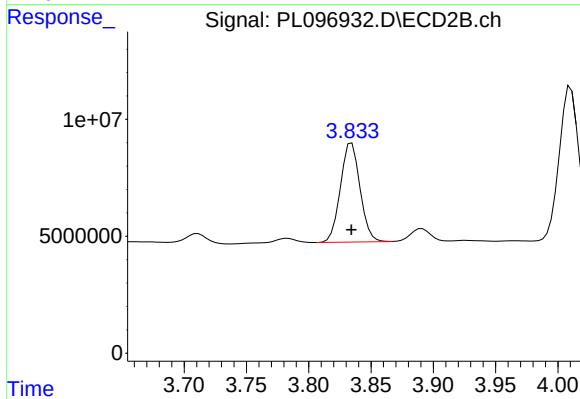

#23 Chlordane-1


R.T.: 3.834 min
Delta R.T.: 0.000 min
Response: 46642943
Conc: 232.81 ng/ml

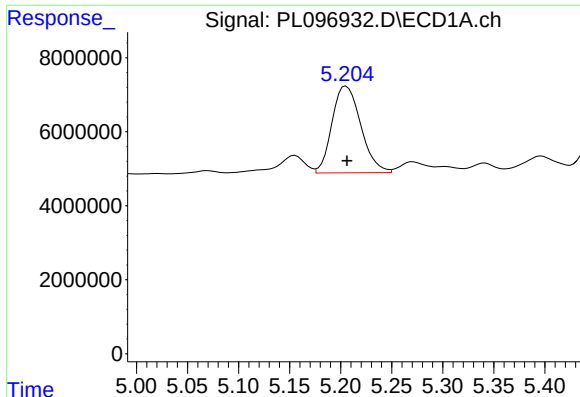

#24 Chlordane-2


R.T.: 5.205 min
Delta R.T.: 0.000 min
Response: 45984109
Conc: 249.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

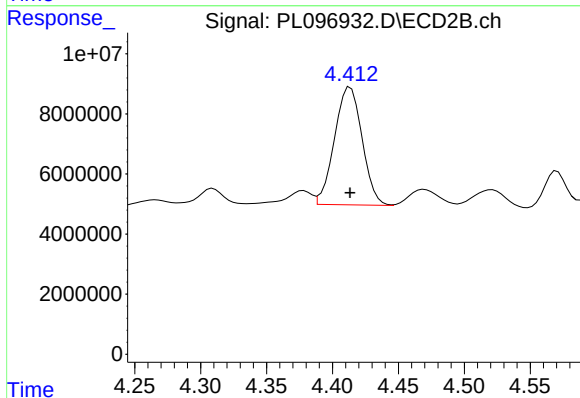


#24 Chlordane-2

R.T.: 4.414 min
Delta R.T.: 0.000 min
Response: 57204534
Conc: 247.03 ng/ml

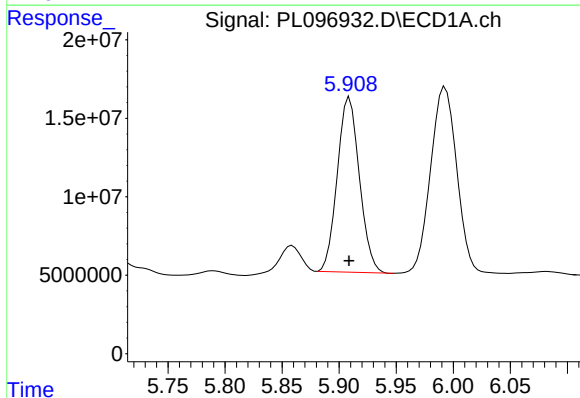


#25 Chlordane-3

R.T.: 5.909 min
Delta R.T.: 0.000 min
Response: 150555273
Conc: 231.90 ng/ml

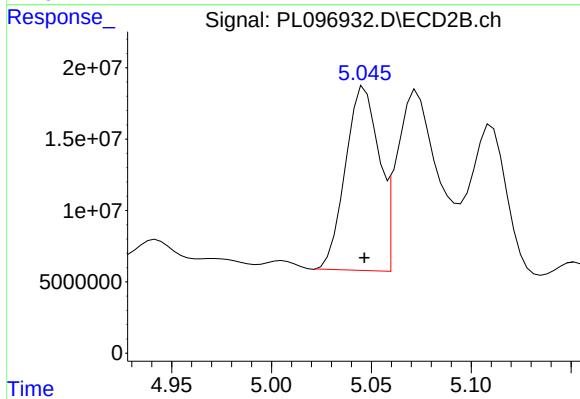

#25 Chlordane-3


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 149766203
Conc: 231.60 ng/ml

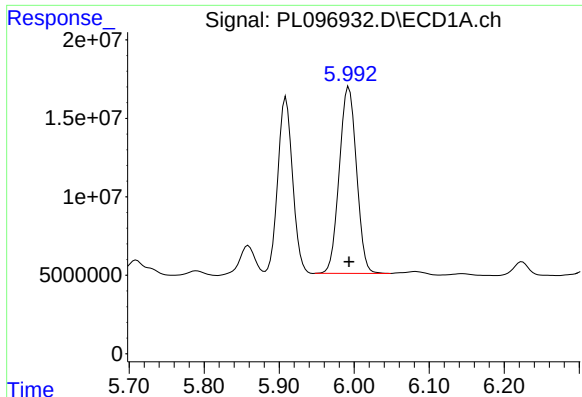

#26 Chlordane-4


R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 189790814
Conc: 233.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

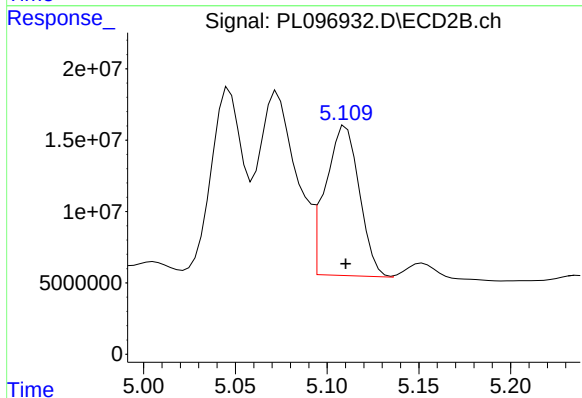


#26 Chlordane-4

R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 134408606
Conc: 232.80 ng/ml

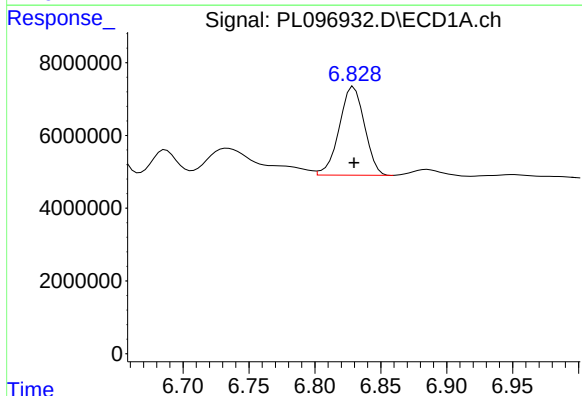


#27 Chlordane-5

R.T.: 6.830 min
Delta R.T.: 0.000 min
Response: 32406098
Conc: 237.92 ng/ml

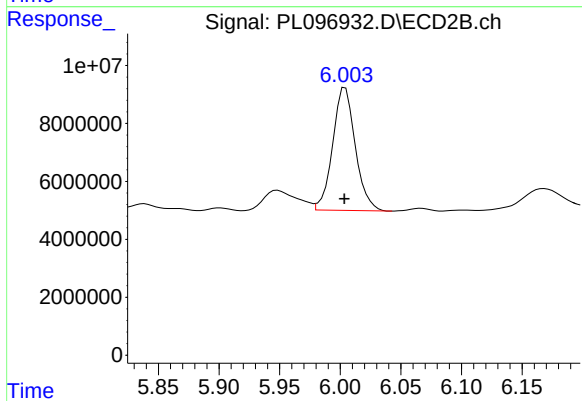

#27 Chlordane-5


R.T.: 6.004 min
Delta R.T.: 0.000 min
Response: 54987817
Conc: 236.57 ng/ml

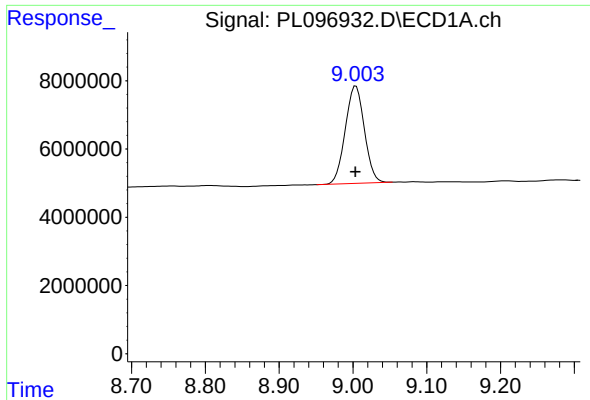

#28 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: 0.000 min
Response: 51261554
Conc: 24.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

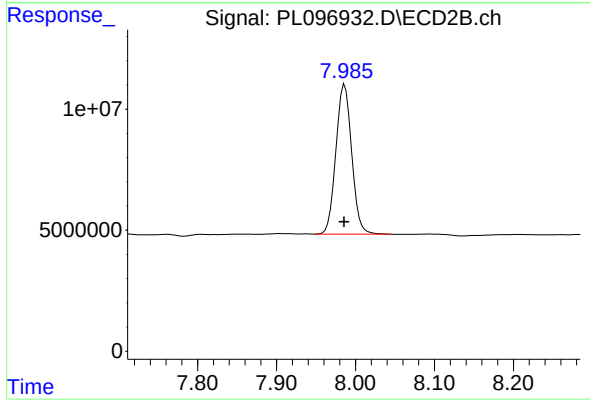

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: 0.000 min
Response: 85996027
Conc: 25.17 ng/ml