

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
 Data File : PL096933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2025 18:28
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 04:51:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 04:50:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.824	12905146	24018405	4.617	4.592
28)	SA Decachlor...	9.004	7.985	10831655	19139192	5.184	5.601
Target Compounds							
23)	Chlordane-1	4.683	3.834	9431027	9513185	54.753	47.484
24)	Chlordane-2	5.208	4.413	9307578	12710157	50.578	54.887
25)	Chlordane-3	5.909	5.046	28952901	27972126	44.596	43.257
26)	Chlordane-4	5.993	5.110	42950738	24259357	52.783	42.019
27)	Chlordane-5	6.829	6.003	6951076	10012533	51.034	43.076



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082025\
Data File : PL096933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2025 18:28
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 04:51:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 04:50:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

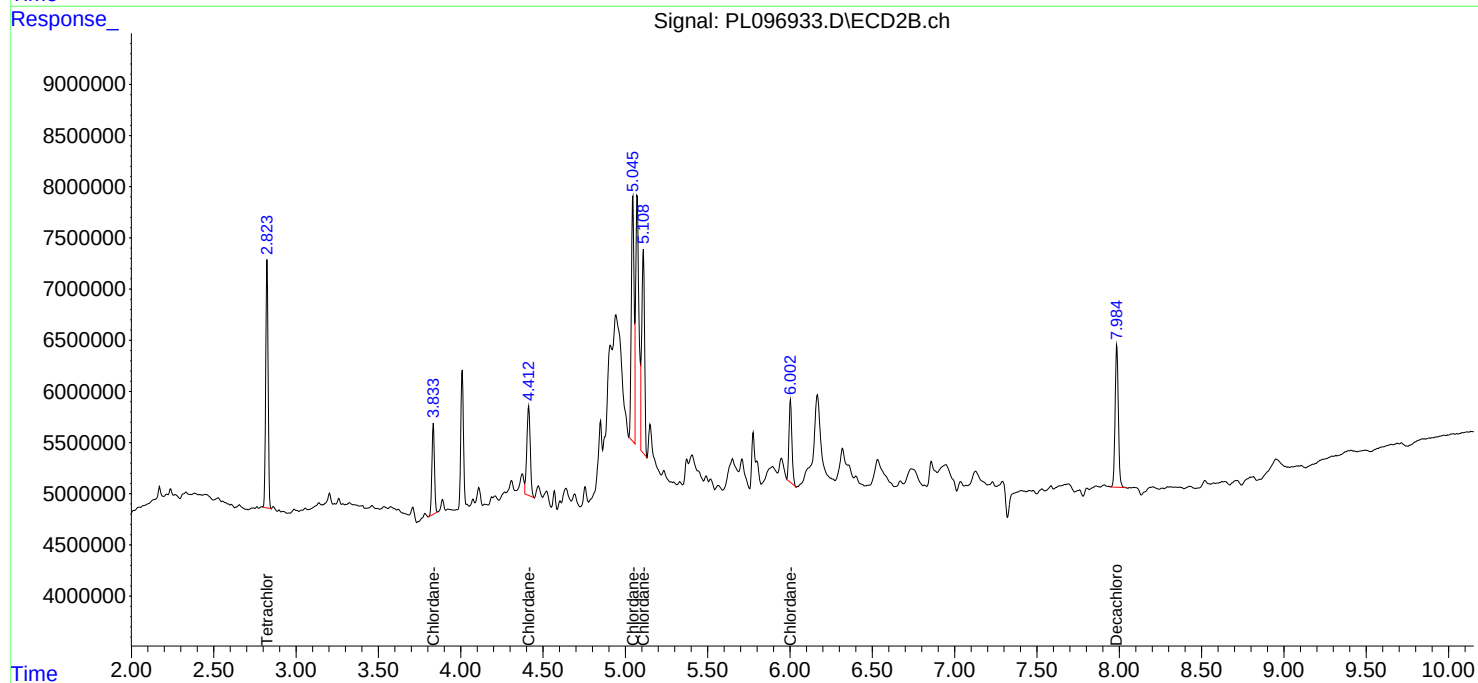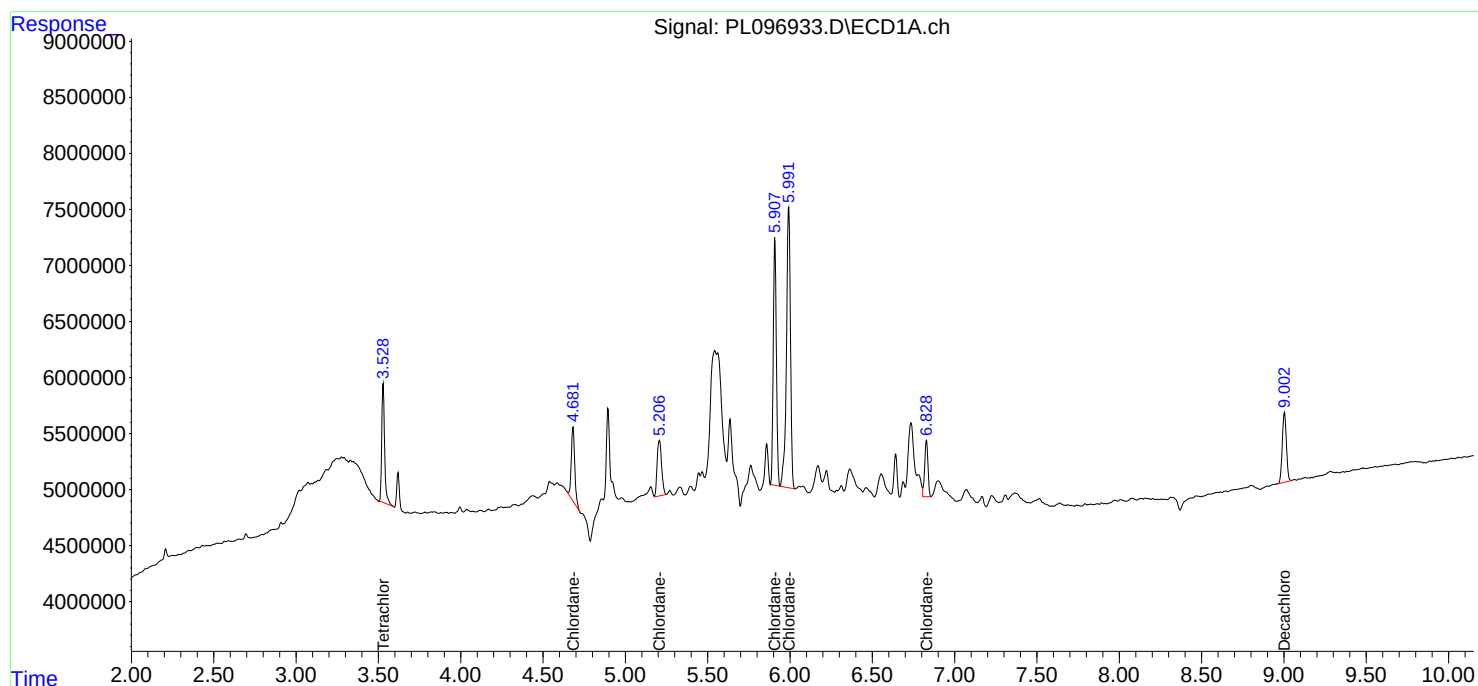


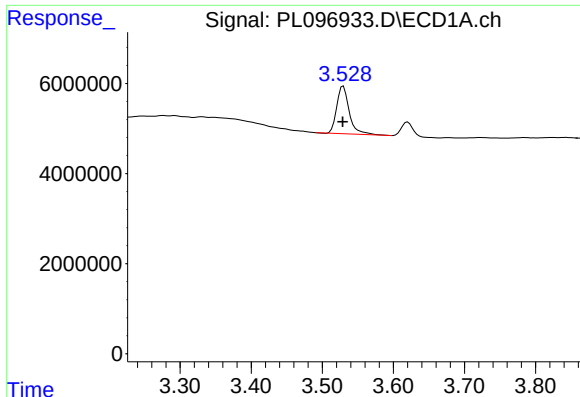

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 12905146
Conc: 4.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

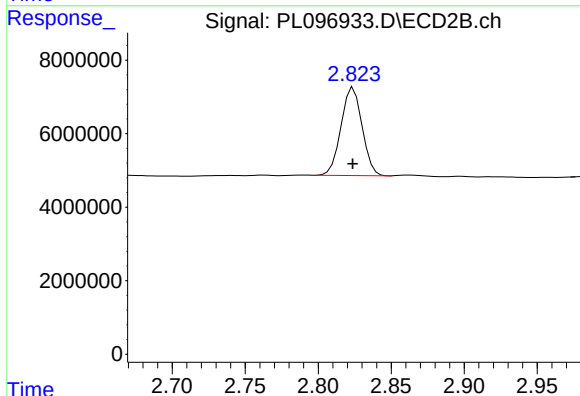


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 24018405
Conc: 4.59 ng/ml

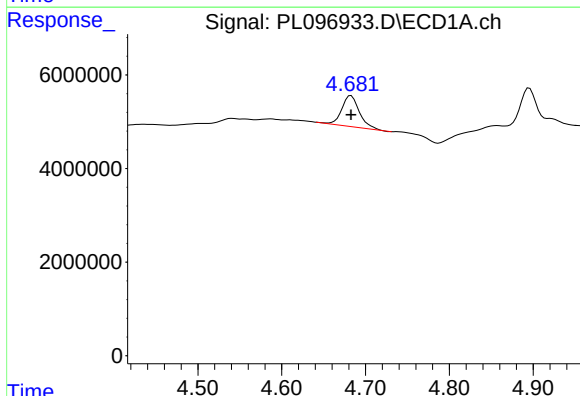


#23 Chlordane-1

R.T.: 4.683 min
Delta R.T.: 0.000 min
Response: 9431027
Conc: 54.75 ng/ml

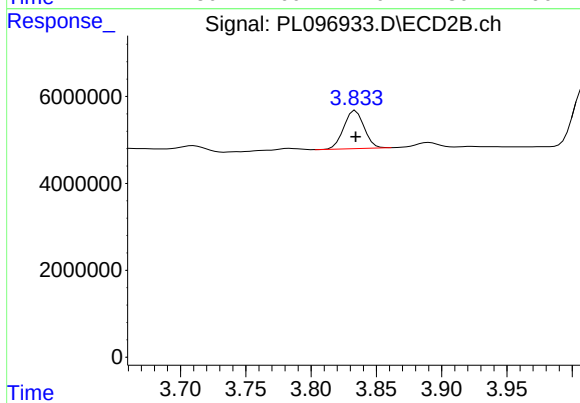

#23 Chlordane-1


R.T.: 3.834 min
Delta R.T.: 0.000 min
Response: 9513185
Conc: 47.48 ng/ml

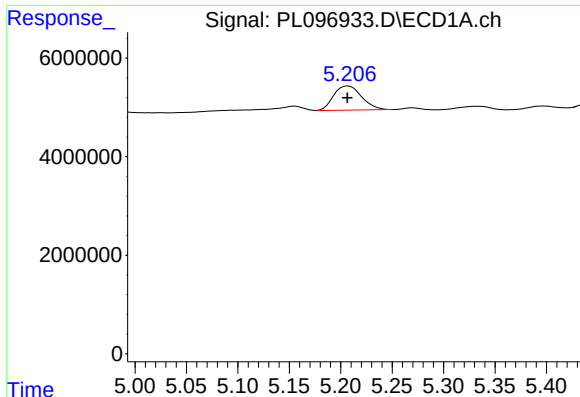

#24 Chlordane-2


R.T.: 5.208 min
Delta R.T.: 0.001 min
Response: 9307578
Conc: 50.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

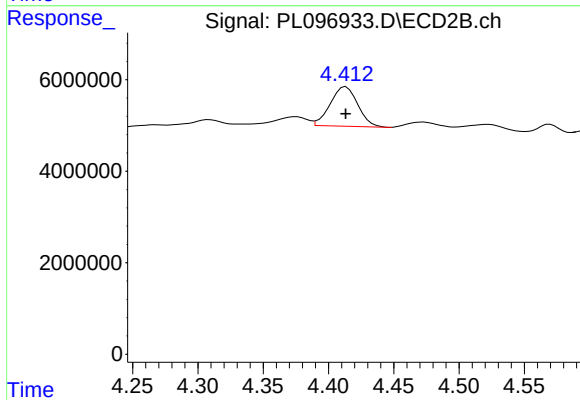


#24 Chlordane-2

R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 12710157
Conc: 54.89 ng/ml

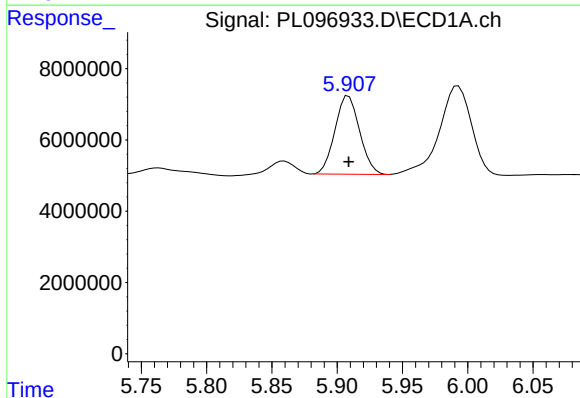


#25 Chlordane-3

R.T.: 5.909 min
Delta R.T.: 0.000 min
Response: 28952901
Conc: 44.60 ng/ml

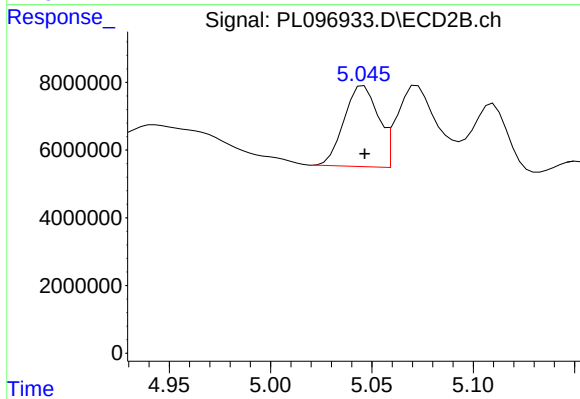

#25 Chlordane-3


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 27972126
Conc: 43.26 ng/ml

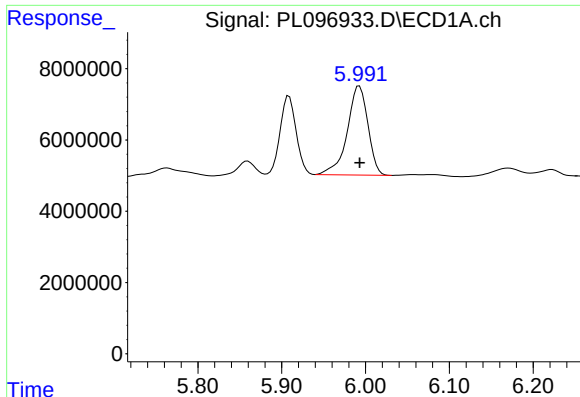

#26 Chlordane-4


R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 42950738
Conc: 52.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

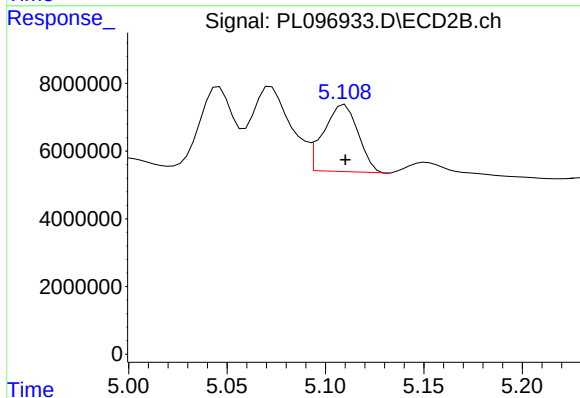


#26 Chlordane-4

R.T.: 5.110 min
Delta R.T.: 0.000 min
Response: 24259357
Conc: 42.02 ng/ml

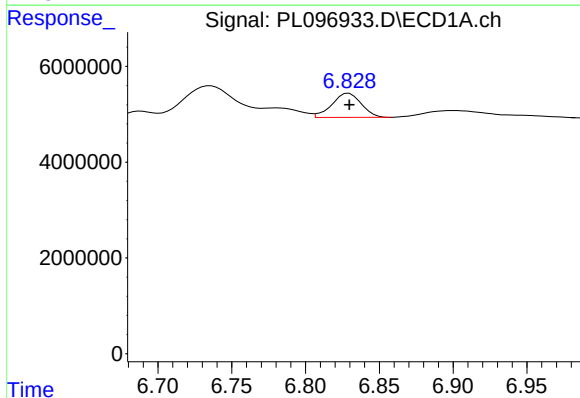


#27 Chlordane-5

R.T.: 6.829 min
Delta R.T.: 0.000 min
Response: 6951076
Conc: 51.03 ng/ml

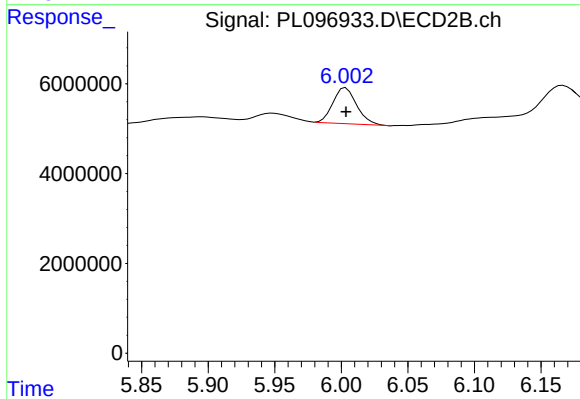

#27 Chlordane-5


R.T.: 6.003 min
Delta R.T.: 0.000 min
Response: 10012533
Conc: 43.08 ng/ml

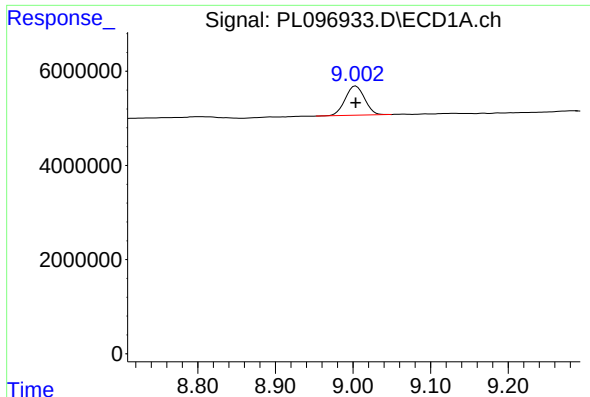

#28 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: 0.000 min
Response: 10831655
Conc: 5.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

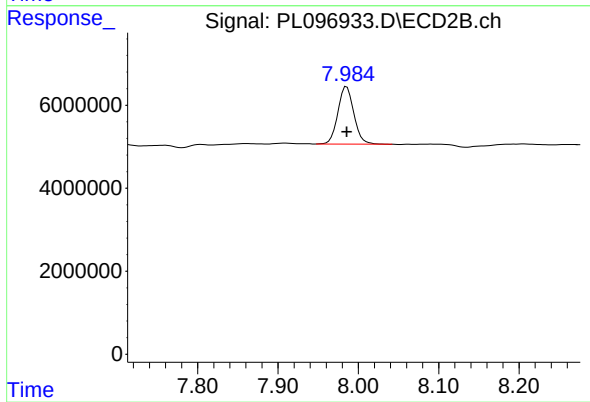

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: 0.000 min
Response: 19139192
Conc: 5.60 ng/ml