

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2018 16:52
 Operator : AJ\SJ
 Sample : J4560-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 00:52:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.906	139.6E6	59131250	19.972	22.057
28)	SA Decachlor...	7.961	8.894	134.4E6	52345617	19.135	22.557
Target Compounds							
3)	MA gamma-BHC...	4.046f	0.000	8939113	0	0.843	N.D. #
6)	B beta-BHC	4.218f	0.000	30685336	0	6.605	N.D. #
7)	B delta-BHC	0.000	4.931	0	15423794	N.D.	3.874 #
19)	B Endosulfa...	6.455	0.000	30103229	0	3.700	N.D. #
20)	A Methoxychlor	6.636f	0.000	43045443	0	10.519	N.D. #
23)	Chlordane-1	0.000	4.931	0	15423794	N.D.	123.455 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2018 16:52
Operator : AJ\SJ
Sample : J4560-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 00:52:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

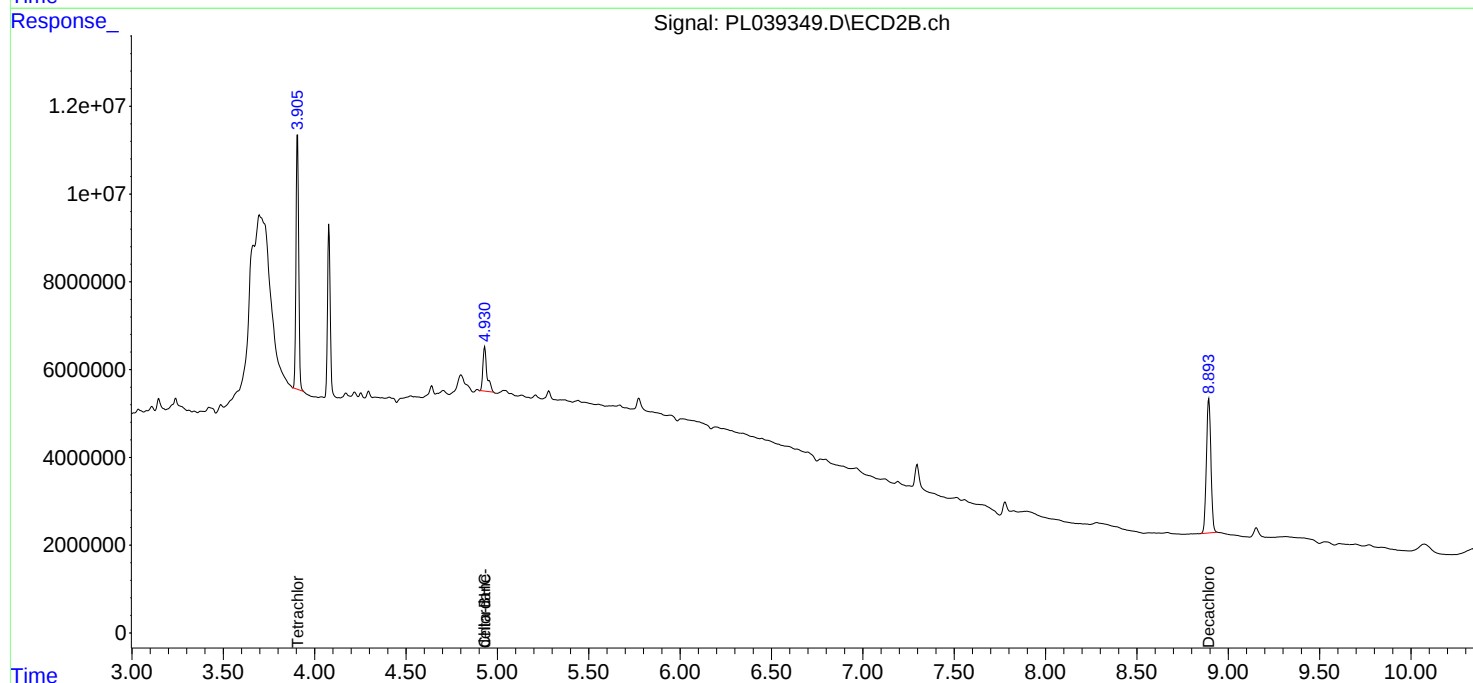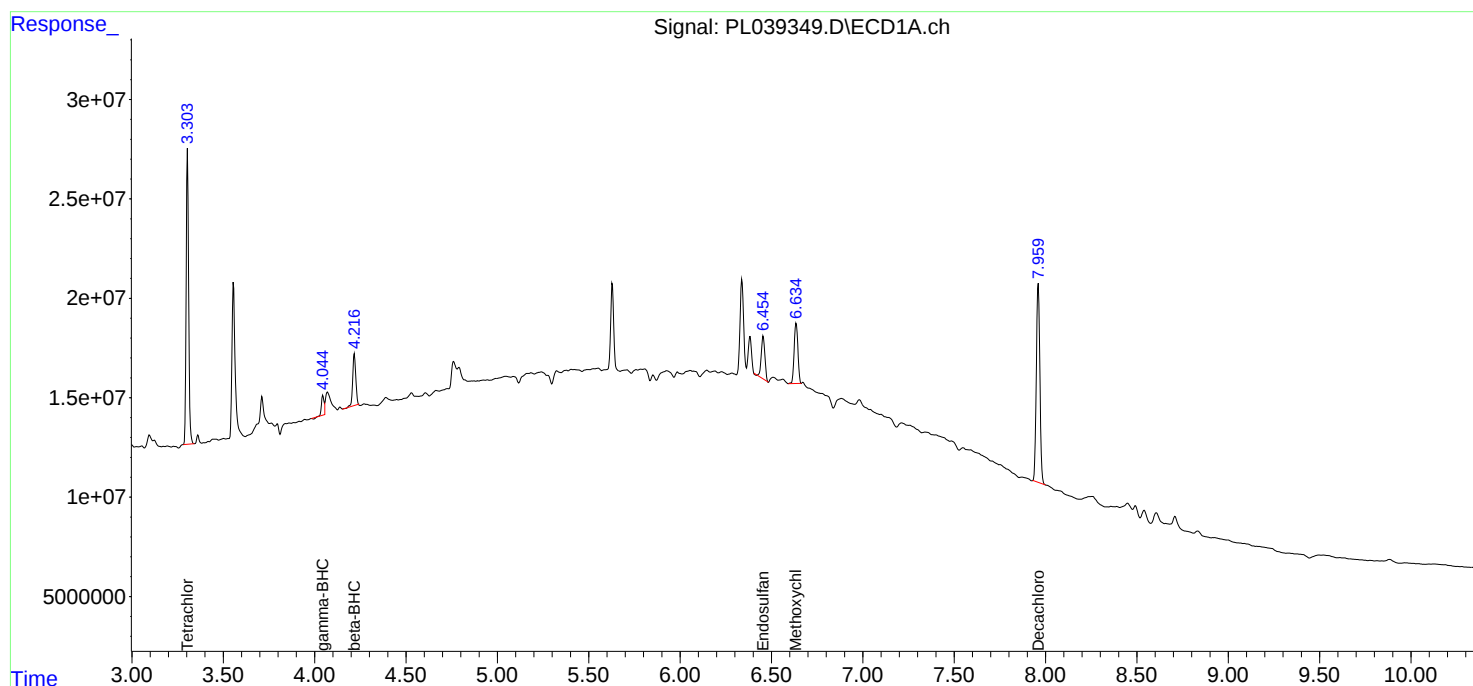


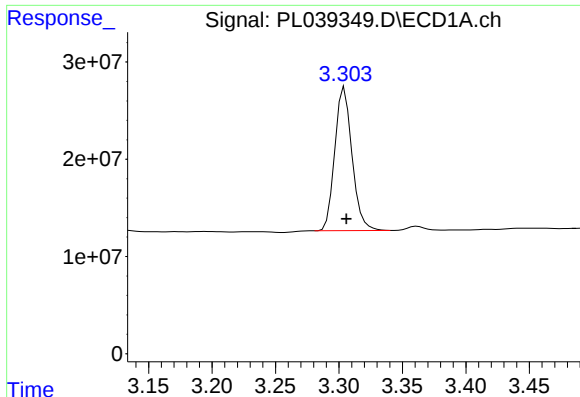

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 139610641
Conc: 19.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

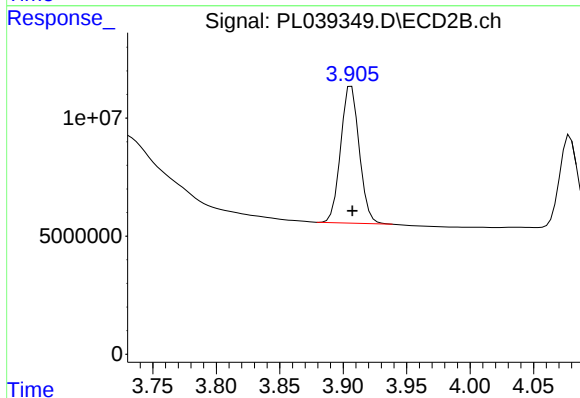


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 59131250
Conc: 22.06 ng/ml

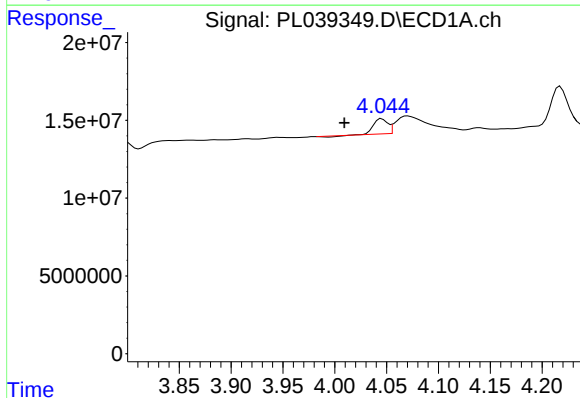


#3 gamma-BHC (Lindane)

R.T.: 4.046 min
Delta R.T.: 0.036 min
Response: 8939113
Conc: 0.84 ng/ml

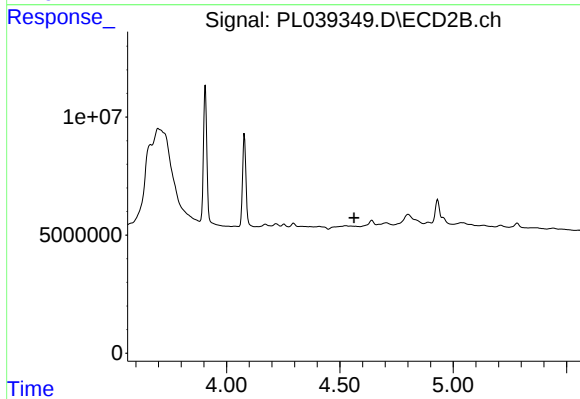

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.563 min
Response: 0
Conc: N.D.

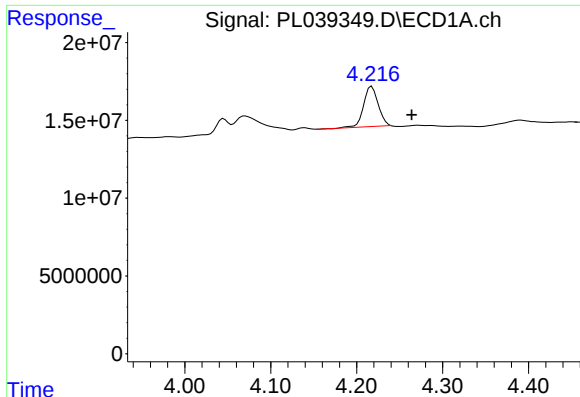

#6 beta-BHC


R.T.: 4.218 min
Delta R.T.: -0.046 min
Response: 30685336
Conc: 6.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

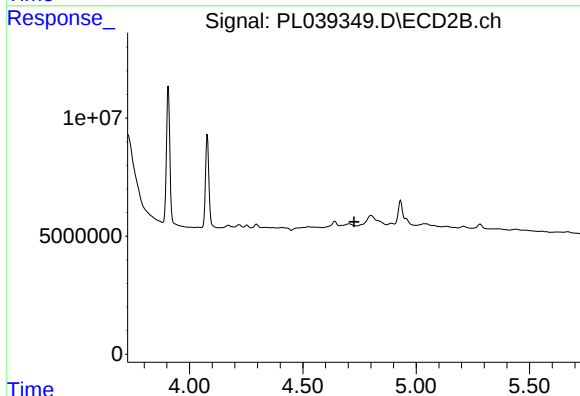


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

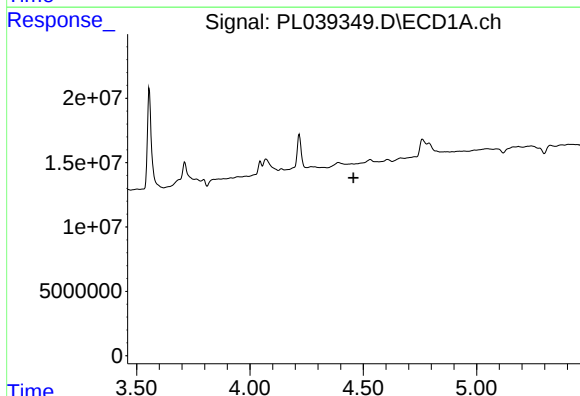


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

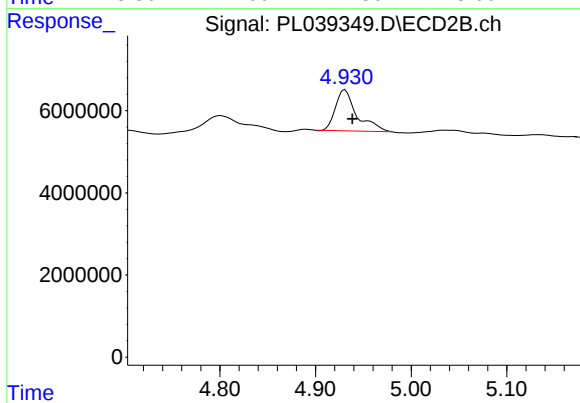

#7 delta-BHC


R.T.: 4.931 min
Delta R.T.: -0.008 min
Response: 15423794
Conc: 3.87 ng/ml

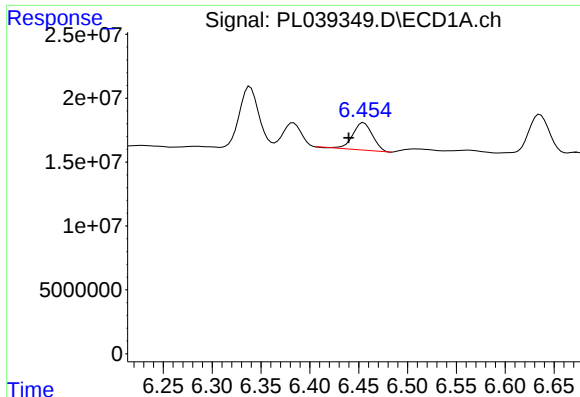

#19 Endosulfan Sulfate


R.T.: 6.455 min
Delta R.T.: 0.015 min
Response: 30103229
Conc: 3.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

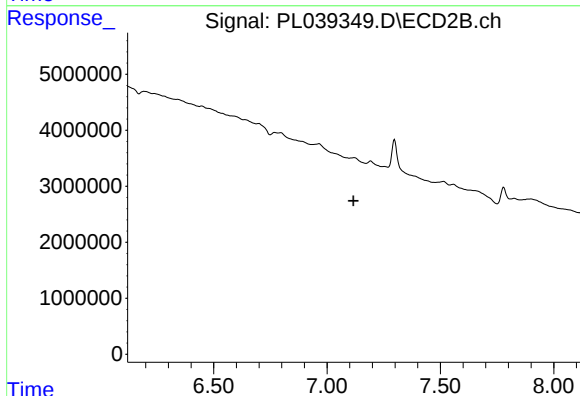


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

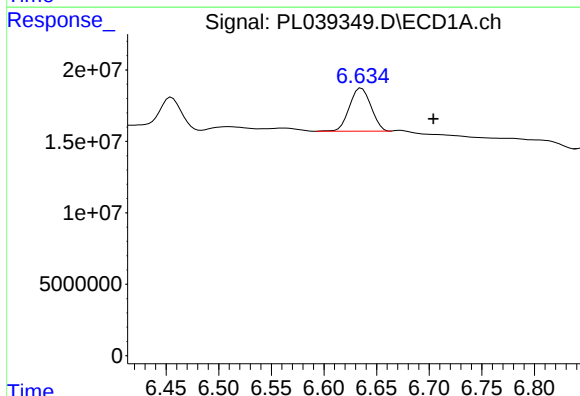


#20 Methoxychlor

R.T.: 6.636 min
Delta R.T.: -0.068 min
Response: 43045443
Conc: 10.52 ng/ml

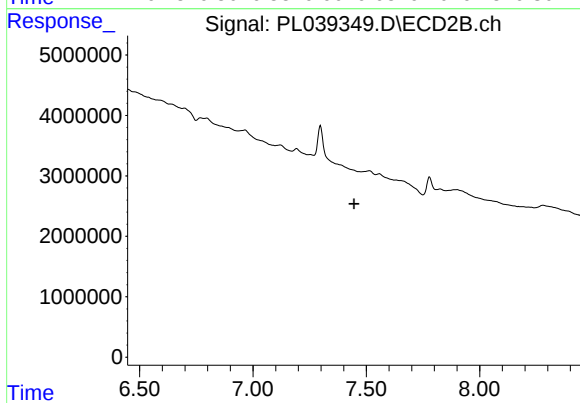

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

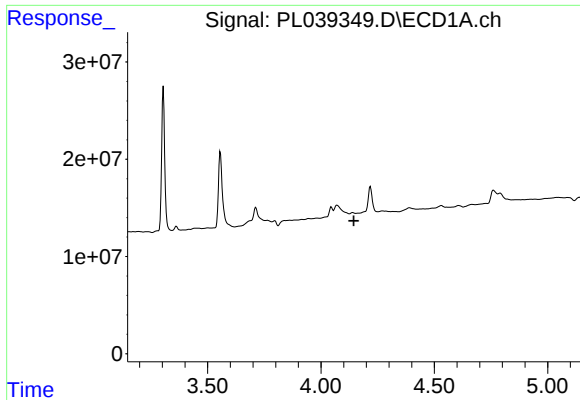

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

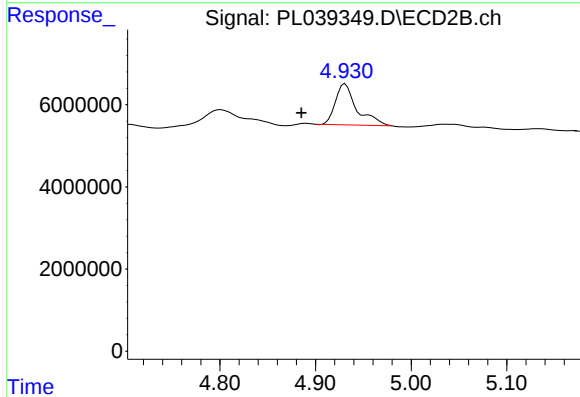


#23 Chlordane-1

R.T.: 4.931 min
Delta R.T.: 0.046 min
Response: 15423794
Conc: 123.45 ng/ml

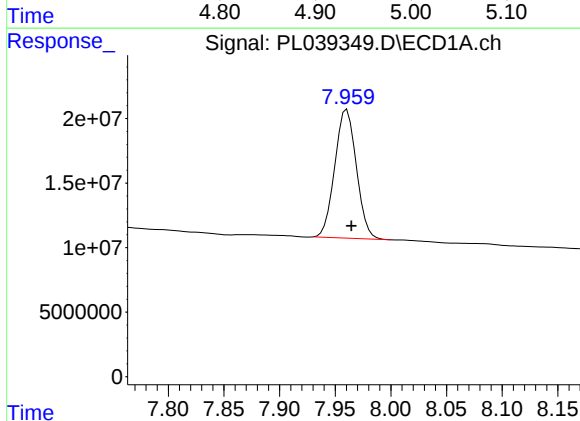

#28 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.004 min
Response: 134391422
Conc: 19.13 ng/ml

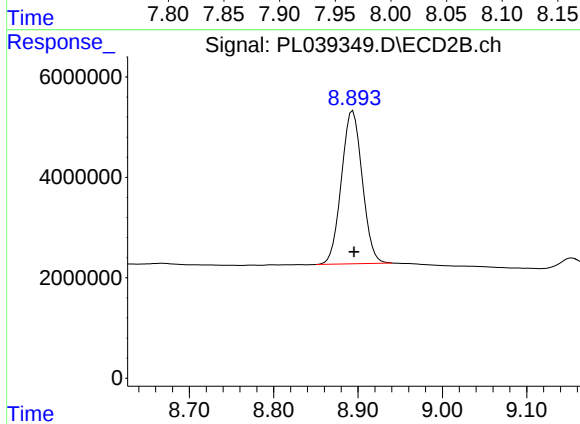

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.002 min
Response: 52345617
Conc: 22.56 ng/ml