

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2018 18:45
 Operator : AJ\SJ
 Sample : J4275-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 00:55:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.907	147.4E6	63470407	21.093	23.675
28)	SA Decachlor...	7.960	8.895	139.9E6	54283839	19.916	23.392
Target Compounds							
6)	B beta-BHC	4.217f	0.000	19874659	0	4.278	N.D. #
7)	B delta-BHC	0.000	4.932	0	3513513	N.D.	0.882 #
8)	B Heptachlo...	0.000	5.775	0	4135989	N.D.	1.230 #
23)	Chlordane-1	0.000	4.932	0	3513513	N.D.	28.123 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2018 18:45
Operator : AJ\SJ
Sample : J4275-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 00:55:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

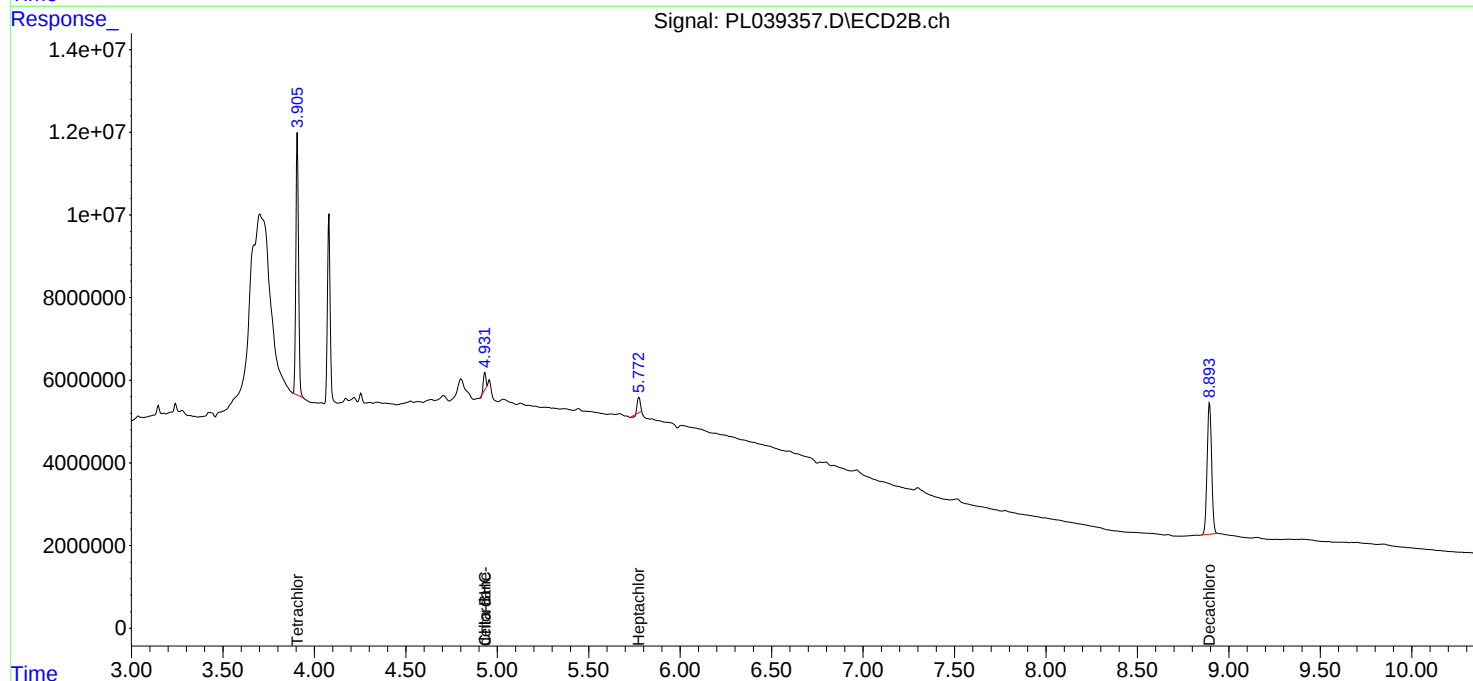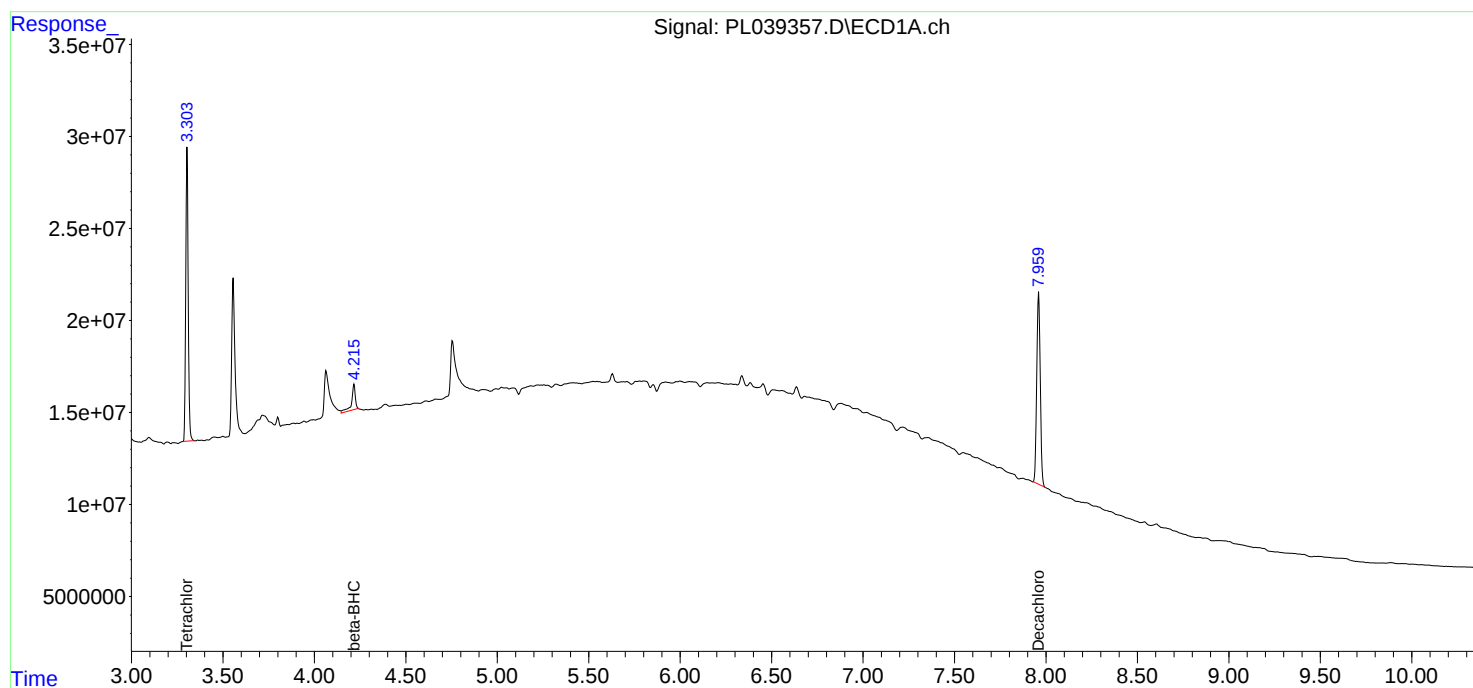


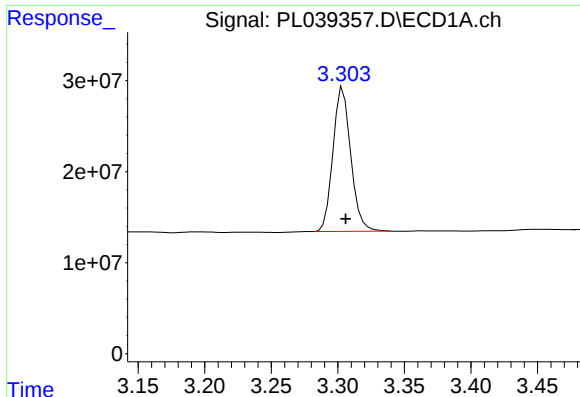

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 147449803
Conc: 21.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

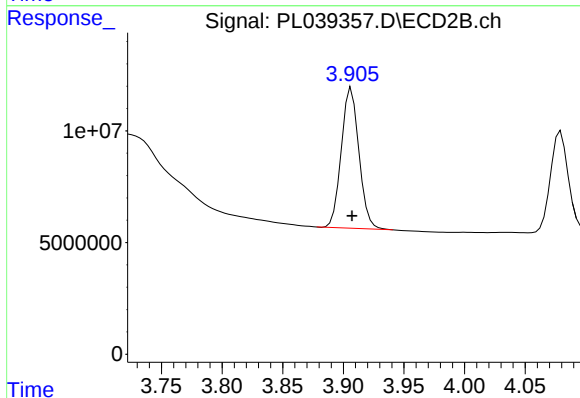


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 63470407
Conc: 23.68 ng/ml

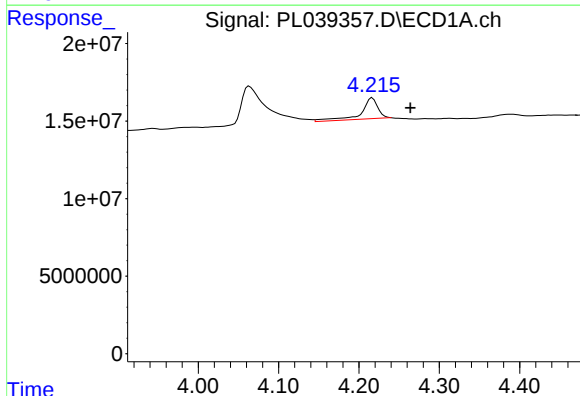


#6 beta-BHC

R.T.: 4.217 min
Delta R.T.: -0.047 min
Response: 19874659
Conc: 4.28 ng/ml

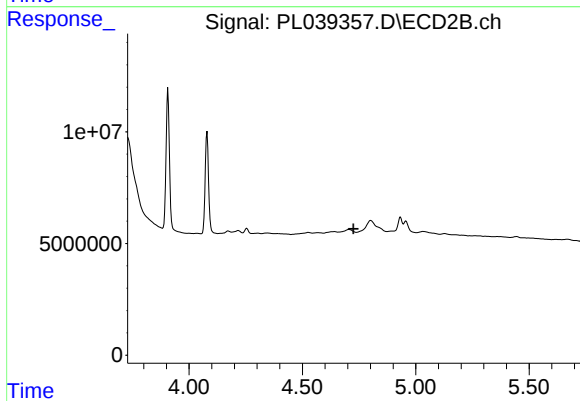

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

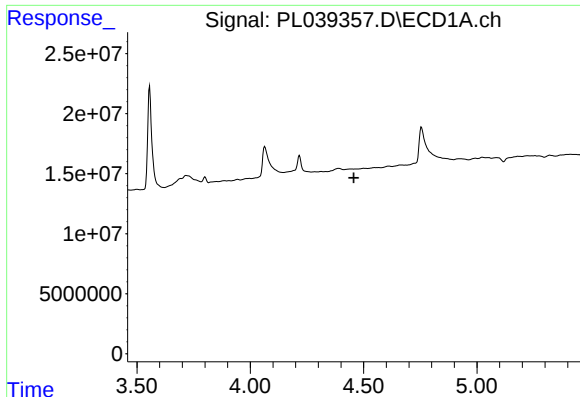

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

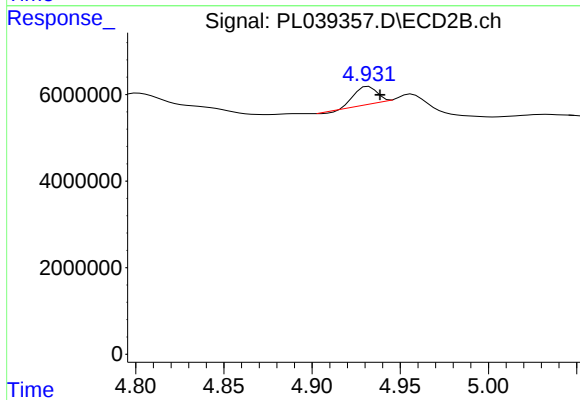


#7 delta-BHC

R.T.: 4.932 min
Delta R.T.: -0.006 min
Response: 3513513
Conc: 0.88 ng/ml

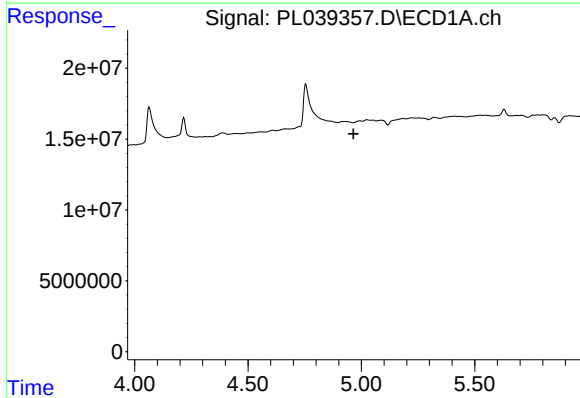


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

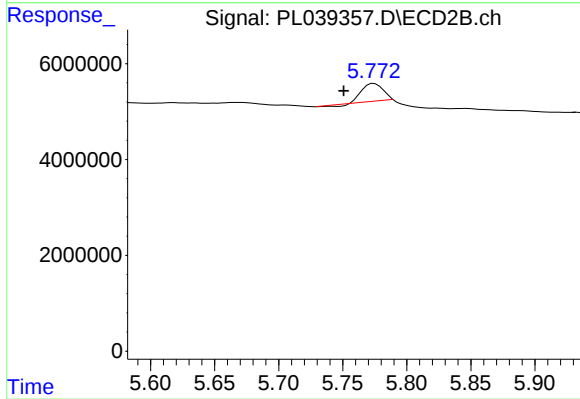

#8 Heptachlor epoxide


R.T.: 5.775 min
Delta R.T.: 0.024 min
Response: 4135989
Conc: 1.23 ng/ml

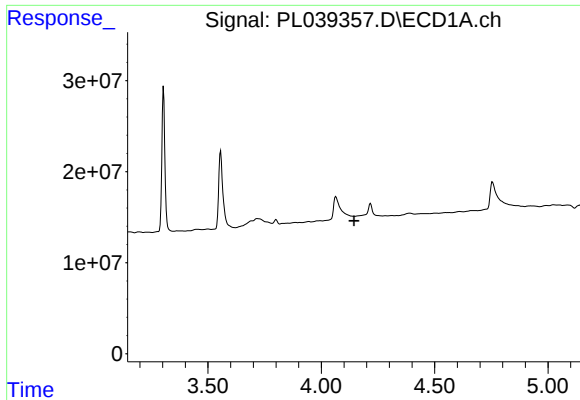

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

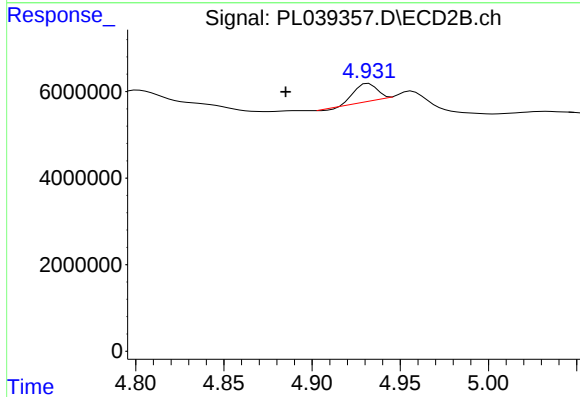


#23 Chlordane-1

R.T.: 4.932 min
Delta R.T.: 0.047 min
Response: 3513513
Conc: 28.12 ng/ml

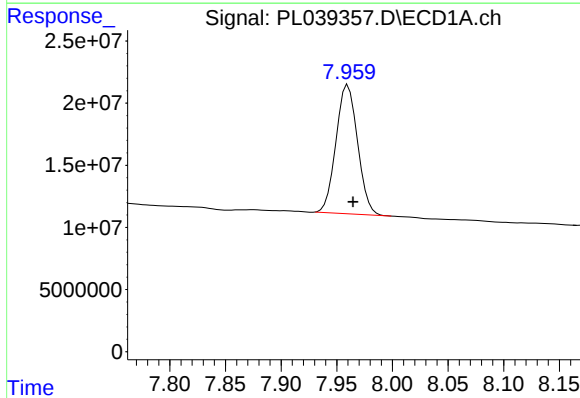

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.004 min
Response: 139877792
Conc: 19.92 ng/ml

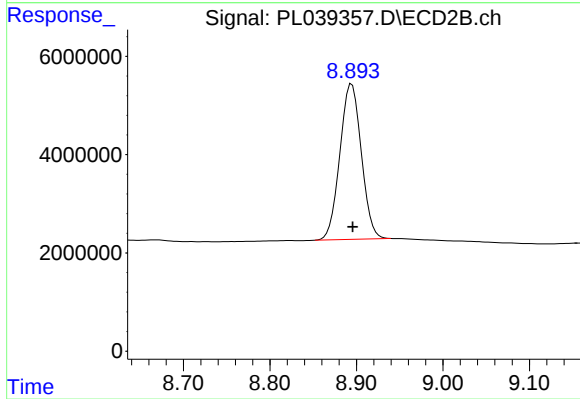

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.000 min
Response: 54283839
Conc: 23.39 ng/ml