

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2018 19:28
 Operator : AJ\SJ
 Sample : J4275-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 00:56:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.907	142.8E6	61614019	20.431	22.983
28)	SA Decachlor...	7.960	8.894	144.5E6	54952785	20.576	23.680
Target Compounds							
3)	MA gamma-BHC...	4.046f	0.000	5484843	0	0.517	N.D. #
6)	B beta-BHC	4.217f	0.000	25475736	0	5.484	N.D. #
7)	B delta-BHC	0.000	4.932	0	11762823	N.D.	2.954 #
19)	B Endosulfa...	6.455	0.000	10316821	0	1.268	N.D. #
20)	A Methoxychlor	6.636f	0.000	17657522	0	4.315	N.D. #
23)	Chlordane-1	4.078	4.932	15666784	11762823	49.487	94.152 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2018 19:28
Operator : AJ\SJ
Sample : J4275-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 00:56:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

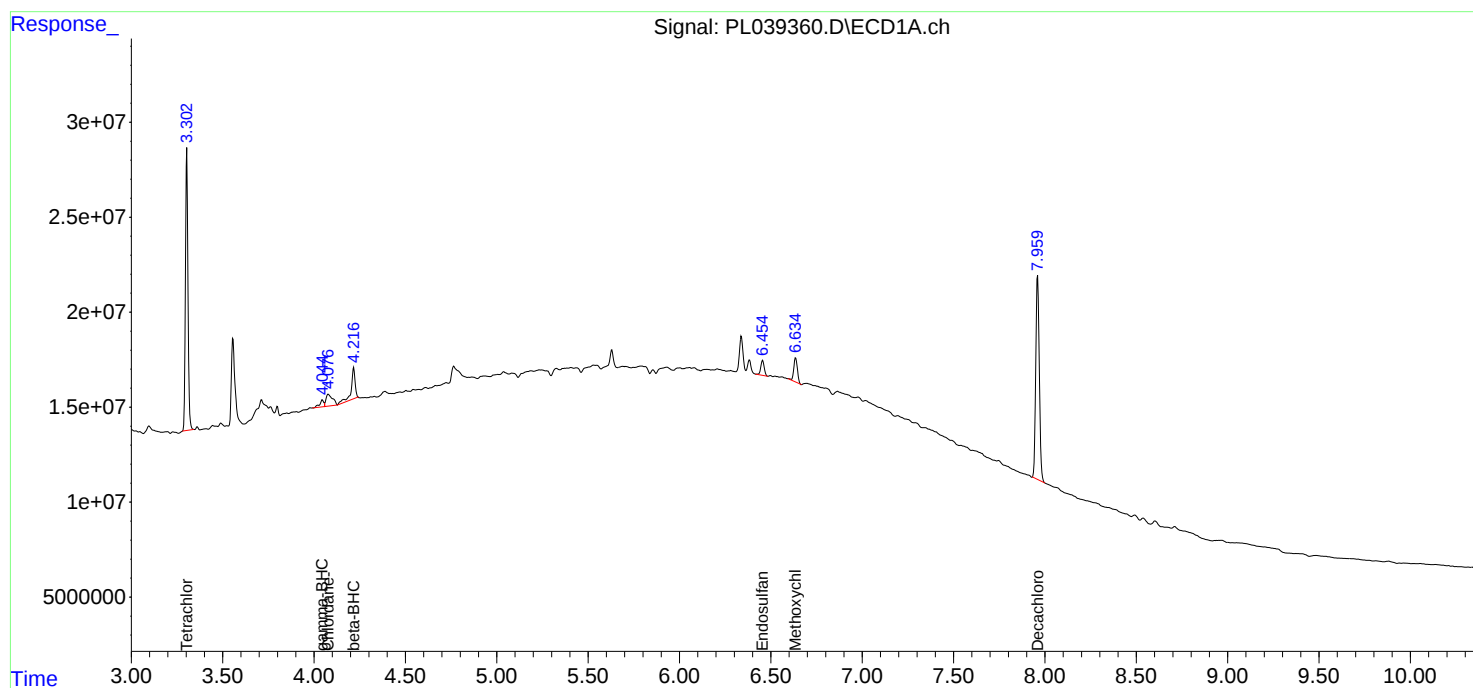


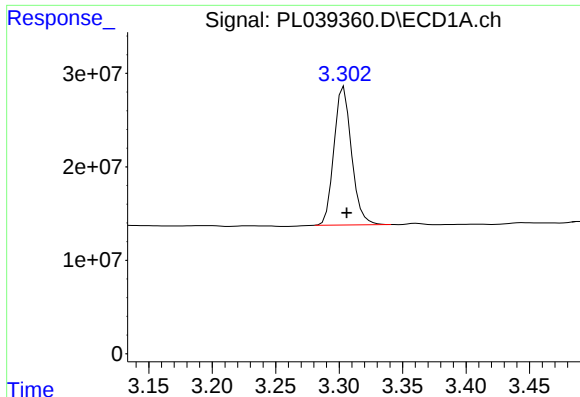

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 142821322
Conc: 20.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

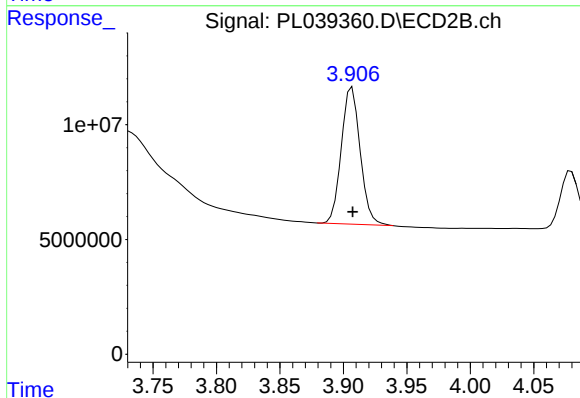


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 61614019
Conc: 22.98 ng/ml

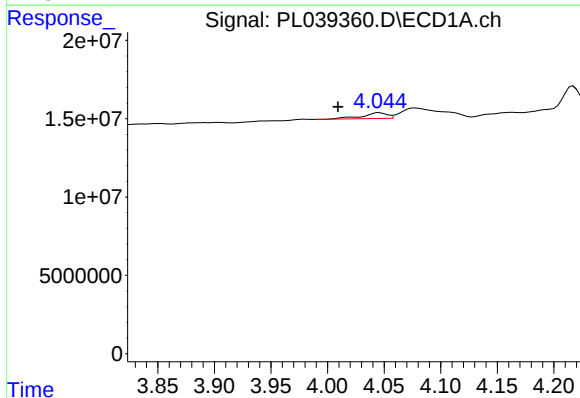


#3 gamma-BHC (Lindane)

R.T.: 4.046 min
Delta R.T.: 0.036 min
Response: 5484843
Conc: 0.52 ng/ml

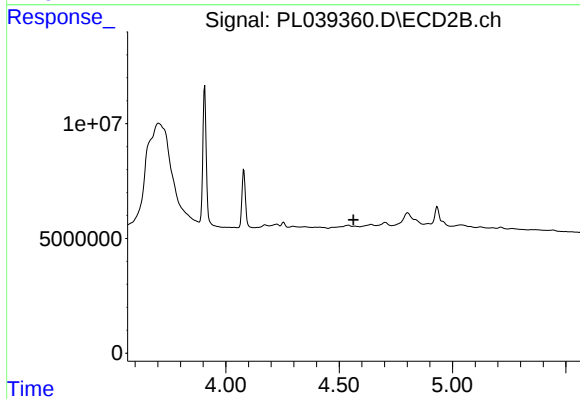

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

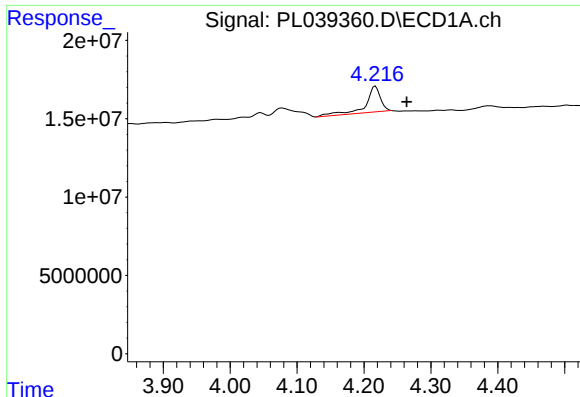

#6 beta-BHC


R.T.: 4.217 min
Delta R.T.: -0.047 min
Response: 25475736
Conc: 5.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

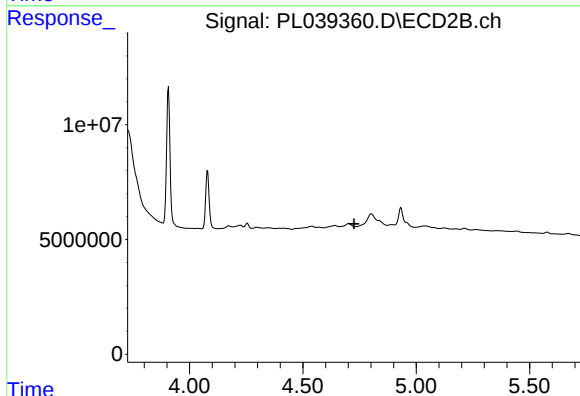


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

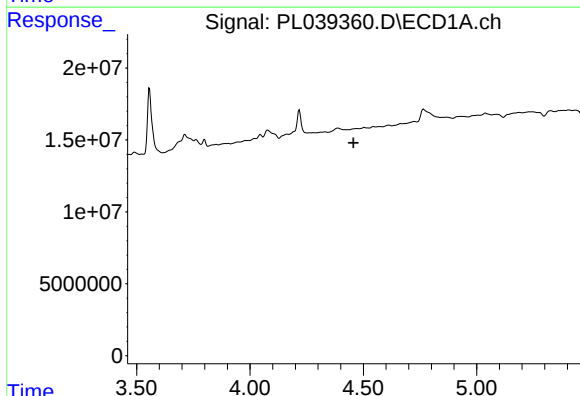


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

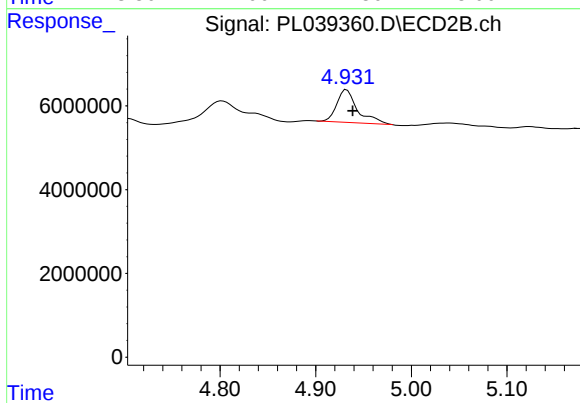

#7 delta-BHC


R.T.: 4.932 min
Delta R.T.: -0.006 min
Response: 11762823
Conc: 2.95 ng/ml

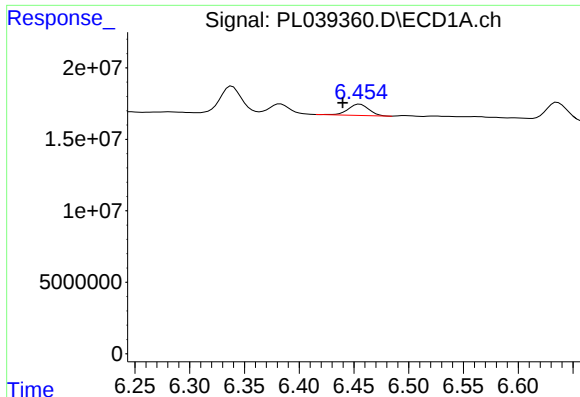

#19 Endosulfan Sulfate


R.T.: 6.455 min
Delta R.T.: 0.016 min
Response: 10316821
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

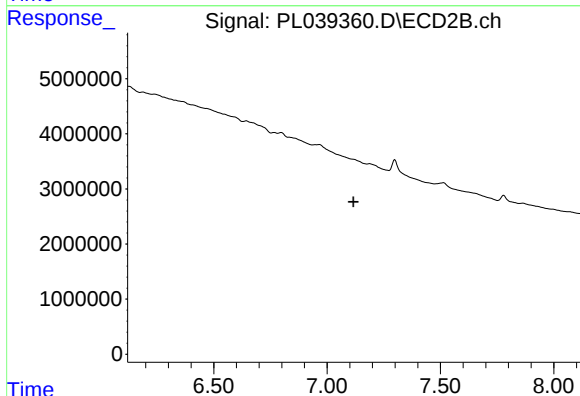


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

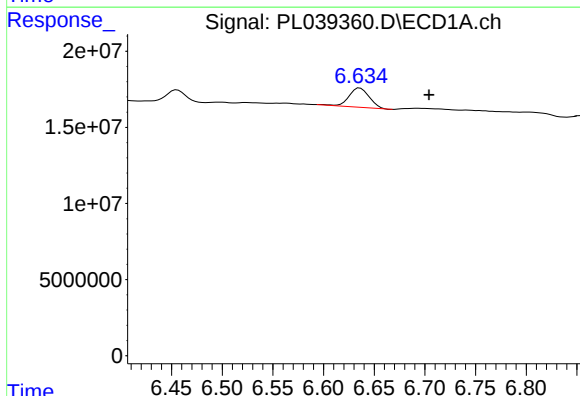


#20 Methoxychlor

R.T.: 6.636 min
Delta R.T.: -0.068 min
Response: 17657522
Conc: 4.31 ng/ml

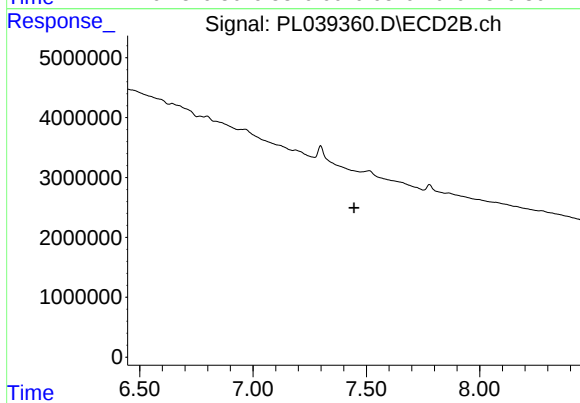

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

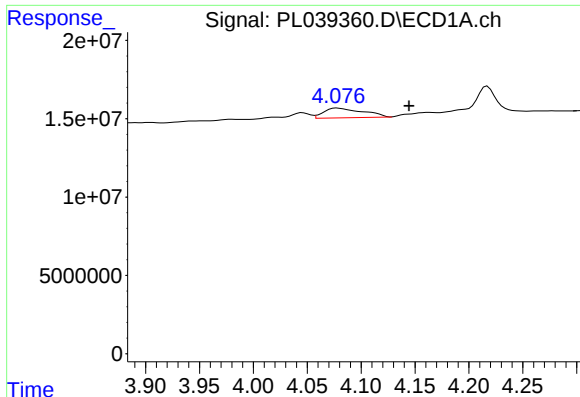

#23 Chlordane-1


R.T.: 4.078 min
Delta R.T.: -0.067 min
Response: 15666784
Conc: 49.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

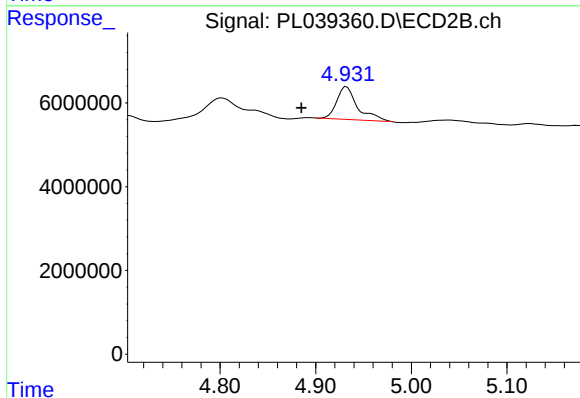


#23 Chlordane-1

R.T.: 4.932 min
Delta R.T.: 0.047 min
Response: 11762823
Conc: 94.15 ng/ml

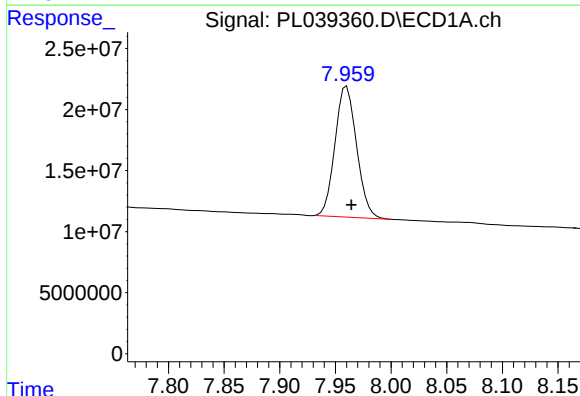

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.004 min
Response: 144511965
Conc: 20.58 ng/ml

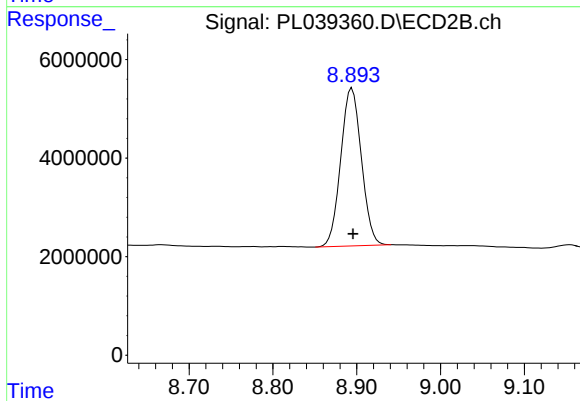

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.001 min
Response: 54952785
Conc: 23.68 ng/ml