

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2018 19:42
 Operator : AJ\SJ
 Sample : J4277-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 00:56:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.907	139.2E6	60427049	19.912	22.540
28)	SA Decachlor...	7.960	8.895	118.4E6	45566104	16.854	19.635
Target Compounds							
5)	MB Aldrin	4.532	0.000	11770680	0	1.175	N.D. #
6)	B beta-BHC	4.217f	0.000	48048261	0	10.343	N.D. #
7)	B delta-BHC	0.000	4.932	0	28173818	N.D.	7.076 #
8)	B Heptachlo...	4.919f	0.000	1865632	0	0.195	N.D. #
14)	MA Endrin	5.855f	0.000	1923757	0	0.215	N.D. #
16)	A 4,4'-DDD	5.855f	0.000	1923757	0	0.241	N.D. #
20)	A Methoxychlor	6.636f	0.000	10405340	0	2.543	N.D. #
23)	Chlordane-1	4.140	4.932	5396582	28173818	17.046	225.508 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2018 19:42
Operator : AJ\SJ
Sample : J4277-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 00:56:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

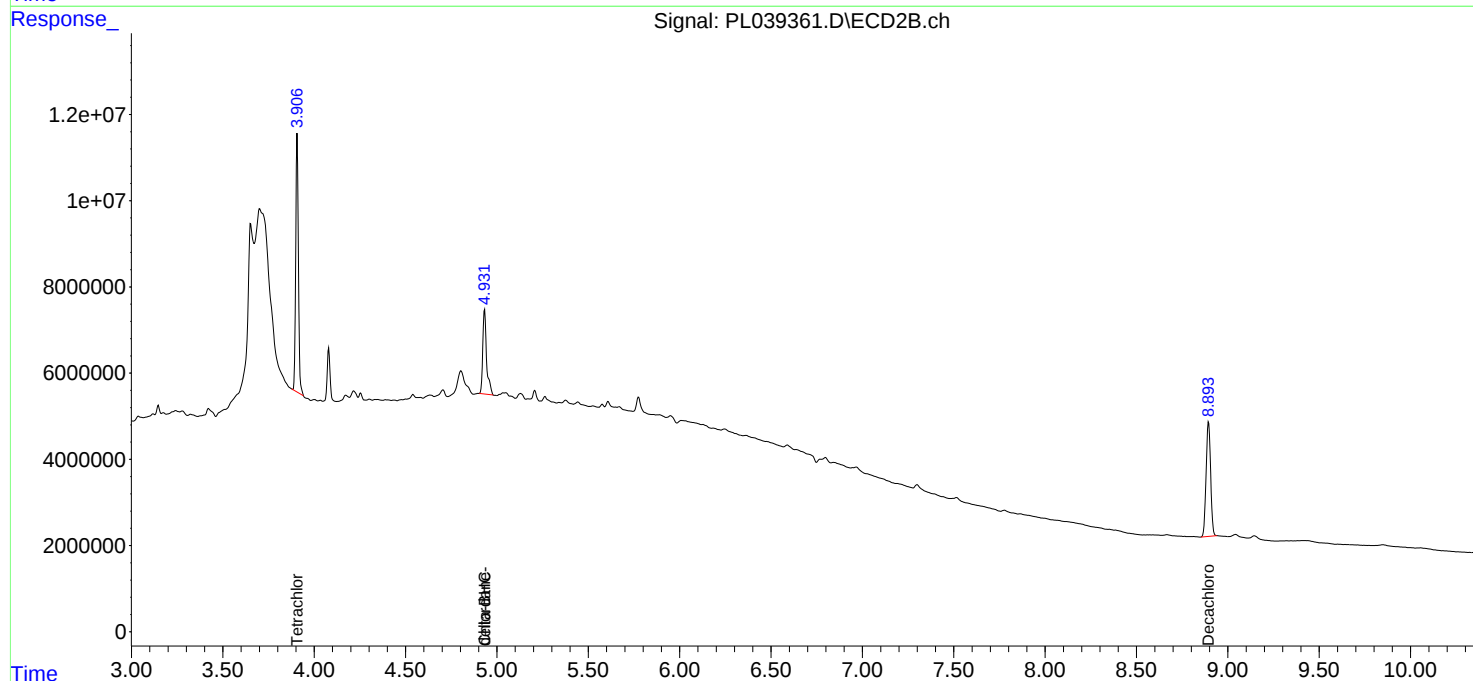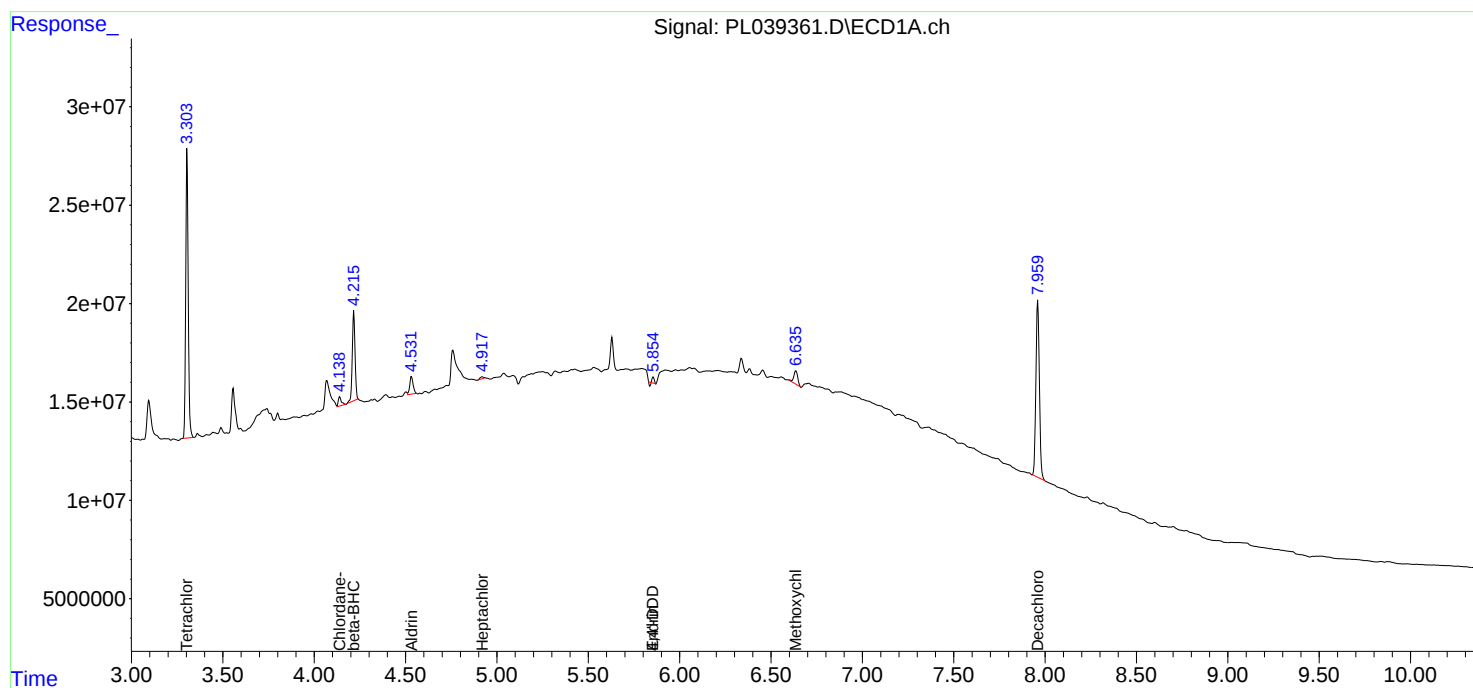


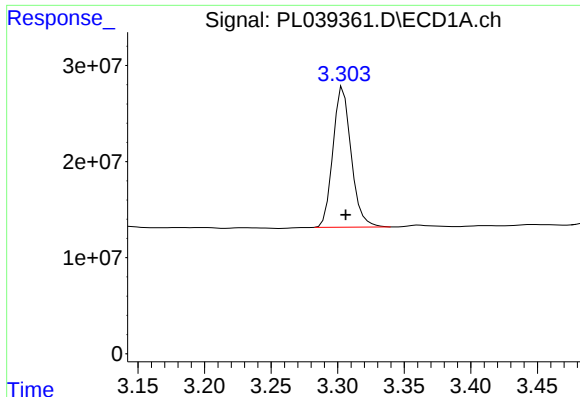

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 139189775
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

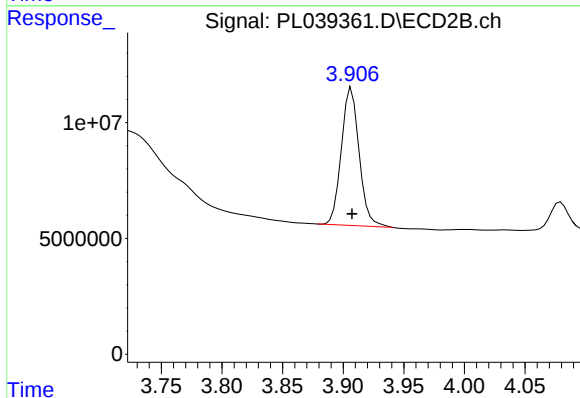


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 60427049
Conc: 22.54 ng/ml

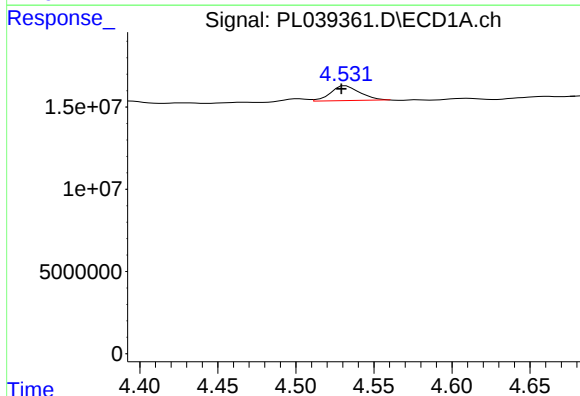


#5 Aldrin

R.T.: 4.532 min
Delta R.T.: 0.003 min
Response: 11770680
Conc: 1.18 ng/ml

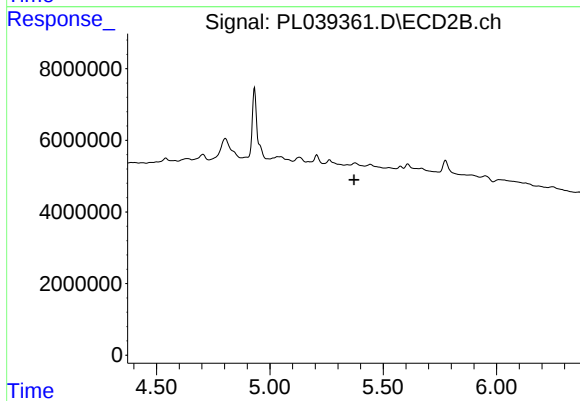

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.372 min
Response: 0
Conc: N.D.

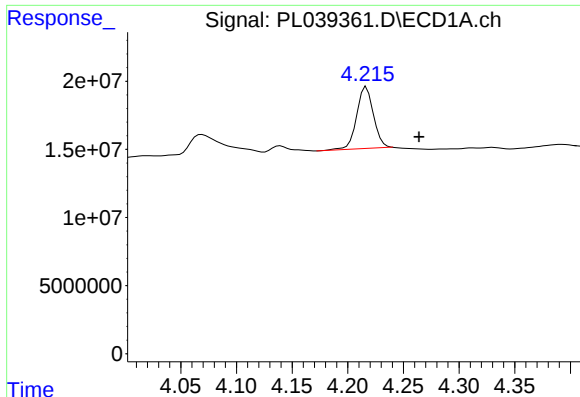

#6 beta-BHC


R.T.: 4.217 min
Delta R.T.: -0.047 min
Response: 48048261
Conc: 10.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

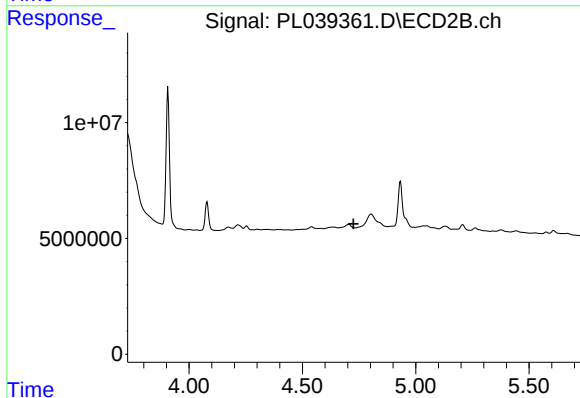


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

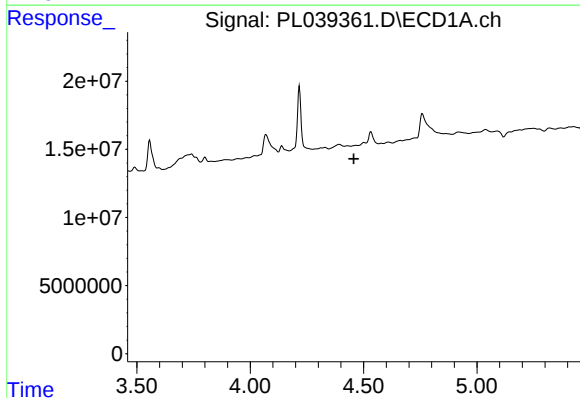


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

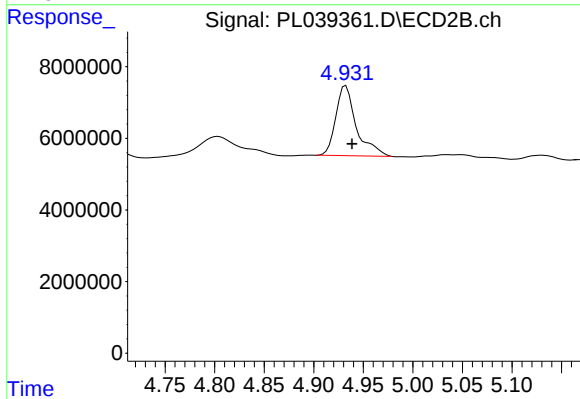

#7 delta-BHC


R.T.: 4.932 min
Delta R.T.: -0.006 min
Response: 28173818
Conc: 7.08 ng/ml

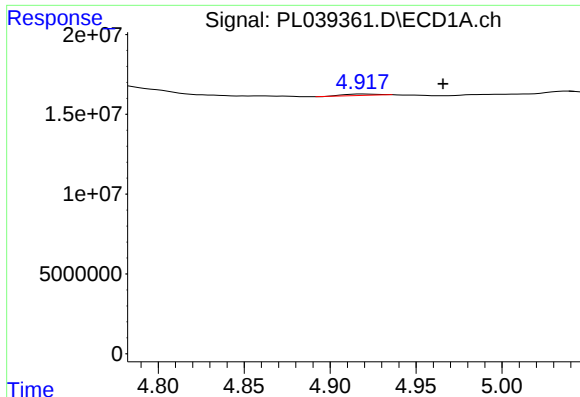

#8 Heptachlor epoxide


R.T.: 4.919 min
Delta R.T.: -0.046 min
Response: 1865632
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

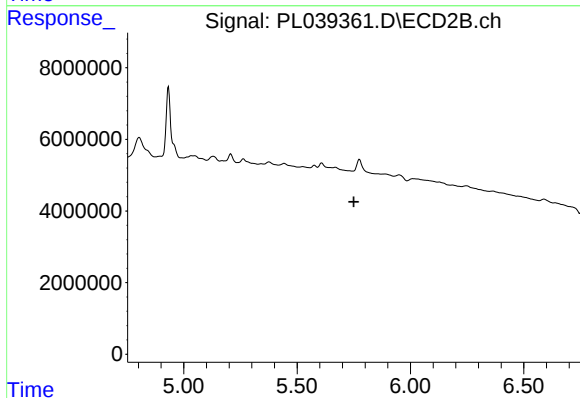


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

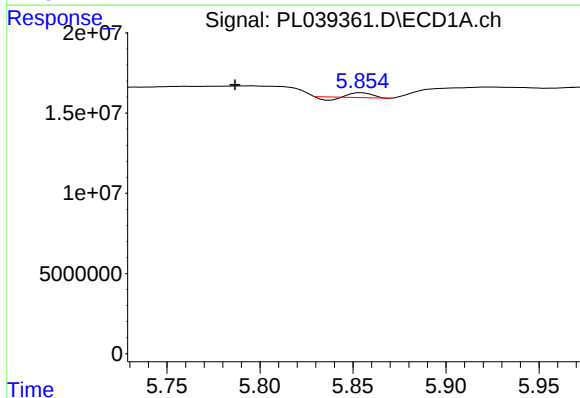


#14 Endrin

R.T.: 5.855 min
Delta R.T.: 0.069 min
Response: 1923757
Conc: 0.21 ng/ml

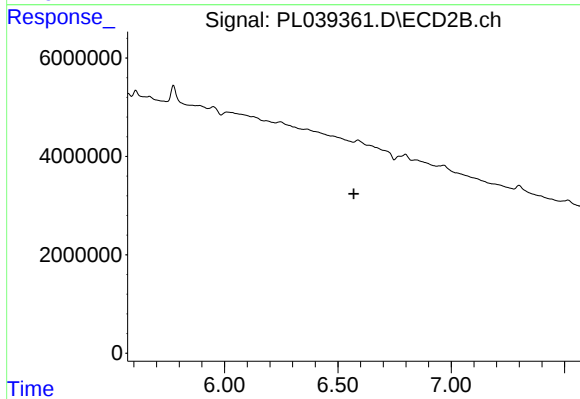

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

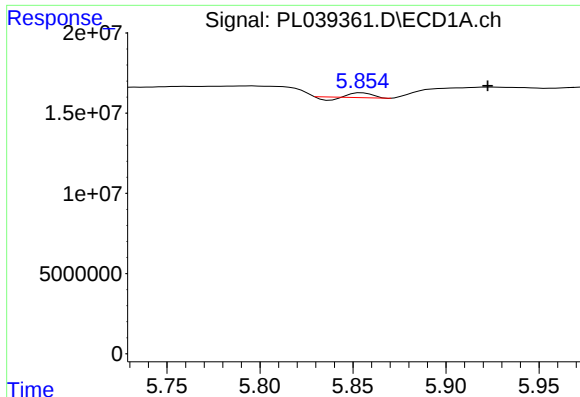

#16 4,4'-DDD


R.T.: 5.855 min
Delta R.T.: -0.067 min
Response: 1923757
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

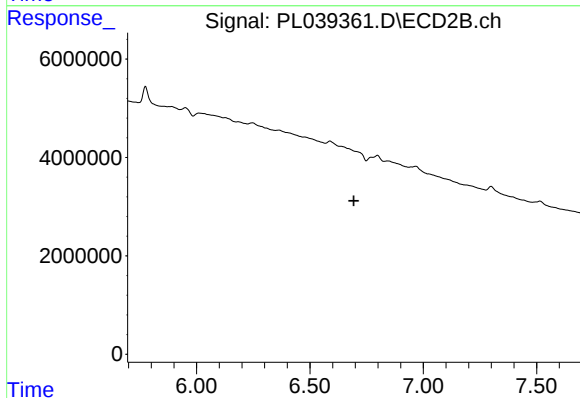


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

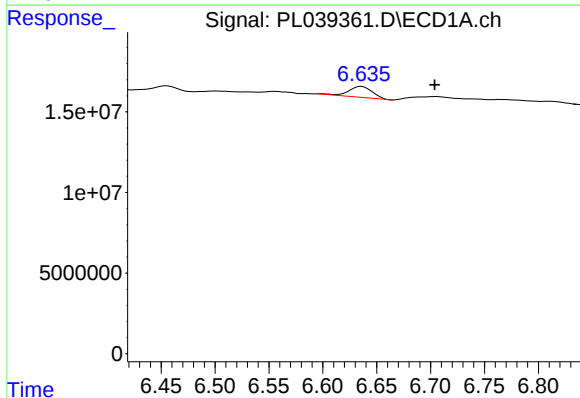


#20 Methoxychlor

R.T.: 6.636 min
Delta R.T.: -0.068 min
Response: 10405340
Conc: 2.54 ng/ml

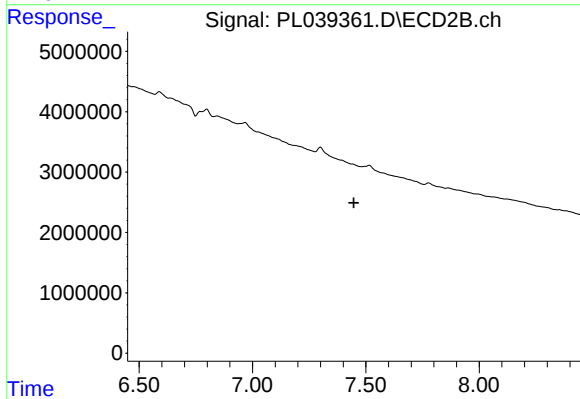

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

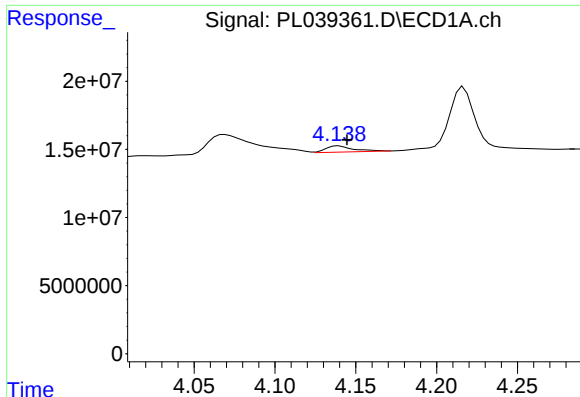

#23 Chlordane-1


R.T.: 4.140 min
Delta R.T.: -0.005 min
Response: 5396582
Conc: 17.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

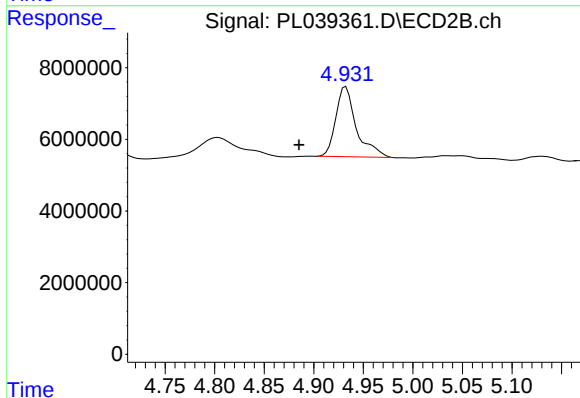


#23 Chlordane-1

R.T.: 4.932 min
Delta R.T.: 0.047 min
Response: 28173818
Conc: 225.51 ng/ml

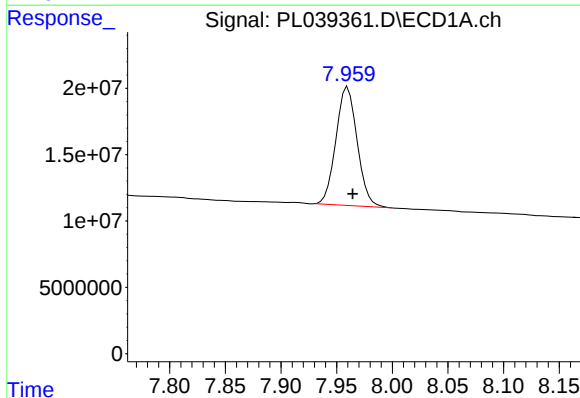

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.004 min
Response: 118372773
Conc: 16.85 ng/ml

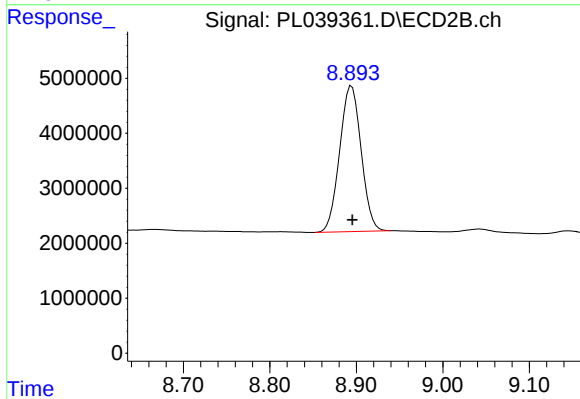

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.000 min
Response: 45566104
Conc: 19.64 ng/ml