

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 02:33
 Operator : AJ\SJ
 Sample : J4553-01
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 05:32:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.907	142.8E6	60562510	20.430	22.590
28)	SA Decachlor...	7.962	8.896	104.2E6	44613079	14.831	19.225 #
Target Compounds							
4)	MA Heptachlor	4.224f	0.000	12242526	0	1.163	N.D. #
6)	B beta-BHC	4.224f	0.000	12242526	0	2.635	N.D. #
10)	B gamma-Chl...	5.144f	0.000	1645125	0	0.167	N.D. #
23)	Chlordane-1	4.163	0.000	4925681	0	15.559	N.D. #
25)	Chlordane-3	5.144	0.000	1645125	0	1.506	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 02:33
Operator : AJ\SJ
Sample : J4553-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 05:32:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

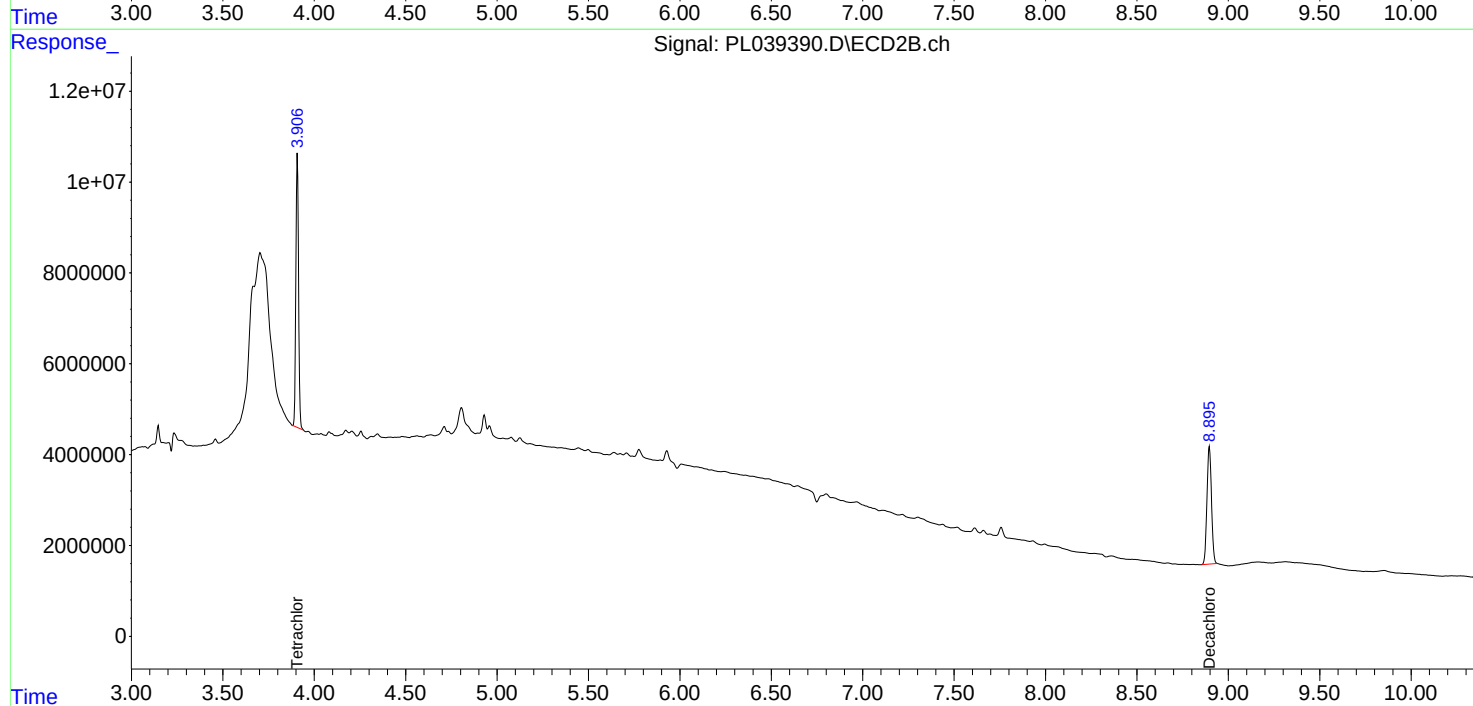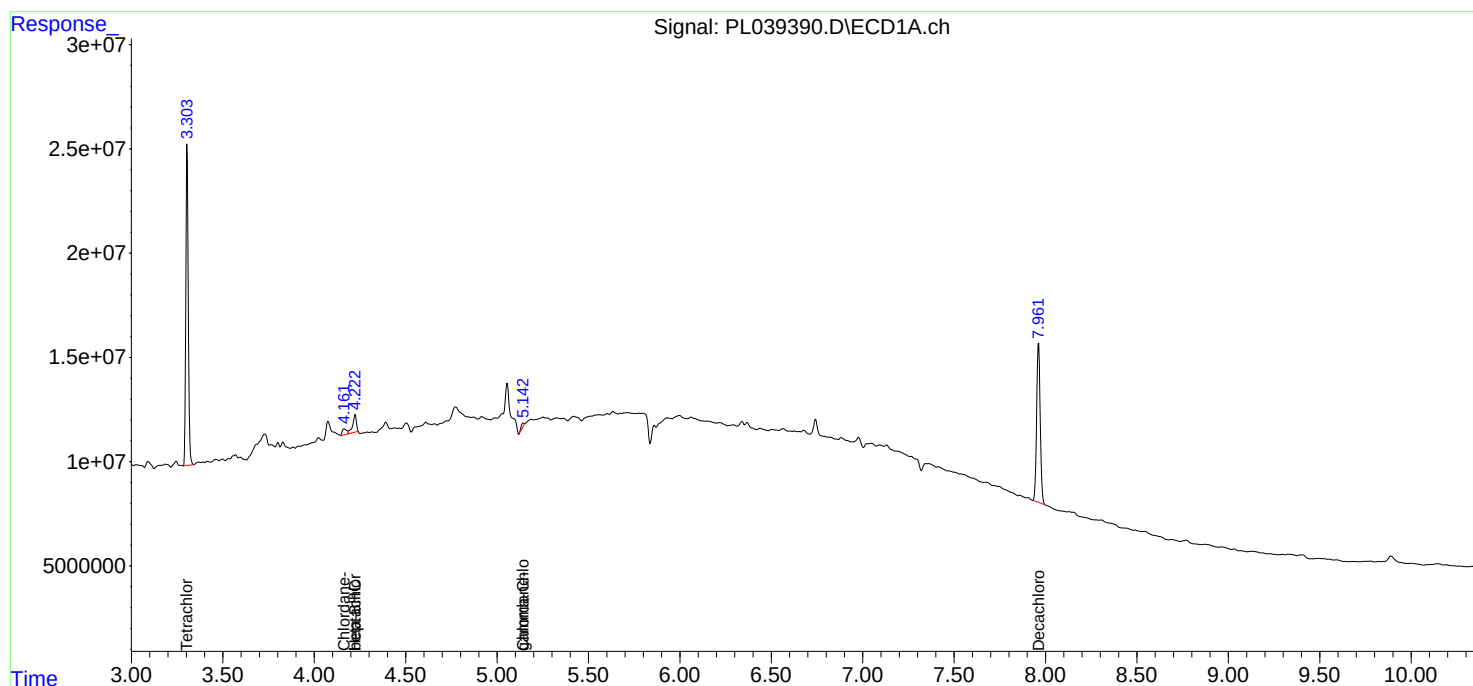


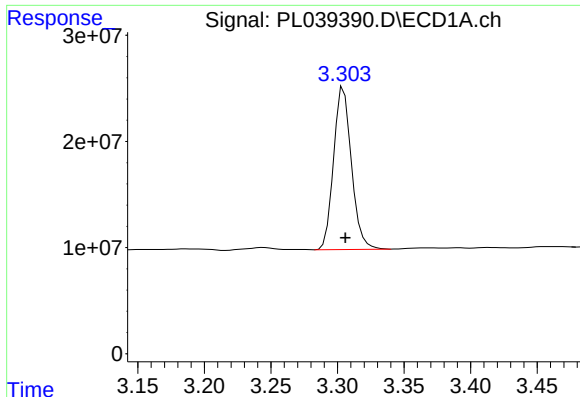

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 142816551
Conc: 20.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

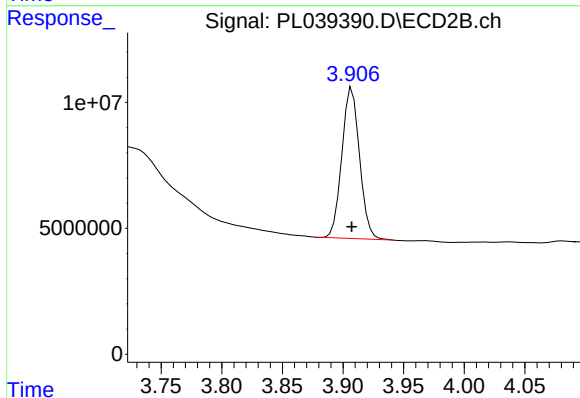


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 60562510
Conc: 22.59 ng/ml

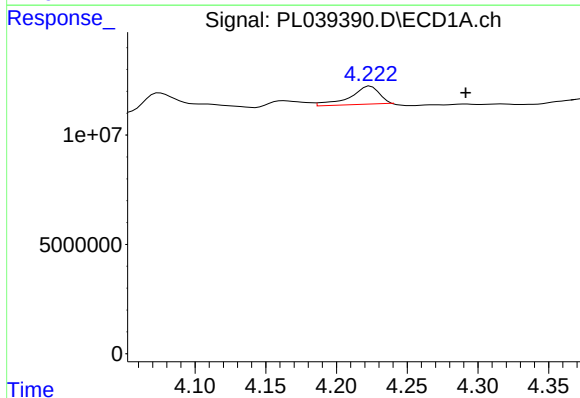


#4 Heptachlor

R.T.: 4.224 min
Delta R.T.: -0.067 min
Response: 12242526
Conc: 1.16 ng/ml

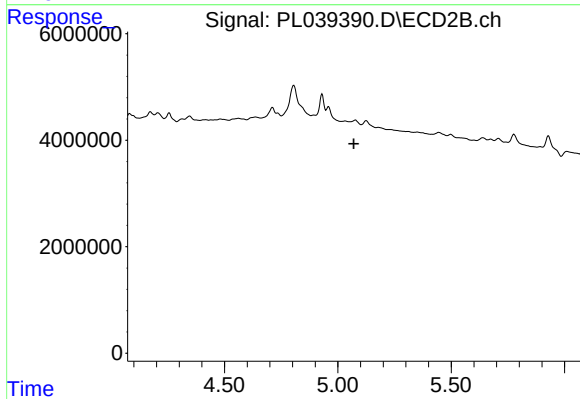

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.071 min
Response: 0
Conc: N.D.

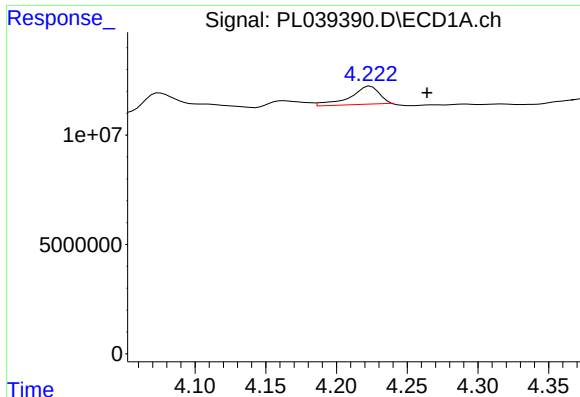

#6 beta-BHC


R.T.: 4.224 min
Delta R.T.: -0.040 min
Response: 12242526
Conc: 2.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

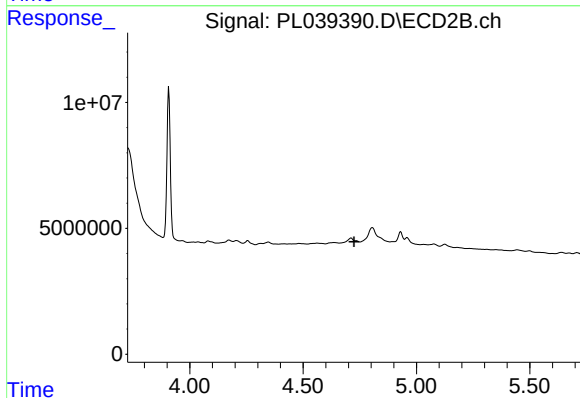


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

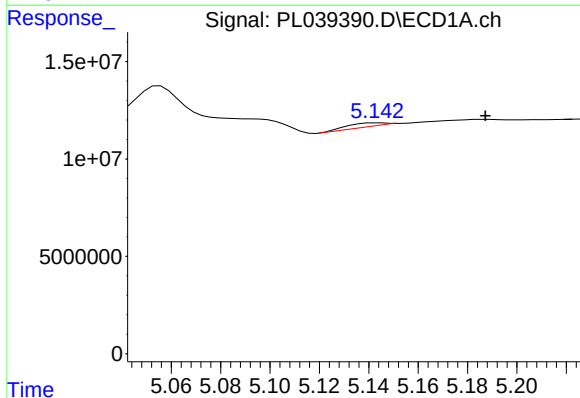


#10 gamma-Chlordane

R.T.: 5.144 min
Delta R.T.: -0.043 min
Response: 1645125
Conc: 0.17 ng/ml

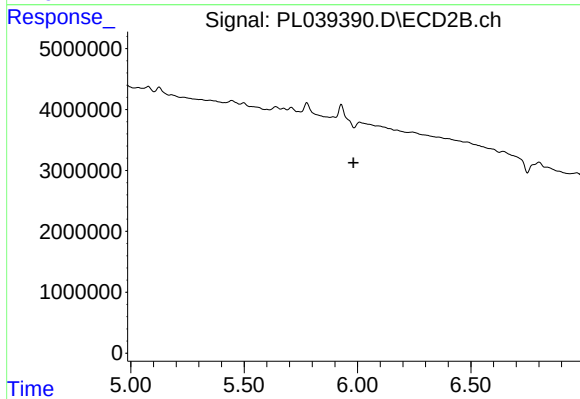

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

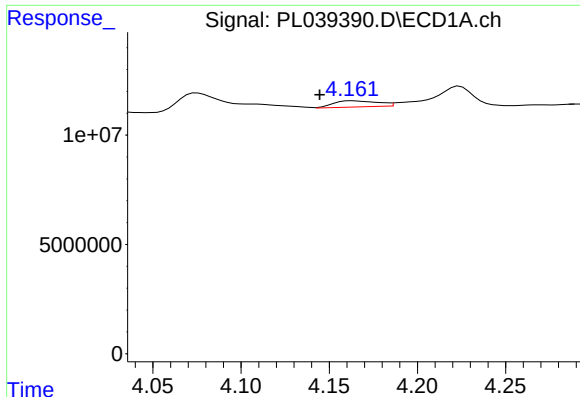

#23 Chlordane-1


R.T.: 4.163 min
Delta R.T.: 0.018 min
Response: 4925681
Conc: 15.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

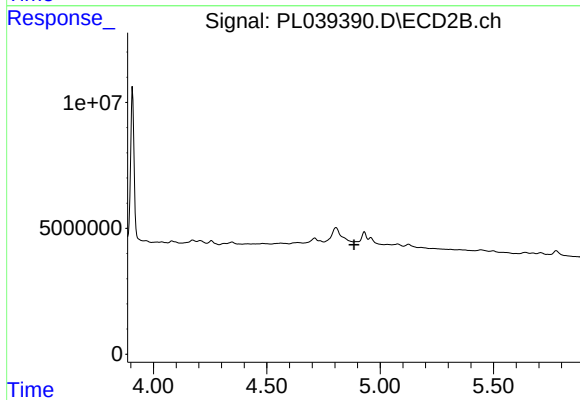


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

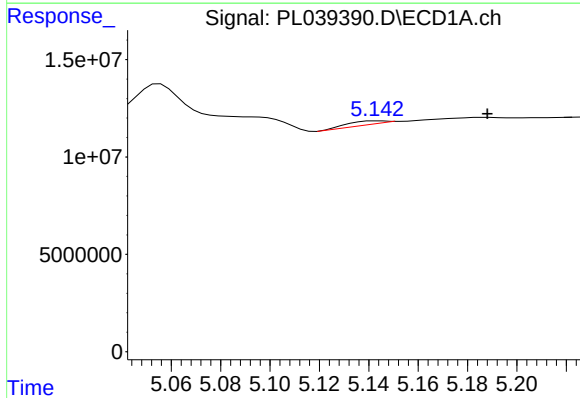


#25 Chlordane-3

R.T.: 5.144 min
Delta R.T.: -0.044 min
Response: 1645125
Conc: 1.51 ng/ml

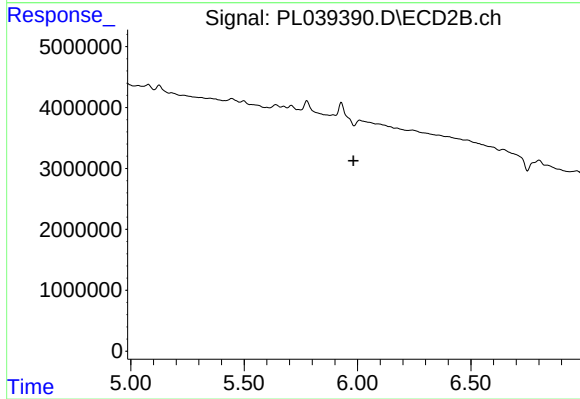

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

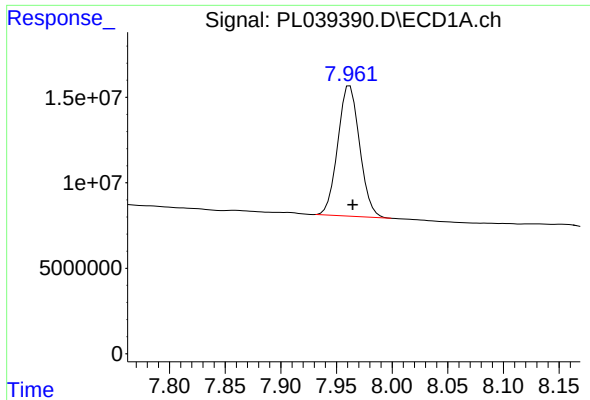

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.002 min
Response: 104161286
Conc: 14.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

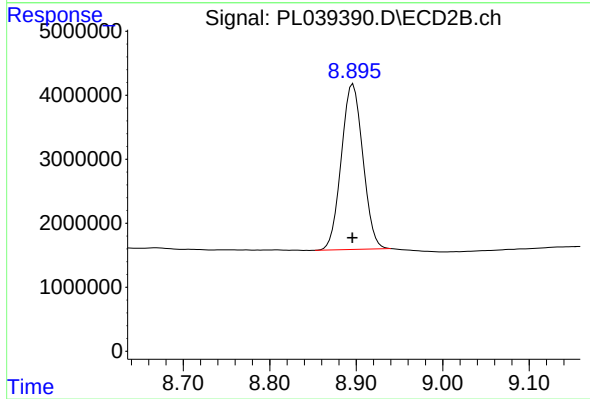

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 44613079
Conc: 19.22 ng/ml