

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 04:27
 Operator : AJ\SJ
 Sample : J4556-03
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 05:35:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.908	184.6E6	79445933	26.410	29.634
28)	SA Decachlor...	7.962	8.898	126.0E6	51286134	17.943	22.100
Target Compounds							
4)	MA Heptachlor	4.307	0.000	4317654	0	0.410	N.D. #
6)	B beta-BHC	4.307f	0.000	4317654	0	0.929	N.D. #
10)	B gamma-Chl...	5.216	0.000	10025643	0	1.015	N.D. #
11)	B alpha-Chl...	5.216	0.000	10025643	0	1.044	N.D. #
16)	A 4,4'-DDD	5.923	0.000	5410740	0	0.679	N.D. #
23)	Chlordane-1	4.169	0.000	4657886	0	14.713	N.D. #
25)	Chlordane-3	5.216	0.000	10025643	0	9.179	N.D. #
26)	Chlordane-4	5.216	0.000	10025643	0	10.032	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 04:27
Operator : AJ\SJ
Sample : J4556-03
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 05:35:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

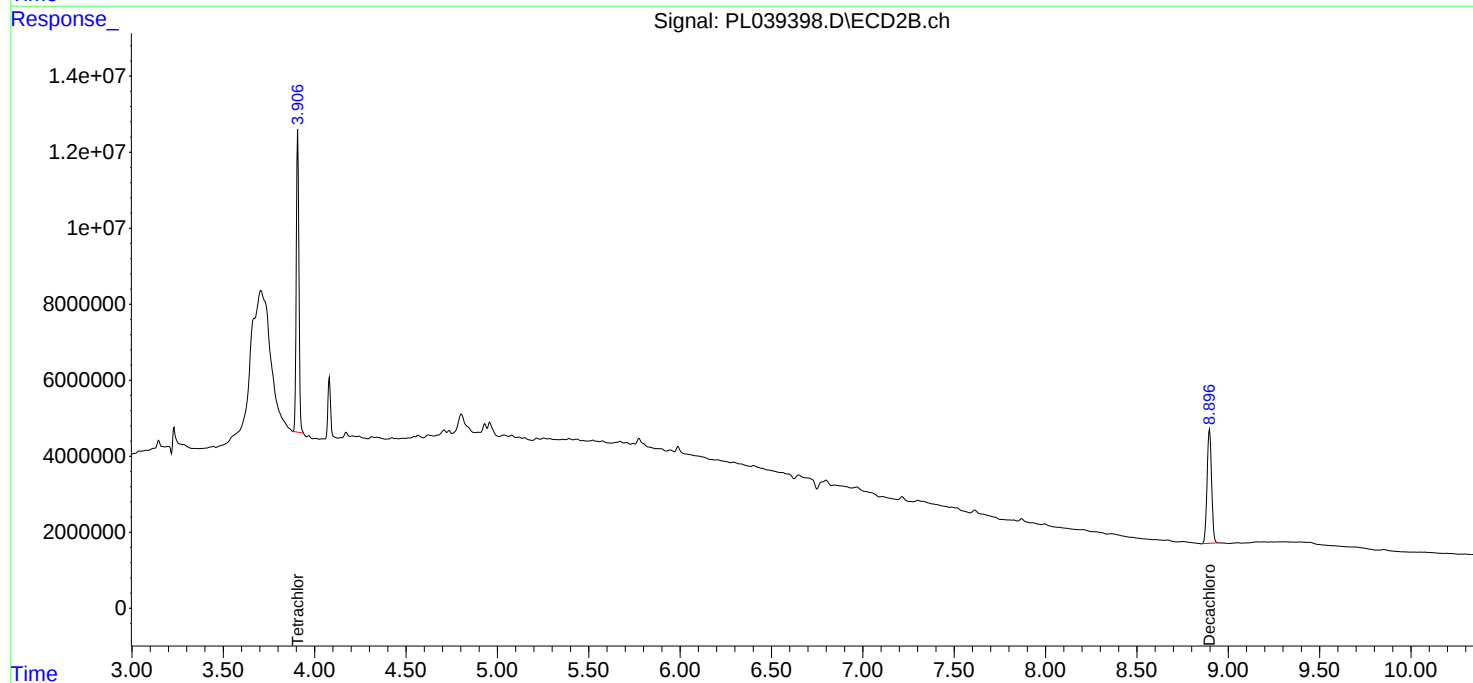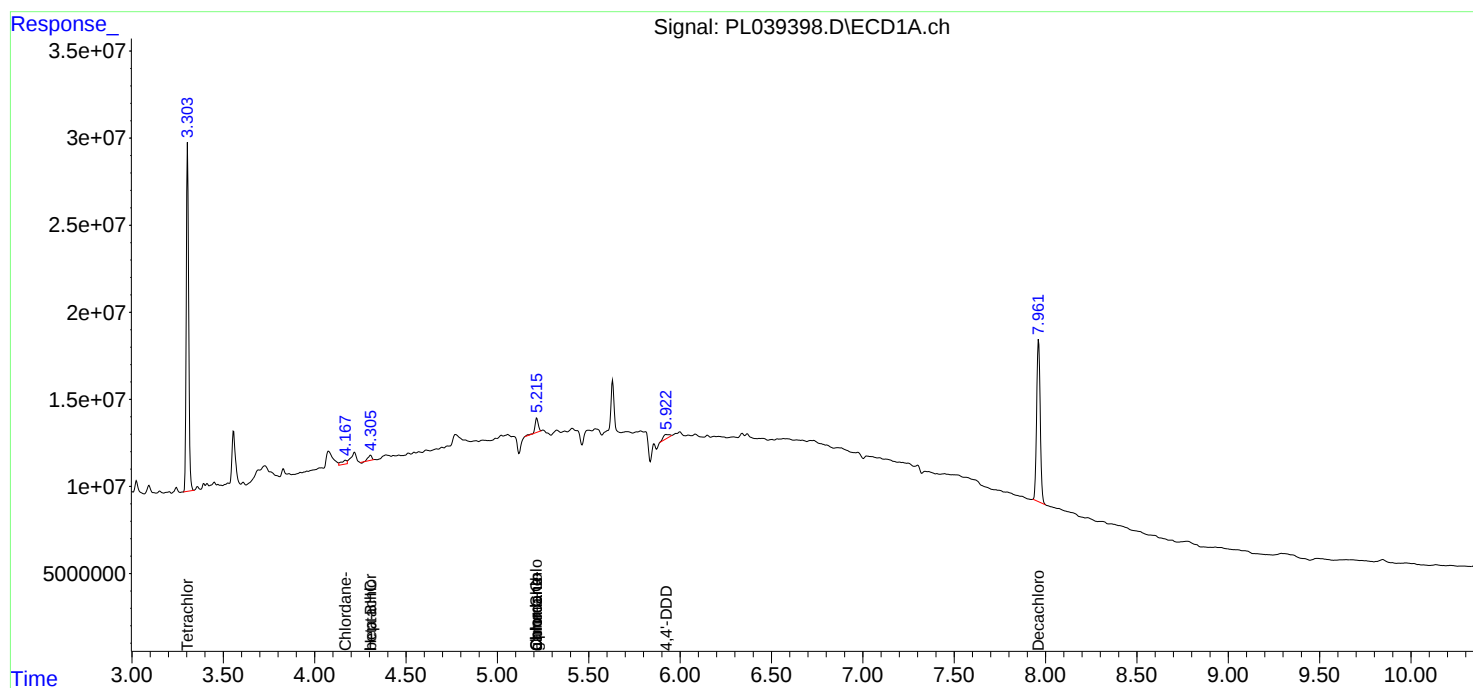


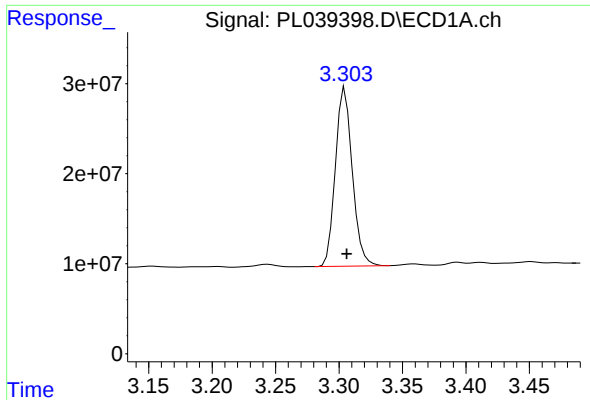

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 184614005
Conc: 26.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

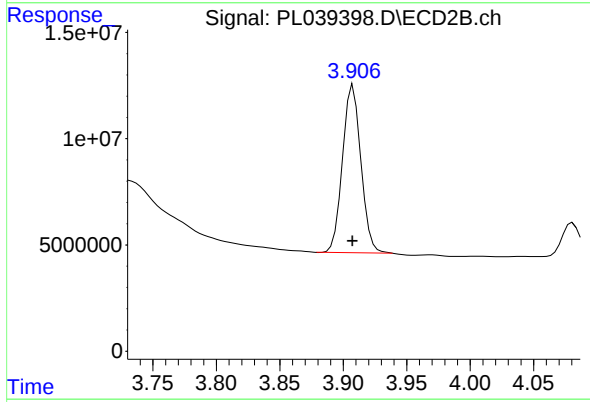


#1 Tetrachloro-m-xylene

R.T.: 3.908 min
Delta R.T.: 0.000 min
Response: 79445933
Conc: 29.63 ng/ml

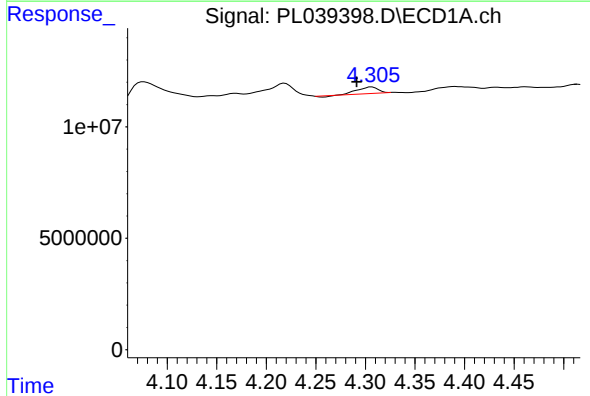


#4 Heptachlor

R.T.: 4.307 min
Delta R.T.: 0.015 min
Response: 4317654
Conc: 0.41 ng/ml

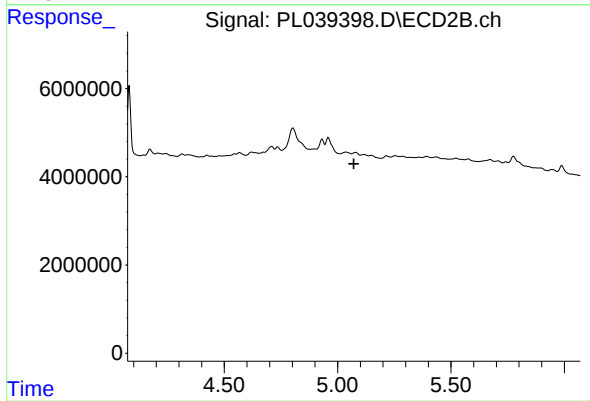

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.071 min
Response: 0
Conc: N.D.

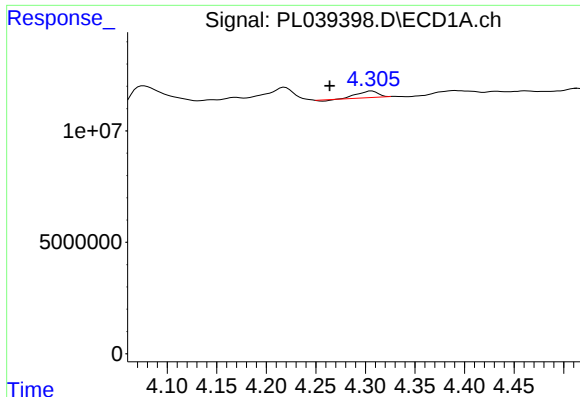

#6 beta-BHC


R.T.: 4.307 min
Delta R.T.: 0.042 min
Response: 4317654
Conc: 0.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

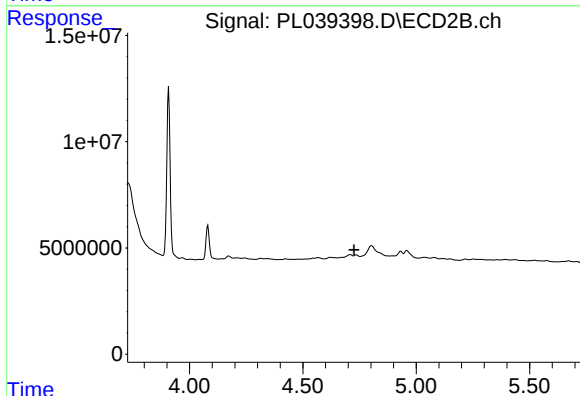


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

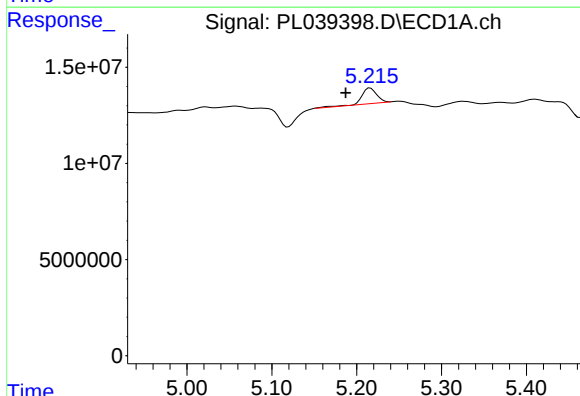


#10 gamma-Chlordane

R.T.: 5.216 min
Delta R.T.: 0.029 min
Response: 10025643
Conc: 1.02 ng/ml

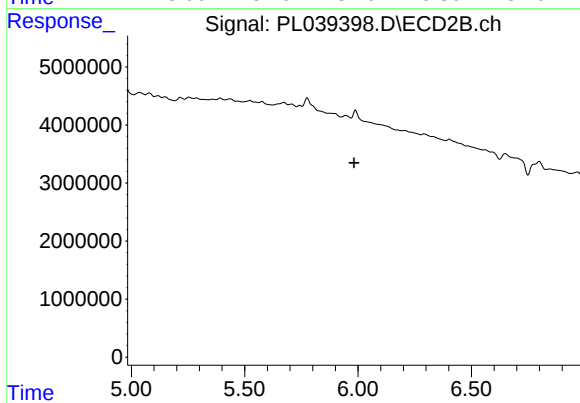

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

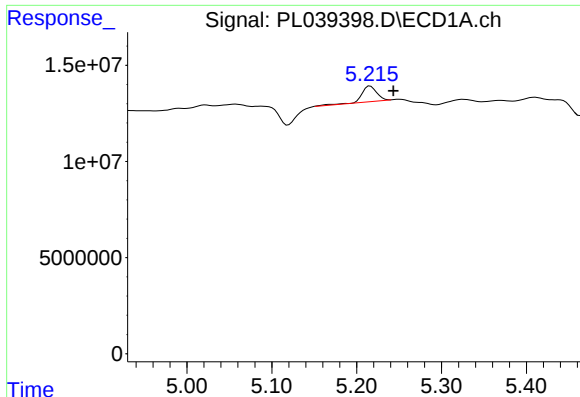

#11 alpha-Chlordane


R.T.: 5.216 min
Delta R.T.: -0.028 min
Response: 10025643
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

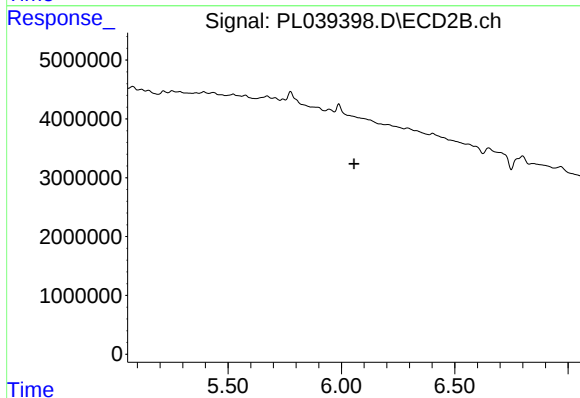


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

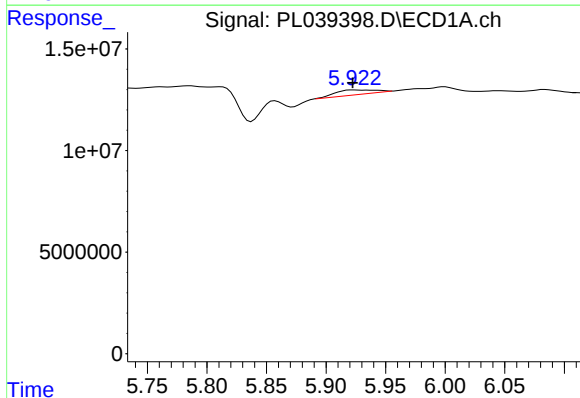


#16 4,4'-DDD

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 5410740
Conc: 0.68 ng/ml

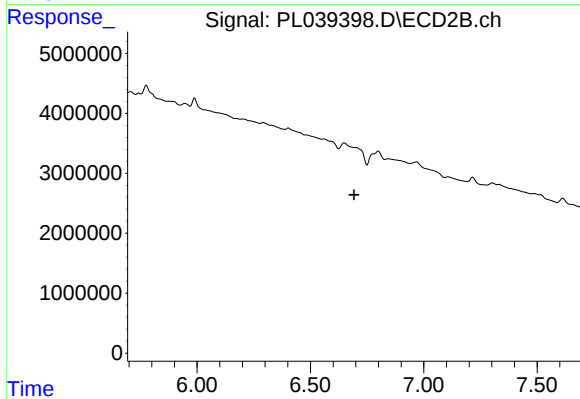

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

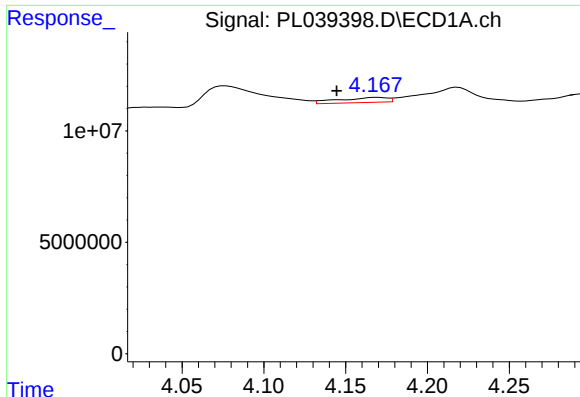

#23 Chlordane-1


R.T.: 4.169 min
Delta R.T.: 0.025 min
Response: 4657886
Conc: 14.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

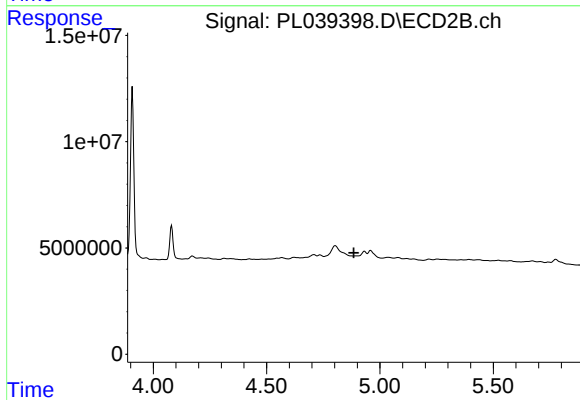


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

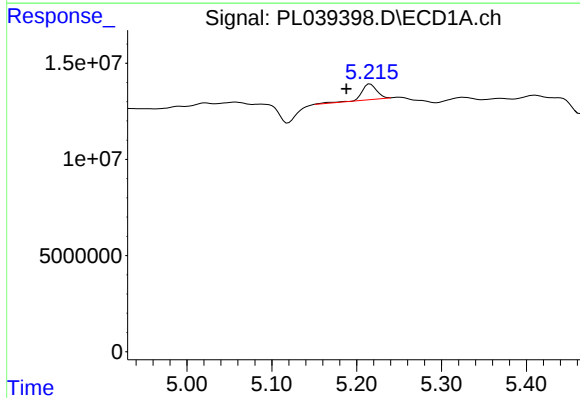


#25 Chlordane-3

R.T.: 5.216 min
Delta R.T.: 0.028 min
Response: 10025643
Conc: 9.18 ng/ml

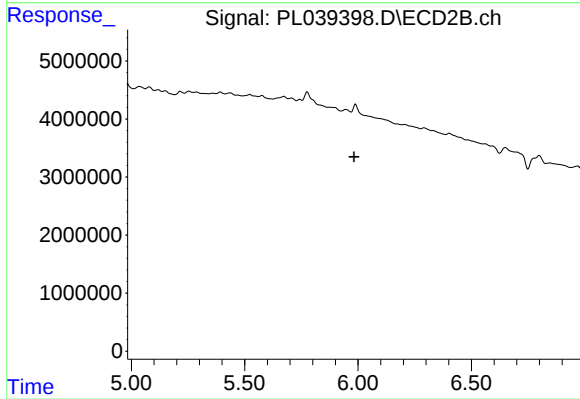

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

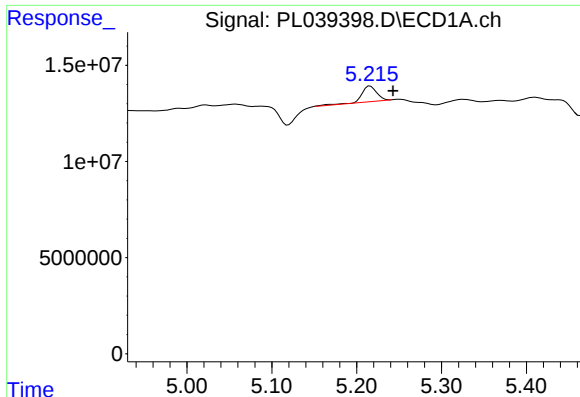

#26 Chlordane-4


R.T.: 5.216 min
Delta R.T.: -0.027 min
Response: 10025643
Conc: 10.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

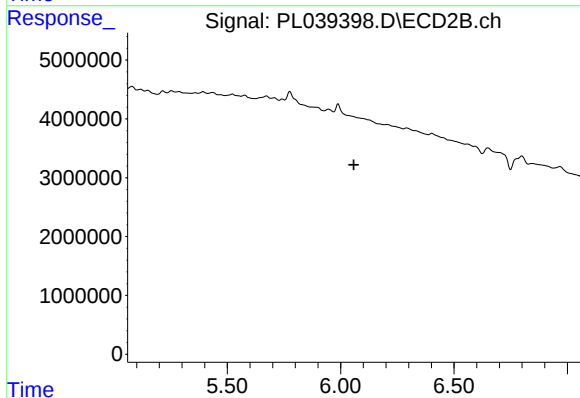


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.058 min
Response: 0
Conc: N.D.

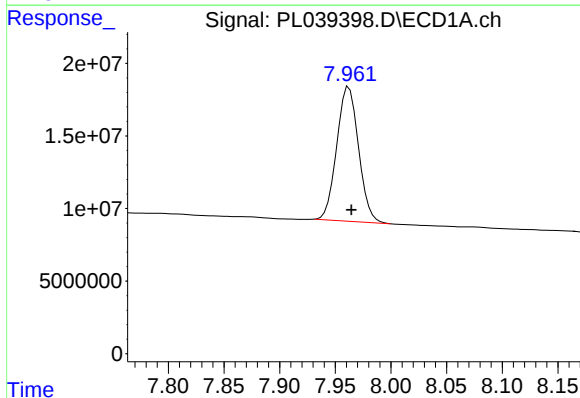

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.002 min
Response: 126021199
Conc: 17.94 ng/ml

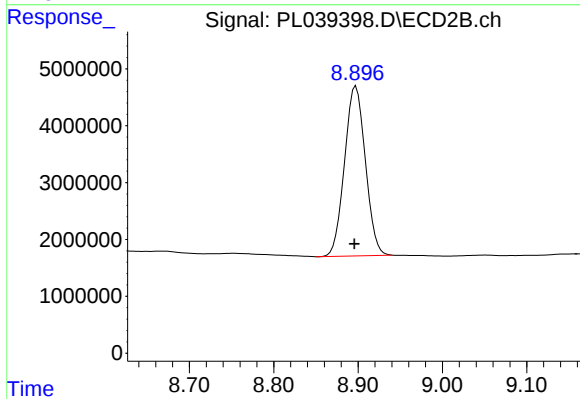

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.002 min
Response: 51286134
Conc: 22.10 ng/ml