

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 04:41
 Operator : AJ\SJ
 Sample : J4556-04
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 05:35:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.907	174.5E6	75195724	24.962	28.049
28)	SA Decachlor...	7.963	8.898	118.3E6	47774596	16.842	20.587
Target Compounds							
2)	A alpha-BHC	3.689f	0.000	5539468	0	0.469	N.D. #
6)	B beta-BHC	4.219f	0.000	12120703	0	2.609	N.D. #
10)	B gamma-Chl...	5.216	0.000	9469107	0	0.959	N.D. #
11)	B alpha-Chl...	5.216	0.000	9469107	0	0.986	N.D. #
14)	MA Endrin	5.856f	0.000	3215004	0	0.359	N.D. #
16)	A 4,4'-DDD	5.930	0.000	6626452	0	0.832	N.D. #
23)	Chlordane-1	4.167	0.000	5793195	0	18.299	N.D. #
25)	Chlordane-3	5.216	0.000	9469107	0	8.669	N.D. #
26)	Chlordane-4	5.216	0.000	9469107	0	9.475	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 04:41
Operator : AJ\SJ
Sample : J4556-04
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 05:35:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

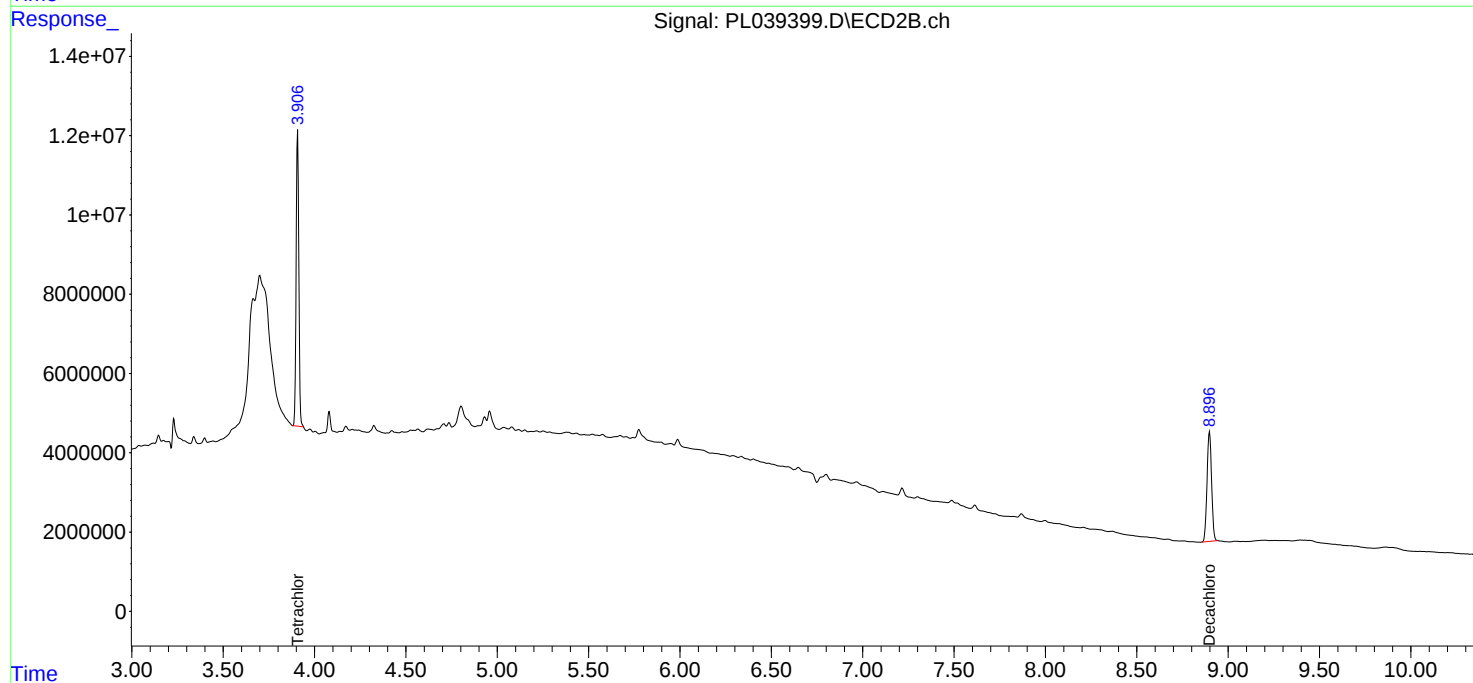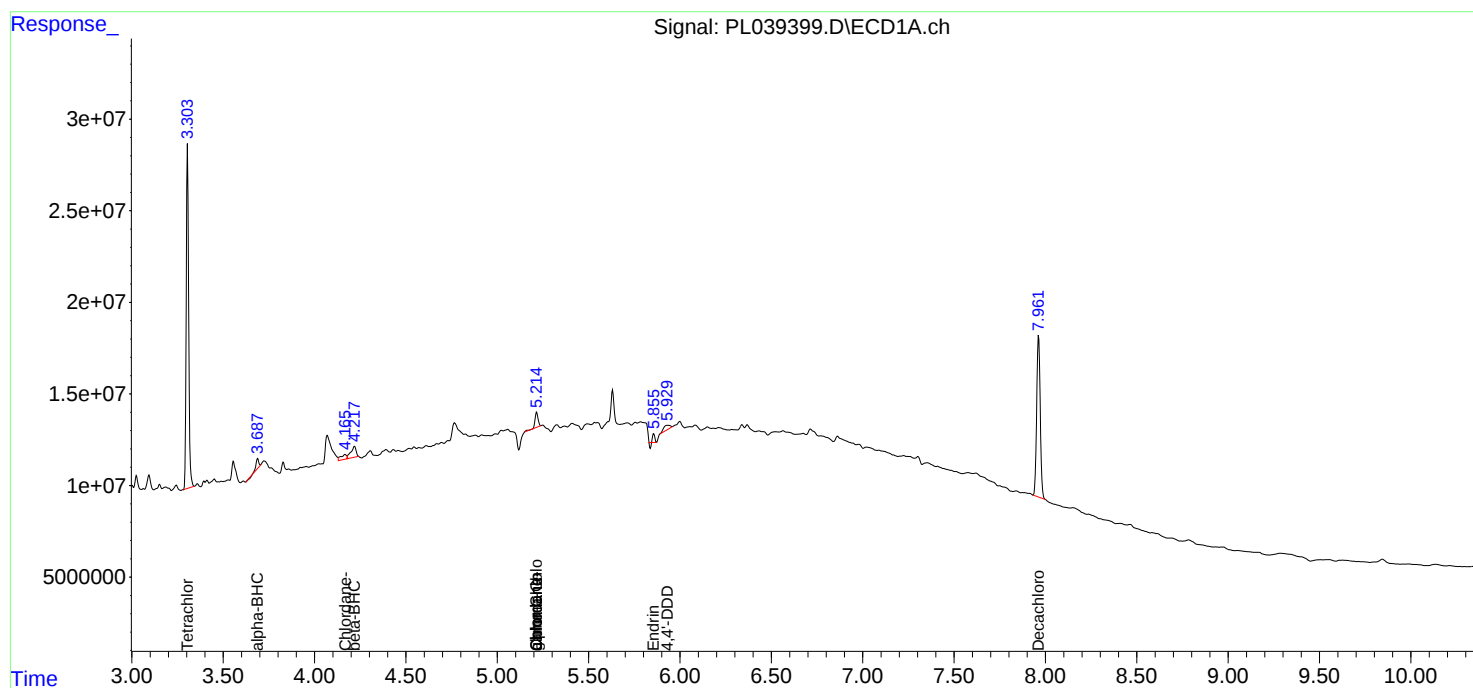


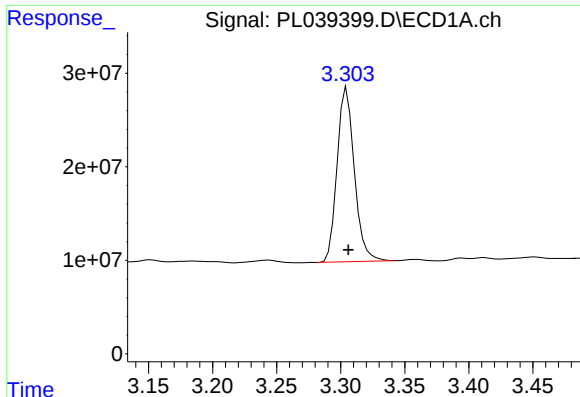

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 174492249
Conc: 24.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

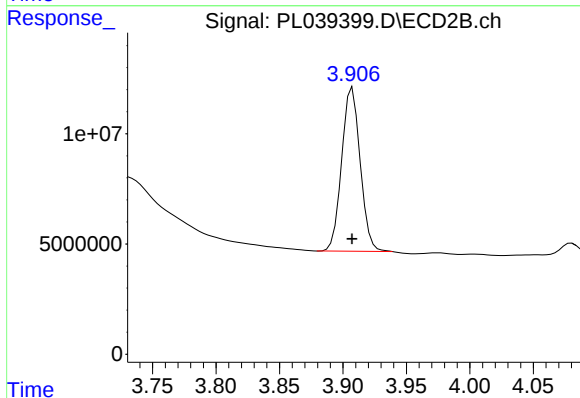


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 75195724
Conc: 28.05 ng/ml

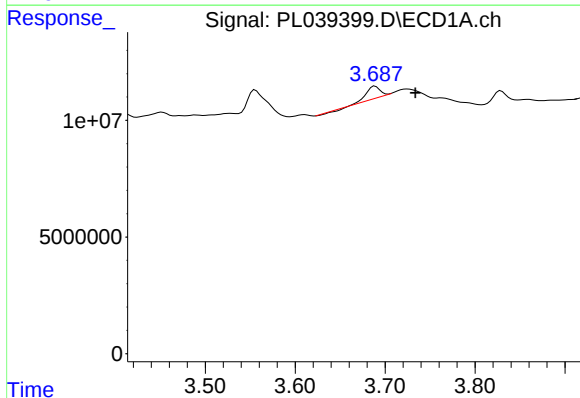


#2 alpha-BHC

R.T.: 3.689 min
Delta R.T.: -0.045 min
Response: 5539468
Conc: 0.47 ng/ml

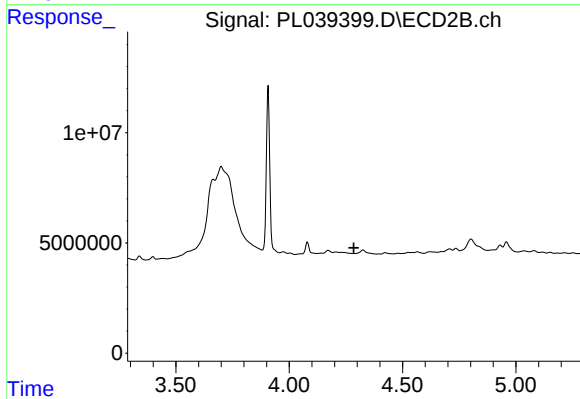

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.285 min
Response: 0
Conc: N.D.

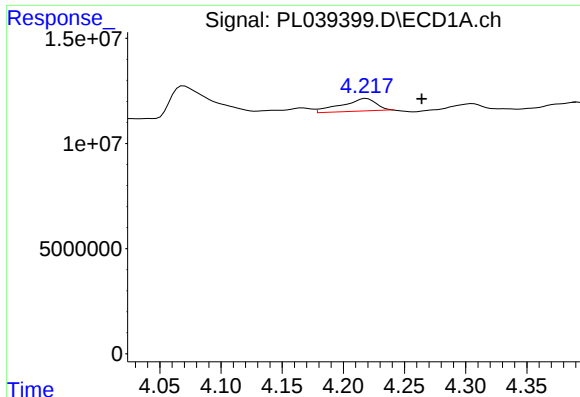

#6 beta-BHC


R.T.: 4.219 min
Delta R.T.: -0.045 min
Response: 12120703
Conc: 2.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

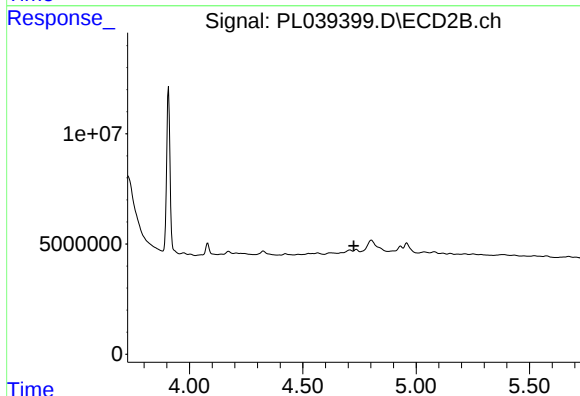


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

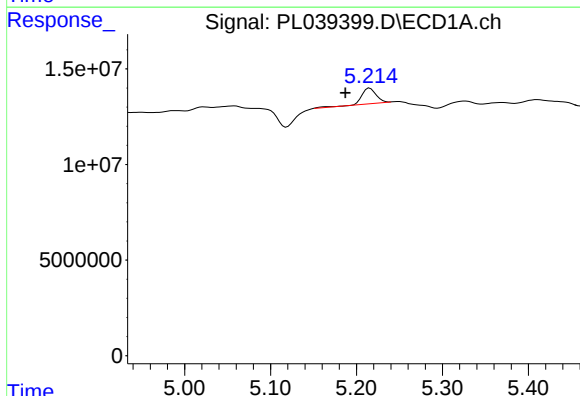


#10 gamma-Chlordane

R.T.: 5.216 min
Delta R.T.: 0.028 min
Response: 9469107
Conc: 0.96 ng/ml

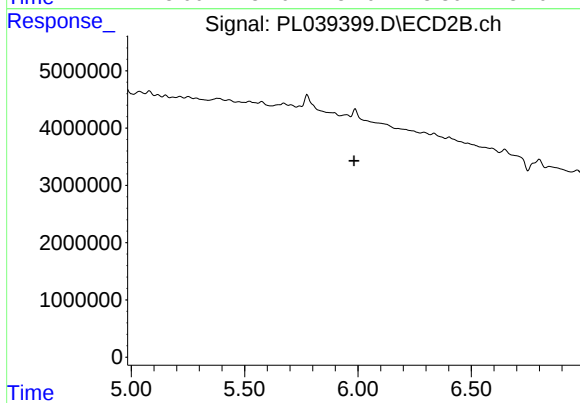

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

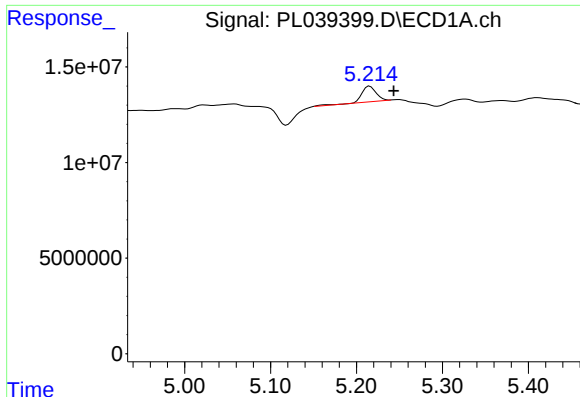

#11 alpha-Chlordane


R.T.: 5.216 min
Delta R.T.: -0.028 min
Response: 9469107
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

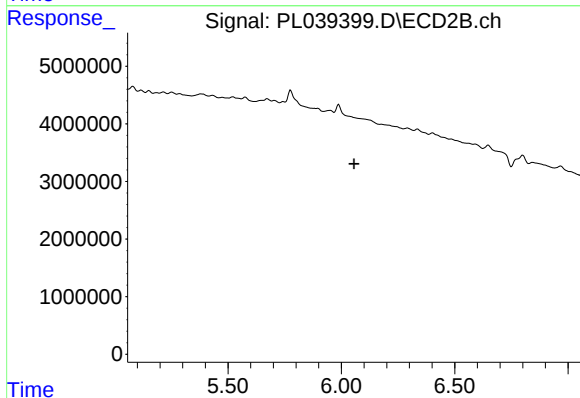


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

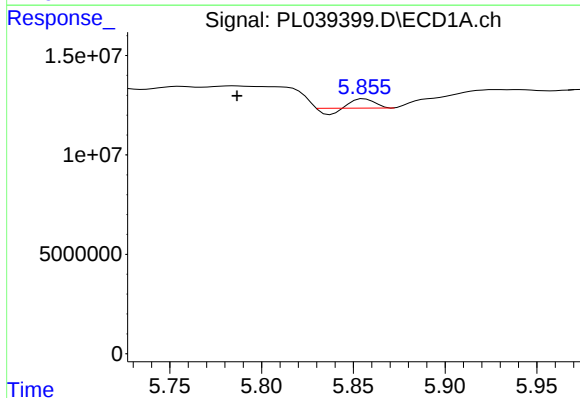


#14 Endrin

R.T.: 5.856 min
Delta R.T.: 0.070 min
Response: 3215004
Conc: 0.36 ng/ml

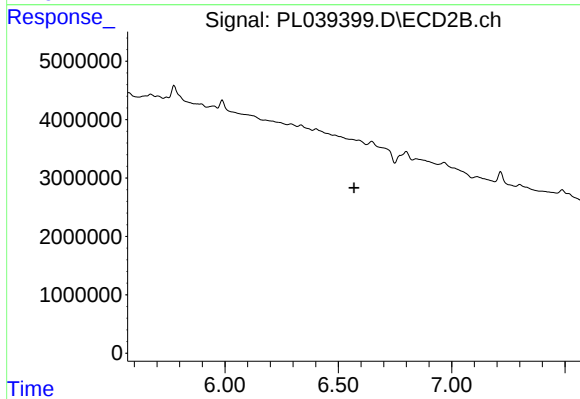

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

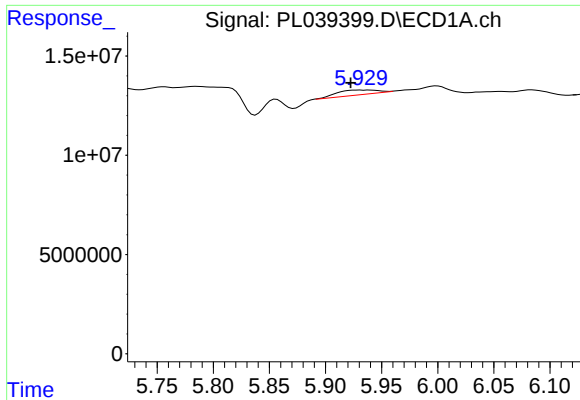

#16 4,4'-DDD


R.T.: 5.930 min
Delta R.T.: 0.008 min
Response: 6626452
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

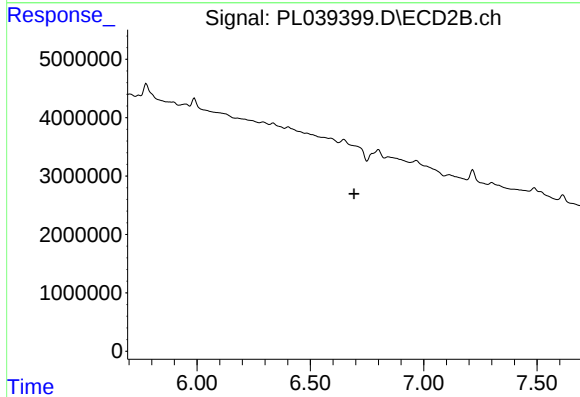


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.

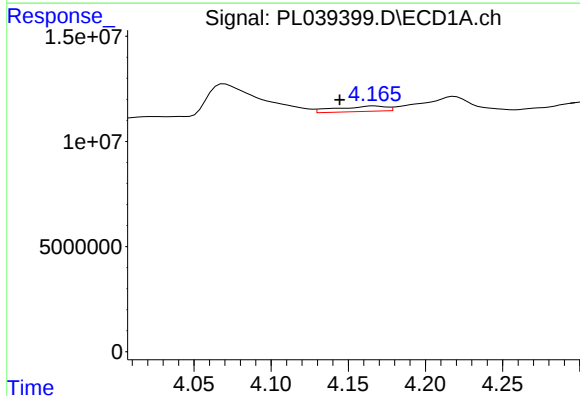


#23 Chlordane-1

R.T.: 4.167 min
Delta R.T.: 0.022 min
Response: 5793195
Conc: 18.30 ng/ml

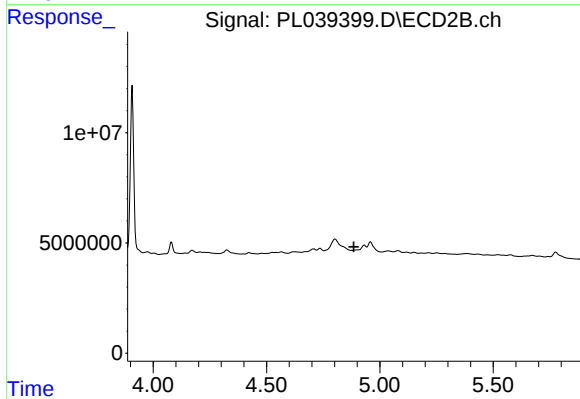

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

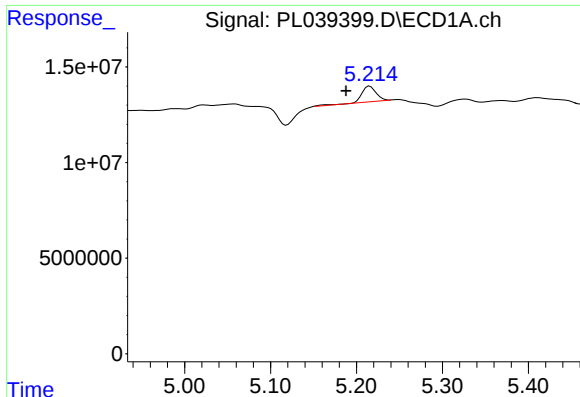

#25 Chlordane-3


R.T.: 5.216 min
Delta R.T.: 0.028 min
Response: 9469107
Conc: 8.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

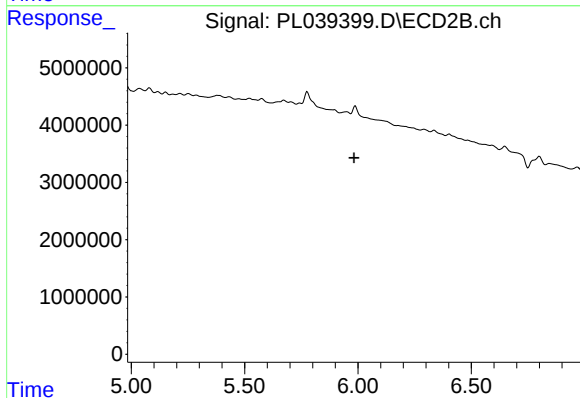


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

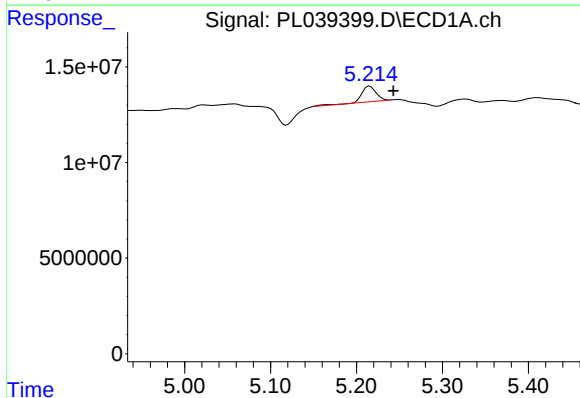


#26 Chlordane-4

R.T.: 5.216 min
Delta R.T.: -0.027 min
Response: 9469107
Conc: 9.48 ng/ml

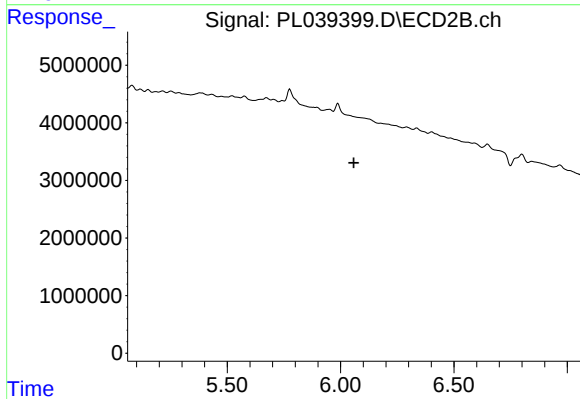

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

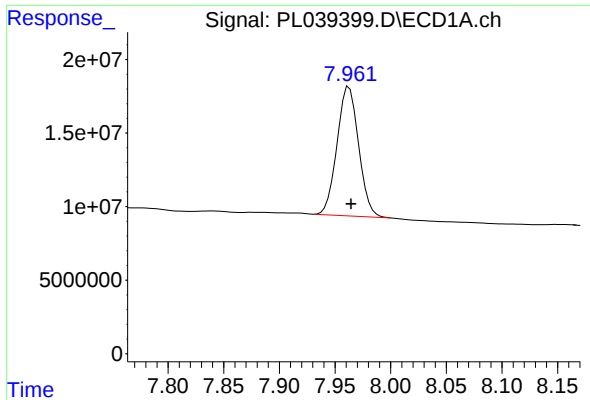

#28 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: -0.002 min
Response: 118286309
Conc: 16.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

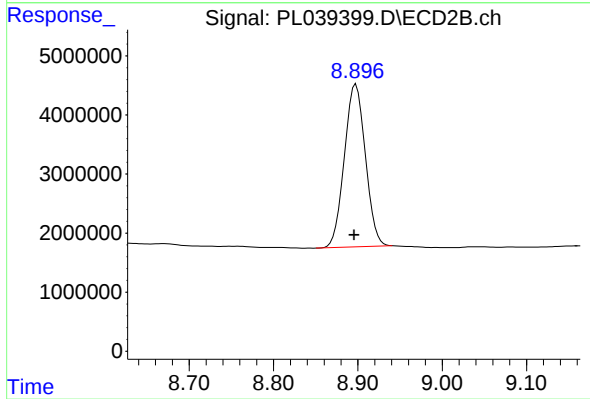

#28 Decachlorobiphenyl

R.T.: 8.898 min
Delta R.T.: 0.002 min
Response: 47774596
Conc: 20.59 ng/ml