

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 05:09
 Operator : AJ\SJ
 Sample : J4556-09
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 05:35:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.908	90452700	40330374	12.940	15.044
28)	SA Decachlor...	7.962	8.897	57464146	24224999	8.182	10.439 #
Target Compounds							
4)	MA Heptachlor	4.305	0.000	17804904	0	1.691	N.D. #
5)	MB Aldrin	4.543	0.000	4229352	0	0.422	N.D. #
6)	B beta-BHC	4.305f	0.000	17804904	0	3.833	N.D. #
8)	B Heptachlo...	5.022f	0.000	6639511	0	0.695	N.D. #
10)	B gamma-Chl...	5.211	0.000	4009031	0	0.406	N.D. #
11)	B alpha-Chl...	5.211	0.000	4009031	0	0.417	N.D. #
12)	B 4,4'-DDE	5.410	0.000	5563102	0	0.581	N.D. #
13)	MA Dieldrin	5.533	0.000	10295111	0	1.056	N.D. #
24)	Chlordane-2	4.695	0.000	2997883	0	8.575	N.D. #
25)	Chlordane-3	5.211	0.000	4009031	0	3.670	N.D. #
26)	Chlordane-4	5.211	0.000	4009031	0	4.012	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 05:09
Operator : AJ\SJ
Sample : J4556-09
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 05:35:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

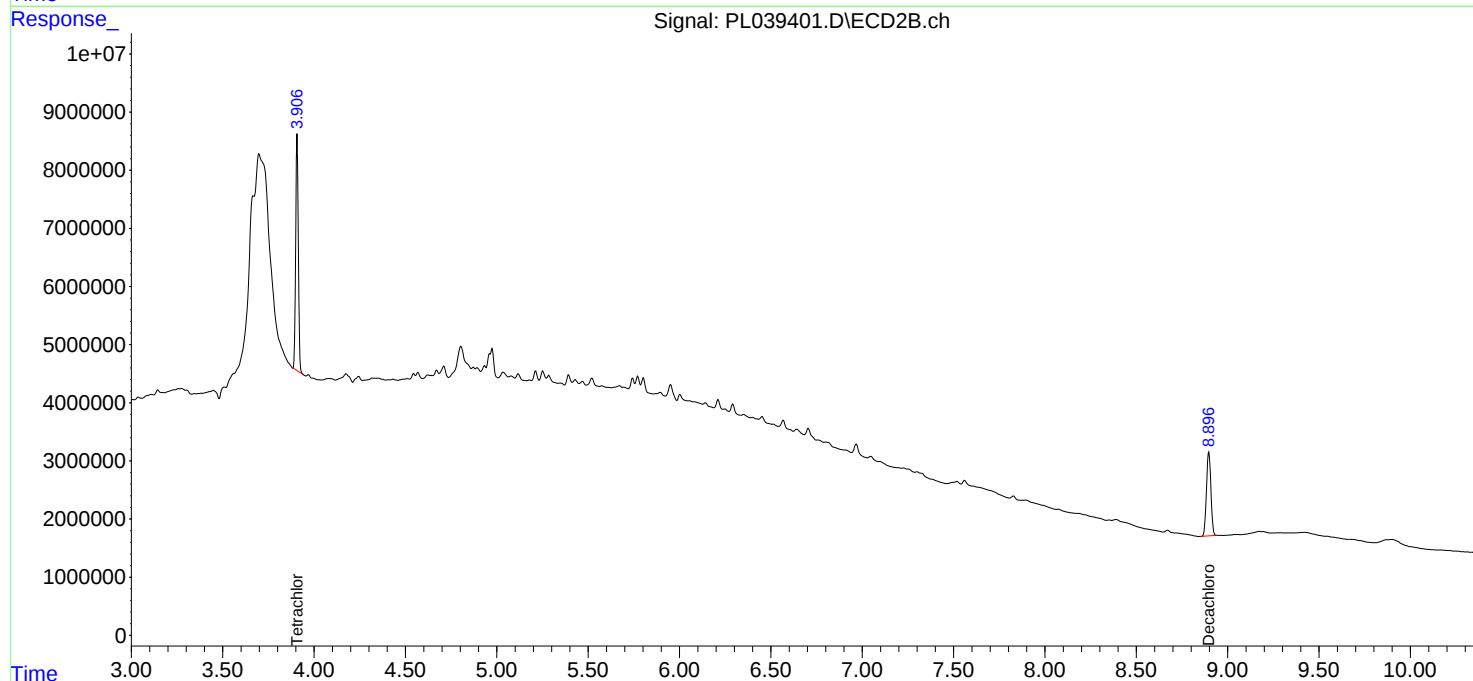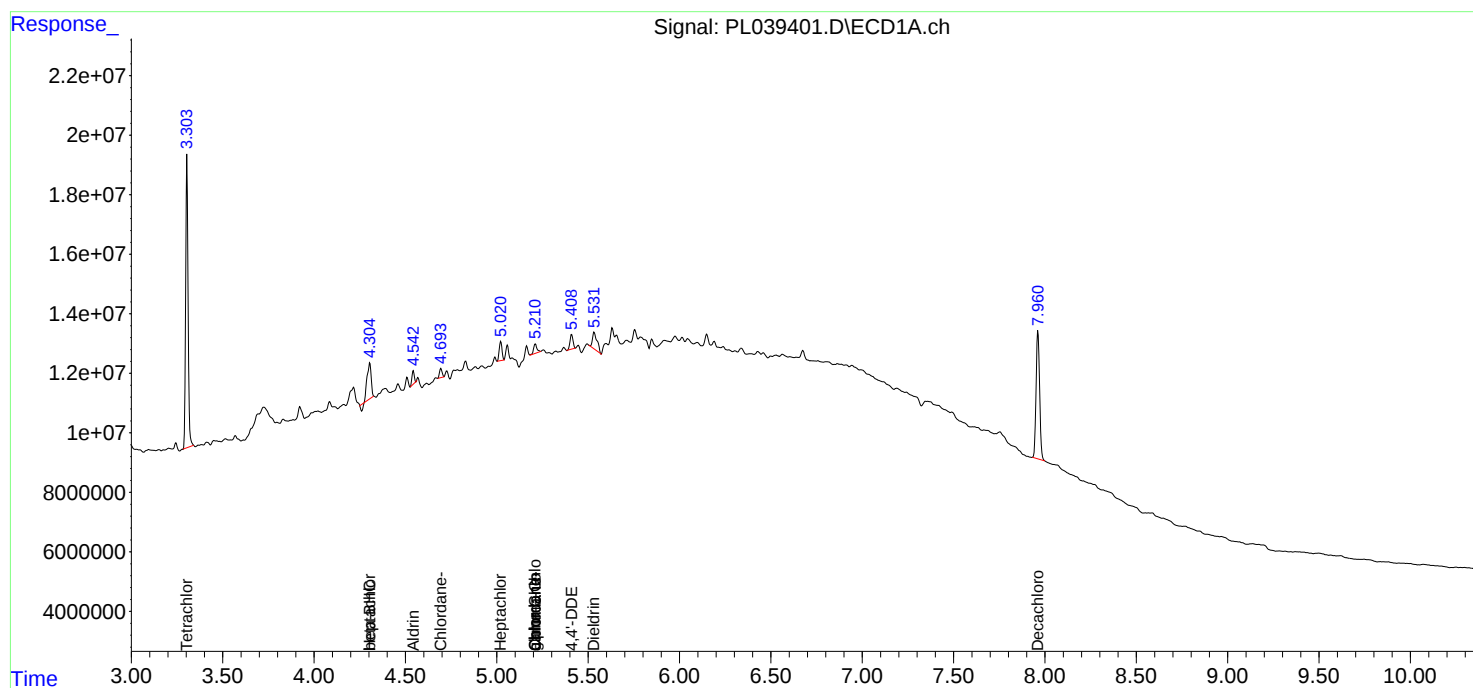


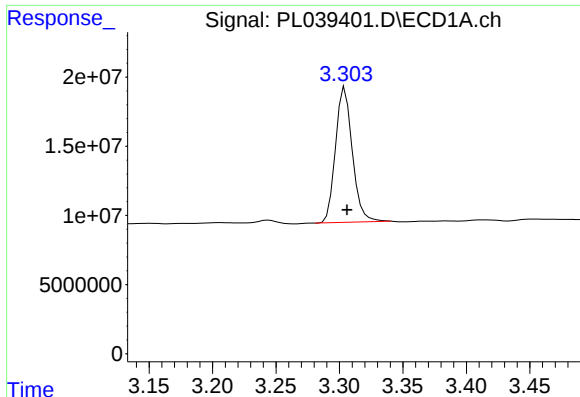

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 90452700
Conc: 12.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

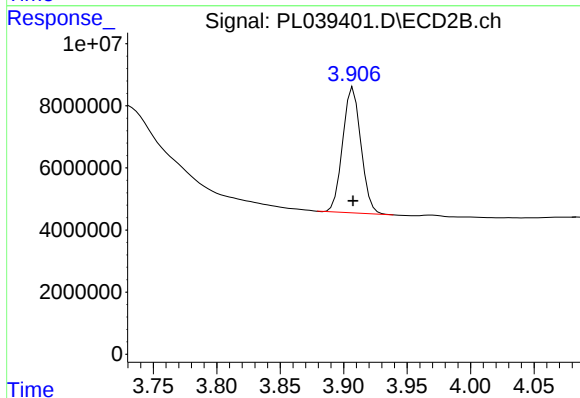


#1 Tetrachloro-m-xylene

R.T.: 3.908 min
Delta R.T.: 0.000 min
Response: 40330374
Conc: 15.04 ng/ml

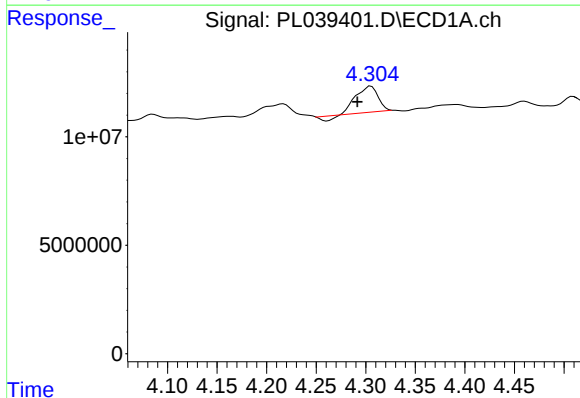


#4 Heptachlor

R.T.: 4.305 min
Delta R.T.: 0.014 min
Response: 17804904
Conc: 1.69 ng/ml

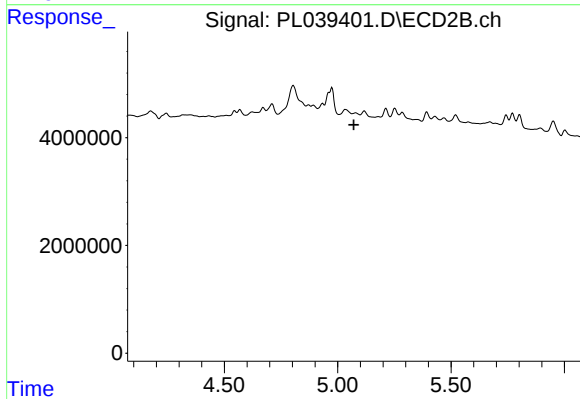

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.071 min
Response: 0
Conc: N.D.

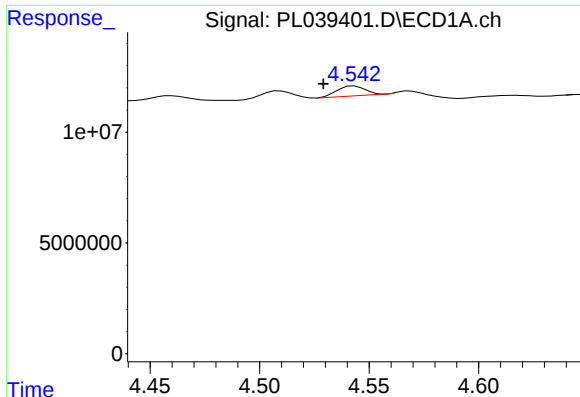

#5 Aldrin


R.T.: 4.543 min
Delta R.T.: 0.014 min
Response: 4229352
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

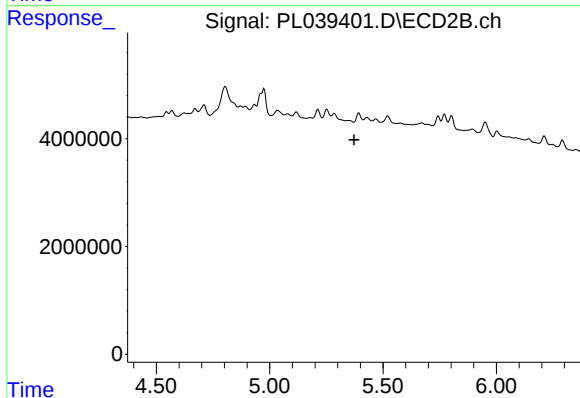


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.372 min
Response: 0
Conc: N.D.

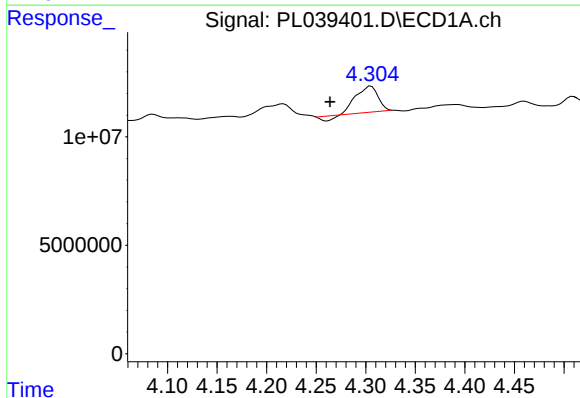


#6 beta-BHC

R.T.: 4.305 min
Delta R.T.: 0.041 min
Response: 17804904
Conc: 3.83 ng/ml

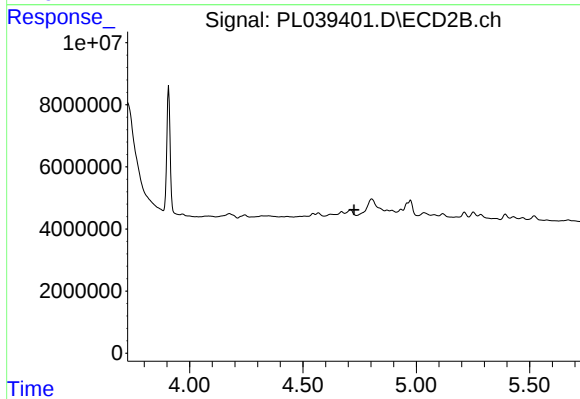

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

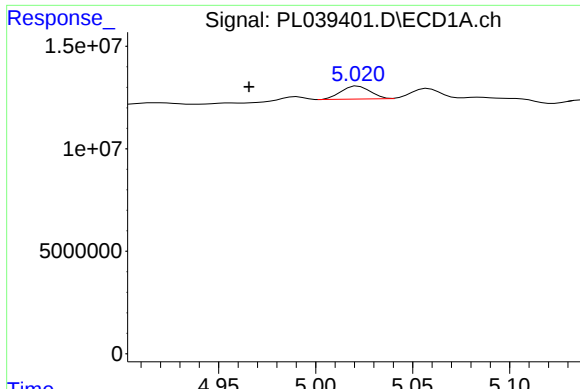

#8 Heptachlor epoxide


R.T.: 5.022 min
Delta R.T.: 0.056 min
Response: 6639511
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

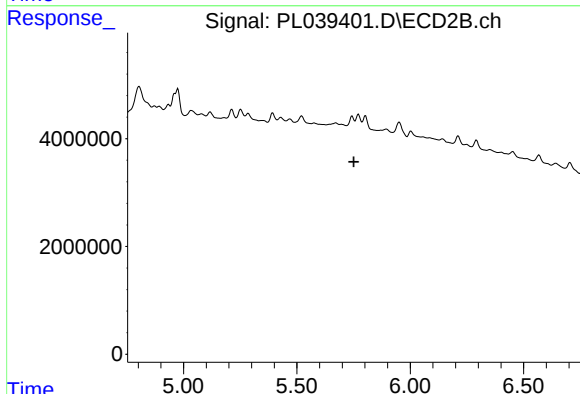


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

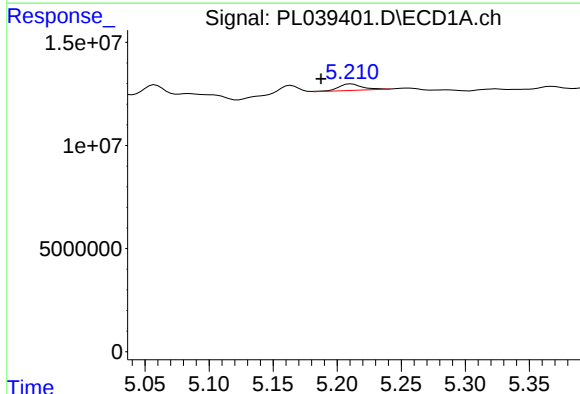


#10 gamma-Chlordane

R.T.: 5.211 min
Delta R.T.: 0.024 min
Response: 4009031
Conc: 0.41 ng/ml

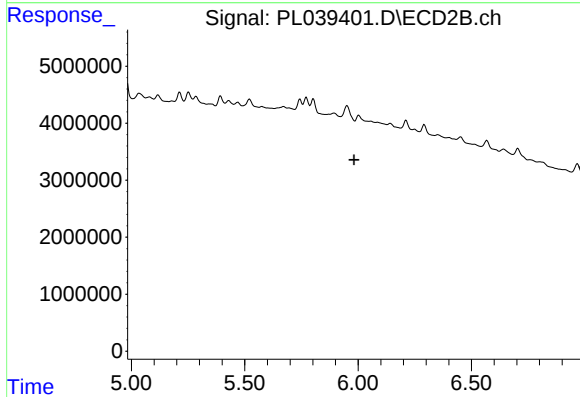

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

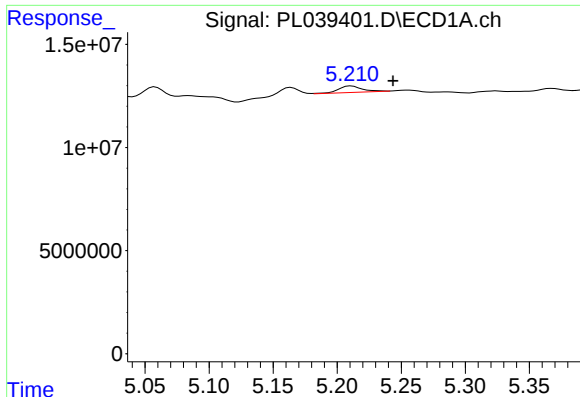

#11 alpha-Chlordane


R.T.: 5.211 min
Delta R.T.: -0.032 min
Response: 4009031
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

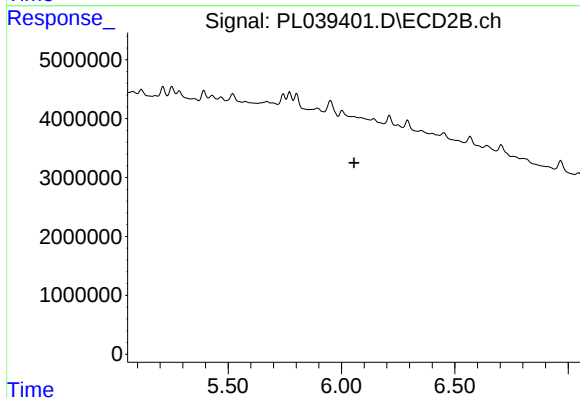


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

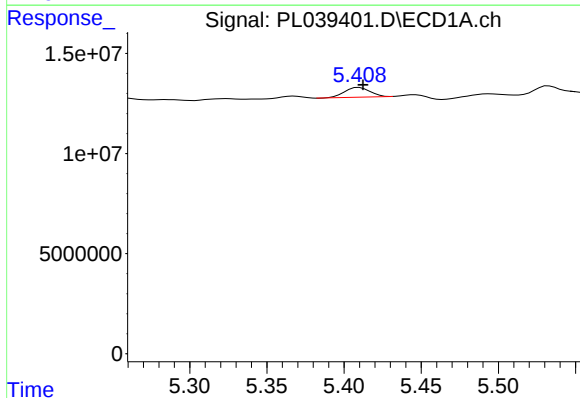


#12 4,4'-DDE

R.T.: 5.410 min
Delta R.T.: -0.003 min
Response: 5563102
Conc: 0.58 ng/ml

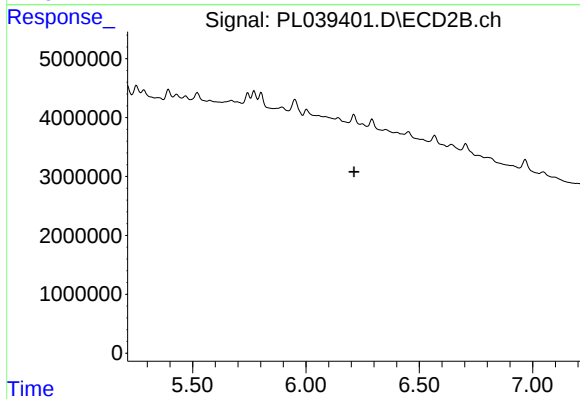

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

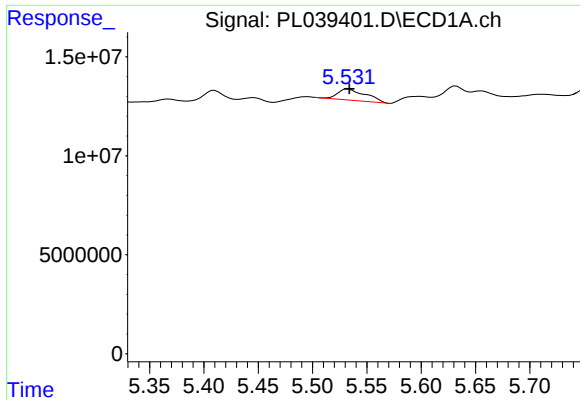

#13 Dieldrin


R.T.: 5.533 min
Delta R.T.: -0.001 min
Response: 10295111
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

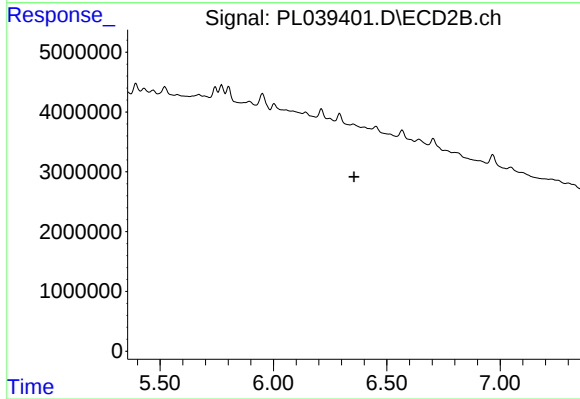


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

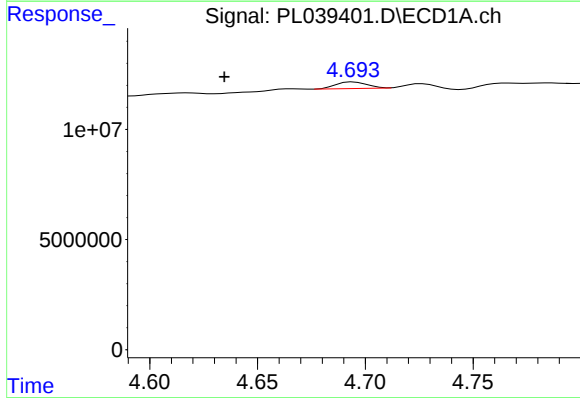


#24 Chlordane-2

R.T.: 4.695 min
Delta R.T.: 0.060 min
Response: 2997883
Conc: 8.58 ng/ml

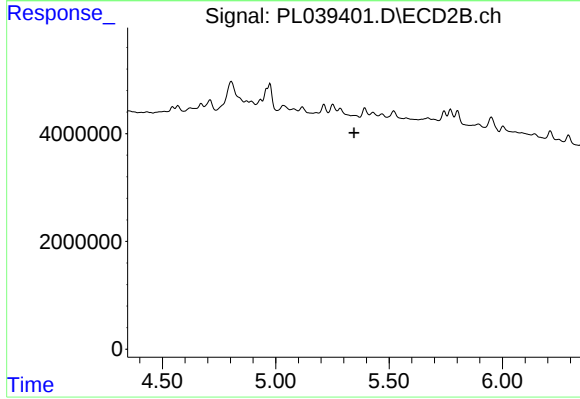

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

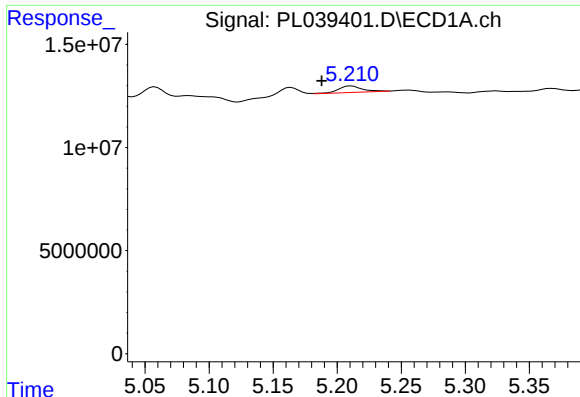

#25 Chlordane-3


R.T.: 5.211 min
Delta R.T.: 0.023 min
Response: 4009031
Conc: 3.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

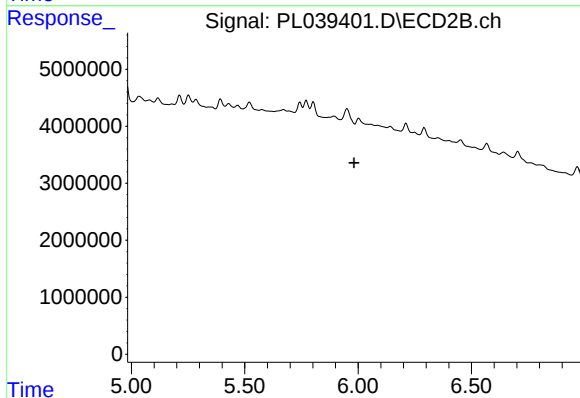


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

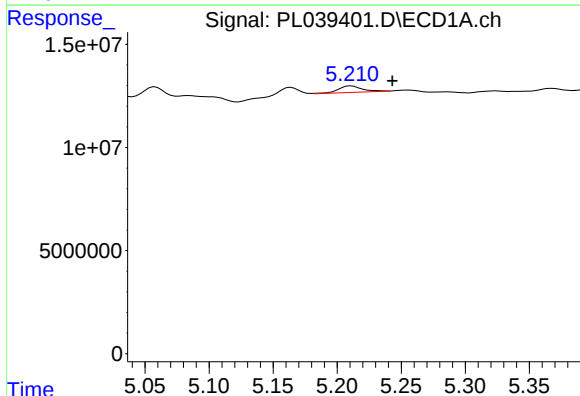


#26 Chlordane-4

R.T.: 5.211 min
Delta R.T.: -0.032 min
Response: 4009031
Conc: 4.01 ng/ml

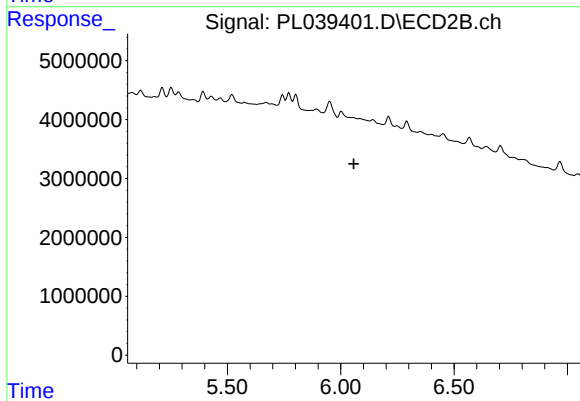

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

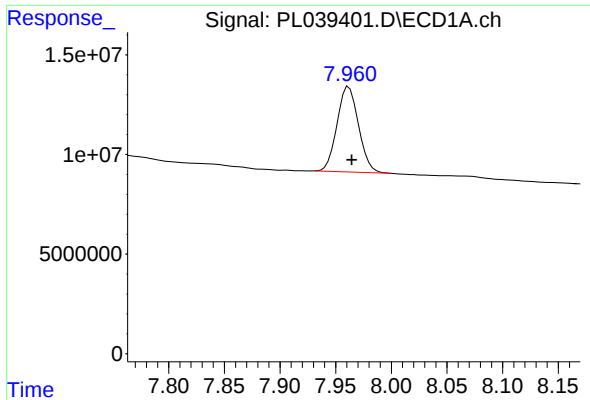

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 57464146
Conc: 8.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

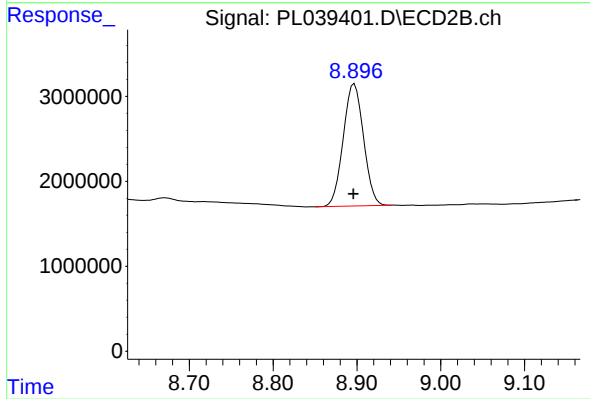

#28 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: 0.001 min
Response: 24224999
Conc: 10.44 ng/ml