

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2018 23:57
 Operator : AJ\SJ
 Sample : J4539-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MS-BASELINE-WATER

Manual Integrations
 APPROVED

Sohil
 8/22/2018 11:45:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 01:02:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.906	127.8E6	55351280	18.282	20.647m
28)	SA Decachlor...	7.960	8.896	125.1E6	47243755	17.819m	20.358

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2018 23:57
Operator : AJ\SJ
Sample : J4539-06
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MS-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
8/22/2018 11:45:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 01:02:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

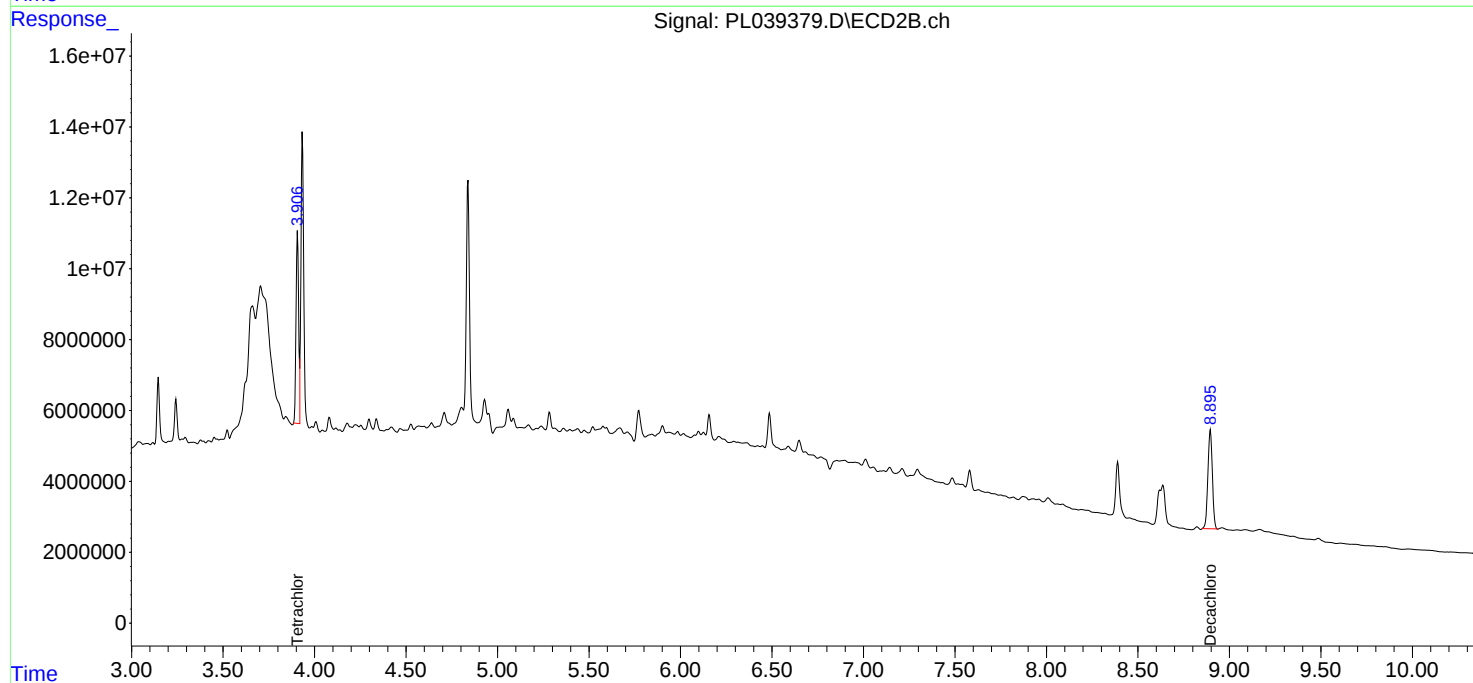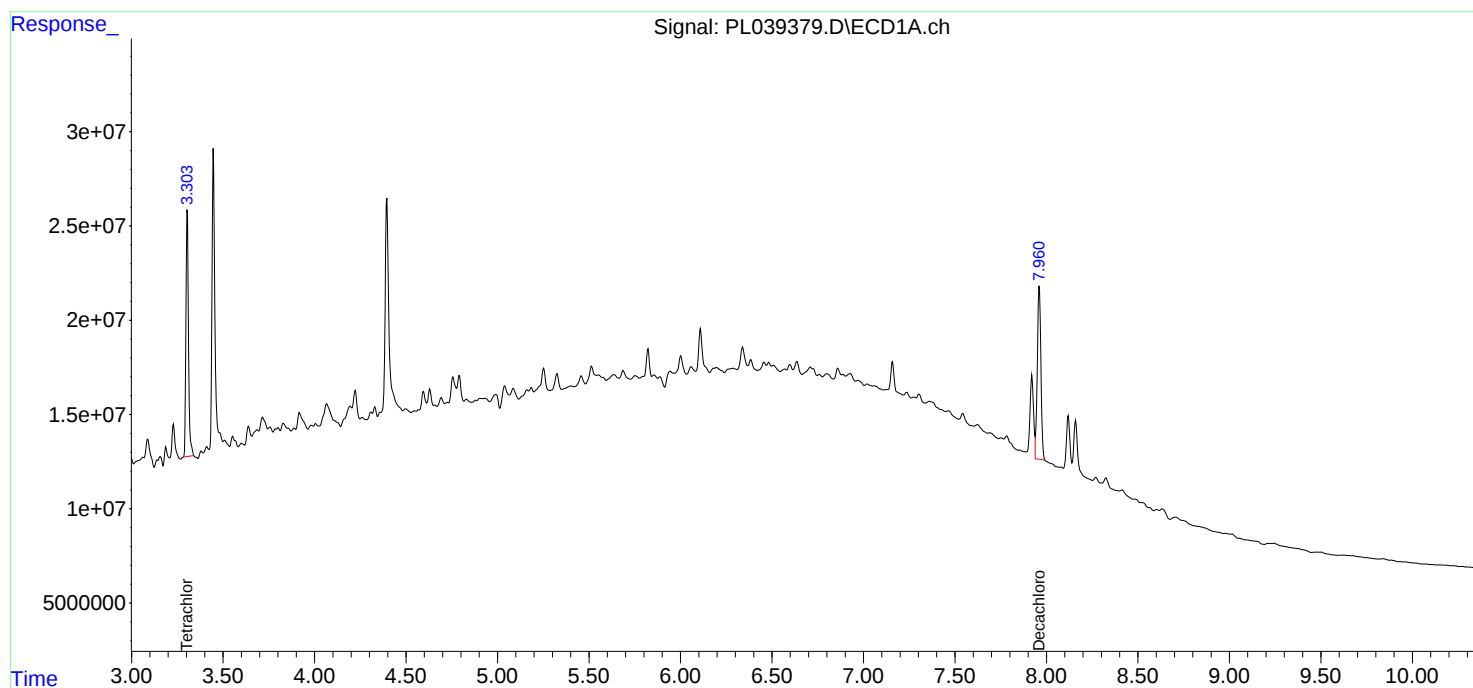

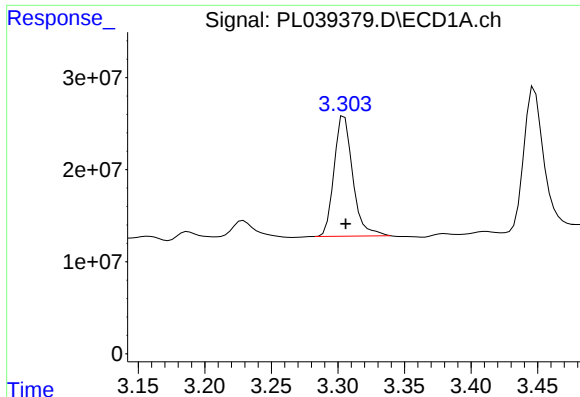


#1 Tetrachloro-m-xylene

R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 127796795
Conc: 18.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
MS-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
8/22/2018 11:45:46 AM

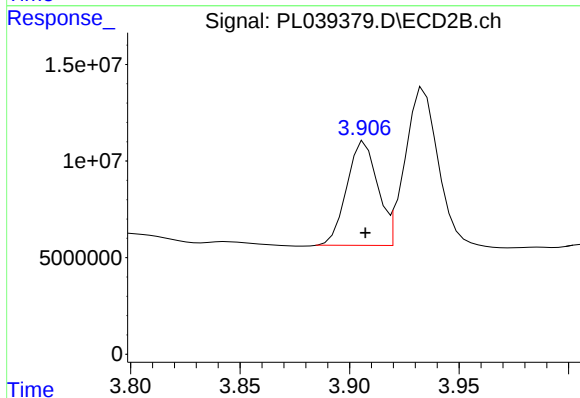


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.002 min
Response: 55351280
Conc: 20.65 ng/ml m

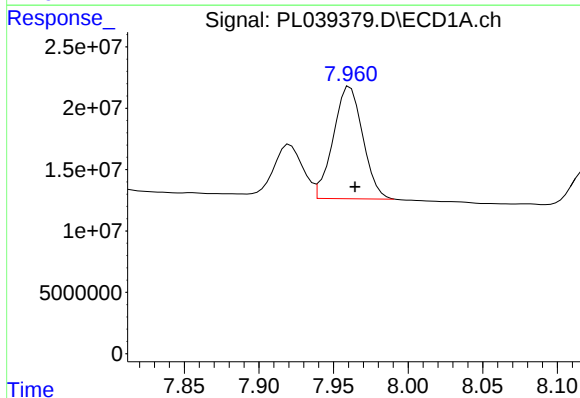

#28 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.005 min
Response: 125148415
Conc: 17.82 ng/ml m

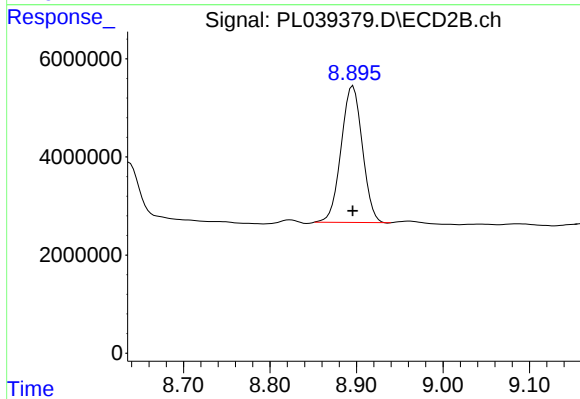

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 47243755
Conc: 20.36 ng/ml