

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
 Data File : PL039409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 07:03
 Operator : AJ\SJ
 Sample : J4545-01 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RB-BASELINE-WATER

Manual Integrations
 APPROVED

Sohil
 8/22/2018 11:46:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 07:18:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.310	3.909	19255142	6831318	2.755m	2.548m
28)	SA Decachlor...	7.964	8.896	10801256	4606144	1.538	1.985m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082118\
Data File : PL039409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 07:03
Operator : AJ\SJ
Sample : J4545-01 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RB-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
8/22/2018 11:46:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 07:18:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

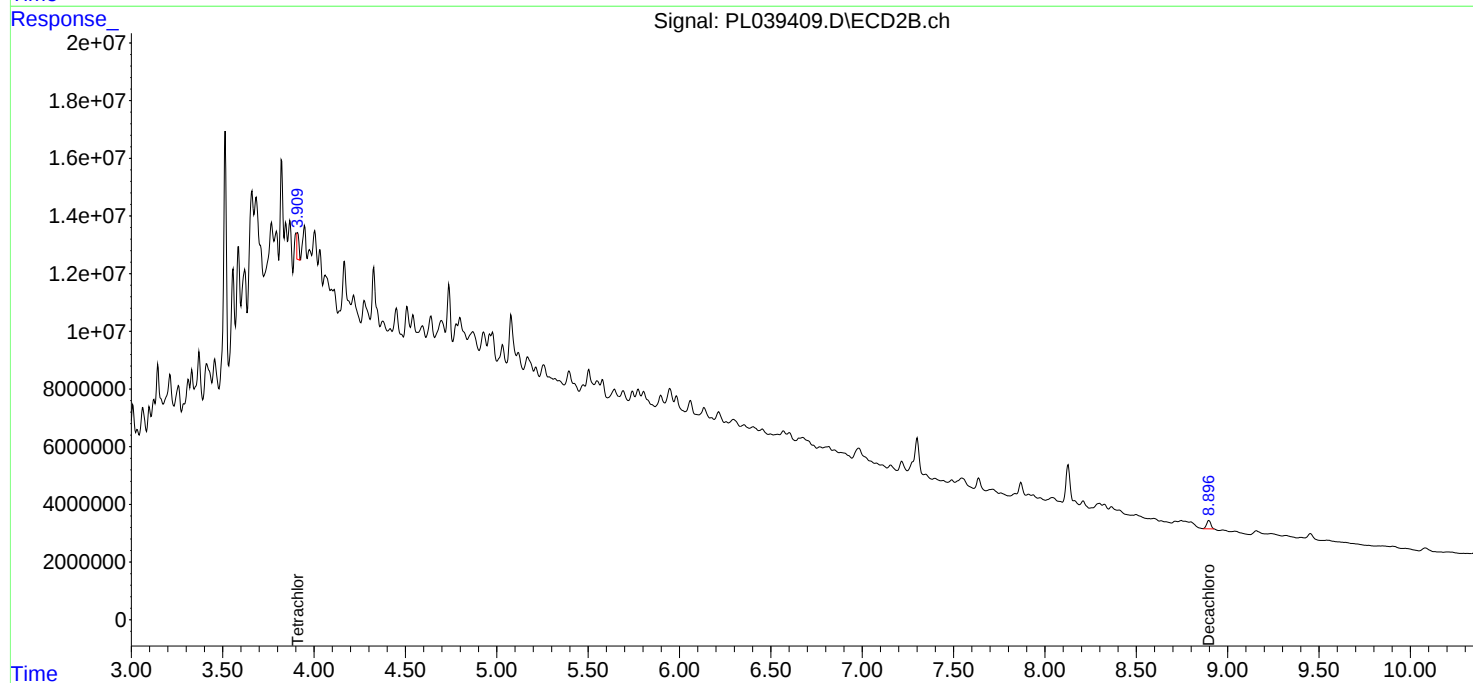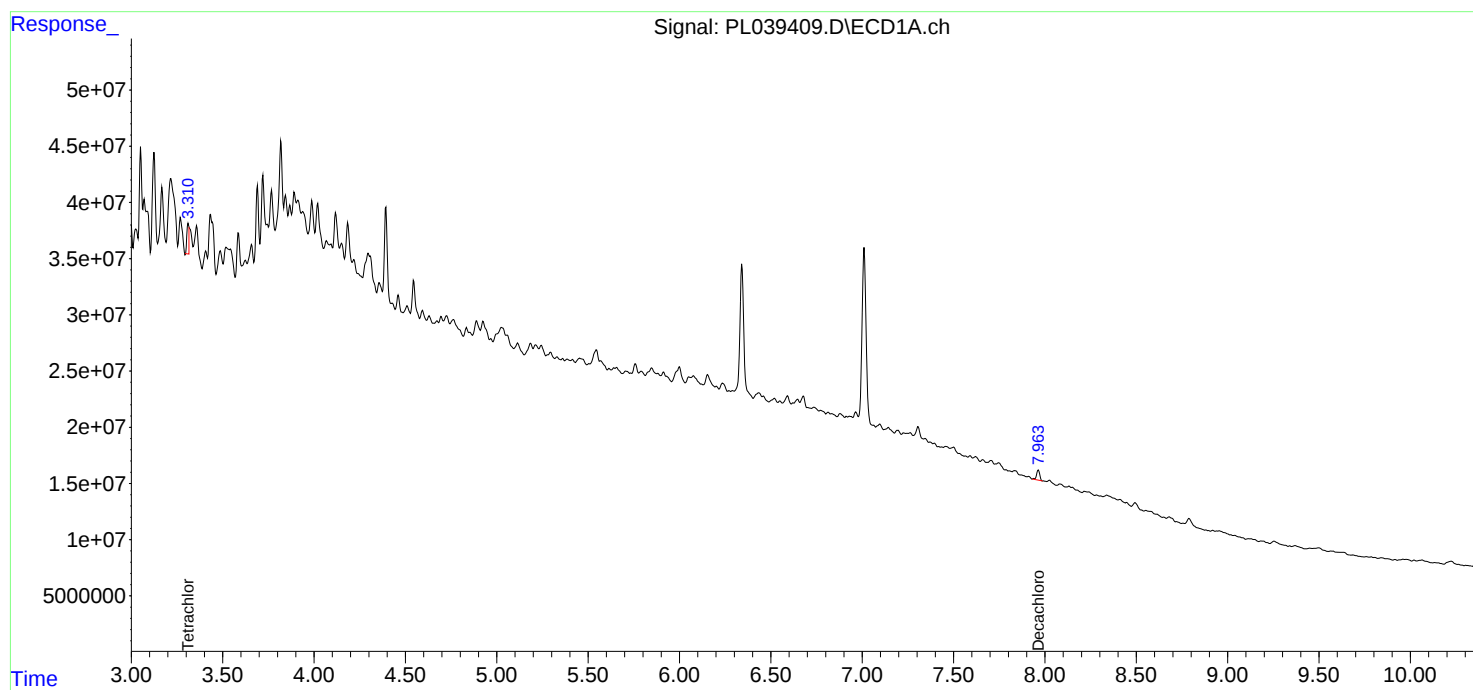

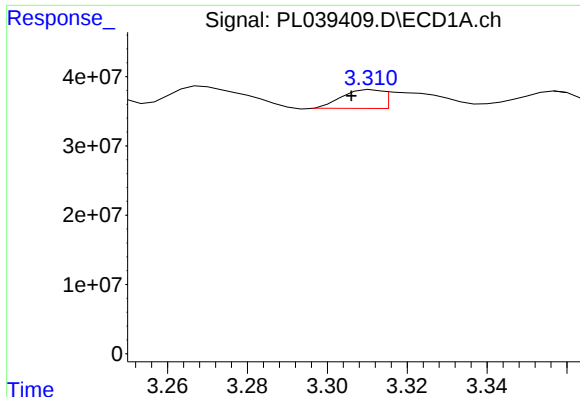


#1 Tetrachloro-m-xylene

R.T.: 3.310 min
Delta R.T.: 0.004 min
Response: 19255142
Conc: 2.75 ng/ml m

Instrument :
ECD_L
ClientSampleId :
RB-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
8/22/2018 11:46:33 AM

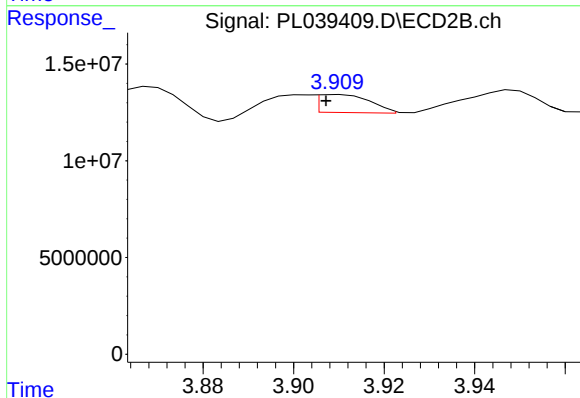


#1 Tetrachloro-m-xylene

R.T.: 3.909 min
Delta R.T.: 0.002 min
Response: 6831318
Conc: 2.55 ng/ml m

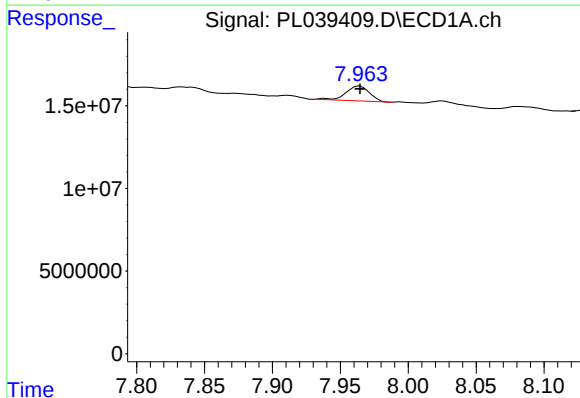

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 10801256
Conc: 1.54 ng/ml

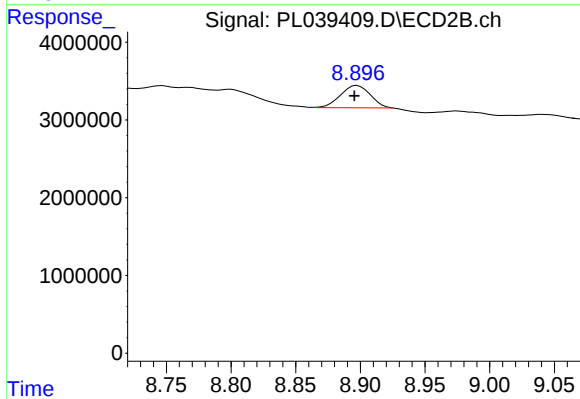

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 4606144
Conc: 1.98 ng/ml m