

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082120\
 Data File : PL060895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2020 12:06
 Operator : DD\AJ
 Sample : L3729-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1-(0-1)

Manual Integrations
 APPROVED

Ankita
 8/24/2020 11:26:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 01:08:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 06:13:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	36342265	50050929	21.769	17.993
28)	SA Decachlor...	8.214	9.097	35816032	41413849	25.074m	20.490
Target Compounds							
14)	MA Endrin	6.017	6.714	8342753	2814397	5.514m	1.083m#
17)	MA 4,4'-DDT	6.379	7.145	6656843	5372560	5.551	2.476 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082120\
Data File : PL060895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2020 12:06
Operator : DD\AJ
Sample : L3729-14
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-1-(0-1)


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 01:08:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 06:13:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

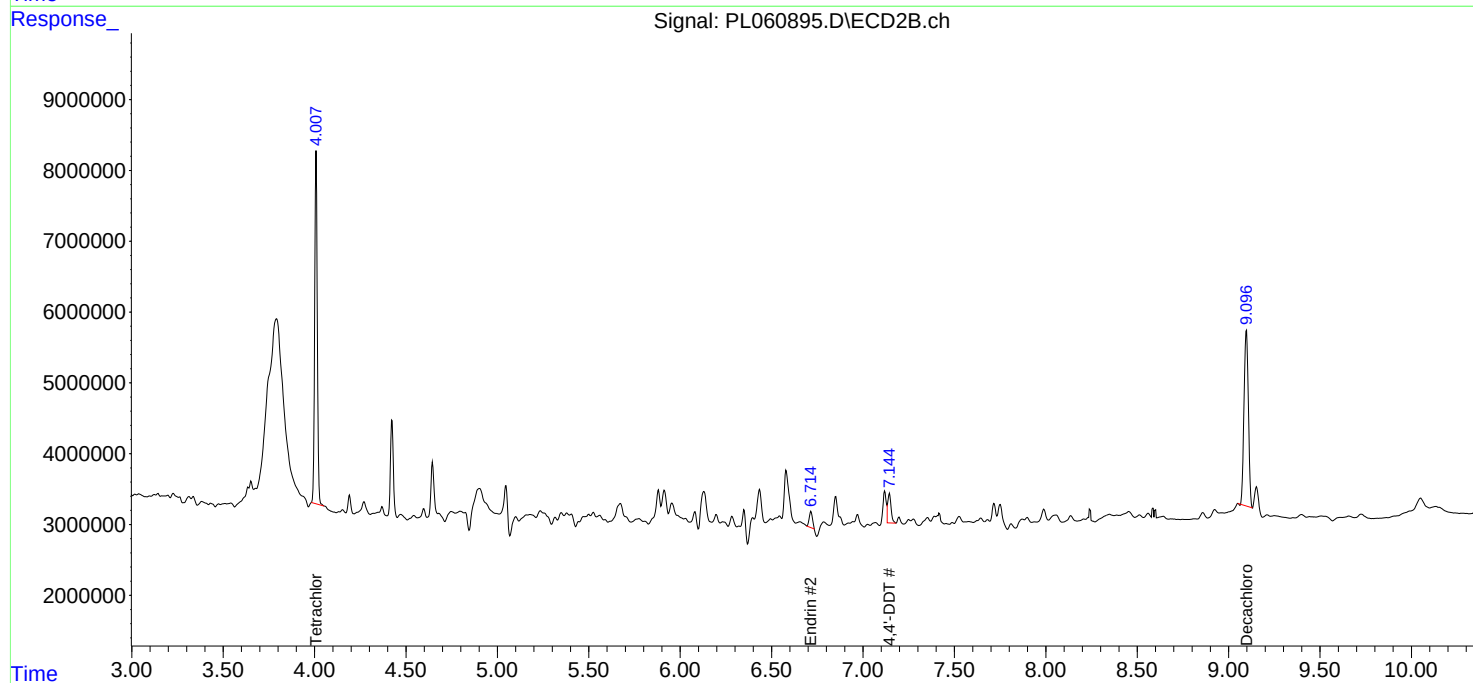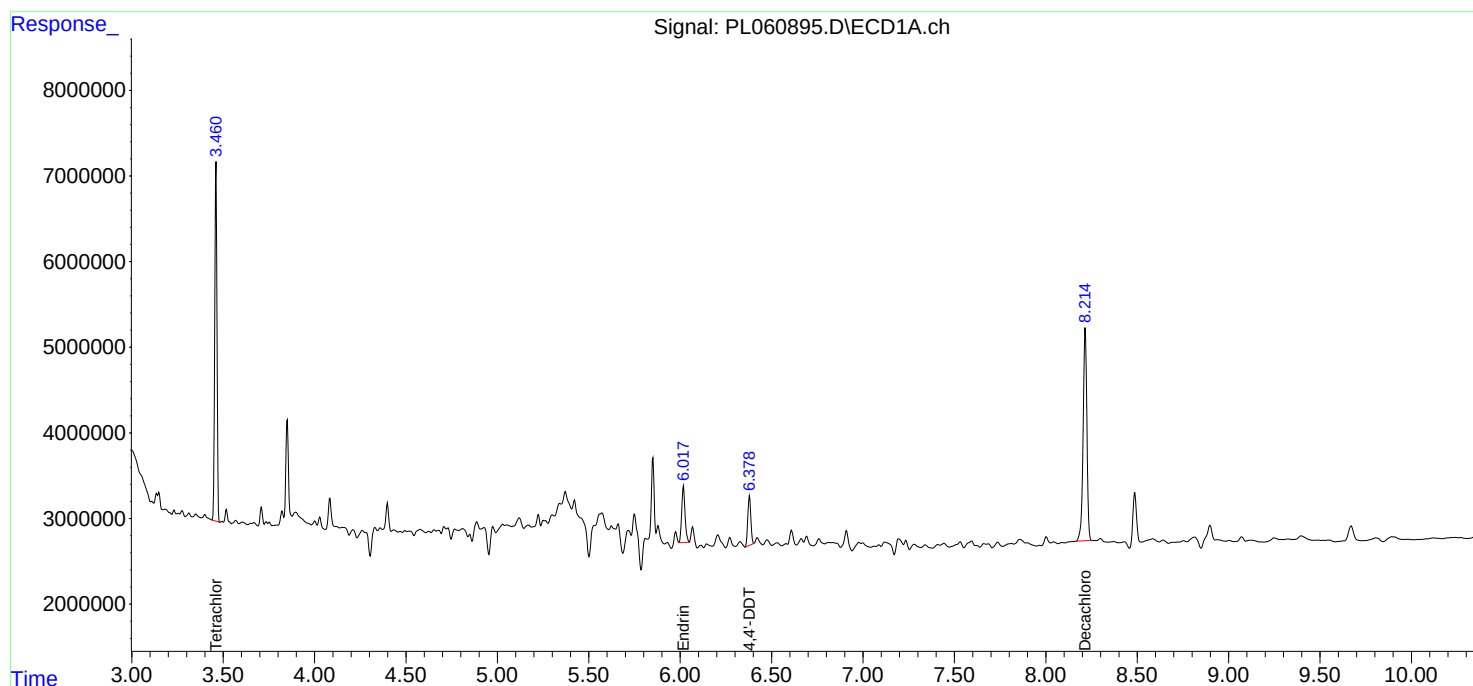

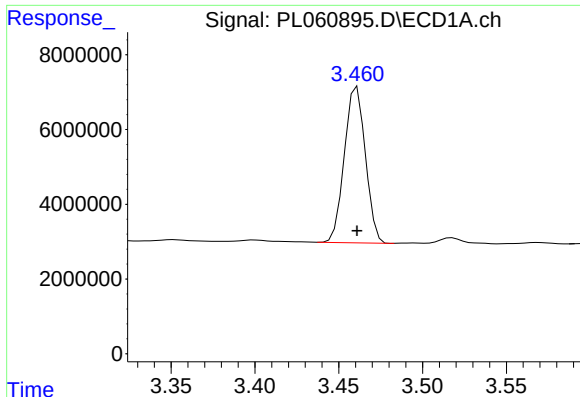


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 36342265
Conc: 21.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1-(0-1)


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:17 AM

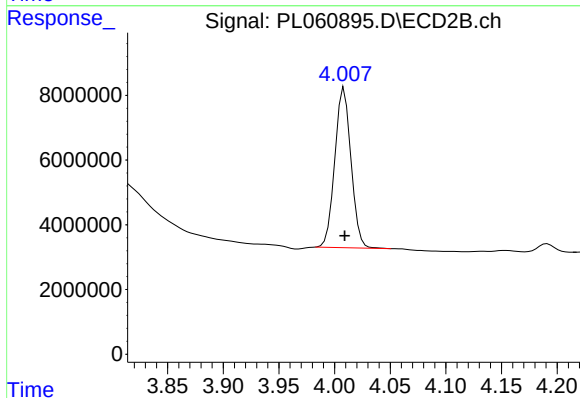


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 50050929
Conc: 17.99 ng/ml

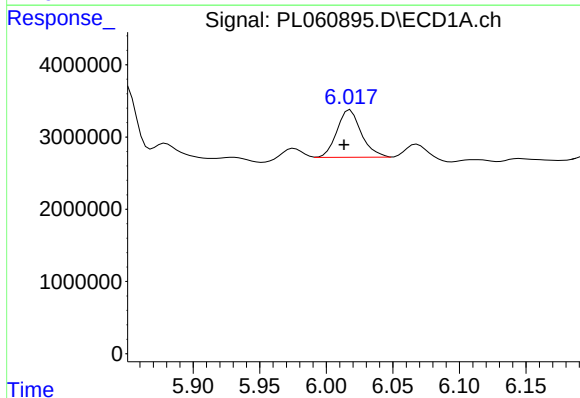


#14 Endrin

R.T.: 6.017 min
Delta R.T.: 0.003 min
Response: 8342753
Conc: 5.51 ng/ml m

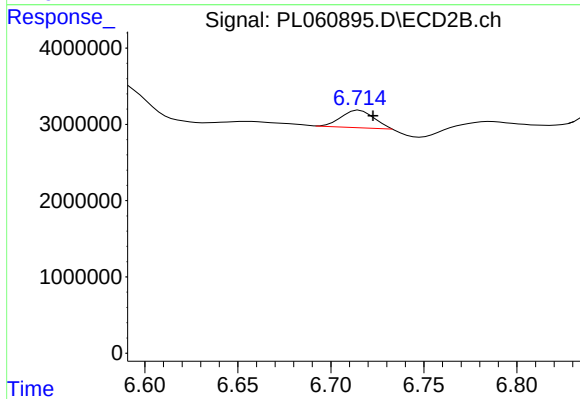

#14 Endrin

R.T.: 6.714 min
Delta R.T.: -0.009 min
Response: 2814397
Conc: 1.08 ng/ml m

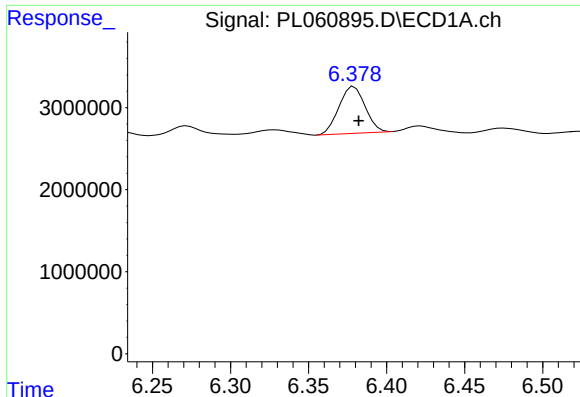


#17 4,4'-DDT

R.T.: 6.379 min
Delta R.T.: -0.003 min
Response: 6656843
Conc: 5.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1-(0-1)


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:17 AM

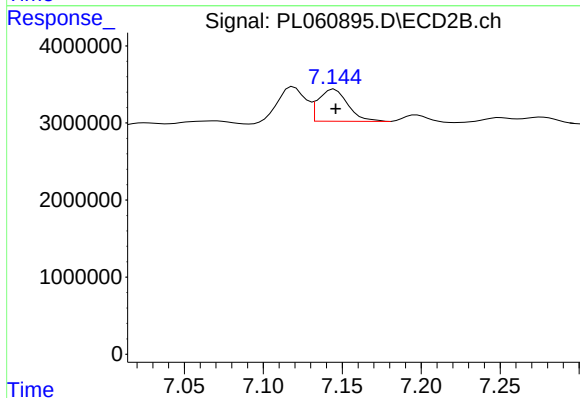


#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 5372560
Conc: 2.48 ng/ml

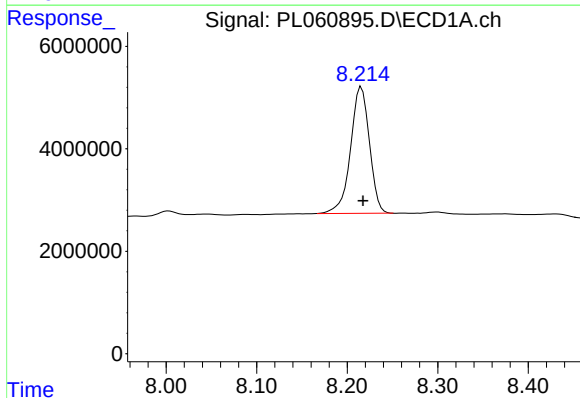

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.003 min
Response: 35816032
Conc: 25.07 ng/ml m

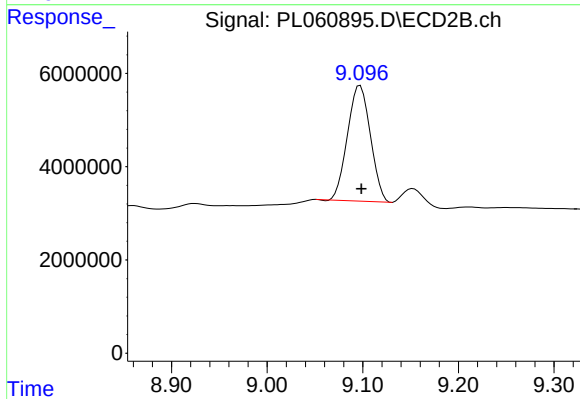

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.001 min
Response: 41413849
Conc: 20.49 ng/ml