

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082120\
 Data File : PL060896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2020 12:20
 Operator : DD\AJ
 Sample : L3729-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-2-(1-2)

Manual Integrations
 APPROVED

Ankita
 8/24/2020 11:26:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 01:08:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 06:13:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.009	23673366	32694470	14.181	11.753
28)	SA Decachlor...	8.215	9.096	25003401	32004786	17.504m	15.835m
Target Compounds							
14)	MA Endrin	6.013	6.715	3348308	3637255	2.213m	1.400 #
17)	MA 4,4'-DDT	6.376	7.143	4702261	2101800	3.921m	0.968m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082120\
Data File : PL060896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2020 12:20
Operator : DD\AJ
Sample : L3729-15
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-2-(1-2)


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 01:08:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 06:13:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

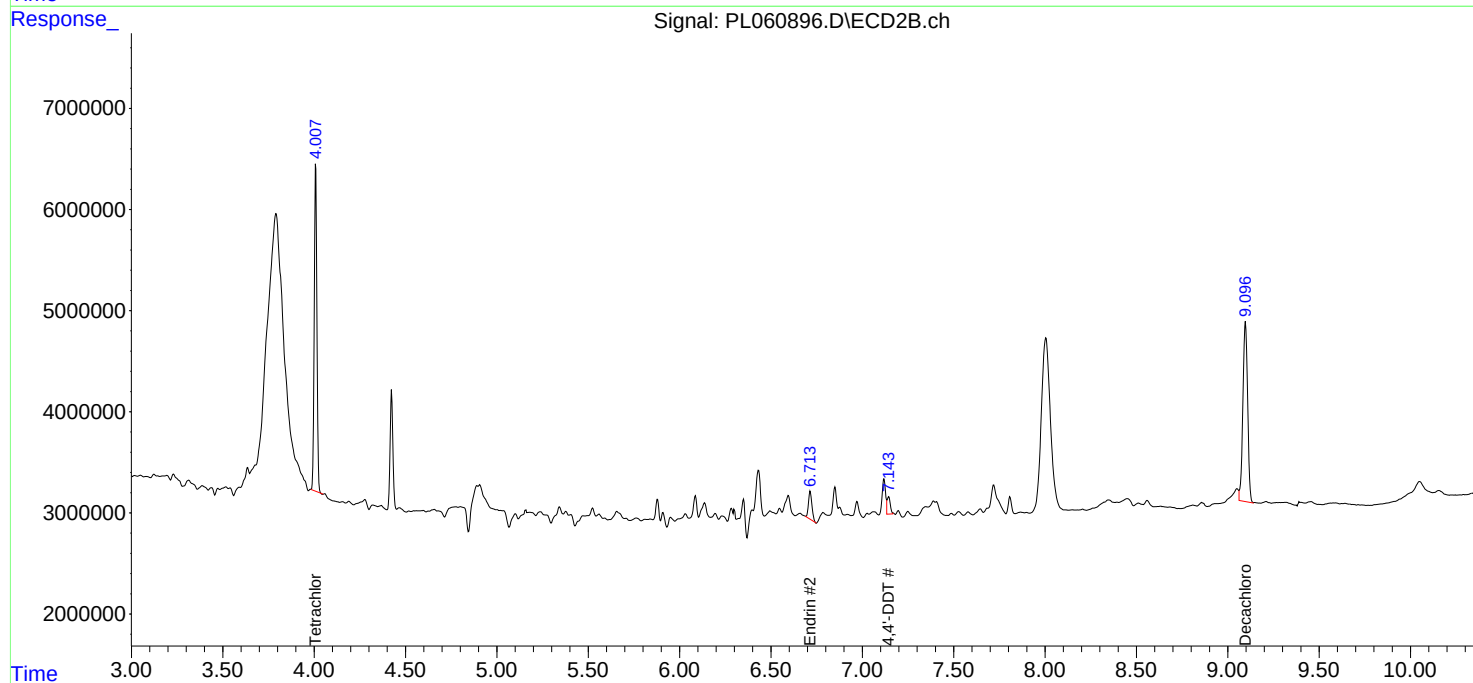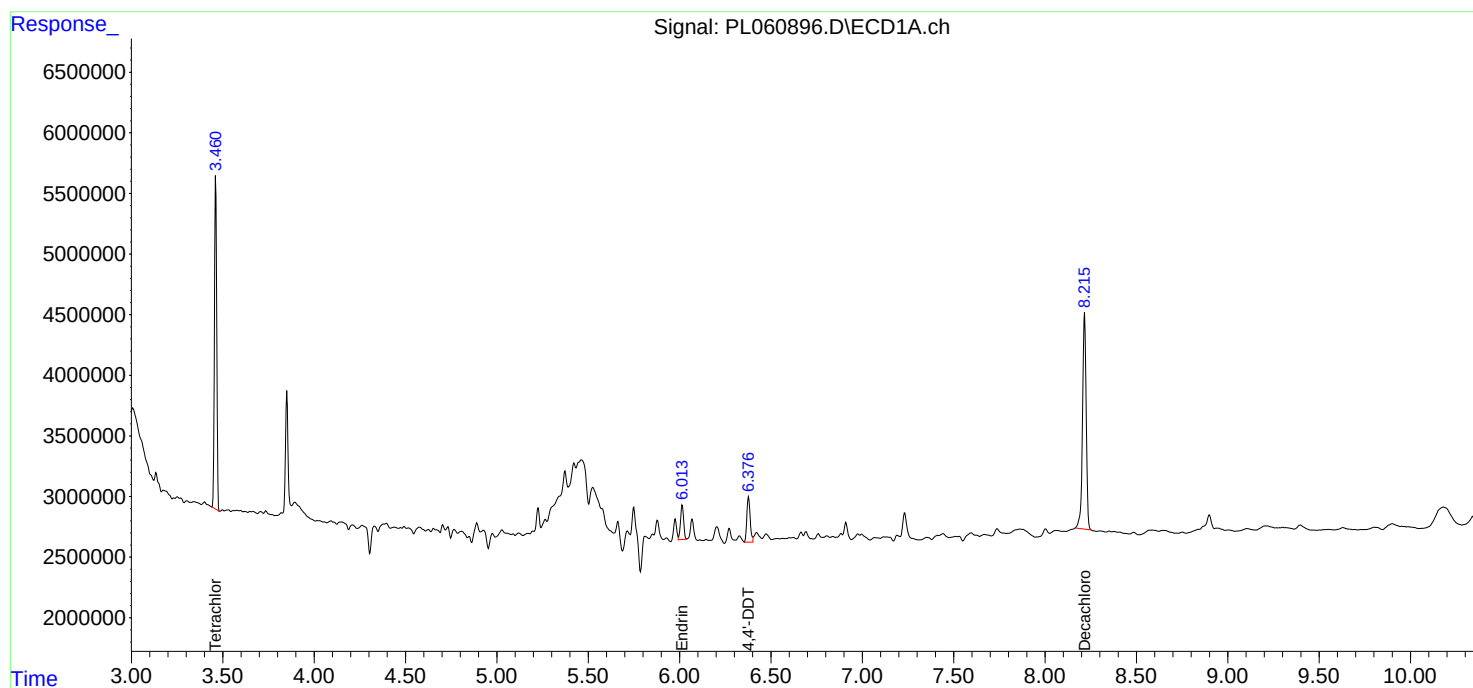

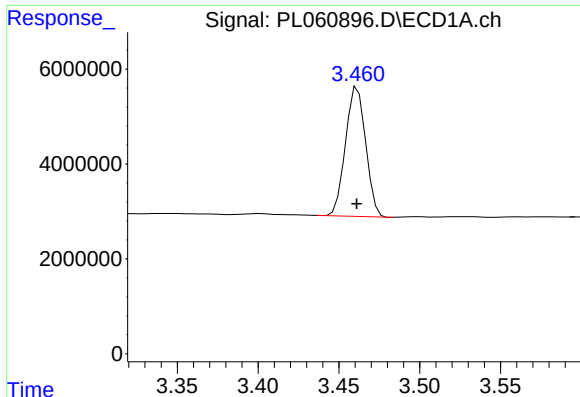


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: 0.000 min
Response: 23673366
Conc: 14.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2-(1-2)


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:19 AM

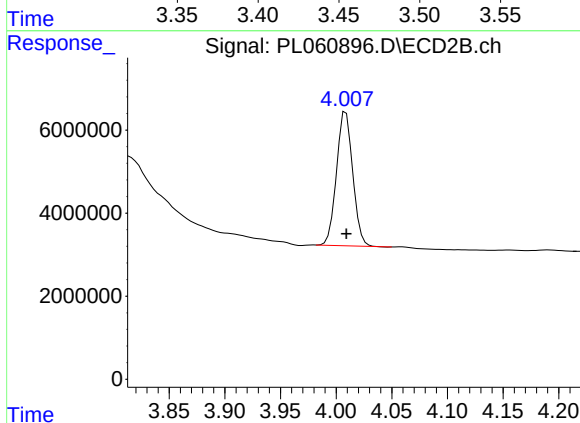


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 32694470
Conc: 11.75 ng/ml

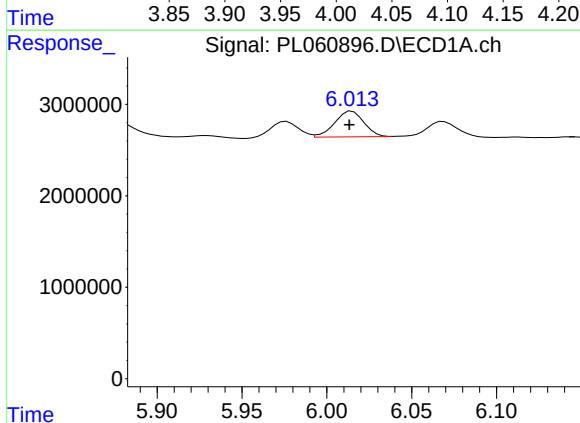


#14 Endrin

R.T.: 6.013 min
Delta R.T.: 0.000 min
Response: 3348308
Conc: 2.21 ng/ml m

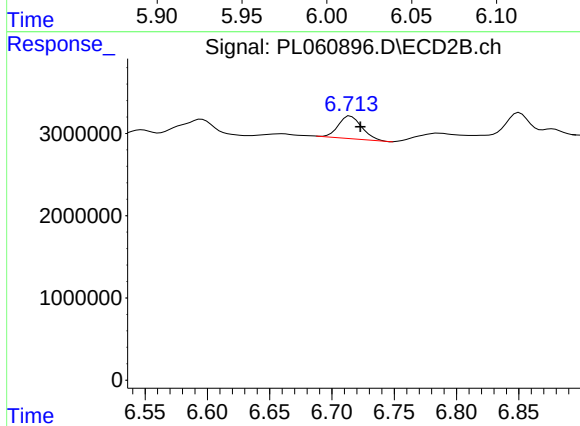

#14 Endrin

R.T.: 6.715 min
Delta R.T.: -0.008 min
Response: 3637255
Conc: 1.40 ng/ml

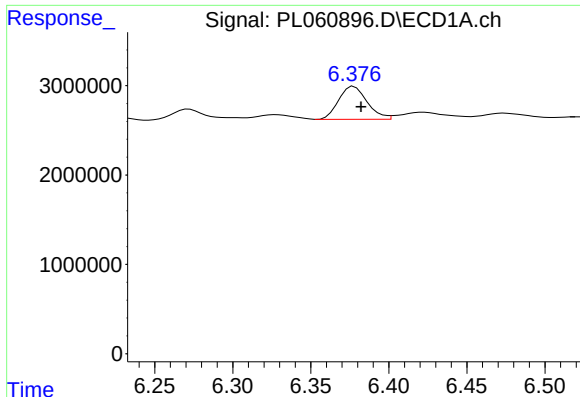


#17 4,4'-DDT

R.T.: 6.376 min
Delta R.T.: -0.006 min
Response: 4702261
Conc: 3.92 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMP-2-(1-2)


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:19 AM

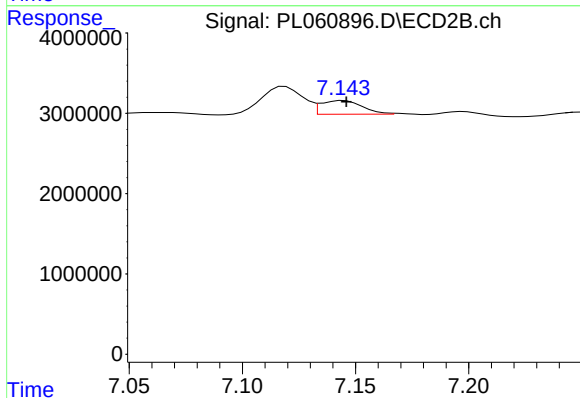


#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: -0.003 min
Response: 2101800
Conc: 0.97 ng/ml m

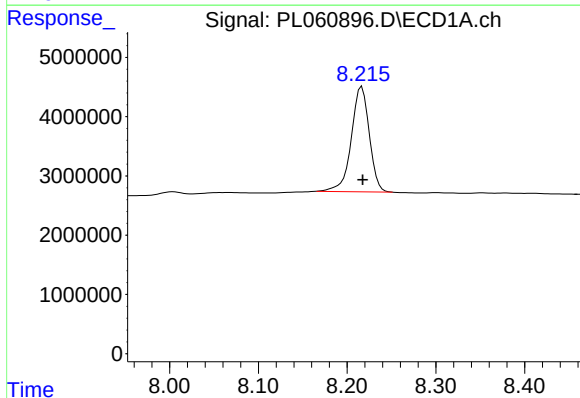

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.002 min
Response: 25003401
Conc: 17.50 ng/ml m

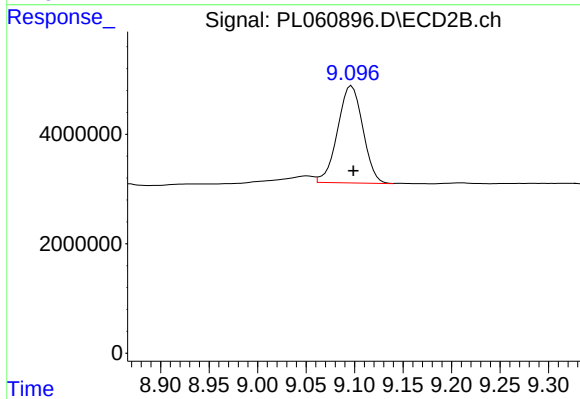

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: -0.003 min
Response: 32004786
Conc: 15.83 ng/ml m