

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082120\
 Data File : PL060897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2020 12:34
 Operator : DD\AJ
 Sample : L3506-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-082020

Manual Integrations
 APPROVED

Ankita
 8/24/2020 11:26:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 01:08:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 06:13:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.461	4.009	23046873	30843598	13.805	11.088
28) SA Decachlor...	8.218	9.097	19960781	28048944	13.974	13.878
Target Compounds						
10) B gamma-Chl...	5.401	6.122	1064512	1438938	0.647m	0.471m#
11) B alpha-Chl...	5.459	6.197	1100380	3203399	0.668m	1.016 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082120\
Data File : PL060897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2020 12:34
Operator : DD\AJ
Sample : L3506-06
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-03-082020


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 01:08:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 06:13:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

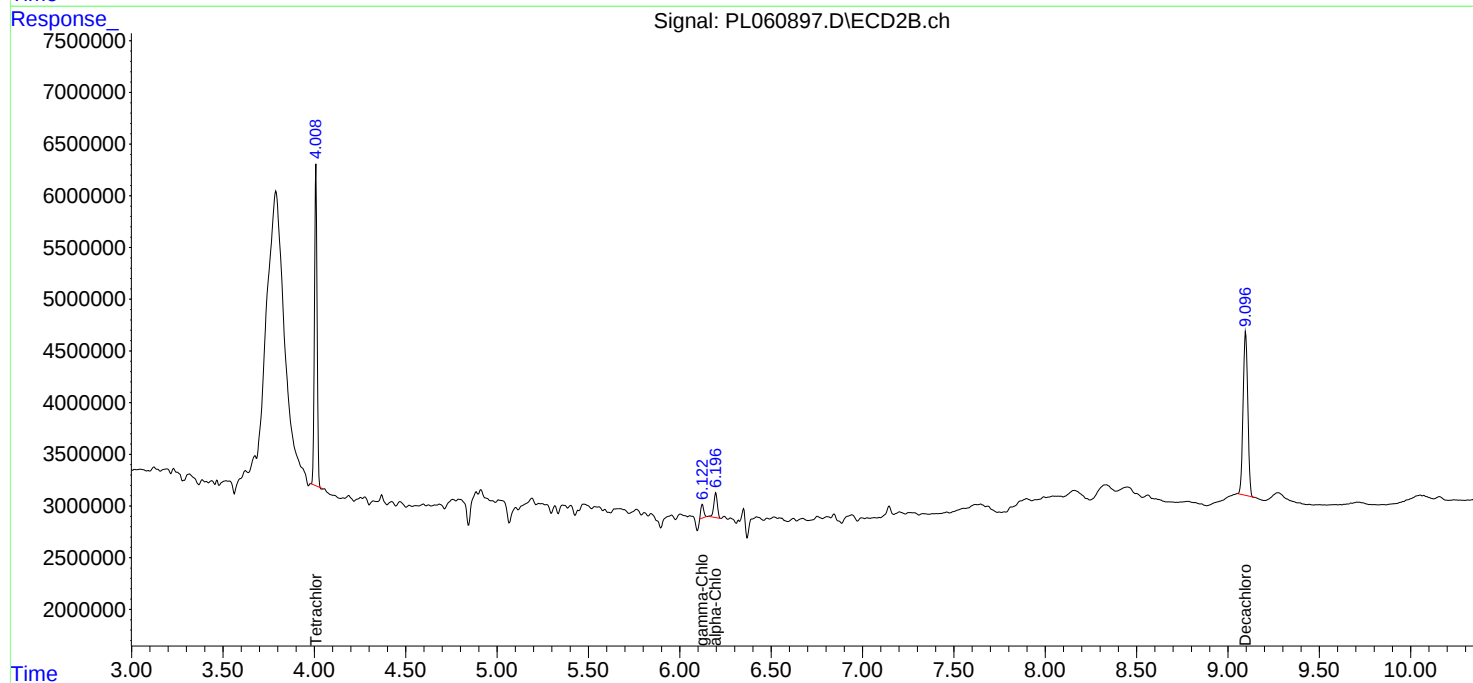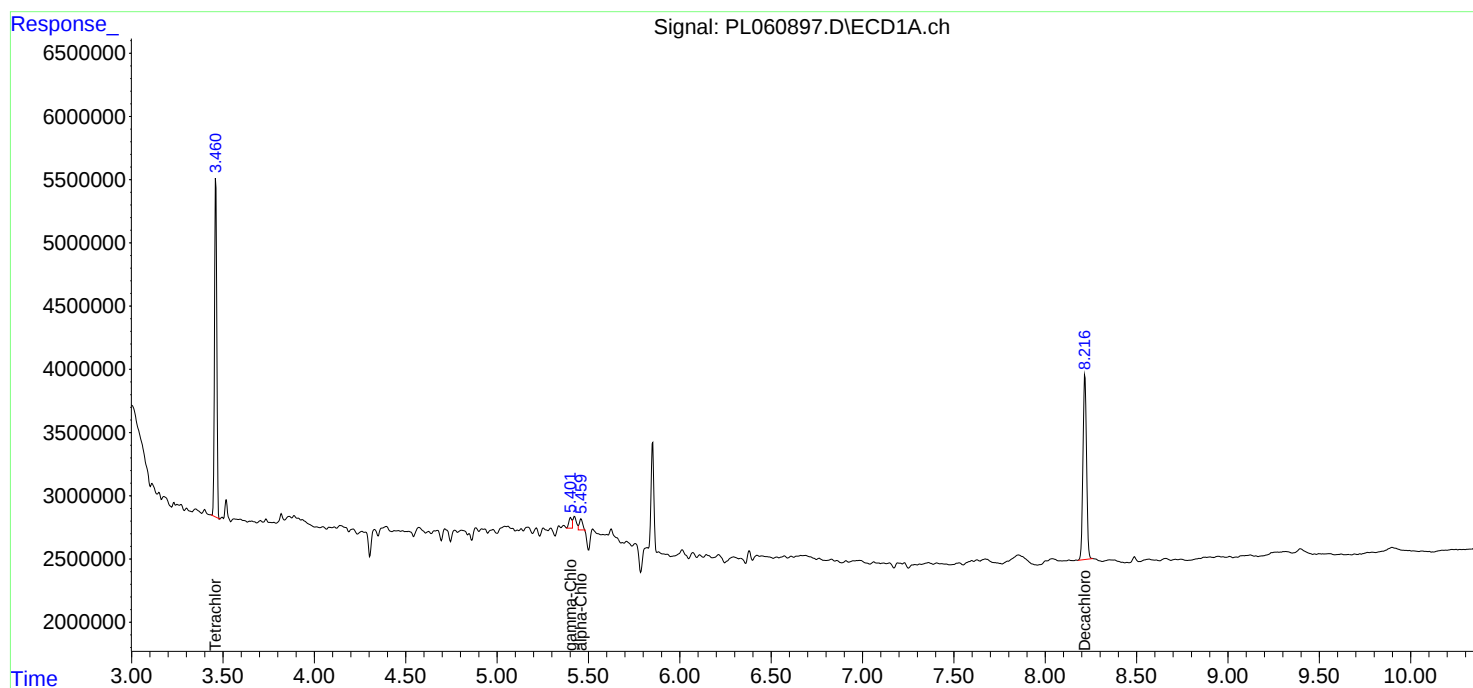

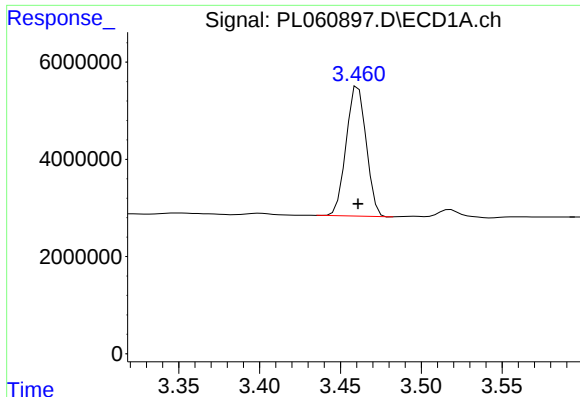


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 23046873
Conc: 13.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-082020


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:24 AM

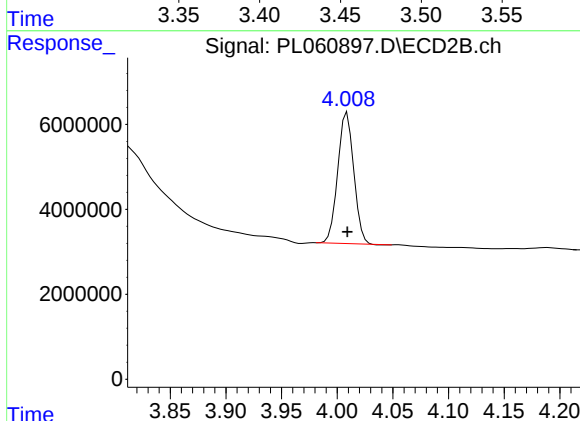


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 30843598
Conc: 11.09 ng/ml

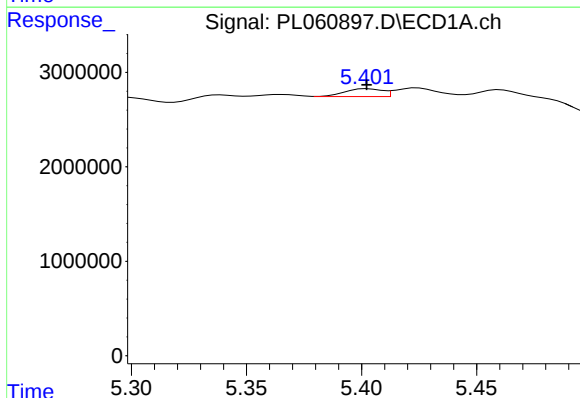


#10 gamma-Chlordane

R.T.: 5.401 min
Delta R.T.: -0.001 min
Response: 1064512
Conc: 0.65 ng/ml m

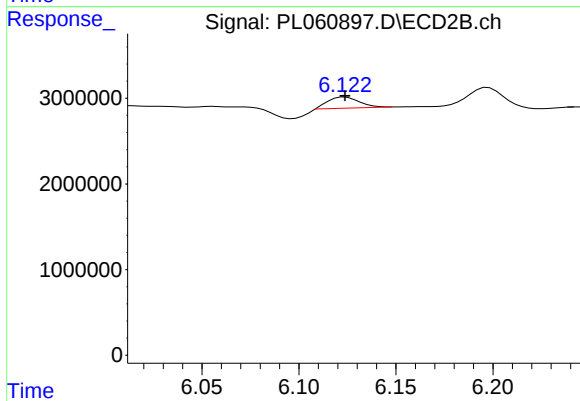

#10 gamma-Chlordane

R.T.: 6.122 min
Delta R.T.: -0.001 min
Response: 1438938
Conc: 0.47 ng/ml m

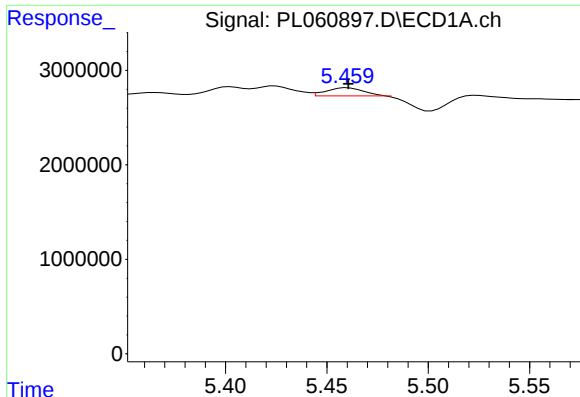


#11 alpha-Chlordane

R.T.: 5.459 min
Delta R.T.: -0.002 min
Response: 1100380
Conc: 0.67 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OR-03-082020


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:24 AM

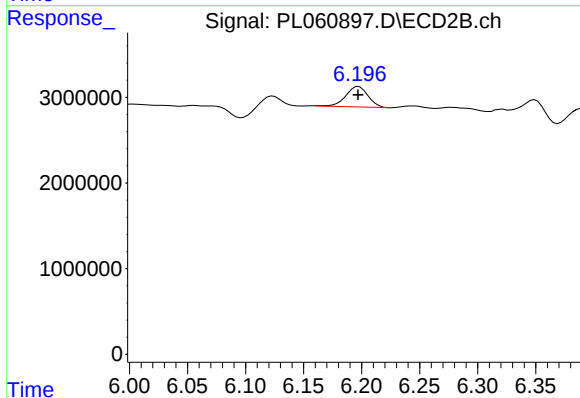


#11 alpha-Chlordane

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 3203399
Conc: 1.02 ng/ml

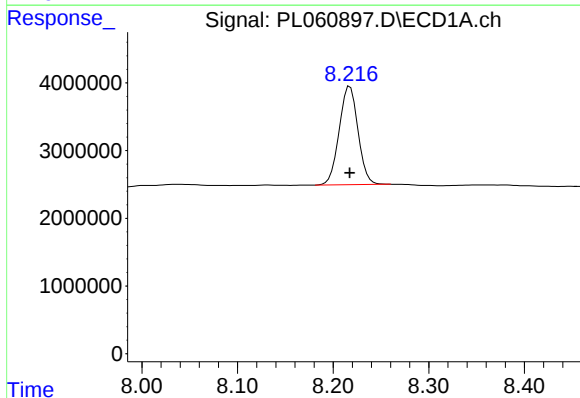

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: 0.000 min
Response: 19960781
Conc: 13.97 ng/ml

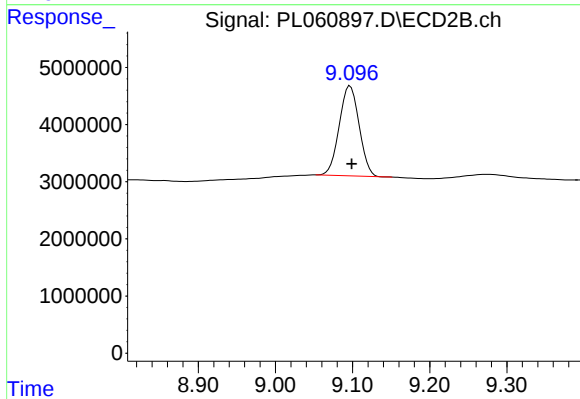

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 28048944
Conc: 13.88 ng/ml