

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082120\
 Data File : PL060915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2020 17:42
 Operator : DD\AJ
 Sample : L3746-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 212

Manual Integrations
 APPROVED

Ankita
 8/24/2020 11:26:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 24 02:30:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 06:13:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.011	24055221	32824105	14.409	11.800
28)	SA Decachlor...	8.218	9.098	20114112	27360648	14.081	13.537
Target Compounds							
12)	B 4,4'-DDE	5.626	6.354	5206997	7786180	3.377	2.572
17)	MA 4,4'-DDT	6.380	7.146	2208667	3656724	1.842m	1.685

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082120\
Data File : PL060915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2020 17:42
Operator : DD\AJ
Sample : L3746-06
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
212


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 24 02:30:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 06:13:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

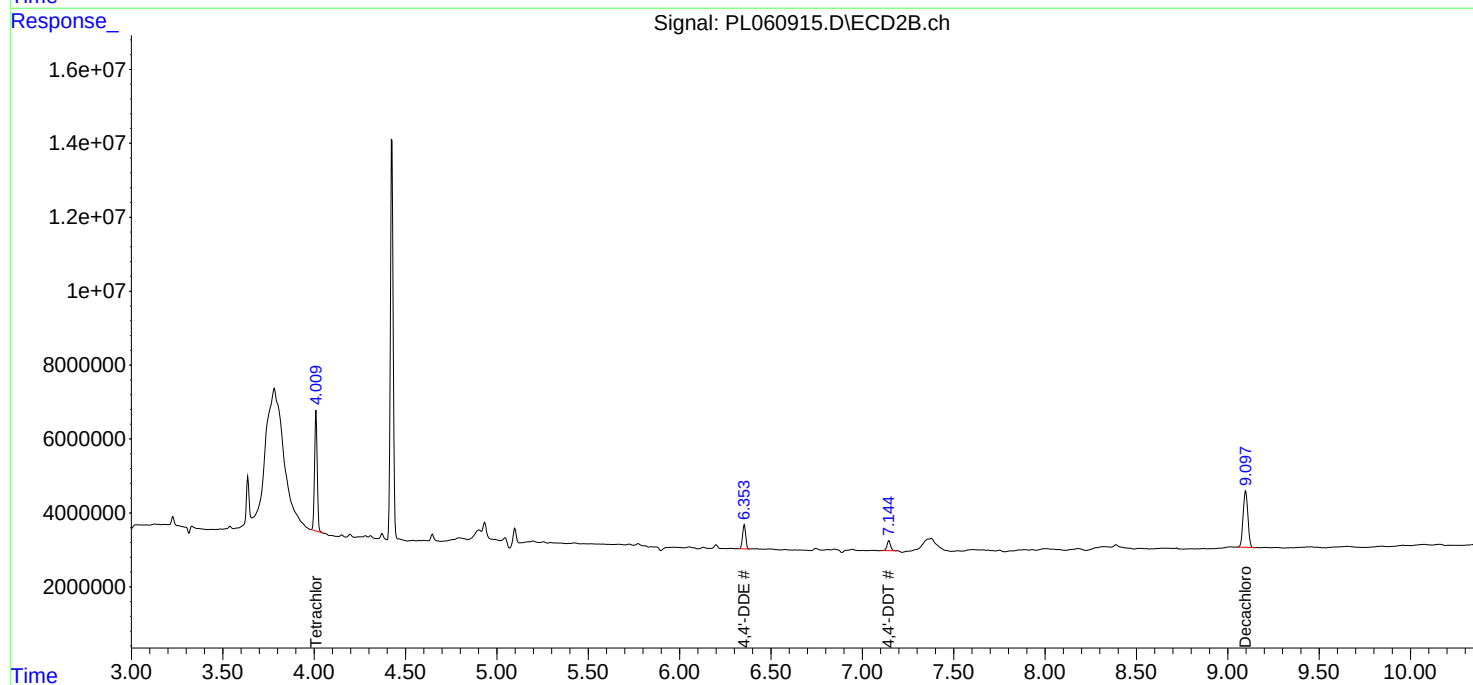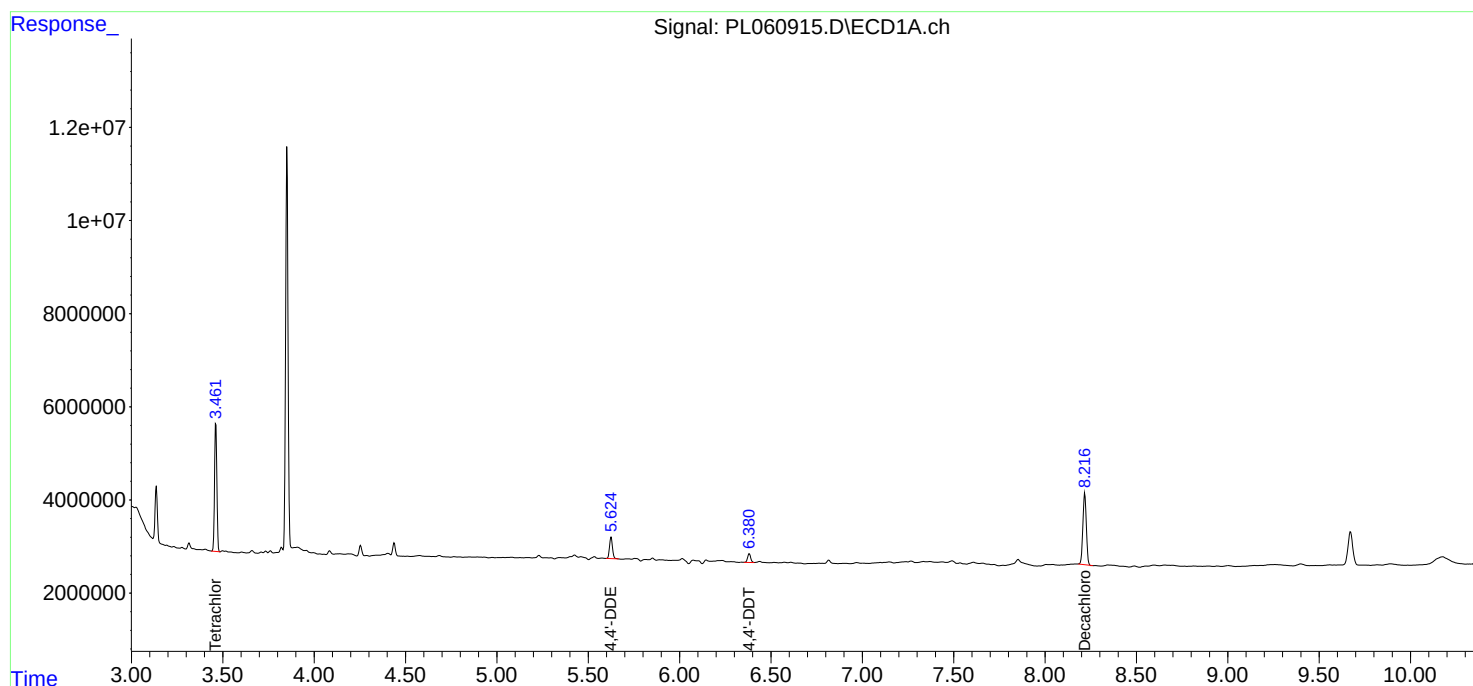

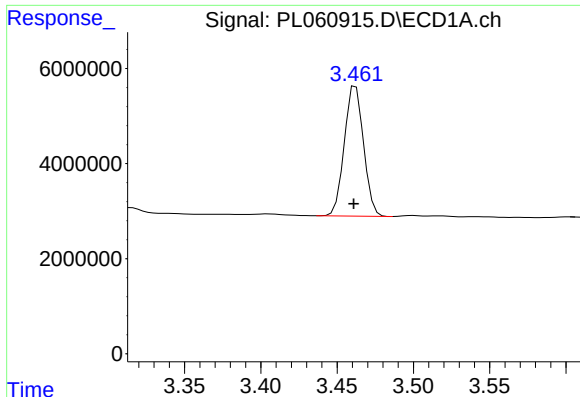


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: 0.001 min
Response: 24055221
Conc: 14.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
212


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:56 AM

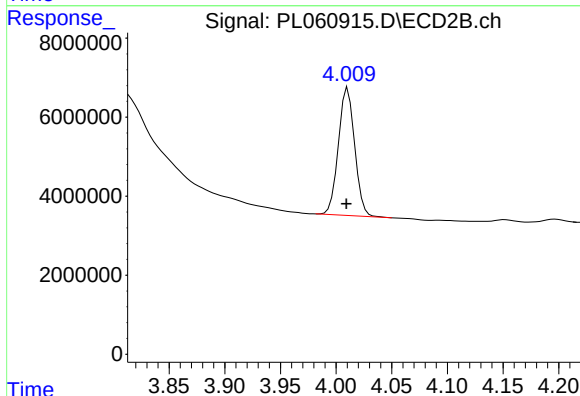


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.001 min
Response: 32824105
Conc: 11.80 ng/ml

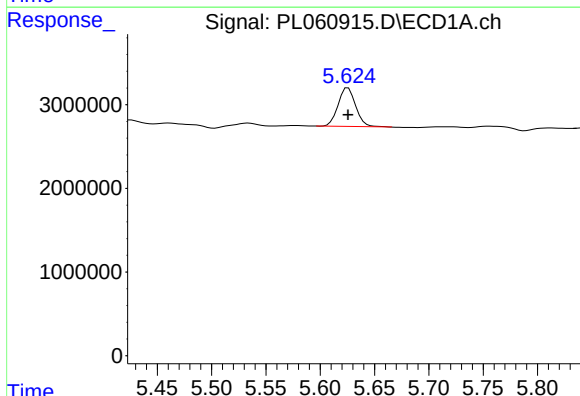


#12 4,4'-DDE

R.T.: 5.626 min
Delta R.T.: 0.000 min
Response: 5206997
Conc: 3.38 ng/ml

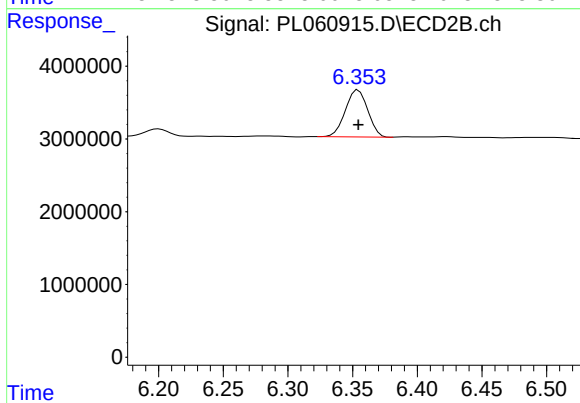

#12 4,4'-DDE

R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 7786180
Conc: 2.57 ng/ml

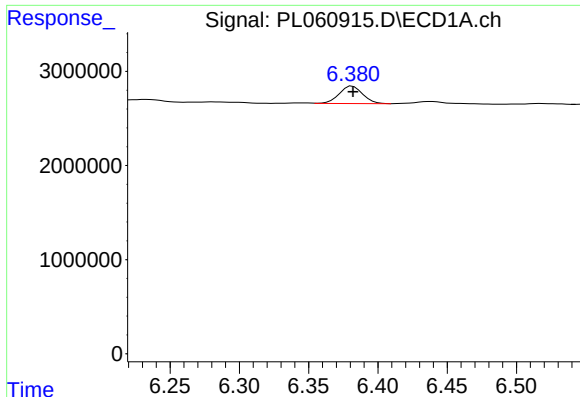


#17 4,4'-DDT

R.T.: 6.380 min
Delta R.T.: -0.002 min
Response: 2208667
Conc: 1.84 ng/ml m

Instrument :
ECD_L
ClientSampleId :
212


Manual Integrations
APPROVED

Ankita
8/24/2020 11:26:56 AM

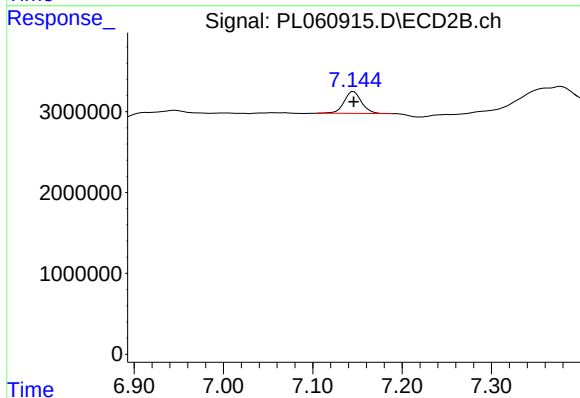


#17 4,4'-DDT

R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 3656724
Conc: 1.68 ng/ml

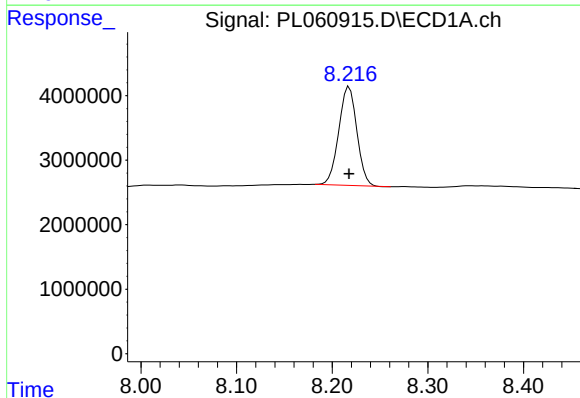

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: 0.000 min
Response: 20114112
Conc: 14.08 ng/ml

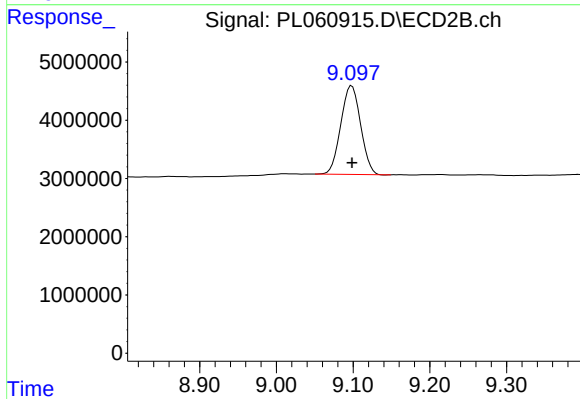

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 27360648
Conc: 13.54 ng/ml