

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
 Data File : PL069314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 04:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 05:02:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.568	9910870	30199314	21.481	21.082
28)	SA Decachlor...	10.399	11.488	13876852	25467276	20.560	20.780
Target Compounds							
4)	MA Heptachlor	6.148f	0.000	736848	0	1.064	N.D. #
7)	B delta-BHC	0.000	7.035f	0	4351742	N.D.	2.356 #
10)	B gamma-Chl...	0.000	8.279f	0	1577046	N.D.	1.025 #
14)	MA Endrin	8.075f	0.000	633130	0	1.096	N.D. #
23)	Chlordane-1	0.000	6.969f	0	1326489	N.D.	23.432 #
25)	Chlordane-3	0.000	8.279f	0	1577046	N.D.	7.364 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
Data File : PL069314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 04:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 05:02:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

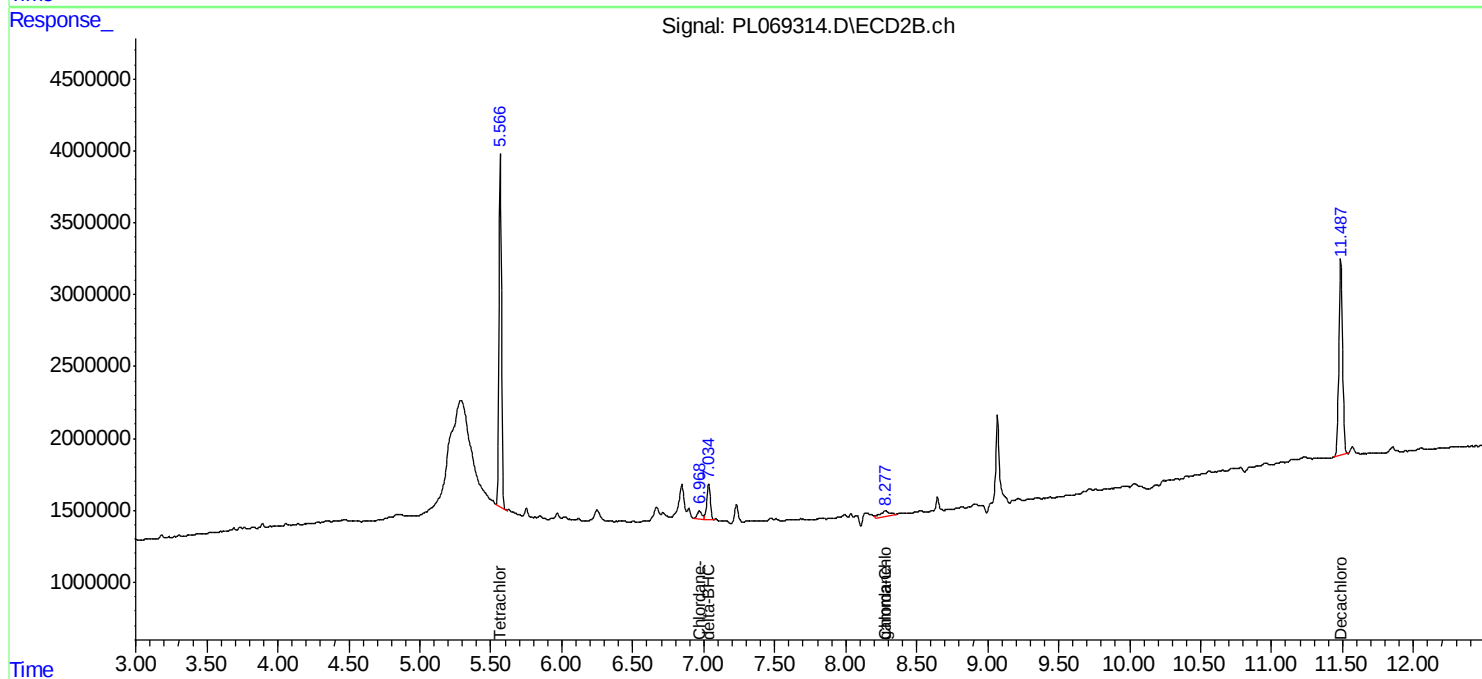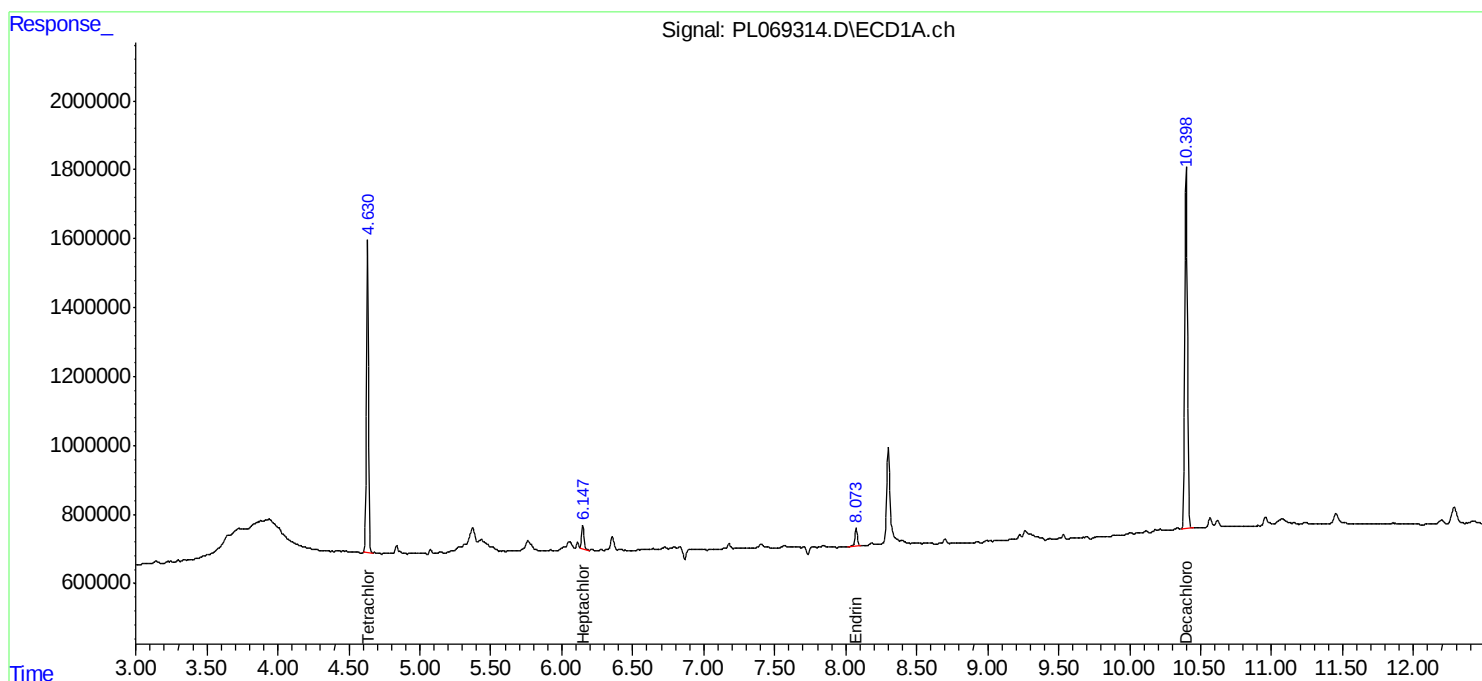


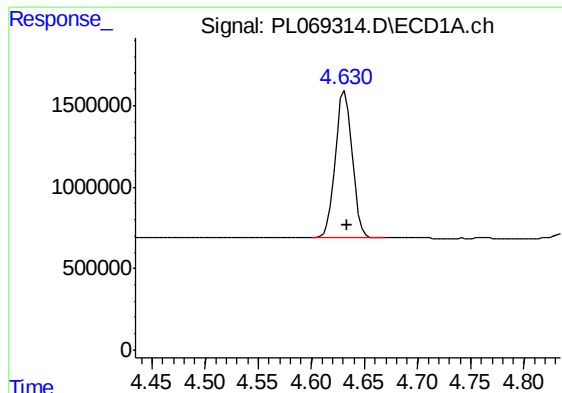

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 9910870
Conc: 21.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

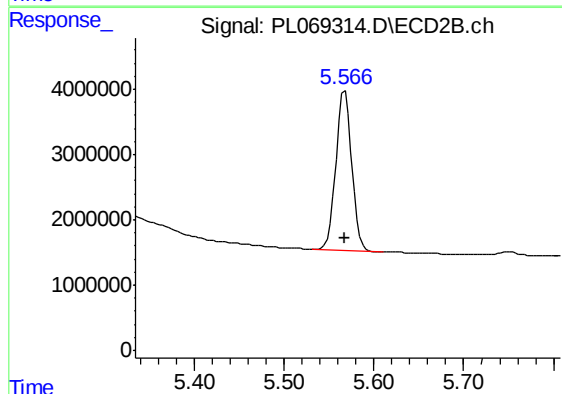


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: 0.000 min
Response: 30199314
Conc: 21.08 ng/ml

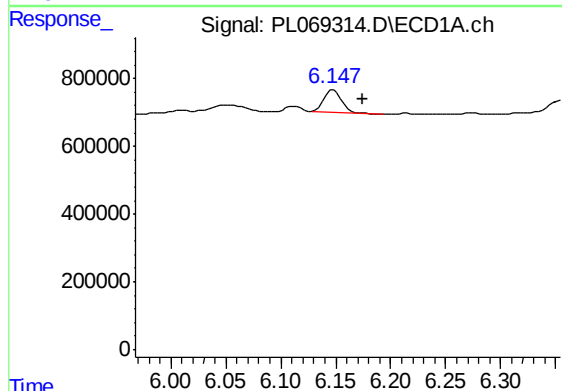


#4 Heptachlor

R.T.: 6.148 min
Delta R.T.: -0.026 min
Response: 736848
Conc: 1.06 ng/ml

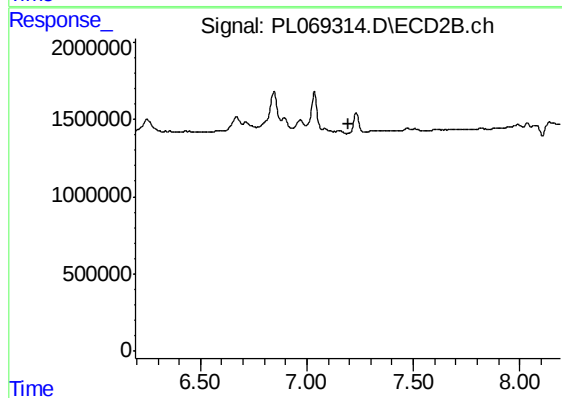

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

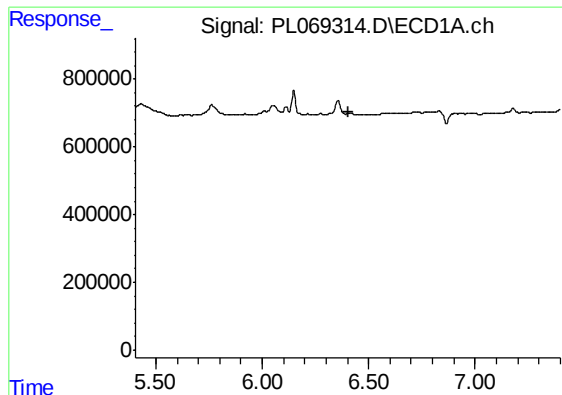

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

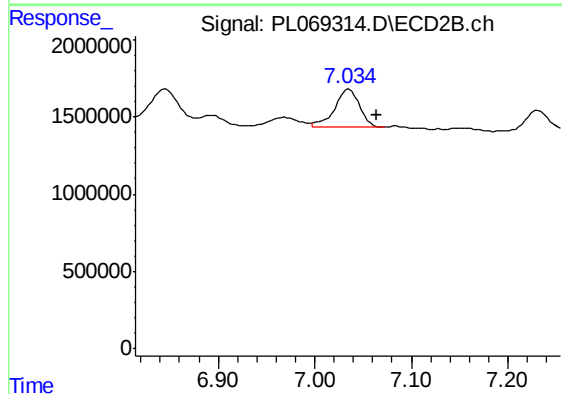


#7 delta-BHC

R.T.: 7.035 min
Delta R.T.: -0.029 min
Response: 4351742
Conc: 2.36 ng/ml

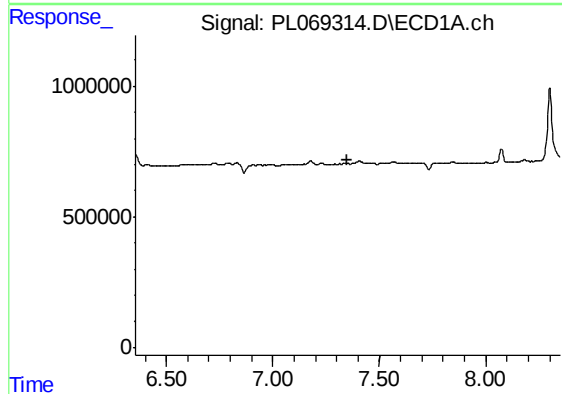


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.352 min
Response: 0
Conc: N.D.

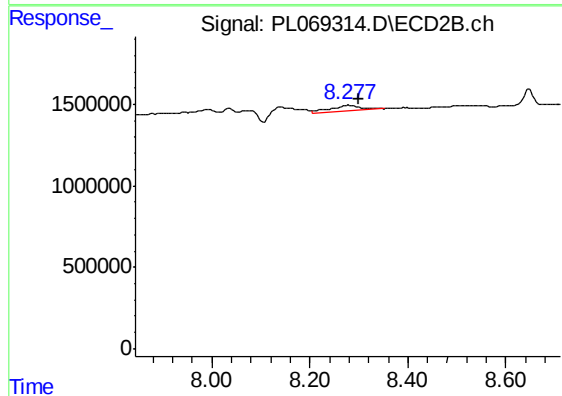

#10 gamma-Chlordane


R.T.: 8.279 min
Delta R.T.: -0.020 min
Response: 1577046
Conc: 1.03 ng/ml

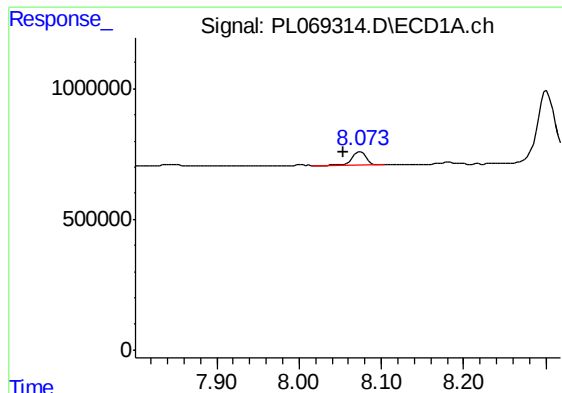

#14 Endrin


R.T.: 8.075 min
Delta R.T.: 0.020 min
Response: 633130
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

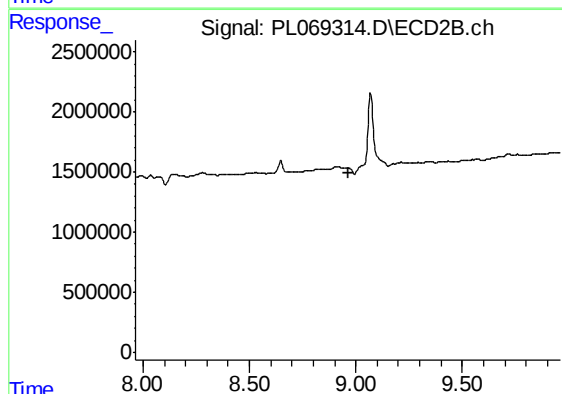


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.964 min
Response: 0
Conc: N.D.

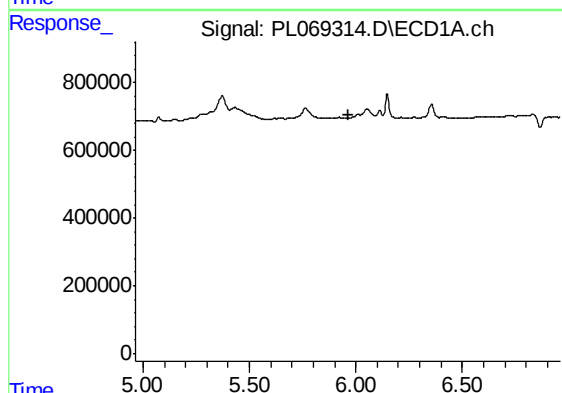


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.964 min
Response: 0
Conc: N.D.

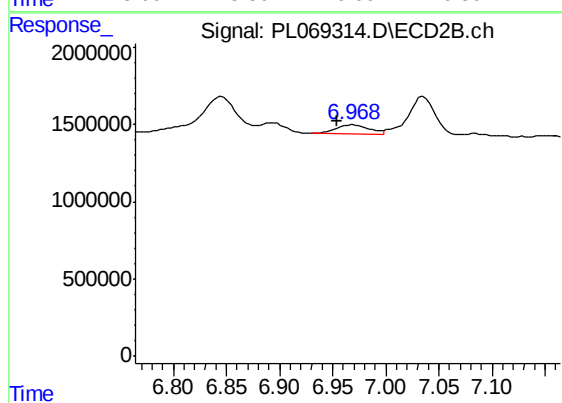

#23 Chlordane-1


R.T.: 6.969 min
Delta R.T.: 0.015 min
Response: 1326489
Conc: 23.43 ng/ml

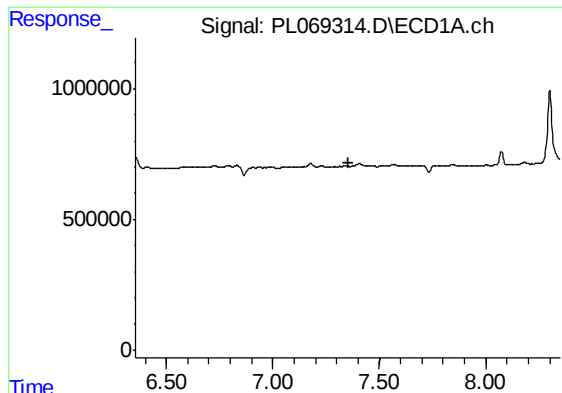

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

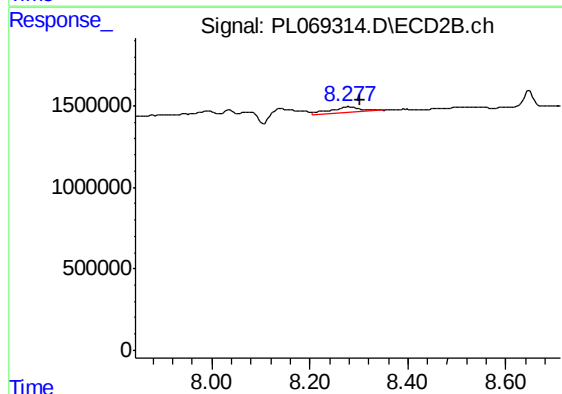


#25 Chlordane-3

R.T.: 8.279 min
Delta R.T.: -0.024 min
Response: 1577046
Conc: 7.36 ng/ml

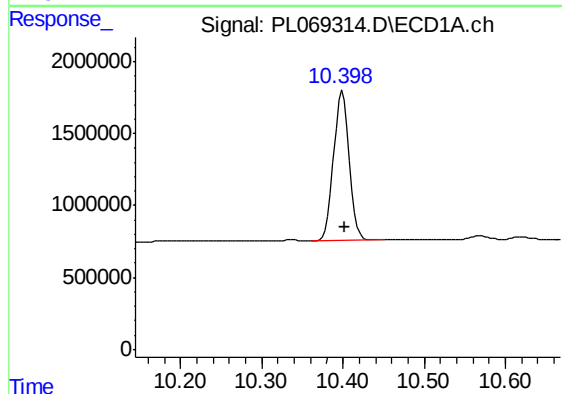

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.002 min
Response: 13876852
Conc: 20.56 ng/ml

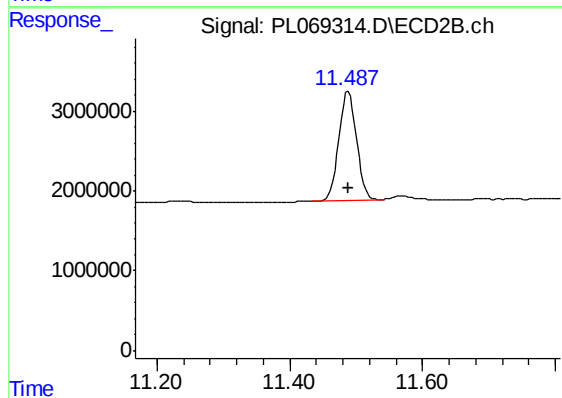

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: 0.000 min
Response: 25467276
Conc: 20.78 ng/ml