

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
 Data File : PL069326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 08:28
 Operator : AR\AJ
 Sample : M3451-04
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5-10-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 04:46:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.634	5.570	5721844	16740311	12.402	11.686
28) SA Decachlor...	10.406	11.496	8036257	14263188	11.907	11.638
Target Compounds						
7) B delta-BHC	0.000	7.043f	0	1772513	N.D.	0.960 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
Data File : PL069326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 08:28
Operator : AR\AJ
Sample : M3451-04
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-5-10-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 04:46:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

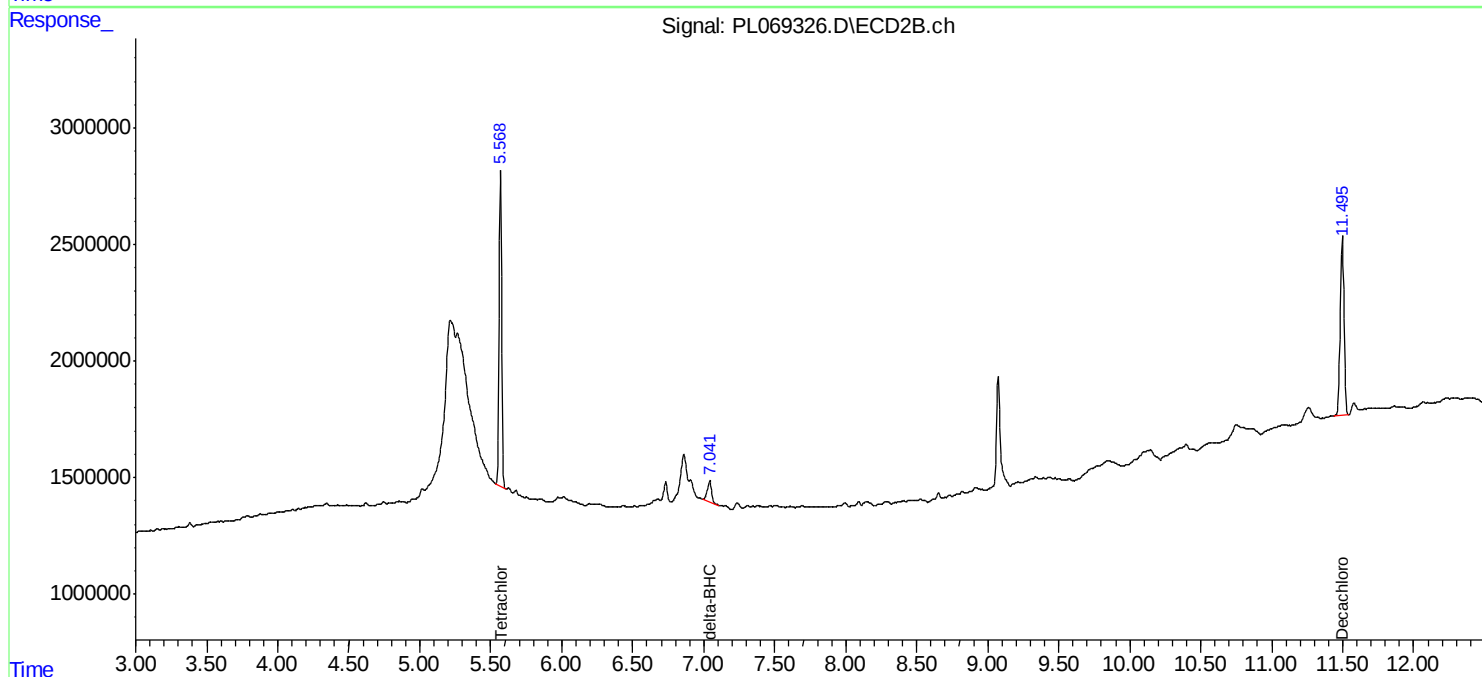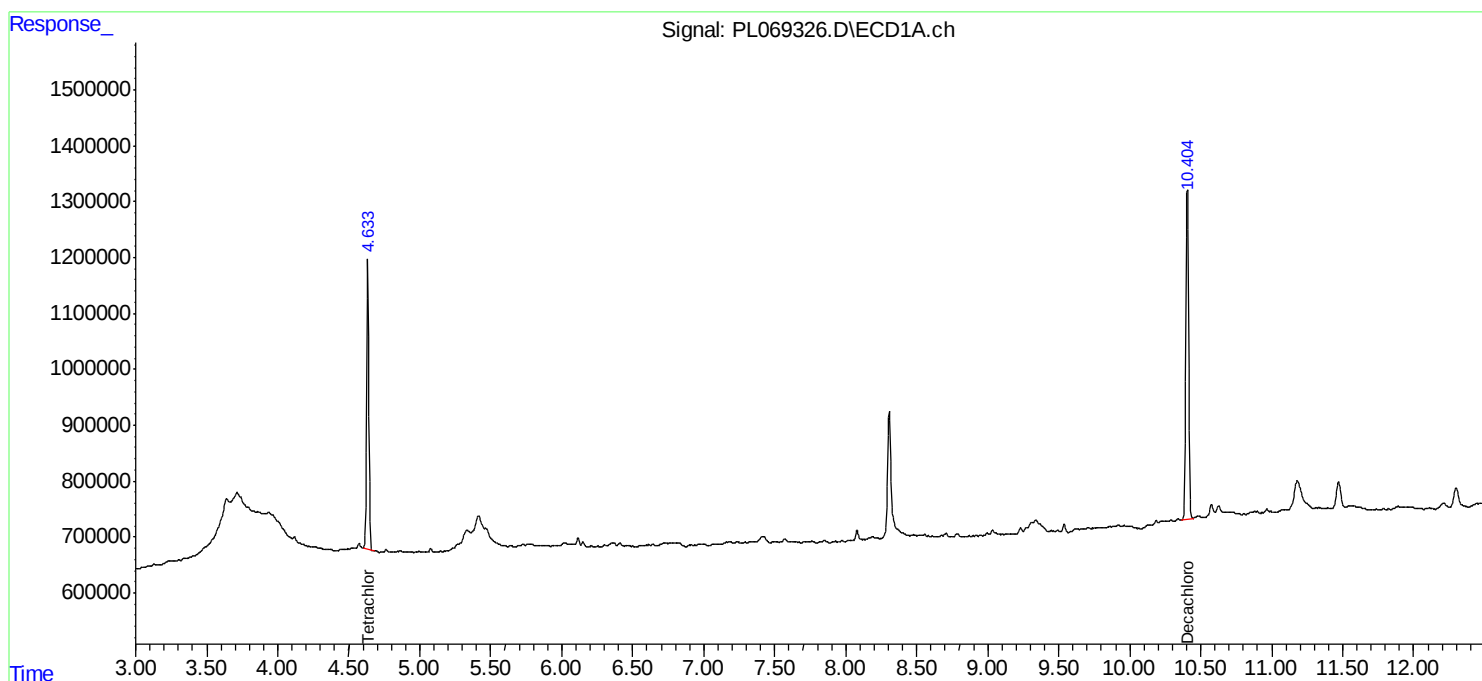


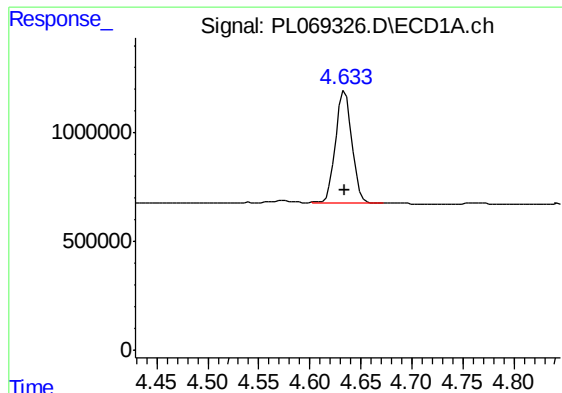

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 5721844
Conc: 12.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-10-COMP

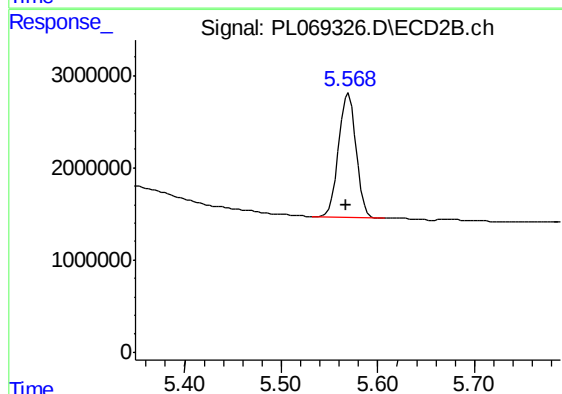


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.003 min
Response: 16740311
Conc: 11.69 ng/ml

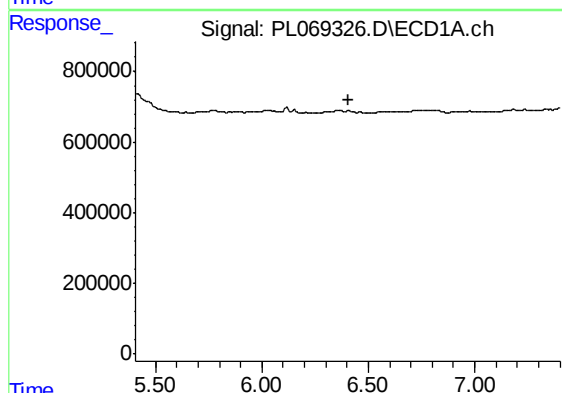


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

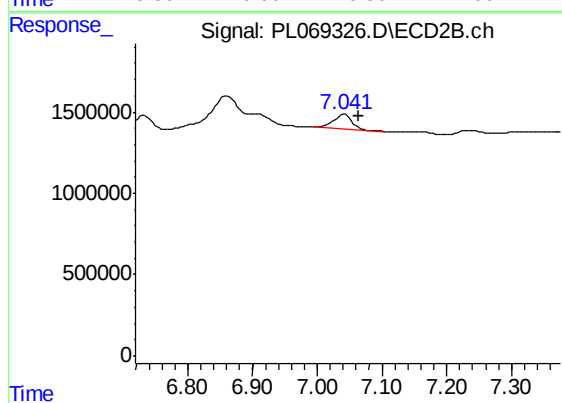

#7 delta-BHC


R.T.: 7.043 min
Delta R.T.: -0.021 min
Response: 1772513
Conc: 0.96 ng/ml

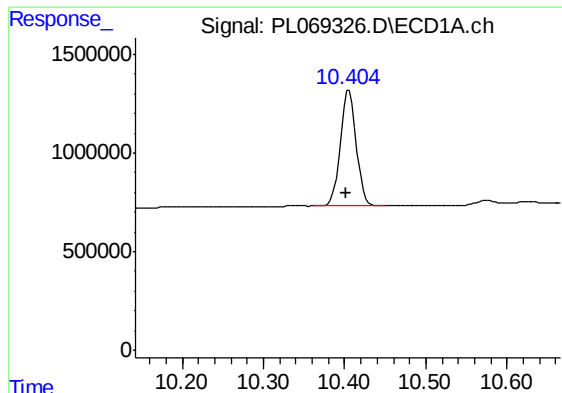

#28 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: 0.004 min
Response: 8036257
Conc: 11.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5-10-COMP

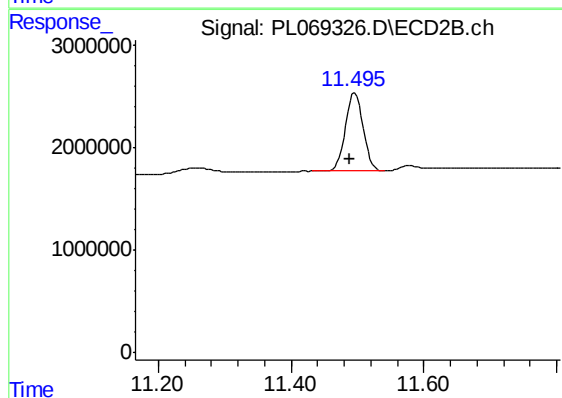

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.008 min
Response: 14263188
Conc: 11.64 ng/ml