

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
 Data File : PL069350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 19:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 04:55:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.632	5.568	10147455	30955191	21.994	21.609
28)	SA Decachlor...	10.398	11.488	13725450	25280158	20.336	20.627
Target Compounds							
4)	MA Heptachlor	6.148f	0.000	735255	0	1.062	N.D. #
7)	B delta-BHC	0.000	7.035f	0	4355350	N.D.	2.358 #
8)	B Heptachlo...	0.000	8.036	0	585426	N.D.	0.389 #
10)	B gamma-Chl...	0.000	8.282f	0	1096785	N.D.	0.713 #
14)	MA Endrin	8.075f	0.000	821043	0	1.422	N.D. #
25)	Chlordane-3	0.000	8.282f	0	1096785	N.D.	5.122 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
Data File : PL069350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 19:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 04:55:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

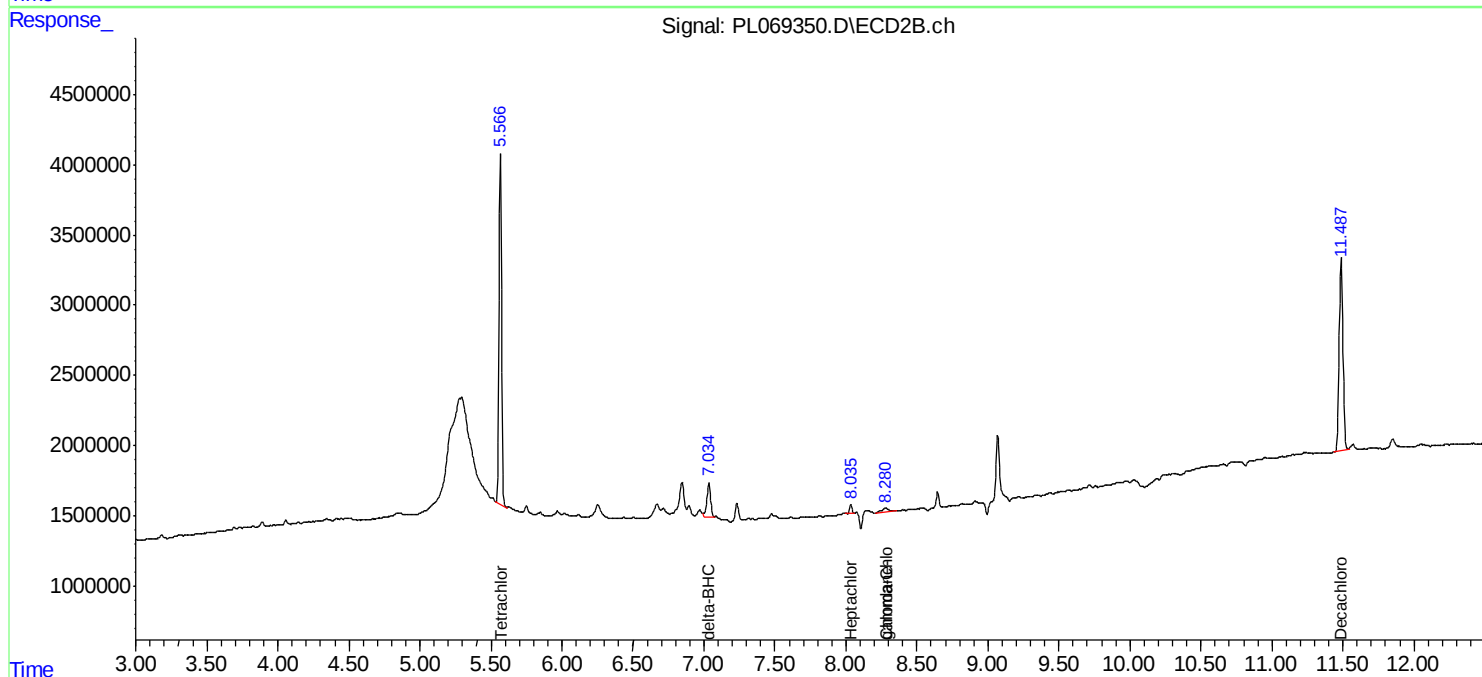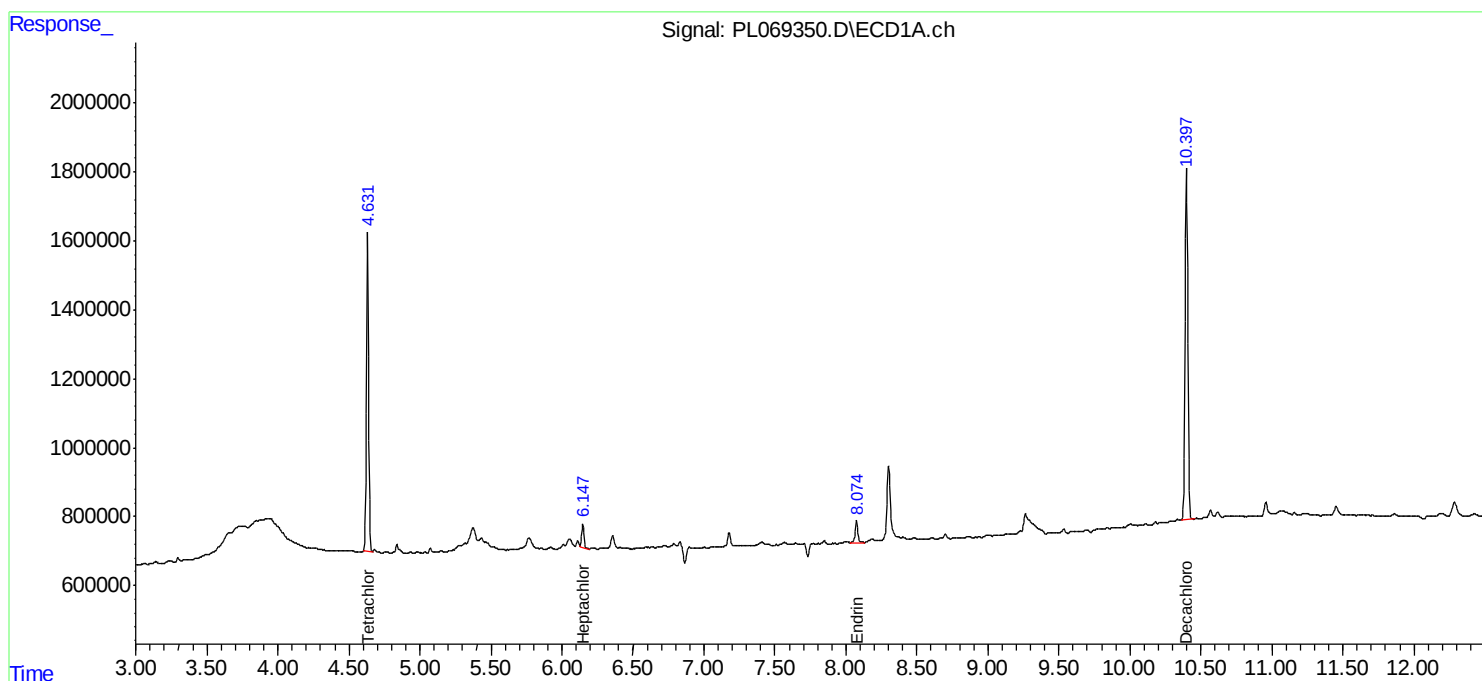


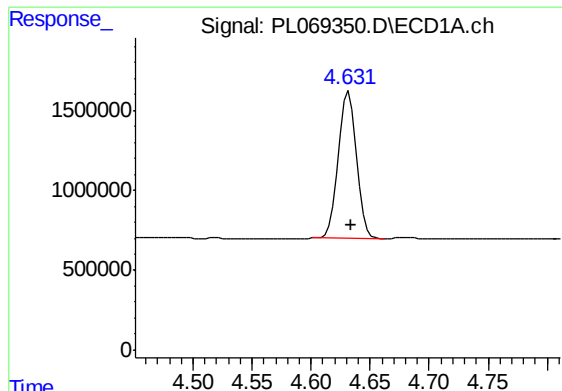

#1 Tetrachloro-m-xylene


R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 10147455
Conc: 21.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

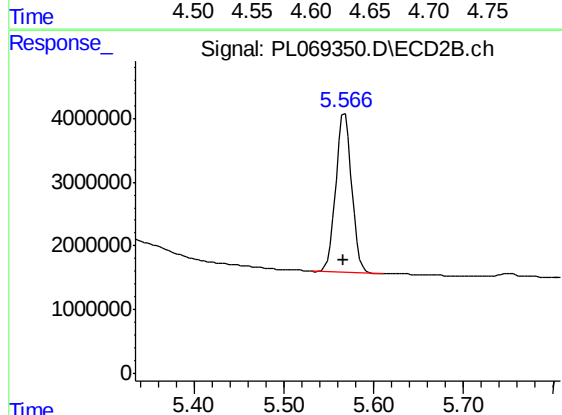


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: 0.000 min
Response: 30955191
Conc: 21.61 ng/ml

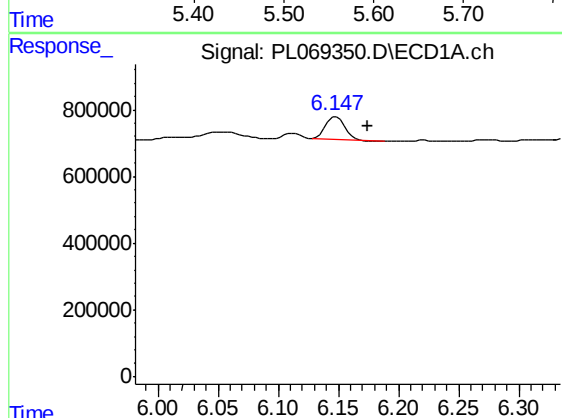


#4 Heptachlor

R.T.: 6.148 min
Delta R.T.: -0.026 min
Response: 735255
Conc: 1.06 ng/ml

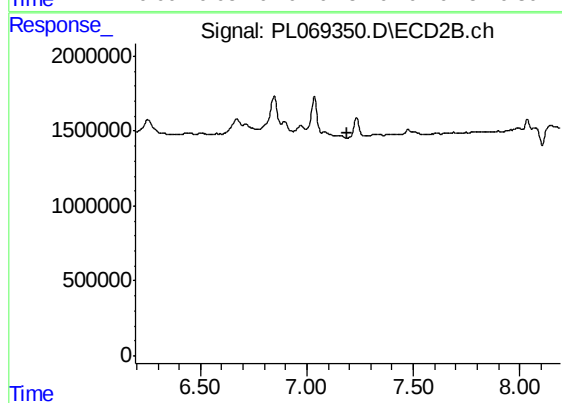

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.193 min
Response: 0
Conc: N.D.

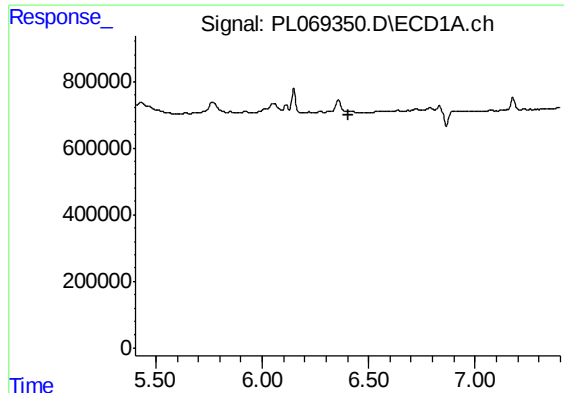

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

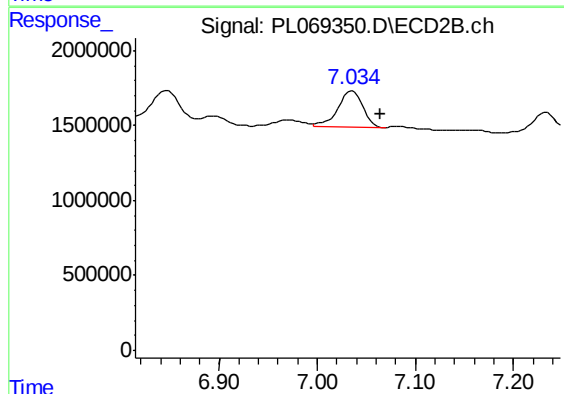


#7 delta-BHC

R.T.: 7.035 min
Delta R.T.: -0.028 min
Response: 4355350
Conc: 2.36 ng/ml

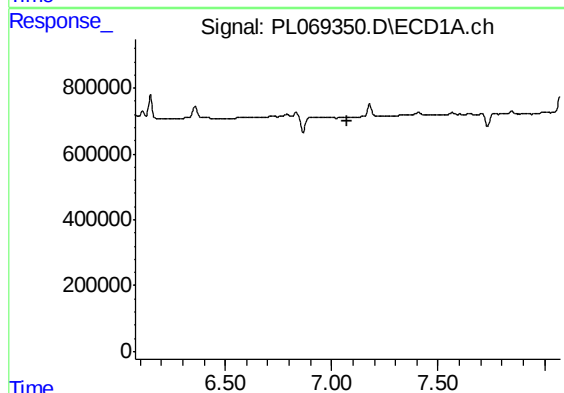


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.075 min
Response: 0
Conc: N.D.

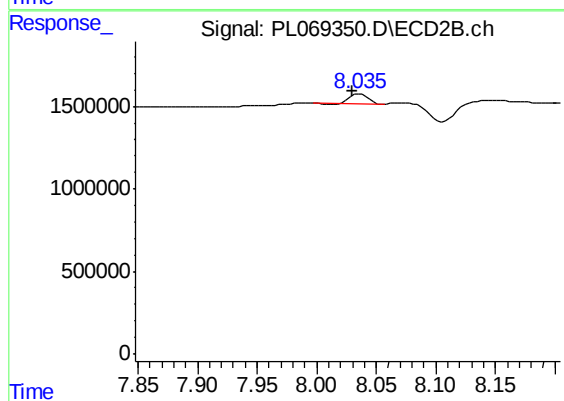

#8 Heptachlor epoxide


R.T.: 8.036 min
Delta R.T.: 0.006 min
Response: 585426
Conc: 0.39 ng/ml

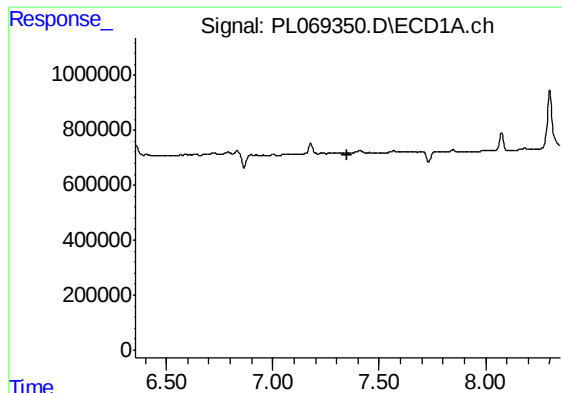

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

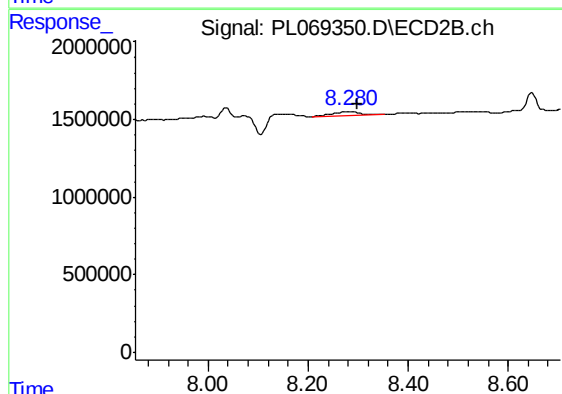


#10 gamma-Chlordane

R.T.: 8.282 min
Delta R.T.: -0.017 min
Response: 1096785
Conc: 0.71 ng/ml

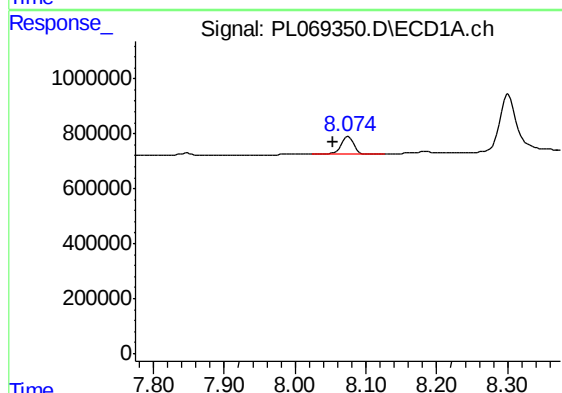


#14 Endrin

R.T.: 8.075 min
Delta R.T.: 0.021 min
Response: 821043
Conc: 1.42 ng/ml

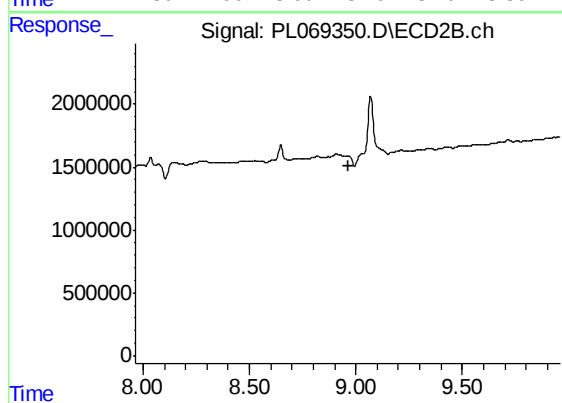

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.964 min
Response: 0
Conc: N.D.

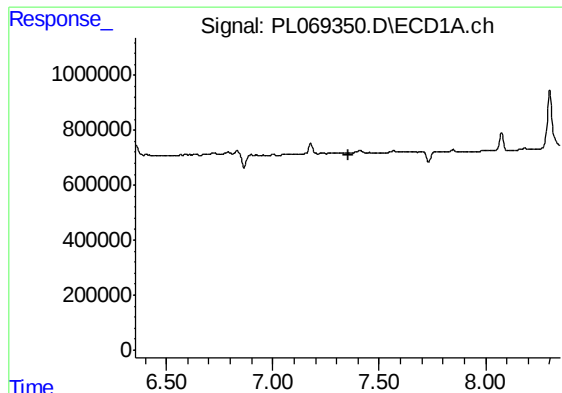

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

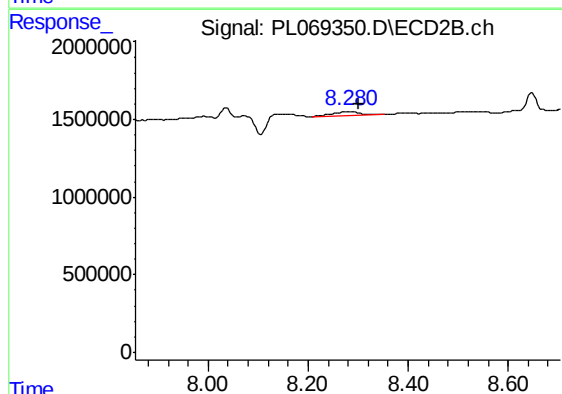


#25 Chlordane-3

R.T.: 8.282 min
Delta R.T.: -0.021 min
Response: 1096785
Conc: 5.12 ng/ml

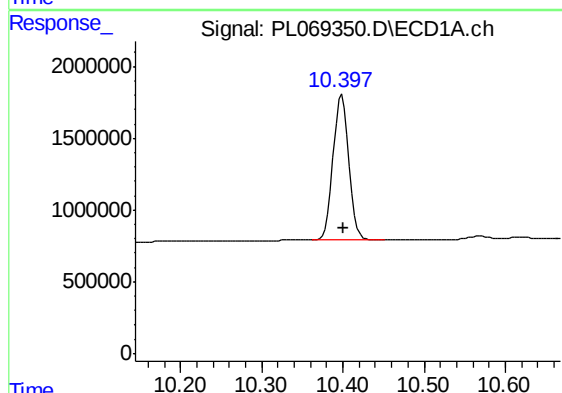

#28 Decachlorobiphenyl

R.T.: 10.398 min
Delta R.T.: -0.003 min
Response: 13725450
Conc: 20.34 ng/ml

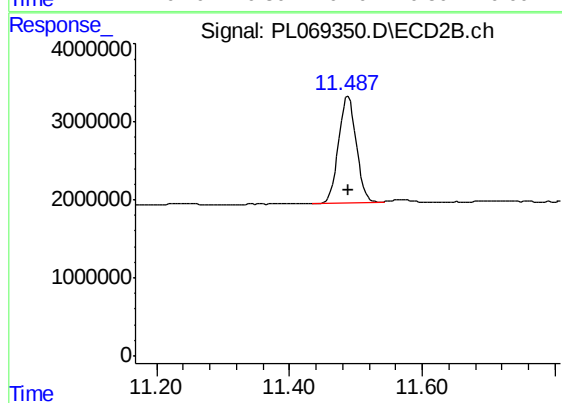

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: 0.000 min
Response: 25280158
Conc: 20.63 ng/ml