

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
 Data File : PL069292.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Aug 2021 20:23
 Operator : AR\AJ
 Sample : M3426-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2021-08-11-FD-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 02:41:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.634	5.567	6494195	19499876	14.076	13.613
28) SA Decachlor...	10.402	11.490	10497928	18092300	15.554	14.762
Target Compounds						
12) B 4,4'-DDE	7.634	8.561	1712787	8695204	3.028	6.216 #
17) MA 4,4'-DDT	8.478	9.424	10517912	8634757	18.273	7.048 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
Data File : PL069292.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Aug 2021 20:23
Operator : AR\AJ
Sample : M3426-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
2021-08-11-FD-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 02:41:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

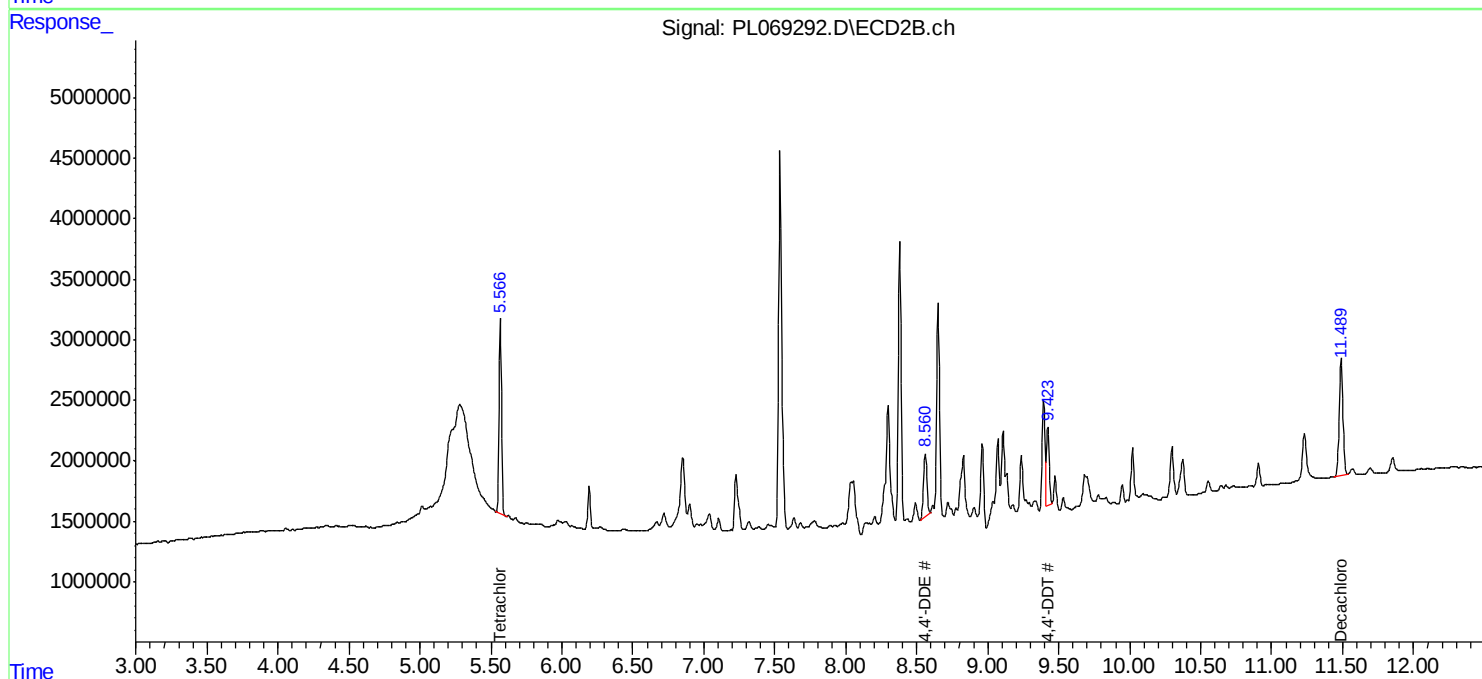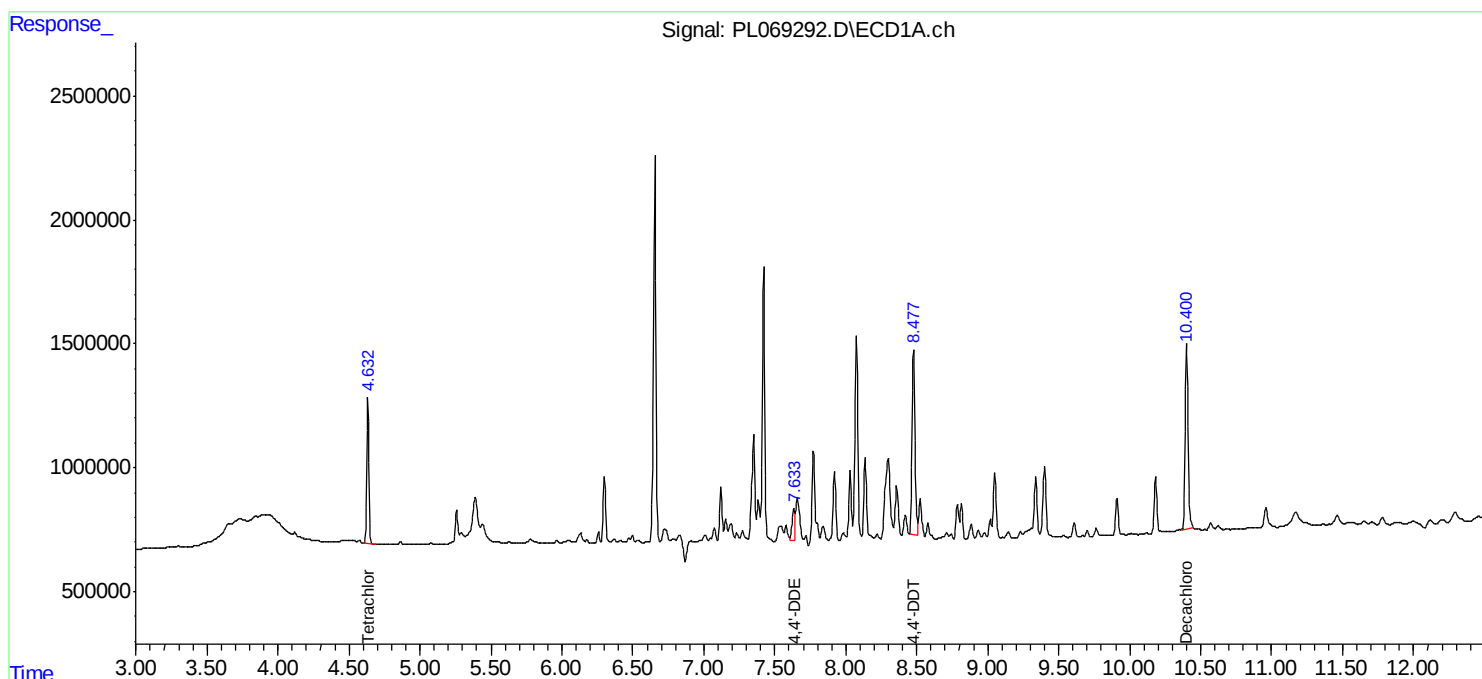


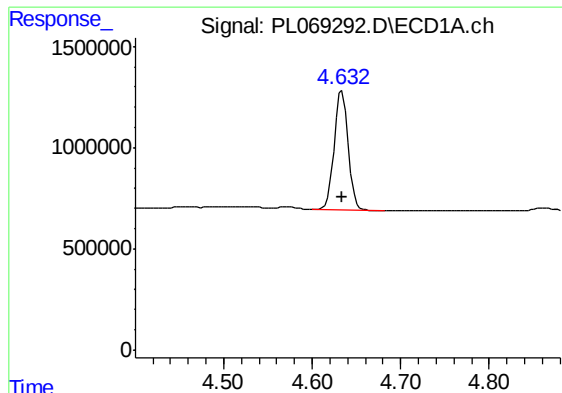

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 6494195
Conc: 14.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
2021-08-11-FD-02

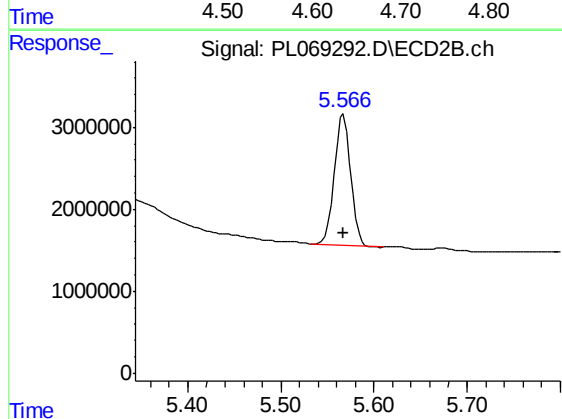


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 19499876
Conc: 13.61 ng/ml

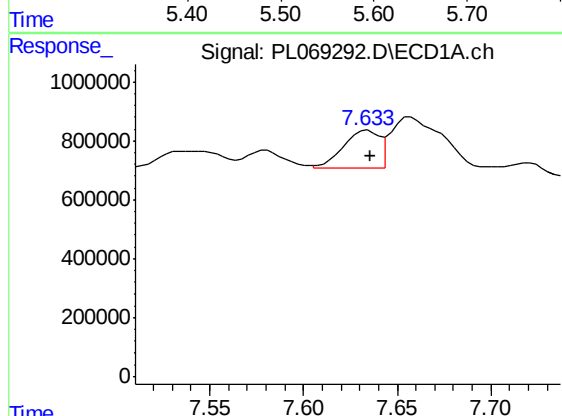


#12 4,4'-DDE

R.T.: 7.634 min
Delta R.T.: -0.001 min
Response: 1712787
Conc: 3.03 ng/ml

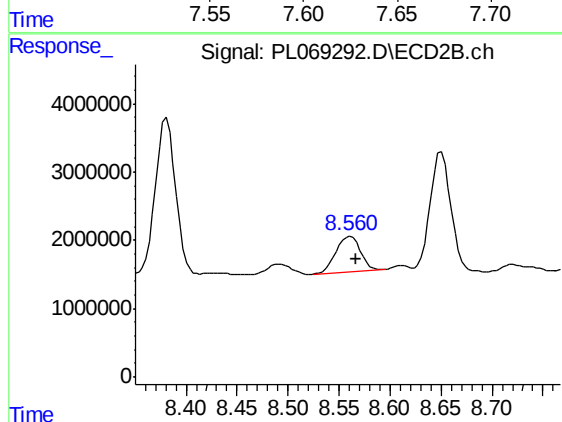

#12 4,4'-DDE


R.T.: 8.561 min
Delta R.T.: -0.006 min
Response: 8695204
Conc: 6.22 ng/ml

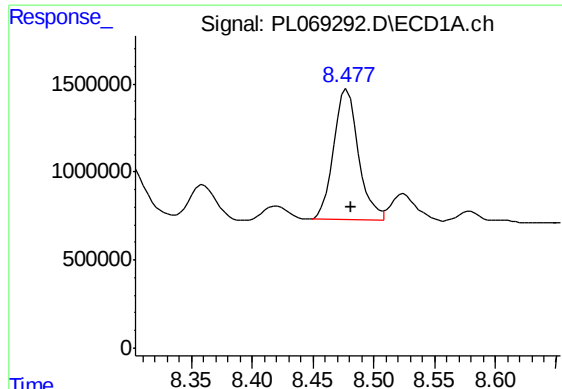

#17 4,4'-DDT


R.T.: 8.478 min
Delta R.T.: -0.004 min
Response: 10517912
Conc: 18.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
2021-08-11-FD-02

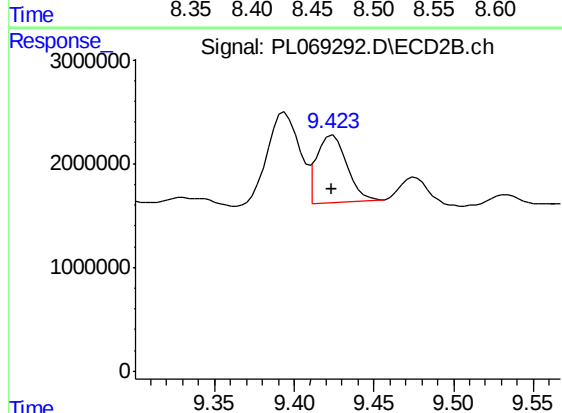


#17 4,4'-DDT

R.T.: 9.424 min
Delta R.T.: 0.000 min
Response: 8634757
Conc: 7.05 ng/ml

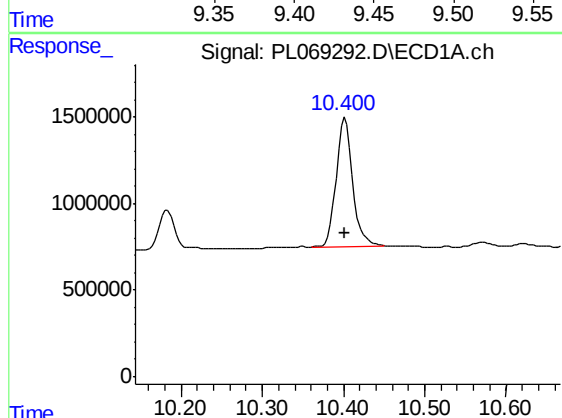

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 10497928
Conc: 15.55 ng/ml

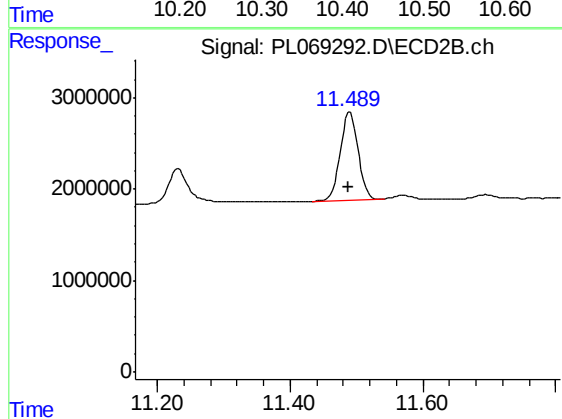

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: 0.002 min
Response: 18092300
Conc: 14.76 ng/ml