

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
 Data File : PL069320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 06:48
 Operator : AR\AJ
 Sample : M3475-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N5868-N34145

Manual Integrations
 APPROVED

mohammad
 8/24/2021 10:26:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 04:45:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.567	6989911	17789237	15.150	12.418
28)	SA Decachlor...	10.400	11.489	7821617	21039700	11.589	17.167 #
Target Compounds							
13)	MA Dieldrin	7.769	8.717	2736355	7472561	4.506m	5.322

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
Data File : PL069320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 06:48
Operator : AR\AJ
Sample : M3475-01
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
N5868-N34145


Manual Integrations
APPROVED

mohammad
8/24/2021 10:26:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 04:45:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

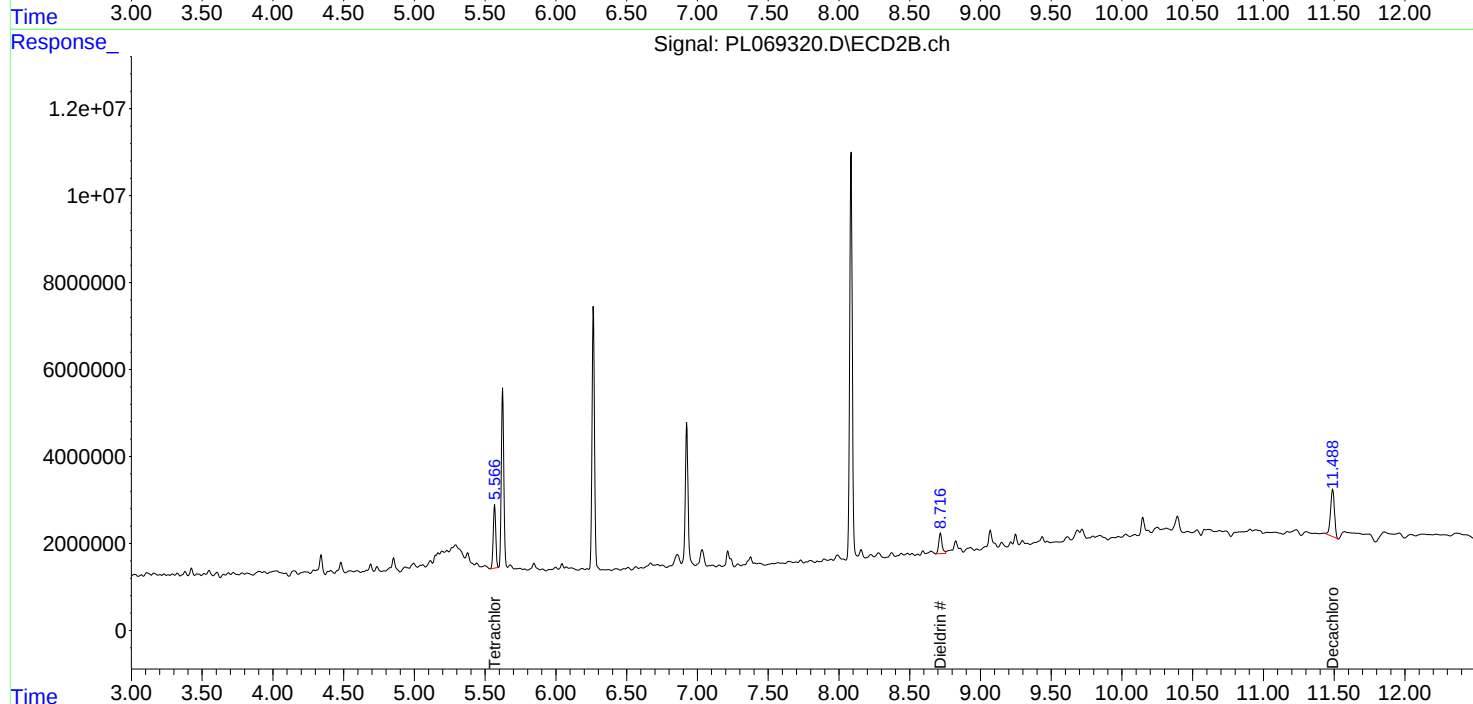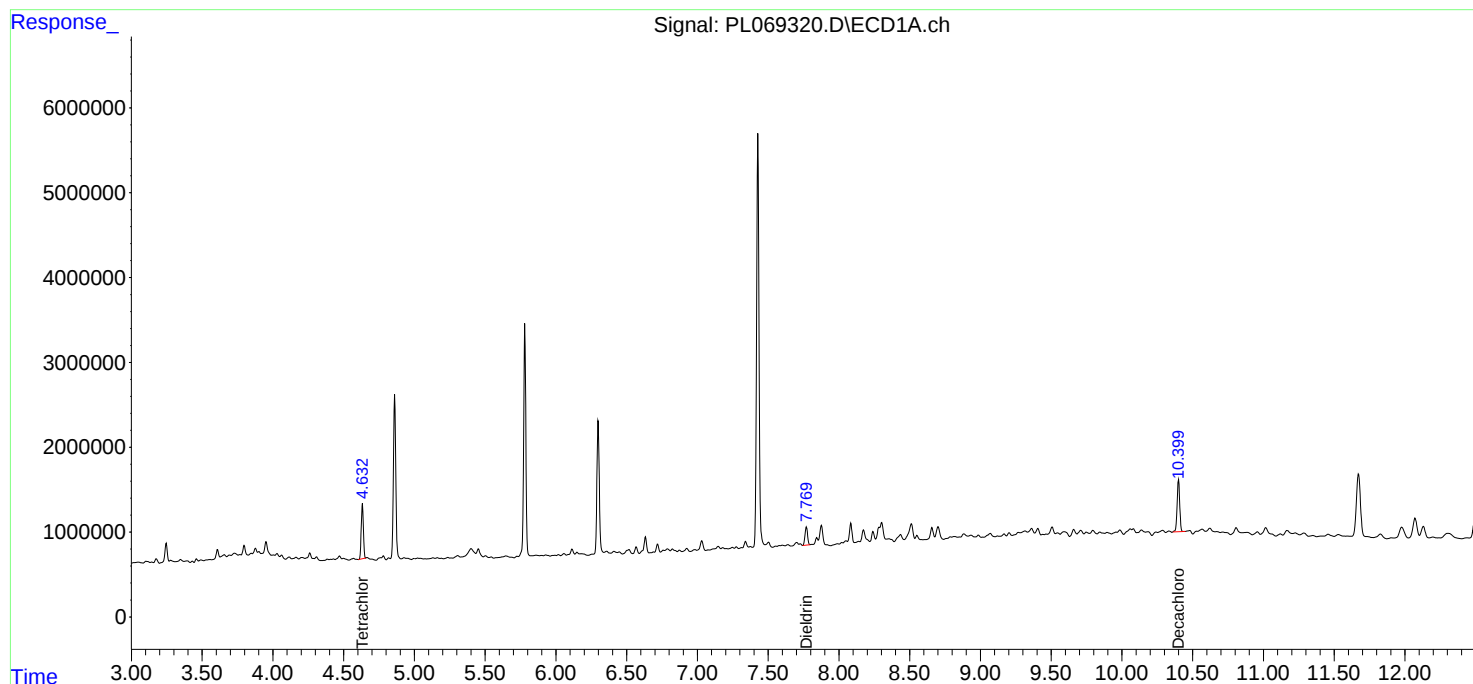

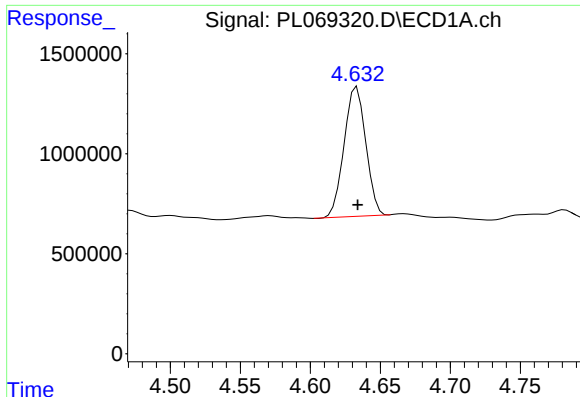


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 6989911
Conc: 15.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
N5868-N34145


Manual Integrations
APPROVED

mohammad
8/24/2021 10:26:50 AM

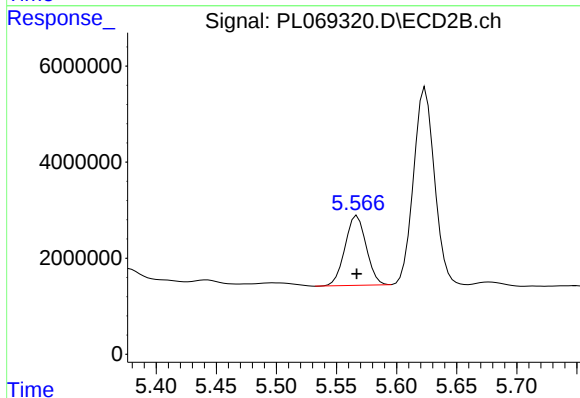


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 17789237
Conc: 12.42 ng/ml

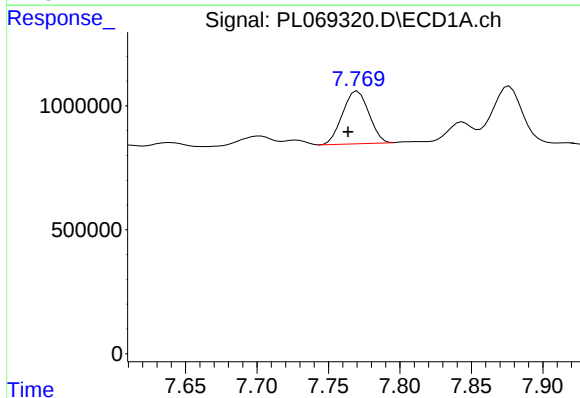


#13 Dieldrin

R.T.: 7.769 min
Delta R.T.: 0.005 min
Response: 2736355
Conc: 4.51 ng/ml m

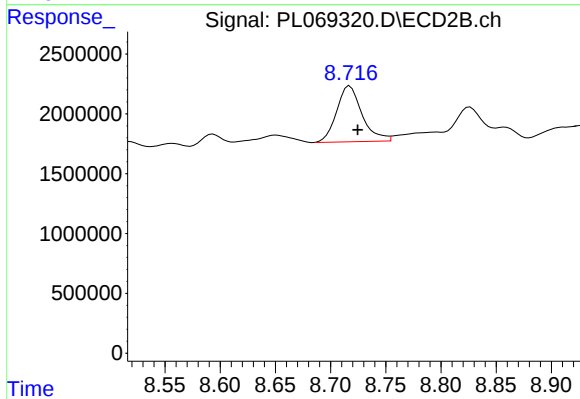

#13 Dieldrin

R.T.: 8.717 min
Delta R.T.: -0.007 min
Response: 7472561
Conc: 5.32 ng/ml

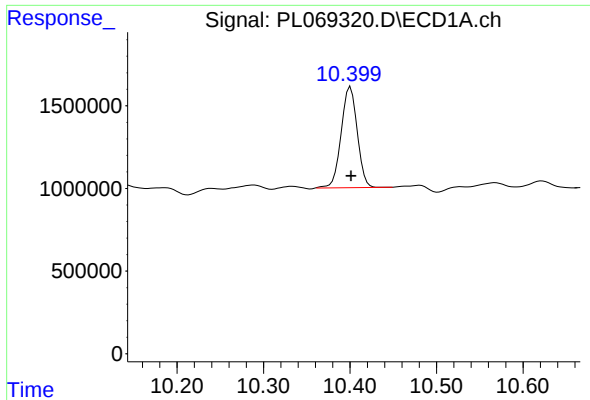


#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: 0.000 min
Response: 7821617
Conc: 11.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
N5868-N34145

Manual Integrations
APPROVED

mohammad
8/24/2021 10:26:50 AM

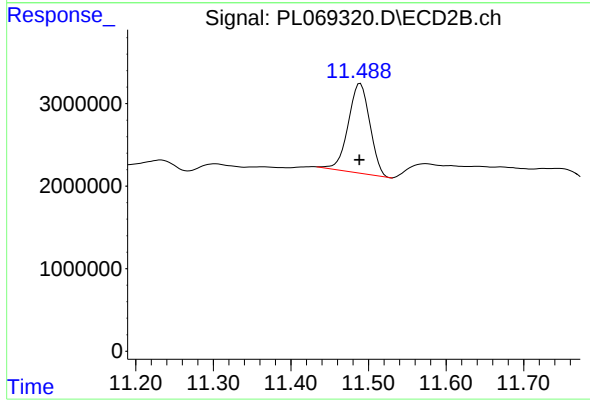

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: 0.001 min
Response: 21039700
Conc: 17.17 ng/ml