

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
 Data File : PL069336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 15:20
 Operator : AR\AJ
 Sample : M3467-03MSD
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-10-(410.75)MSD

Manual Integrations
 APPROVED

mohammad
 8/24/2021 10:25:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 04:50:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.568	9570980	31783418	20.745	22.188
28)	SA Decachlor...	10.402	11.489	10365461	21773590	15.357	17.766m
Target Compounds							
2)	A alpha-BHC	5.340	6.148	29339444	90311797	45.834	46.170
3)	MA gamma-BHC...	5.763	6.544	30220889	82747180	47.302	45.092
4)	MA Heptachlor	6.173	7.193	32707860	83585799	47.226	45.866
5)	MB Aldrin	6.498	7.564	31219596	77949396	50.598	46.898
6)	B beta-BHC	6.142	6.796	15597497	41385071	49.160	44.037
7)	B delta-BHC	6.403	7.064	15162964	43503808	24.390	23.555
8)	B Heptachlo...	7.074	8.031	30207034	70579450	48.662	46.920
9)	A Endosulfan I	7.477	8.436	29431802	65867486	49.713m	47.622
10)	B gamma-Chl...	7.352	8.300	31856380	75851903	49.772	49.308
11)	B alpha-Chl...	7.422	8.381	31090464	72412752	47.713	48.463
12)	B 4,4'-DDE	7.636	8.567	28879604	60057305	51.063	42.934
13)	MA Dieldrin	7.763	8.726	32196347	66465353	53.021m	47.333
14)	MA Endrin	8.055	8.965	28944644	56675641	50.117	48.287
15)	B Endosulfa...	8.365	9.198	27479205	57592583	49.457	48.671
16)	A 4,4'-DDD	8.220	9.108	24117182	59295388	47.421	48.341
17)	MA 4,4'-DDT	8.482	9.425	27158169	54043347	47.182	44.111
18)	B Endrin al...	8.553	9.333	23972637	48690296	52.855	51.187
19)	B Endosulfa...	8.784	9.571	26687592	49501413	44.951	43.571
20)	A Methoxychlor	9.075	9.909	16336385	28532705	43.617m	44.444m
21)	B Endrin ke...	9.303	10.069	31894899	56775568	45.966	43.882
22)	Mirex	9.490	10.536	26271292	43563820	44.171m	46.483

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
Data File : PL069336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 15:20
Operator : AR\AJ
Sample : M3467-03MSD
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 04:50:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

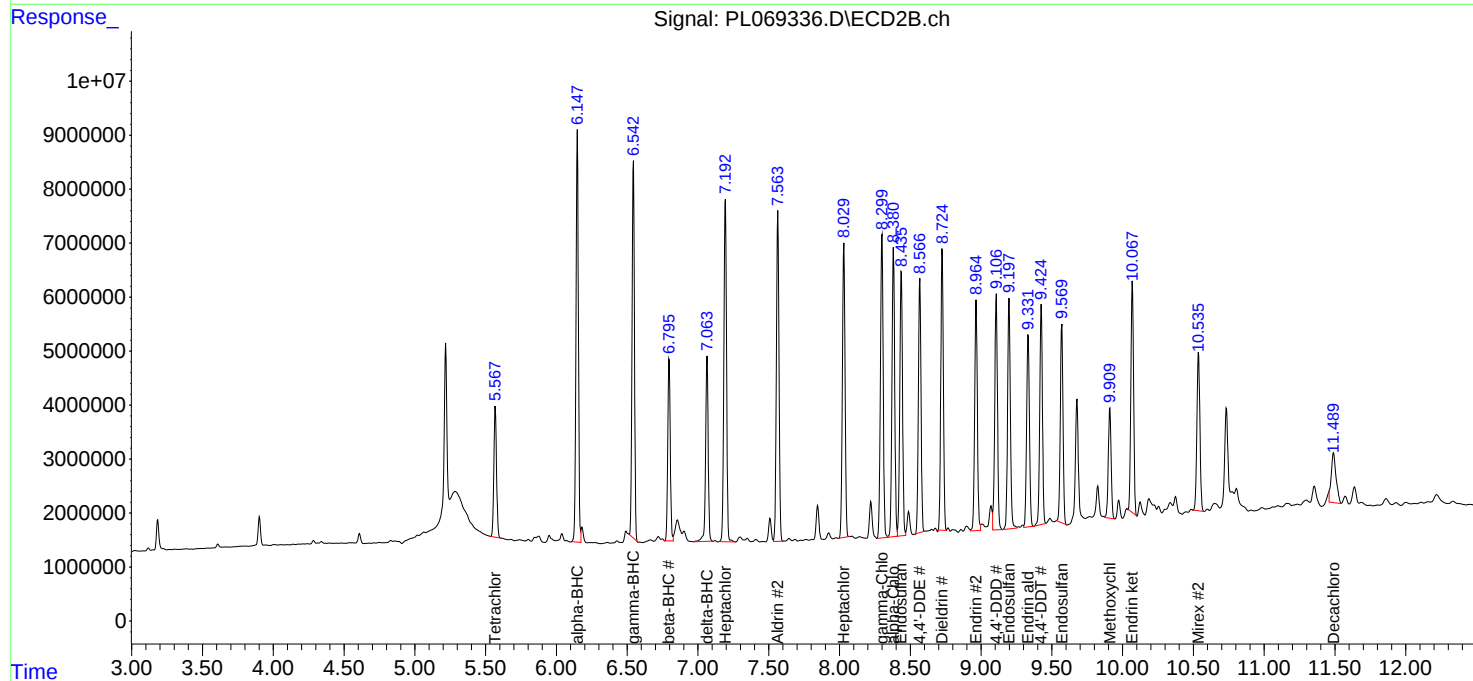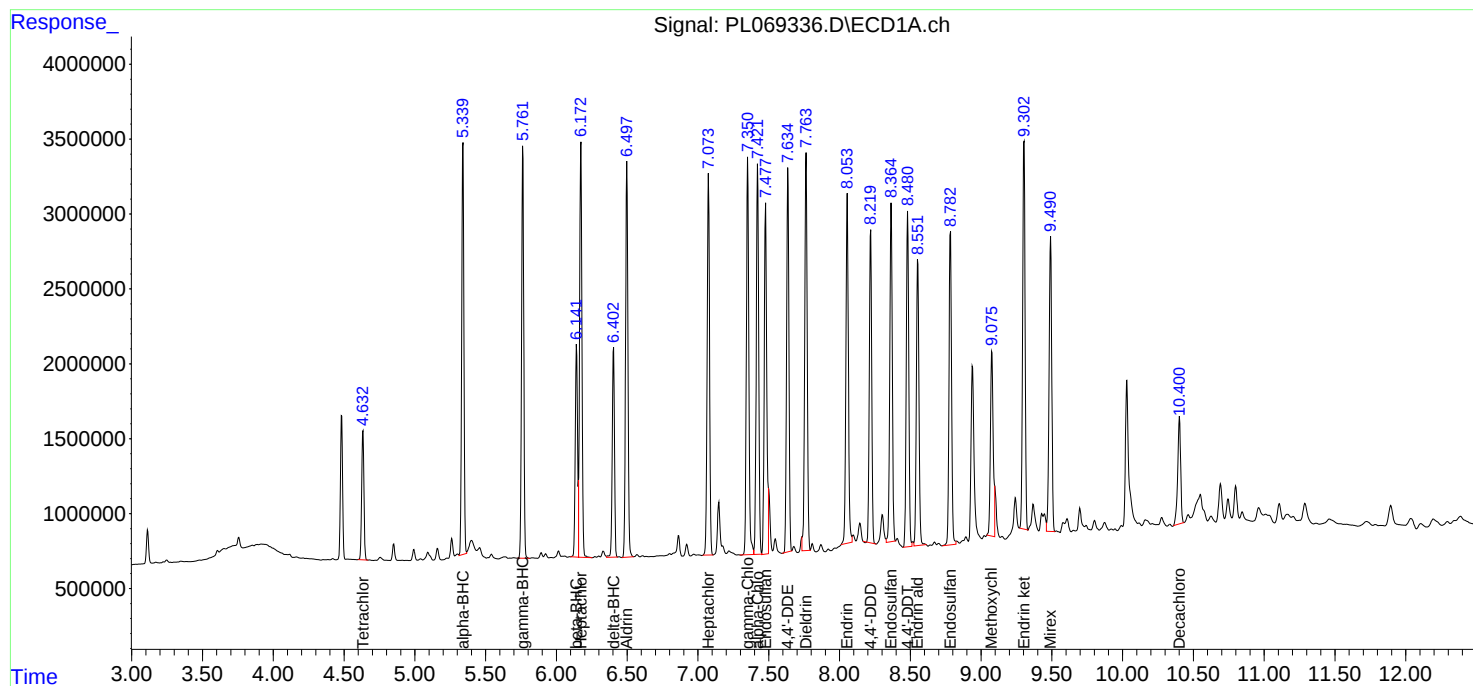

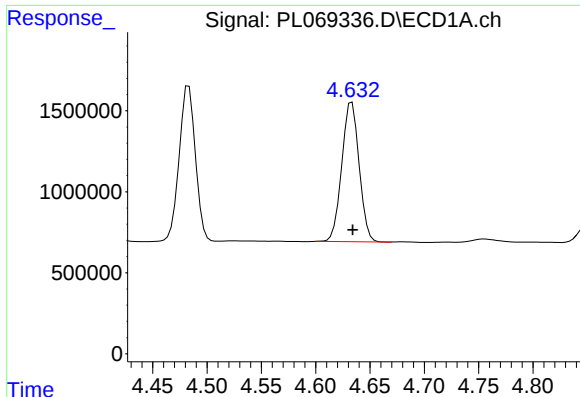


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 9570980
Conc: 20.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

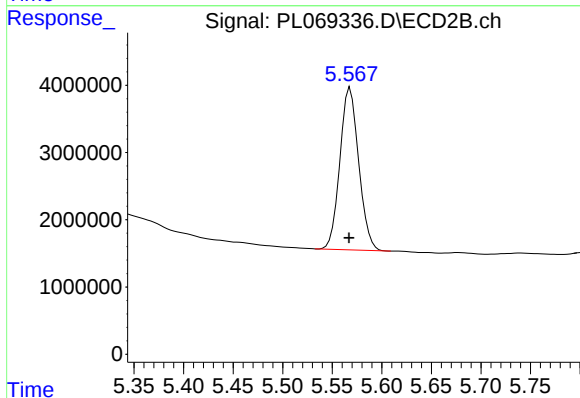


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: 0.001 min
Response: 31783418
Conc: 22.19 ng/ml

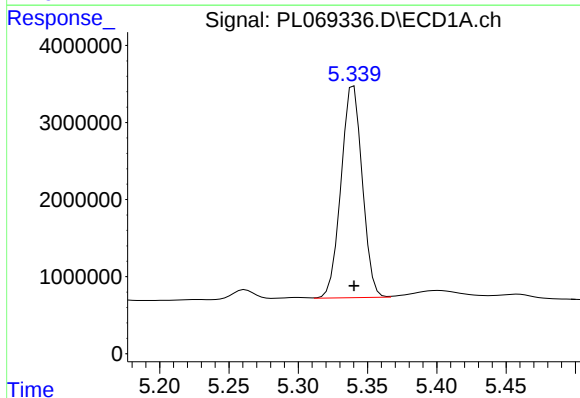


#2 alpha-BHC

R.T.: 5.340 min
Delta R.T.: 0.000 min
Response: 29339444
Conc: 45.83 ng/ml

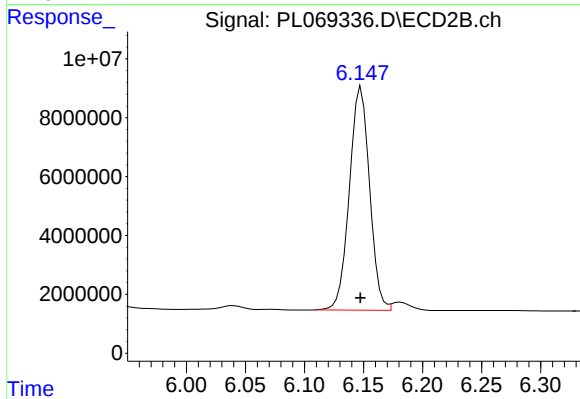

#2 alpha-BHC

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 90311797
Conc: 46.17 ng/ml

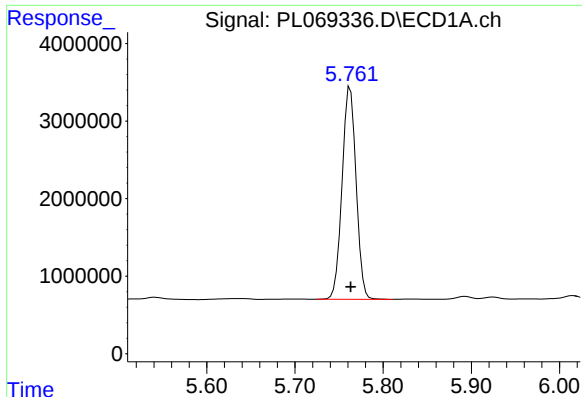


#3 gamma-BHC (Lindane)

R.T.: 5.763 min
Delta R.T.: 0.000 min
Response: 30220889
Conc: 47.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

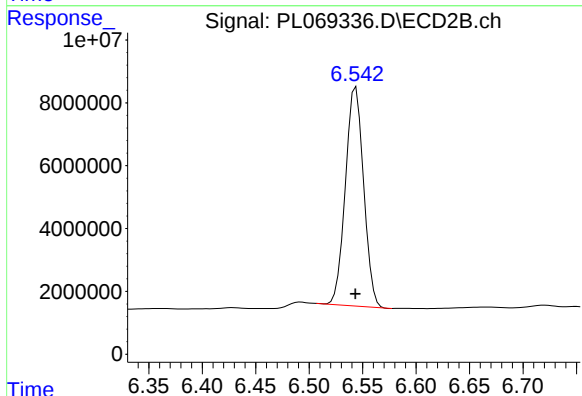


#3 gamma-BHC (Lindane)

R.T.: 6.544 min
Delta R.T.: 0.000 min
Response: 82747180
Conc: 45.09 ng/ml

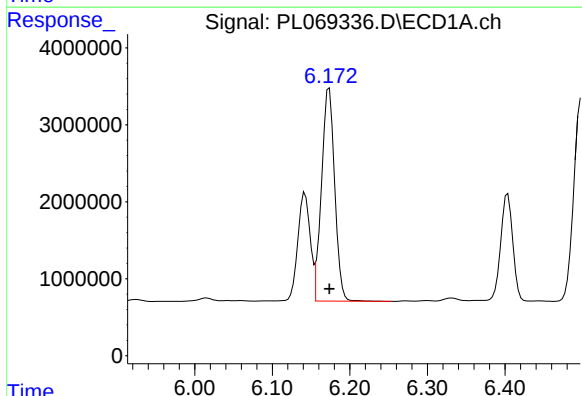


#4 Heptachlor

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 32707860
Conc: 47.23 ng/ml

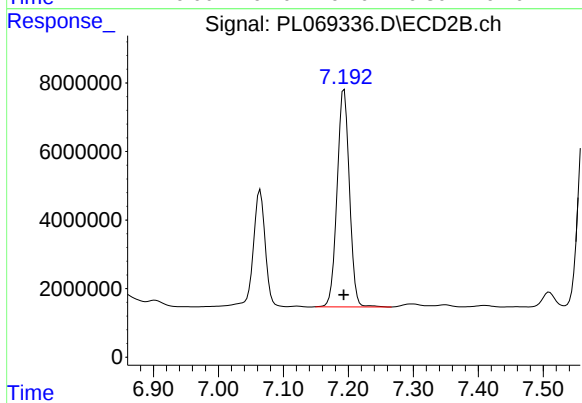

#4 Heptachlor

R.T.: 7.193 min
Delta R.T.: 0.000 min
Response: 83585799
Conc: 45.87 ng/ml

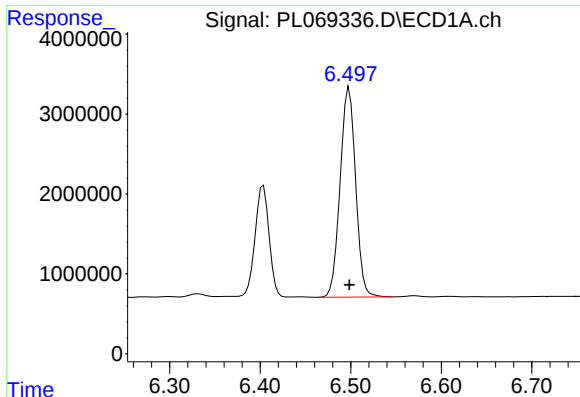


#5 Aldrin

R.T.: 6.498 min
Delta R.T.: 0.000 min
Response: 31219596
Conc: 50.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

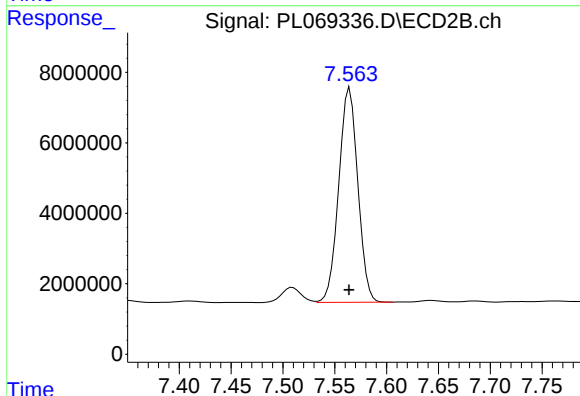


#5 Aldrin

R.T.: 7.564 min
Delta R.T.: 0.000 min
Response: 77949396
Conc: 46.90 ng/ml

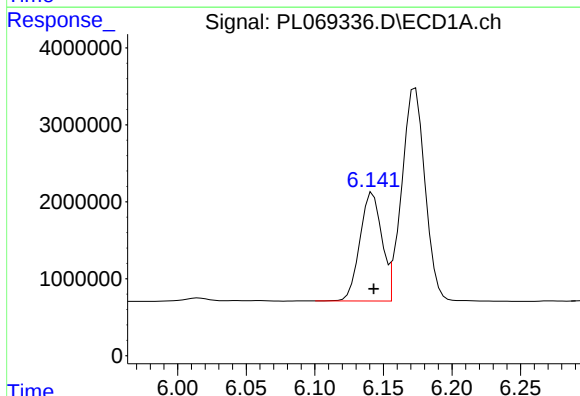


#6 beta-BHC

R.T.: 6.142 min
Delta R.T.: 0.000 min
Response: 15597497
Conc: 49.16 ng/ml

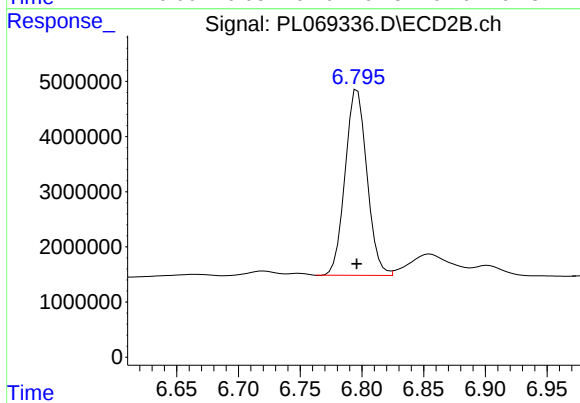

#6 beta-BHC

R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 41385071
Conc: 44.04 ng/ml

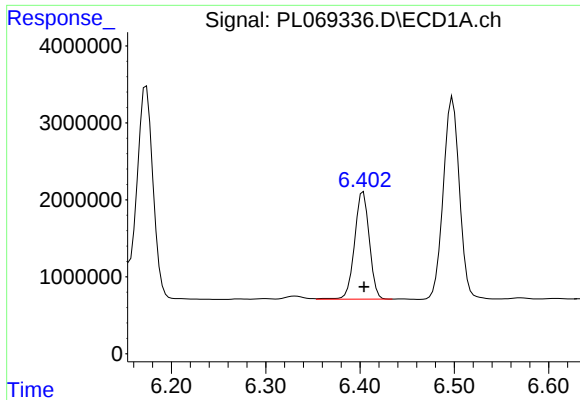


#7 delta-BHC

R.T.: 6.403 min
Delta R.T.: 0.000 min
Response: 15162964
Conc: 24.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

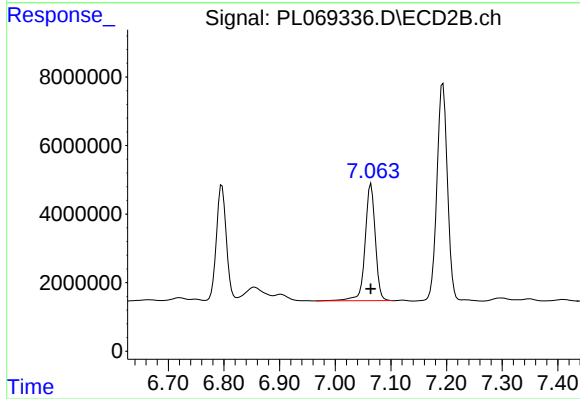


#7 delta-BHC

R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 43503808
Conc: 23.55 ng/ml

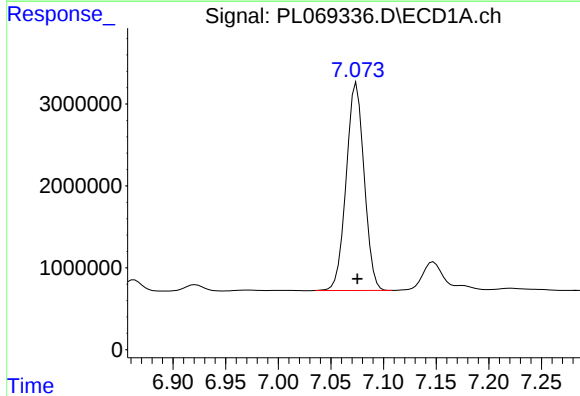


#8 Heptachlor epoxide

R.T.: 7.074 min
Delta R.T.: 0.000 min
Response: 30207034
Conc: 48.66 ng/ml

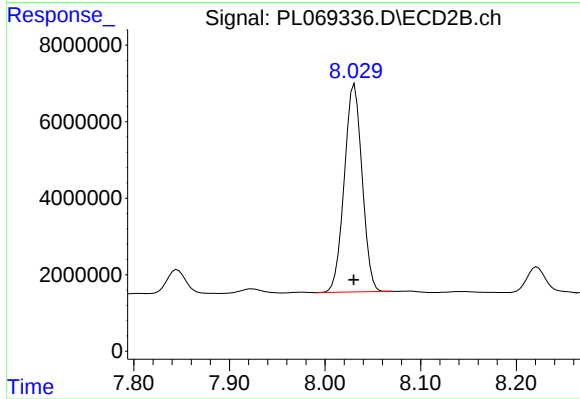

#8 Heptachlor epoxide

R.T.: 8.031 min
Delta R.T.: 0.000 min
Response: 70579450
Conc: 46.92 ng/ml

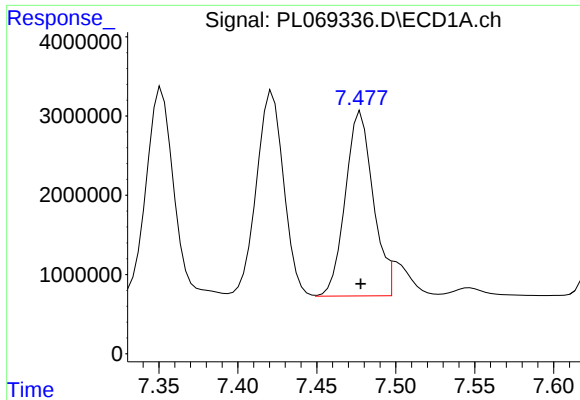


#9 Endosulfan I

R.T.: 7.477 min
Delta R.T.: -0.001 min
Response: 29431802
Conc: 49.71 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

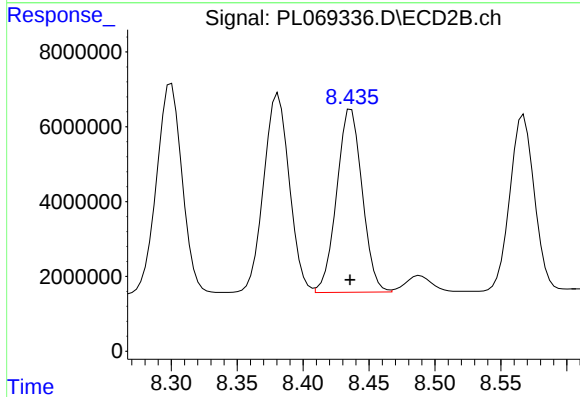


#9 Endosulfan I

R.T.: 8.436 min
Delta R.T.: 0.000 min
Response: 65867486
Conc: 47.62 ng/ml

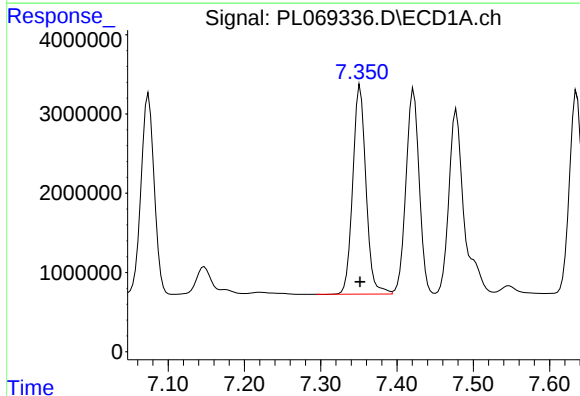


#10 gamma-Chlordane

R.T.: 7.352 min
Delta R.T.: 0.000 min
Response: 31856380
Conc: 49.77 ng/ml

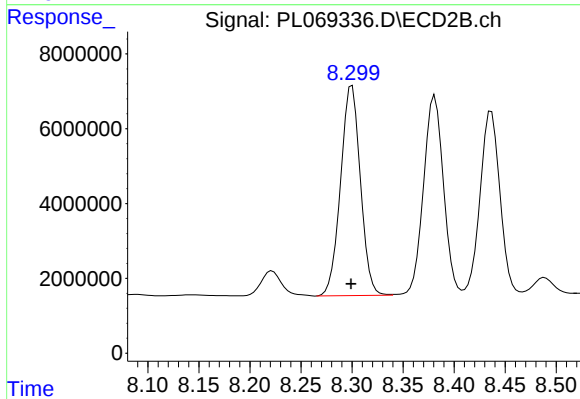

#10 gamma-Chlordane

R.T.: 8.300 min
Delta R.T.: 0.001 min
Response: 75851903
Conc: 49.31 ng/ml

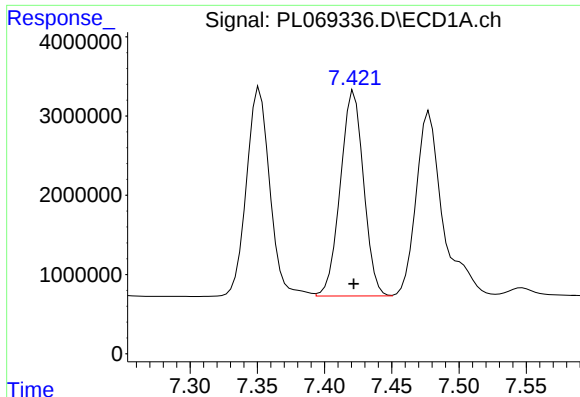


#11 alpha-Chlordane

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 31090464
Conc: 47.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

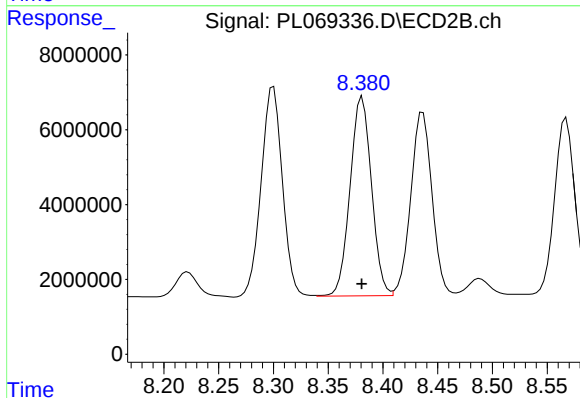


#11 alpha-Chlordane

R.T.: 8.381 min
Delta R.T.: 0.000 min
Response: 72412752
Conc: 48.46 ng/ml

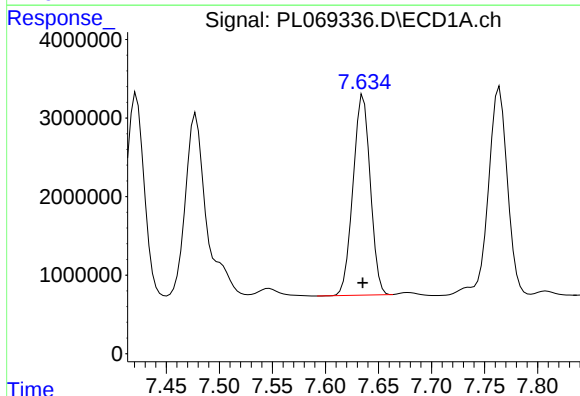


#12 4,4'-DDE

R.T.: 7.636 min
Delta R.T.: 0.000 min
Response: 28879604
Conc: 51.06 ng/ml

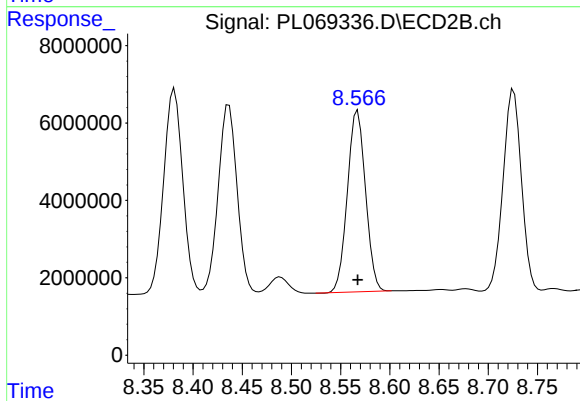

#12 4,4'-DDE

R.T.: 8.567 min
Delta R.T.: 0.000 min
Response: 60057305
Conc: 42.93 ng/ml

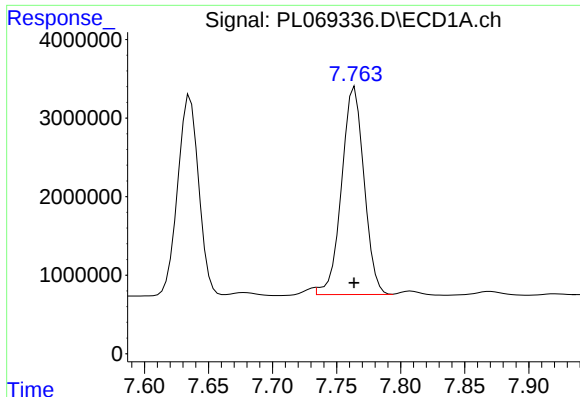


#13 Dieldrin

R.T.: 7.763 min
Delta R.T.: 0.000 min
Response: 32196347
Conc: 53.02 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

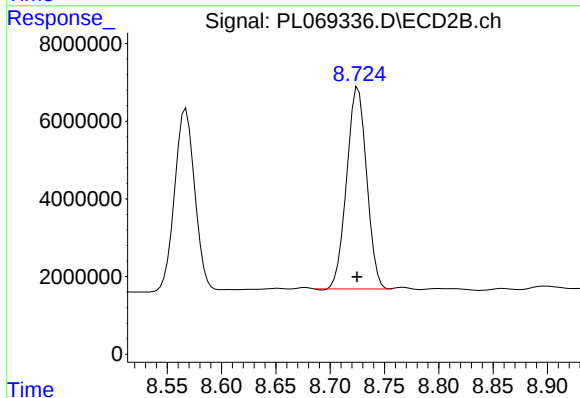


#13 Dieldrin

R.T.: 8.726 min
Delta R.T.: 0.001 min
Response: 66465353
Conc: 47.33 ng/ml

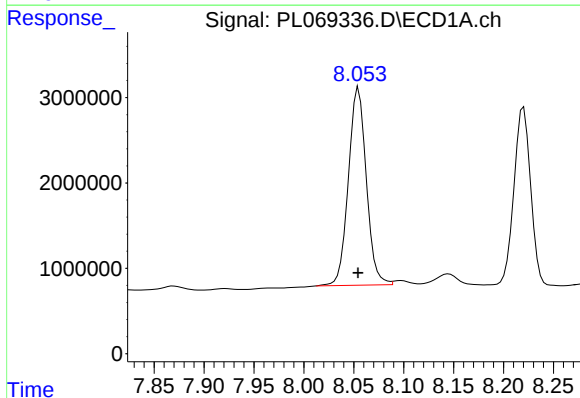


#14 Endrin

R.T.: 8.055 min
Delta R.T.: 0.000 min
Response: 28944644
Conc: 50.12 ng/ml

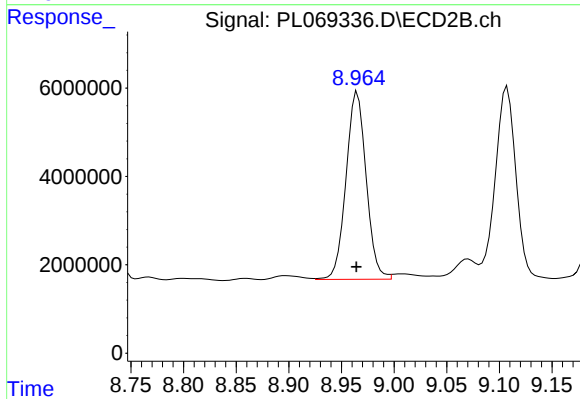

#14 Endrin

R.T.: 8.965 min
Delta R.T.: 0.001 min
Response: 56675641
Conc: 48.29 ng/ml

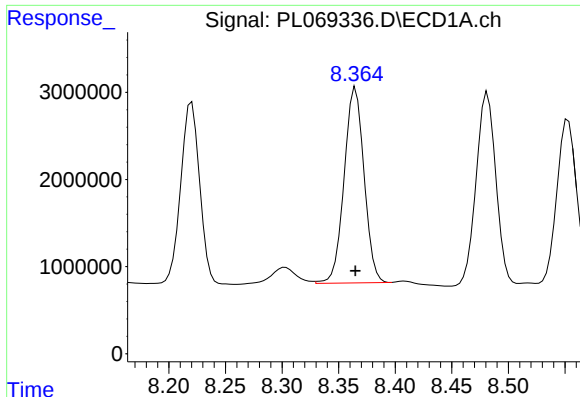


#15 Endosulfan II

R.T.: 8.365 min
Delta R.T.: 0.000 min
Response: 27479205
Conc: 49.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

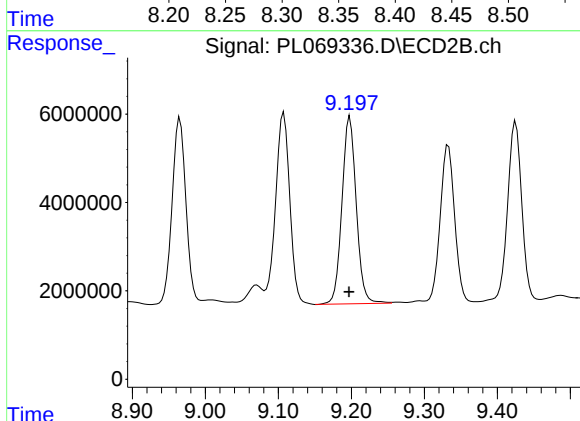


#15 Endosulfan II

R.T.: 9.198 min
Delta R.T.: 0.001 min
Response: 57592583
Conc: 48.67 ng/ml

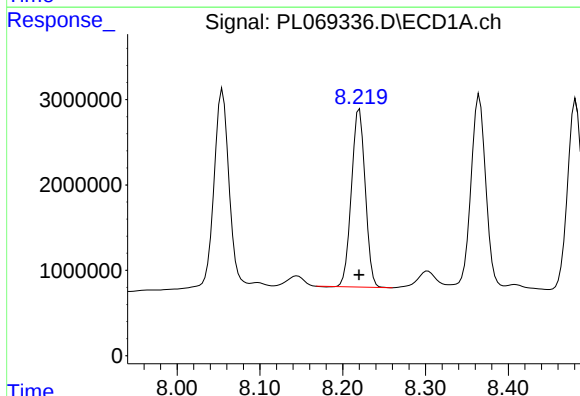


#16 4,4'-DDD

R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 24117182
Conc: 47.42 ng/ml

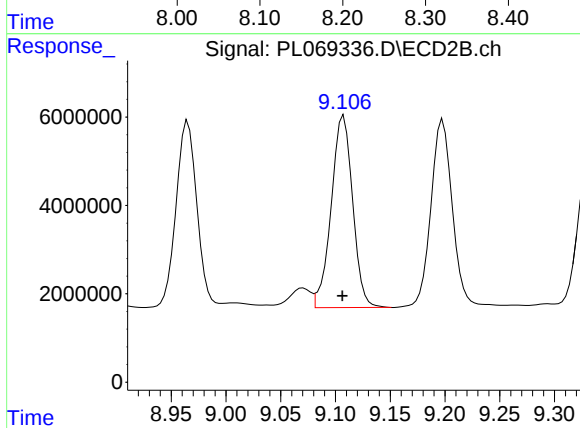

#16 4,4'-DDD

R.T.: 9.108 min
Delta R.T.: 0.001 min
Response: 59295388
Conc: 48.34 ng/ml

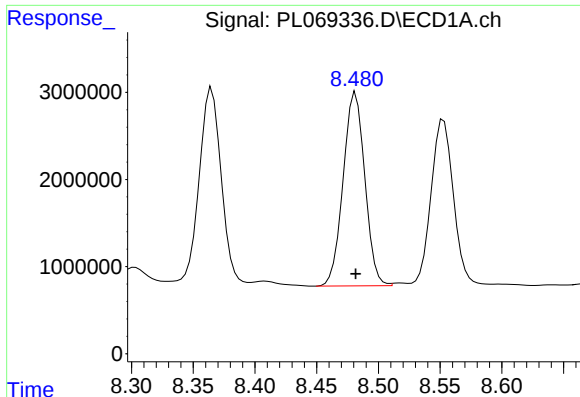


#17 4,4'-DDT

R.T.: 8.482 min
Delta R.T.: 0.000 min
Response: 27158169
Conc: 47.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

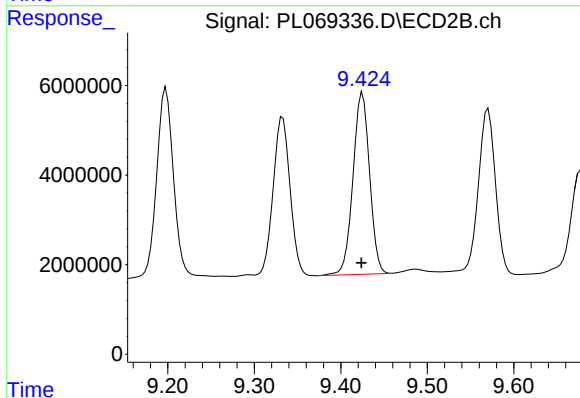


#17 4,4'-DDT

R.T.: 9.425 min
Delta R.T.: 0.001 min
Response: 54043347
Conc: 44.11 ng/ml

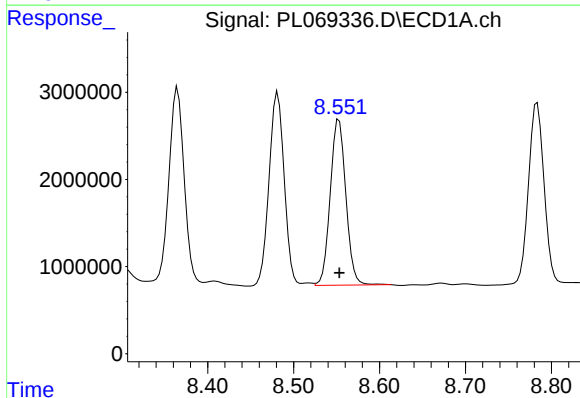


#18 Endrin aldehyde

R.T.: 8.553 min
Delta R.T.: 0.000 min
Response: 23972637
Conc: 52.86 ng/ml

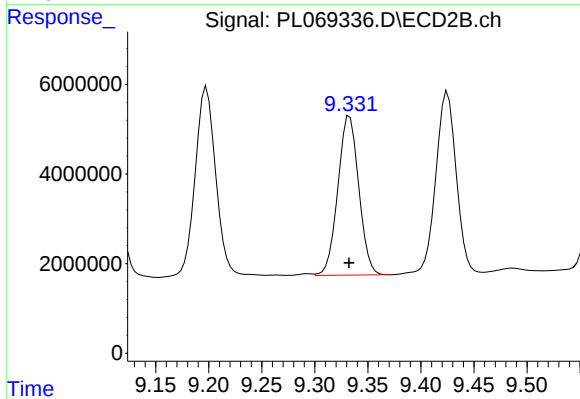

#18 Endrin aldehyde

R.T.: 9.333 min
Delta R.T.: 0.000 min
Response: 48690296
Conc: 51.19 ng/ml

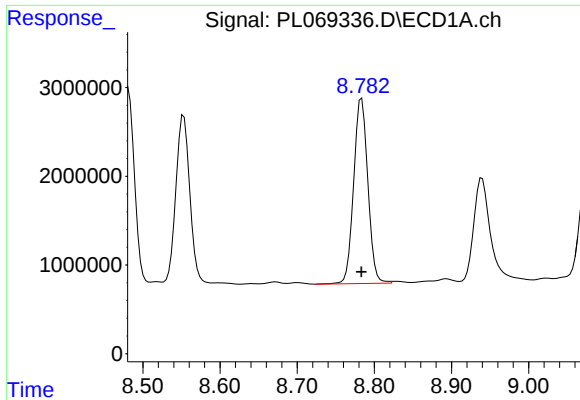


#19 Endosulfan Sulfate

R.T.: 8.784 min
Delta R.T.: 0.000 min
Response: 26687592
Conc: 44.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

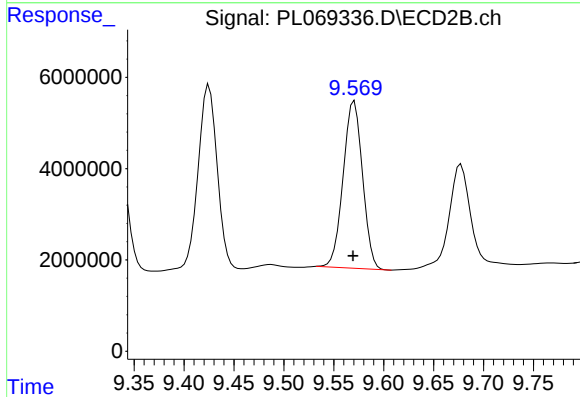


#19 Endosulfan Sulfate

R.T.: 9.571 min
Delta R.T.: 0.001 min
Response: 49501413
Conc: 43.57 ng/ml

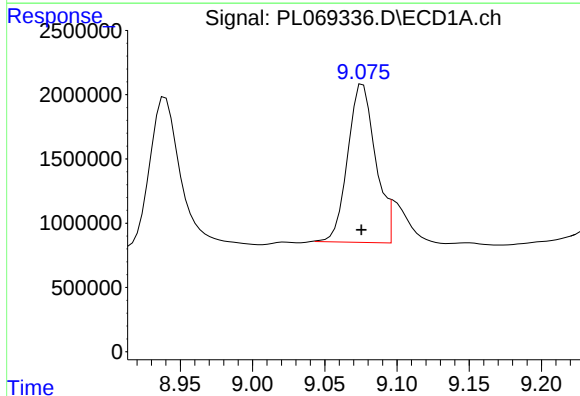


#20 Methoxychlor

R.T.: 9.075 min
Delta R.T.: 0.000 min
Response: 16336385
Conc: 43.62 ng/ml m

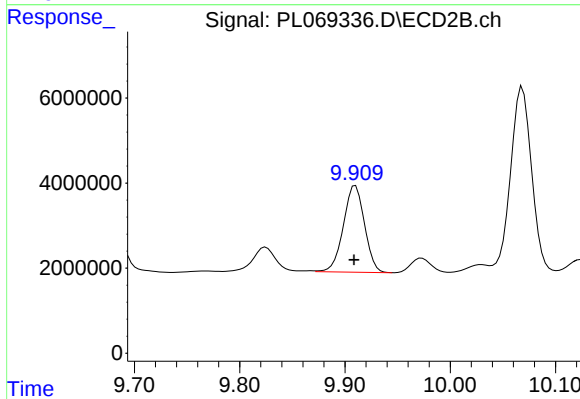

#20 Methoxychlor

R.T.: 9.909 min
Delta R.T.: 0.000 min
Response: 28532705
Conc: 44.44 ng/ml m

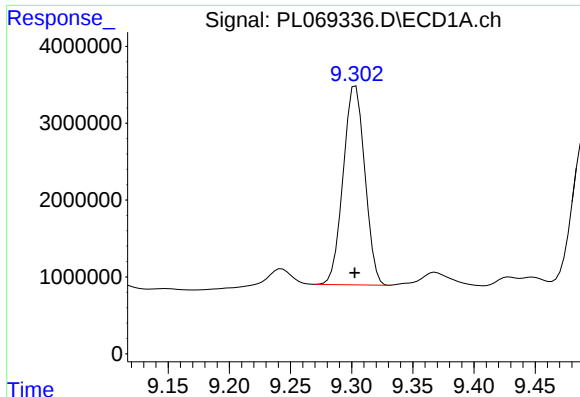


#21 Endrin ketone

R.T.: 9.303 min
Delta R.T.: 0.000 min
Response: 31894899
Conc: 45.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD


Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

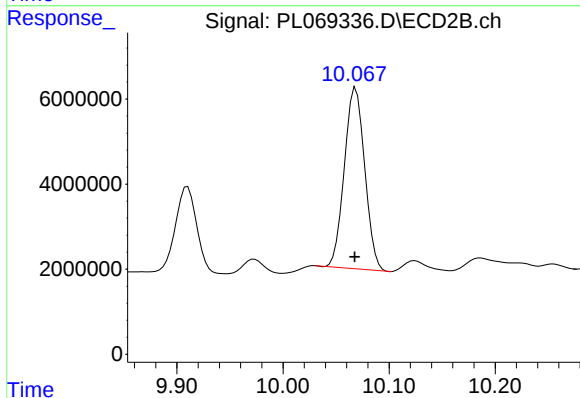


#21 Endrin ketone

R.T.: 10.069 min
Delta R.T.: 0.001 min
Response: 56775568
Conc: 43.88 ng/ml

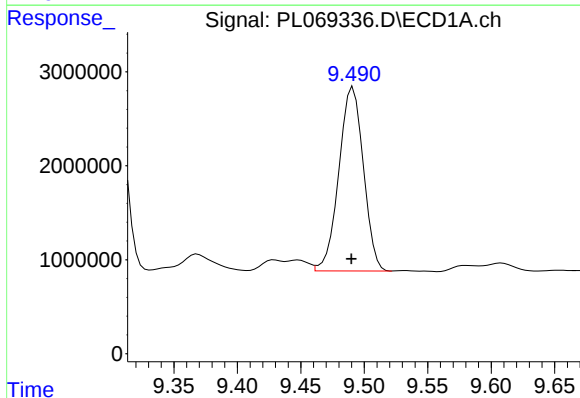


#22 Mirex

R.T.: 9.490 min
Delta R.T.: 0.000 min
Response: 26271292
Conc: 44.17 ng/ml m

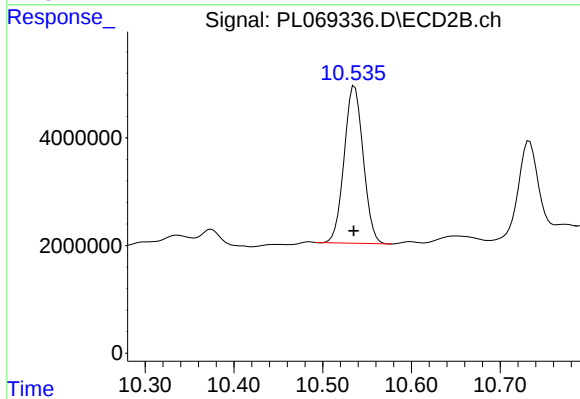

#22 Mirex

R.T.: 10.536 min
Delta R.T.: 0.001 min
Response: 43563820
Conc: 46.48 ng/ml

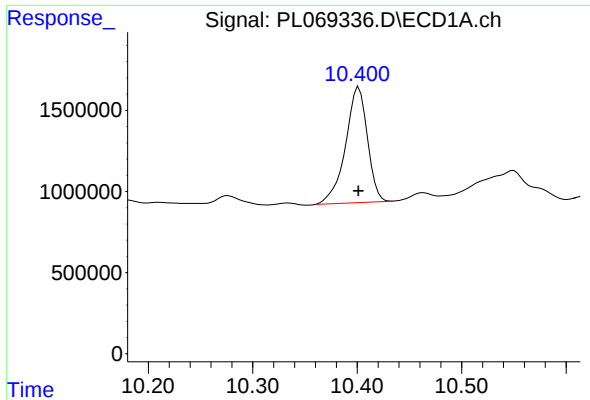


#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: 0.000 min
Response: 10365461
Conc: 15.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-10-(410.75)MSD

Manual Integrations
APPROVED

mohammad
8/24/2021 10:25:57 AM

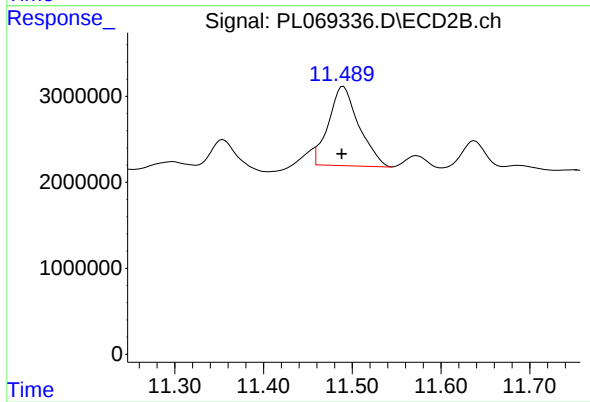

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: 0.000 min
Response: 21773590
Conc: 17.77 ng/ml m