

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
 Data File : PL069338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2021 15:53
 Operator : AR\AJ
 Sample : M3467-07
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-8-(309.00)

Manual Integrations
 APPROVED

mohammad
 8/24/2021 10:26:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 04:51:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.567	4636310	13238614	10.049	9.242
28)	SA Decachlor...	10.400	11.490	4591033	7873648	6.802	6.424
Target Compounds							
10)	B gamma-Chl...	7.349	8.298	343583	862422	0.537m	0.561m
11)	B alpha-Chl...	7.418	8.382	586119	1362333	0.899m	0.912

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082121\
Data File : PL069338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2021 15:53
Operator : AR\AJ
Sample : M3467-07
Misc :
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SAMPLE-8-(309.00)


Manual Integrations
APPROVED

mohammad
8/24/2021 10:26:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 04:51:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

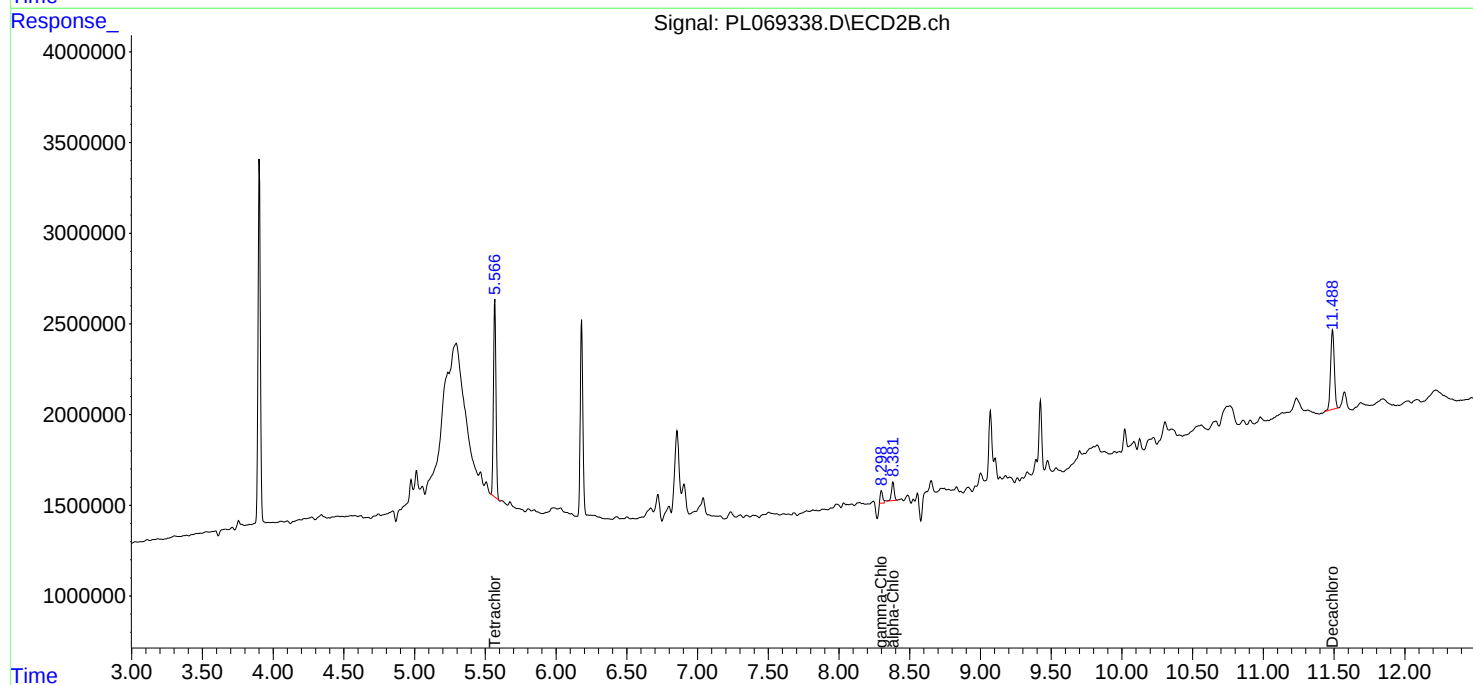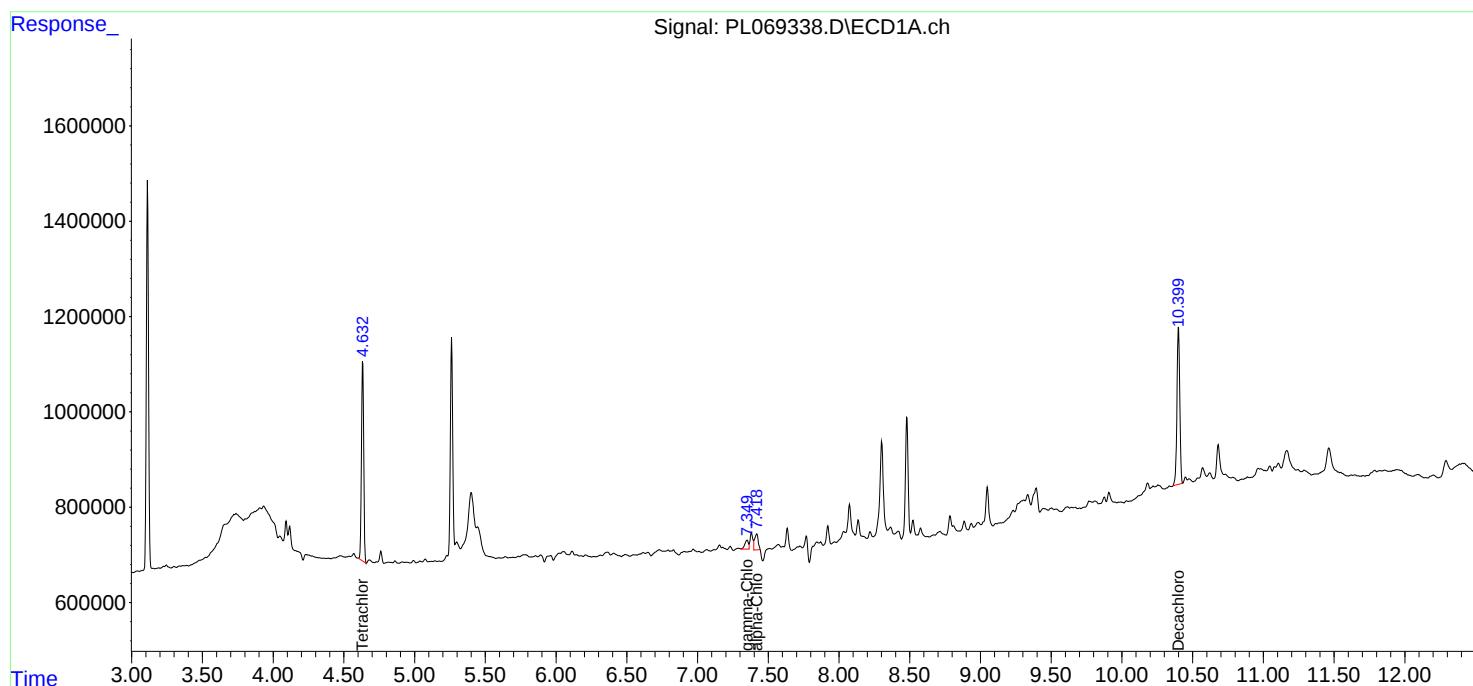

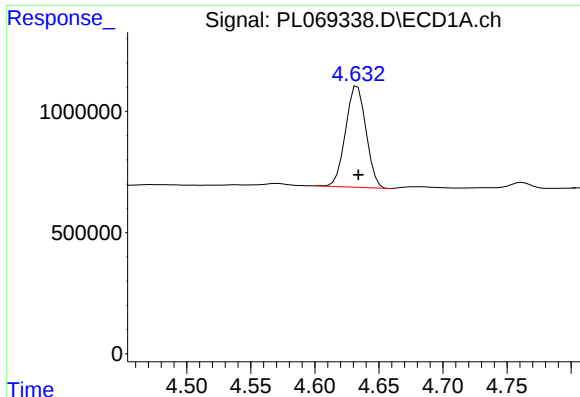


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: 0.000 min
Response: 4636310
Conc: 10.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-8-(309.00)


Manual Integrations
APPROVED

mohammad
8/24/2021 10:26:03 AM

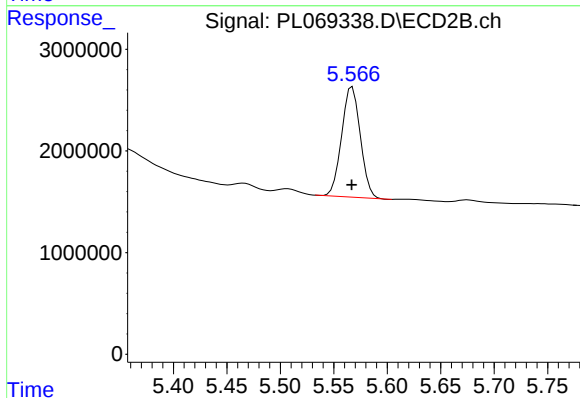


#1 Tetrachloro-m-xylene

R.T.: 5.567 min
Delta R.T.: 0.000 min
Response: 13238614
Conc: 9.24 ng/ml

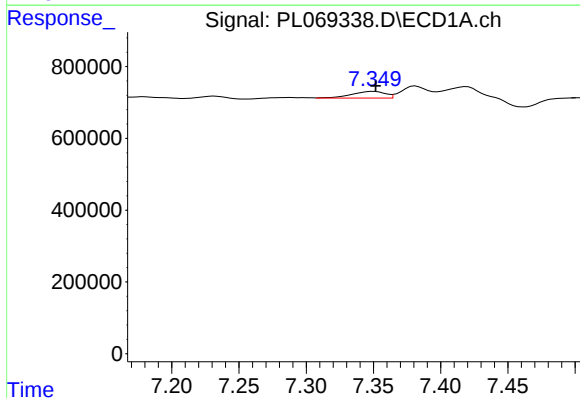


#10 gamma-Chlordane

R.T.: 7.349 min
Delta R.T.: -0.003 min
Response: 343583
Conc: 0.54 ng/ml m

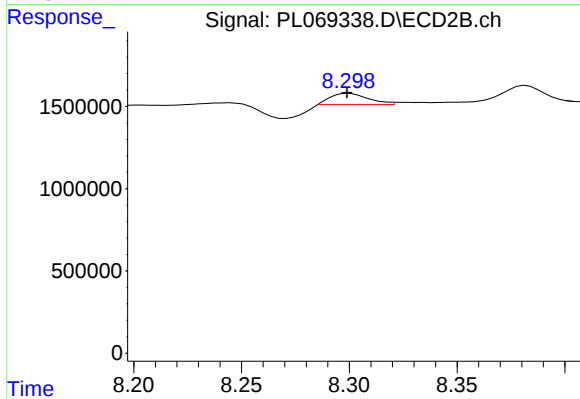

#10 gamma-Chlordane

R.T.: 8.298 min
Delta R.T.: 0.000 min
Response: 862422
Conc: 0.56 ng/ml m

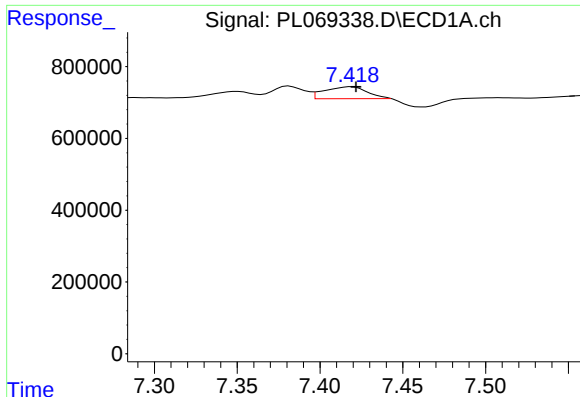


#11 alpha-Chlordane

R.T.: 7.418 min
Delta R.T.: -0.004 min
Response: 586119
Conc: 0.90 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SAMPLE-8-(309.00)


Manual Integrations
APPROVED

mohammad
8/24/2021 10:26:03 AM

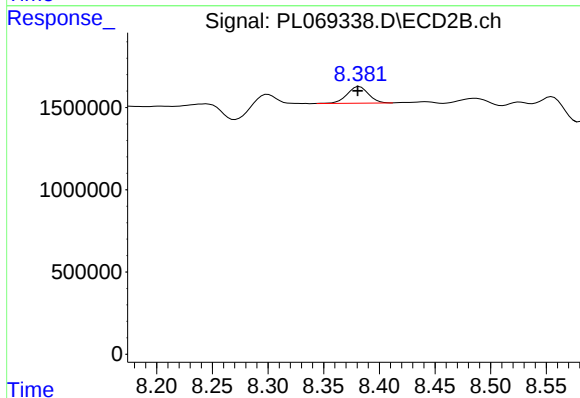


#11 alpha-Chlordane

R.T.: 8.382 min
Delta R.T.: 0.002 min
Response: 1362333
Conc: 0.91 ng/ml

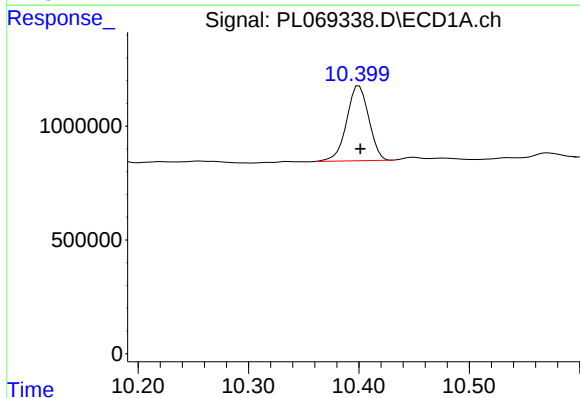

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.001 min
Response: 4591033
Conc: 6.80 ng/ml

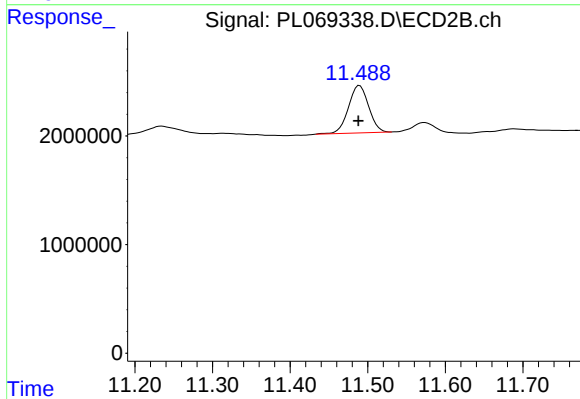

#28 Decachlorobiphenyl

R.T.: 11.490 min
Delta R.T.: 0.001 min
Response: 7873648
Conc: 6.42 ng/ml