

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
 Data File : PL084888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 16:34
 Operator : AR\AJ
 Sample : 04049-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:35:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.478	2.686	50742374	24345429	20.241	20.623
27)	SA Decachlor...	9.028	7.865	55822662	43775008	32.573	32.321
Target Compounds							
2)	A alpha-BHC	3.964f	0.000	448002	0	0.124	N.D. #
3)	MA gamma-BHC...	4.250	0.000	394859	0	0.114	N.D. #
4)	MA Heptachlor	4.859	0.000	3880231	0	1.002	N.D. #
5)	MB Aldrin	5.213	0.000	228845	0	<MDL	N.D. #
6)	B beta-BHC	4.457	3.791f	361778	26703983	0.205	32.506 #
7)	B delta-BHC	4.717	0.000	85353412	0	23.391	N.D. #
9)	A Endosulfan I	6.032	0.000	428333	0	0.150	N.D. #
10)	B trans-Chl...	5.887	0.000	2086384	0	0.661	N.D. #
11)	B cis-Chlor...	6.032f	0.000	428333	0	0.134	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 16:34
Operator : AR\AJ
Sample : 04049-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:35:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

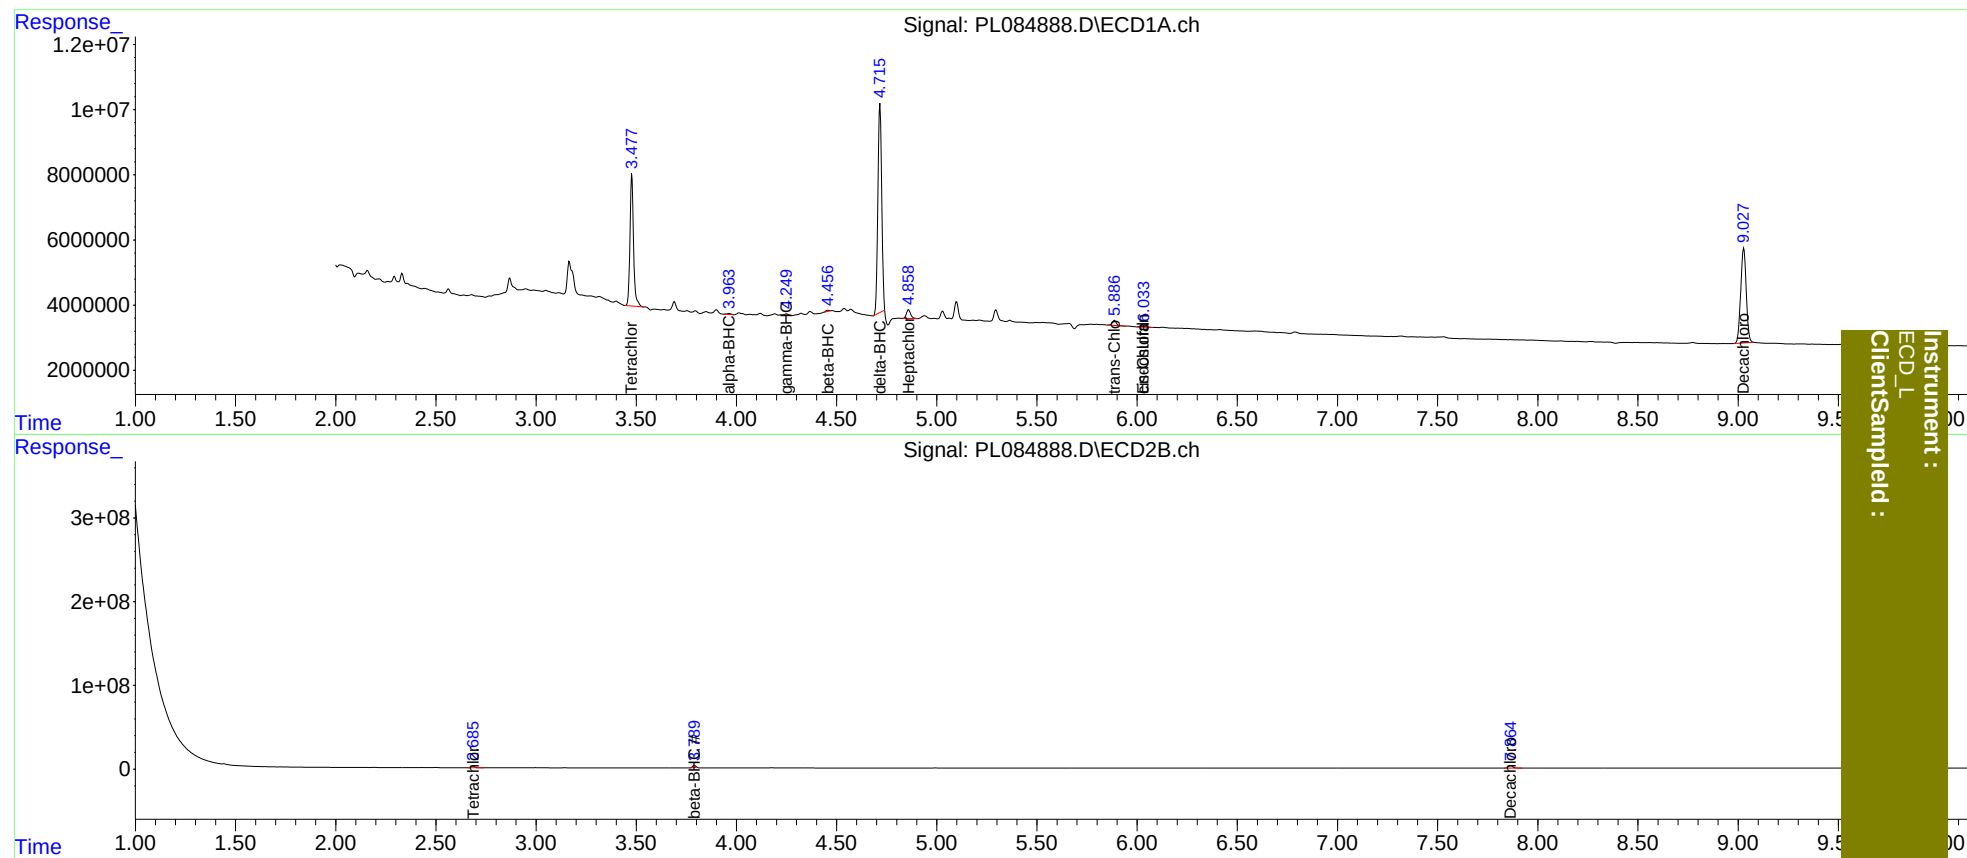


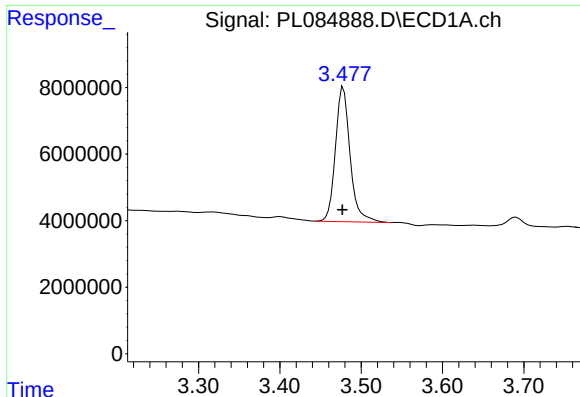

#1 Tetrachloro-m-xylene


R.T.: 3.478 min
Delta R.T.: 0.001 min
Response: 50742374
Conc: 20.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

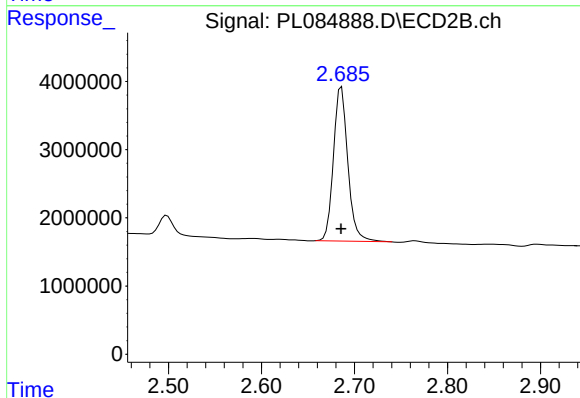


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 24345429
Conc: 20.62 ng/ml

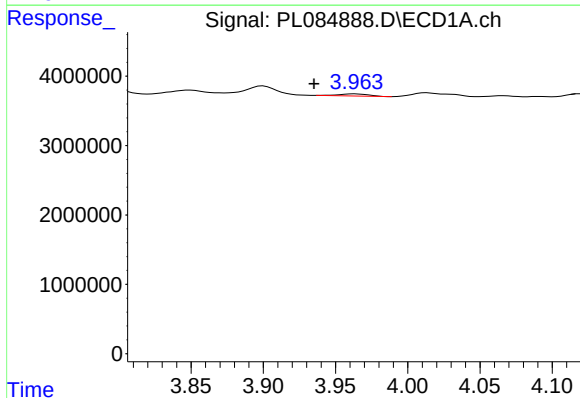


#2 alpha-BHC

R.T.: 3.964 min
Delta R.T.: 0.029 min
Response: 448002
Conc: 0.12 ng/ml

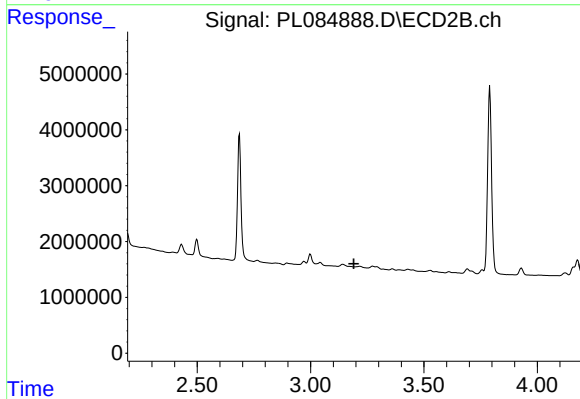

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.190 min
Response: 0
Conc: N.D.

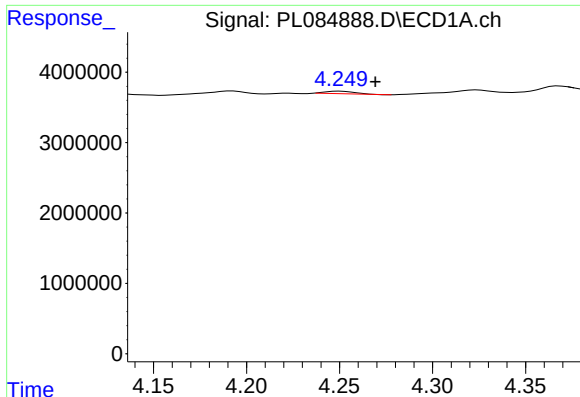

#3 gamma-BHC (Lindane)


R.T.: 4.250 min
Delta R.T.: -0.020 min
Response: 394859
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

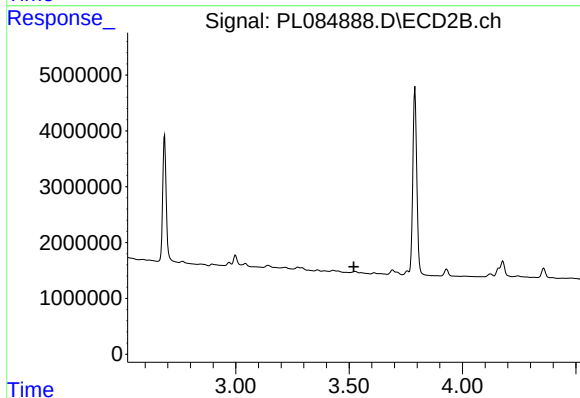


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.521 min
Response: 0
Conc: N.D.

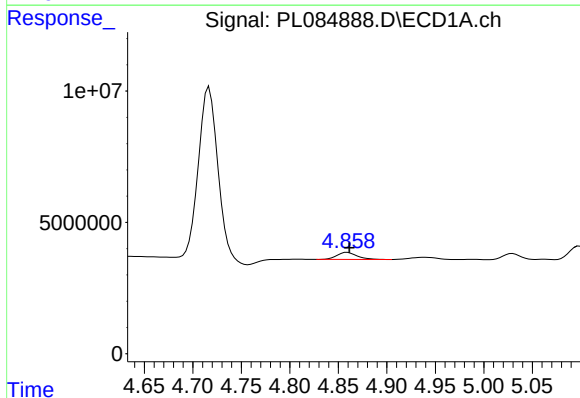


#4 Heptachlor

R.T.: 4.859 min
Delta R.T.: -0.002 min
Response: 3880231
Conc: 1.00 ng/ml

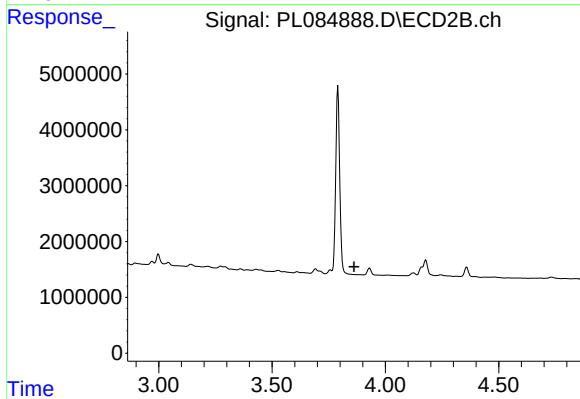

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

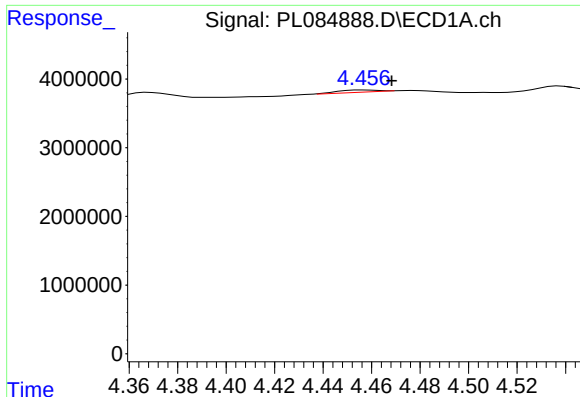

#6 beta-BHC


R.T.: 4.457 min
Delta R.T.: -0.011 min
Response: 361778
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

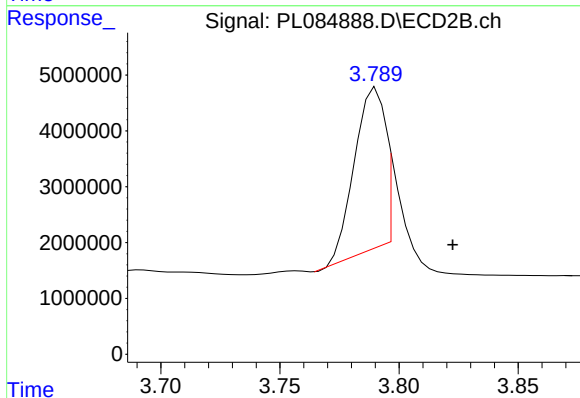


#6 beta-BHC

R.T.: 3.791 min
Delta R.T.: -0.032 min
Response: 26703983
Conc: 32.51 ng/ml

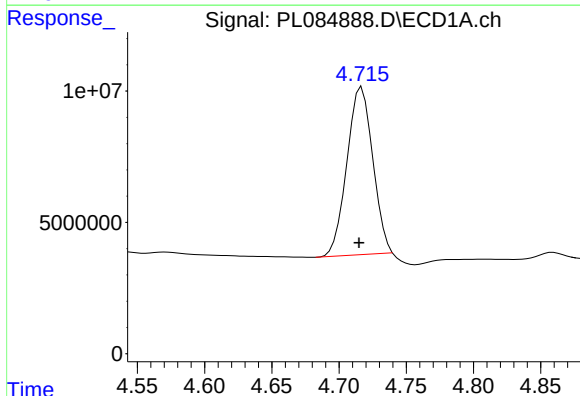


#7 delta-BHC

R.T.: 4.717 min
Delta R.T.: 0.002 min
Response: 85353412
Conc: 23.39 ng/ml

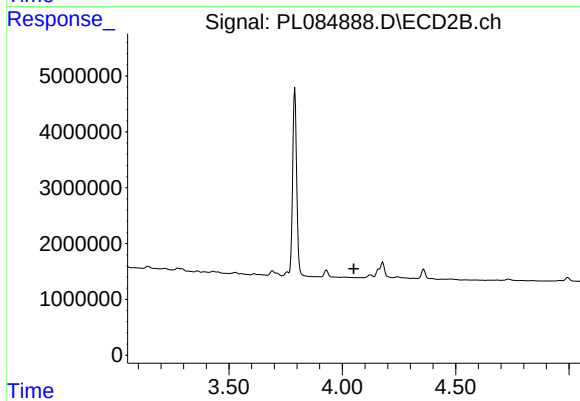

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.051 min
Response: 0
Conc: N.D.

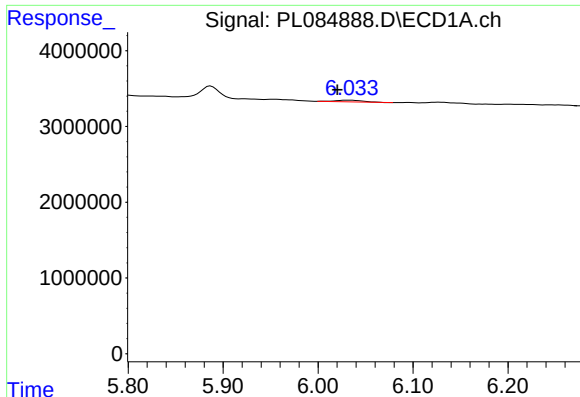

#9 Endosulfan I


R.T.: 6.032 min
Delta R.T.: 0.012 min
Response: 428333
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

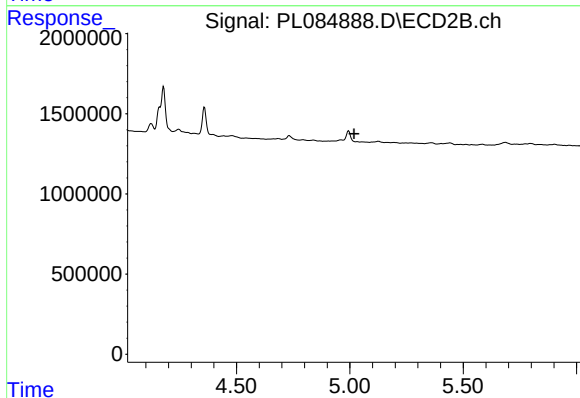


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.019 min
Response: 0
Conc: N.D.

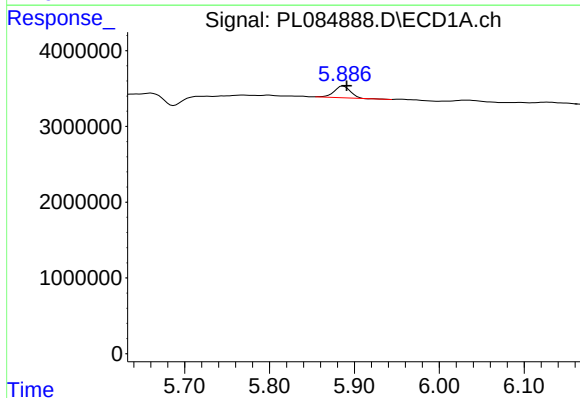


#10 trans-Chlordane

R.T.: 5.887 min
Delta R.T.: -0.004 min
Response: 2086384
Conc: 0.66 ng/ml

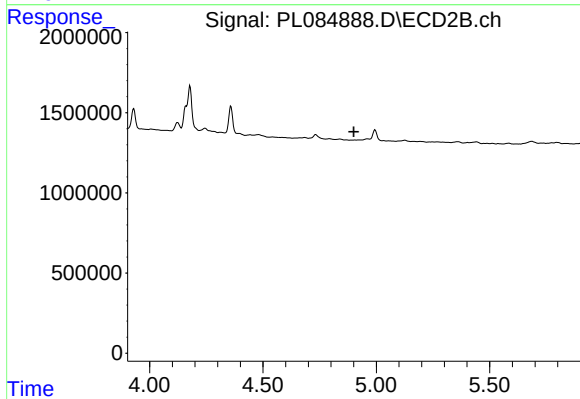

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.901 min
Response: 0
Conc: N.D.

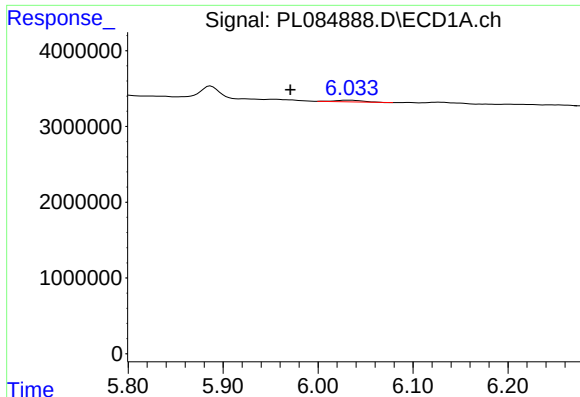

#11 cis-Chlordane


R.T.: 6.032 min
Delta R.T.: 0.061 min
Response: 428333
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

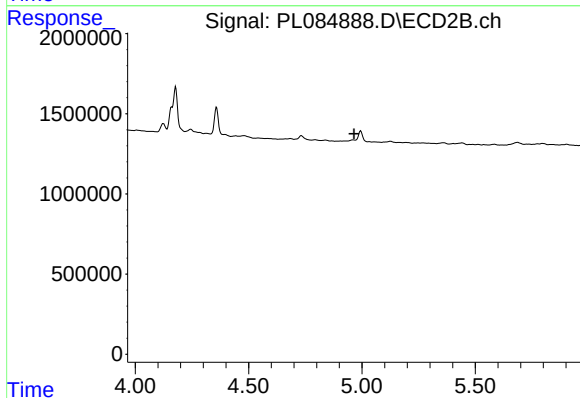


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

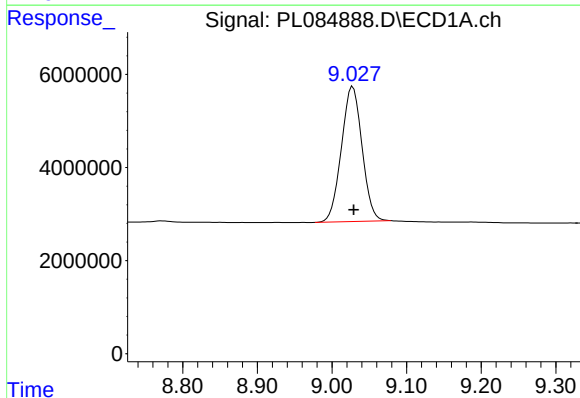

#27 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.001 min
Response: 55822662
Conc: 32.57 ng/ml

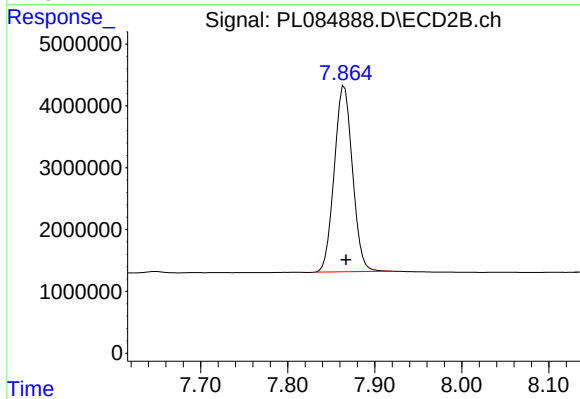

#27 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.002 min
Response: 43775008
Conc: 32.32 ng/ml