

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
 Data File : PL084892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 17:29
 Operator : AR\AJ
 Sample : 04049-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:37:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.685	42462938	19694805	16.938	16.683
27)	SA Decachlor...	9.026	7.865	27696855	21442100	16.162	15.831
Target Compounds							
2)	A alpha-BHC	3.963f	0.000	602501	0	0.167	N.D. #
3)	MA gamma-BHC...	4.260	0.000	1744796	0	0.504	N.D. #
4)	MA Heptachlor	4.862	0.000	366306	0	<MDL	N.D. #
6)	B beta-BHC	4.488	0.000	1719807	0	0.974	N.D. #
7)	B delta-BHC	4.719	0.000	2504077	0	0.686	N.D. #
8)	B Heptachlo...	5.627	0.000	35198	0	<MDL	N.D. #
9)	A Endosulfan I	6.013	0.000	2011656	0	0.706	N.D. #
11)	B cis-Chlor...	6.013f	0.000	2011656	0	0.631	N.D. #
12)	B 4,4'-DDE	6.188f	0.000	237384	0	<MDL	N.D. #
14)	MA Endrin	6.595f	0.000	52168	0	<MDL	N.D. #
15)	B Endosulfa...	6.734	0.000	581541	0	0.247	N.D. #
16)	A 4,4'-DDD	6.734f	0.000	581541	0	0.307	N.D. #
20)	A Methoxychlor	7.508f	0.000	52125	0	<MDL	N.D. #
21)	B Endrin ke...	7.641f	0.000	214098	0	<MDL	N.D. #
22)	Toxaphene-1	6.188	0.000	237384	0	11.544	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 17:29
Operator : AR\AJ
Sample : 04049-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:37:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

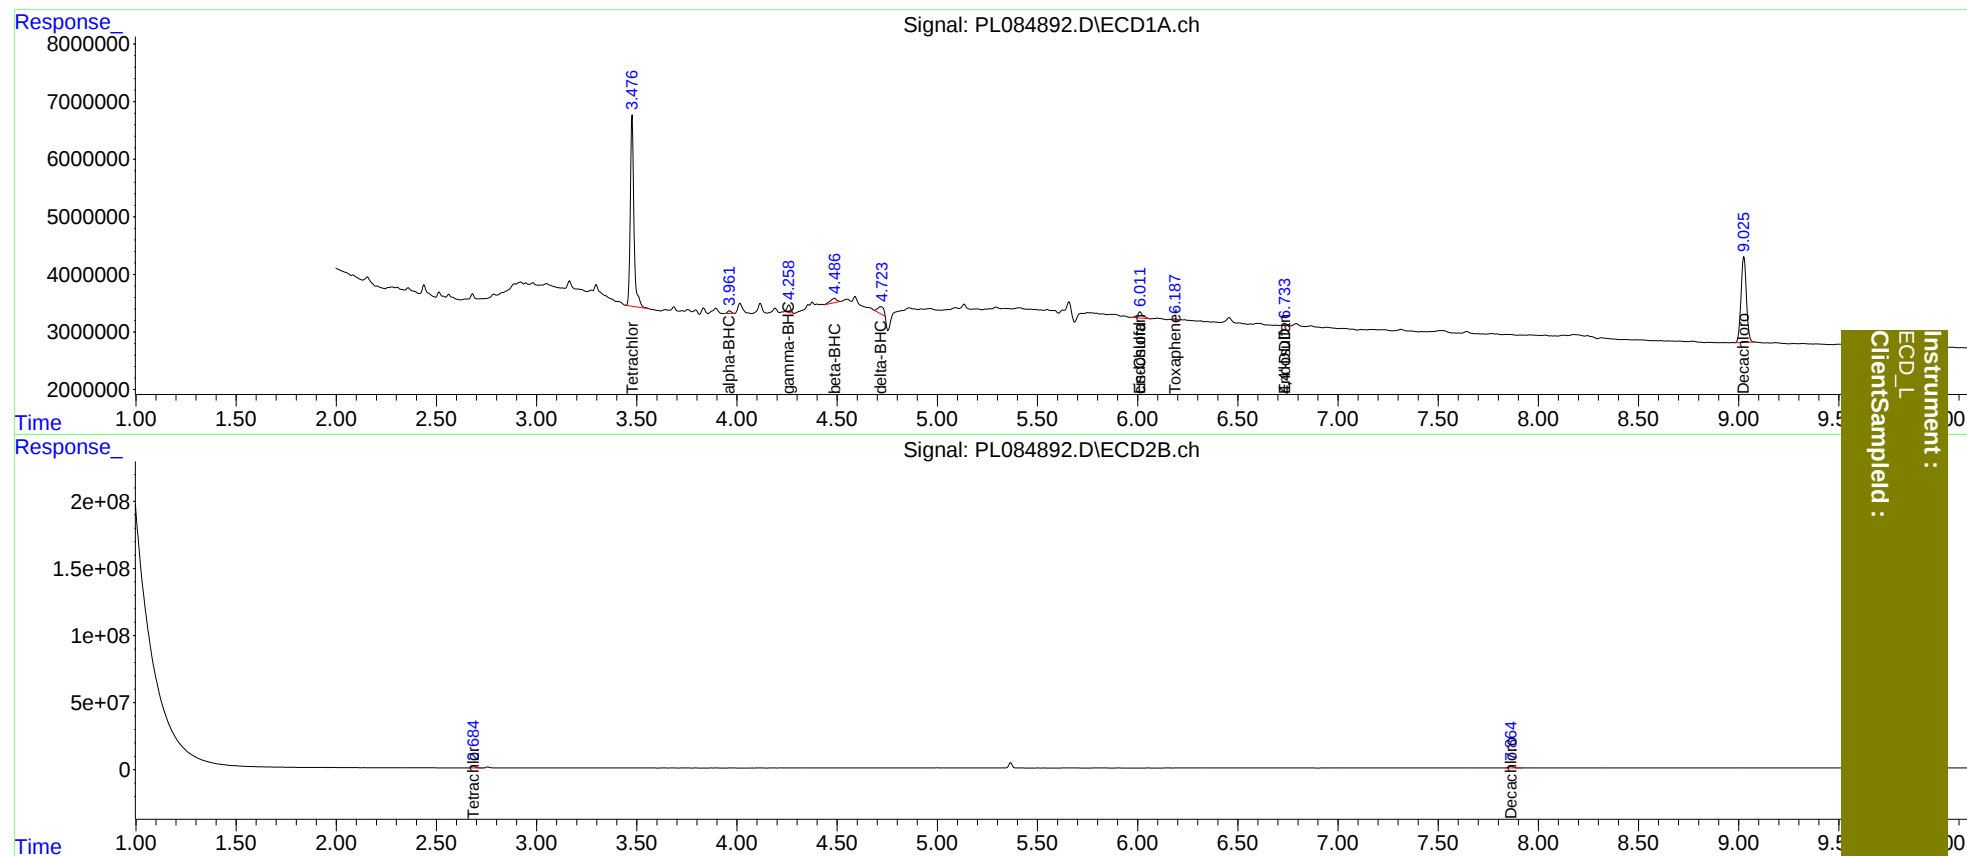


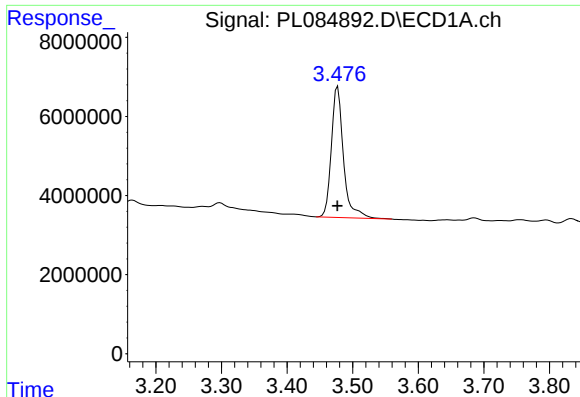

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 42462938
Conc: 16.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

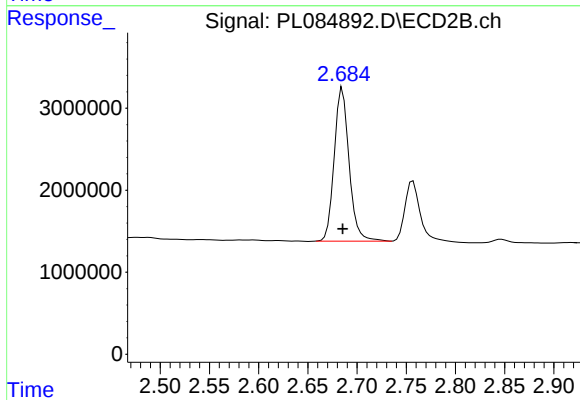


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: 0.000 min
Response: 19694805
Conc: 16.68 ng/ml

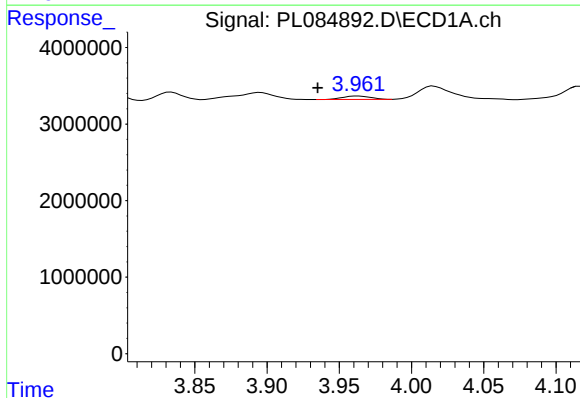


#2 alpha-BHC

R.T.: 3.963 min
Delta R.T.: 0.028 min
Response: 602501
Conc: 0.17 ng/ml

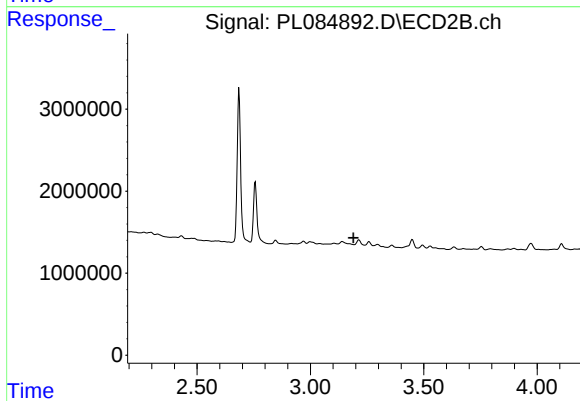

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.190 min
Response: 0
Conc: N.D.

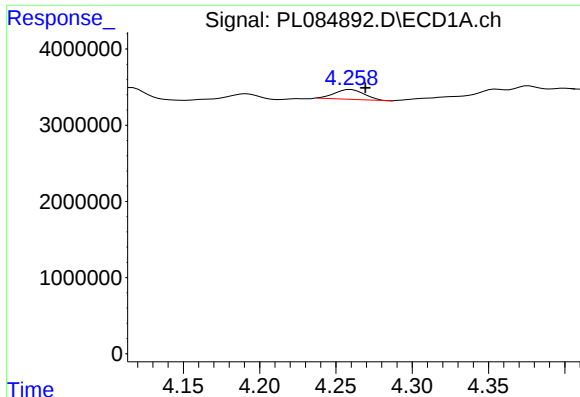

#3 gamma-BHC (Lindane)


R.T.: 4.260 min
Delta R.T.: -0.009 min
Response: 1744796
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

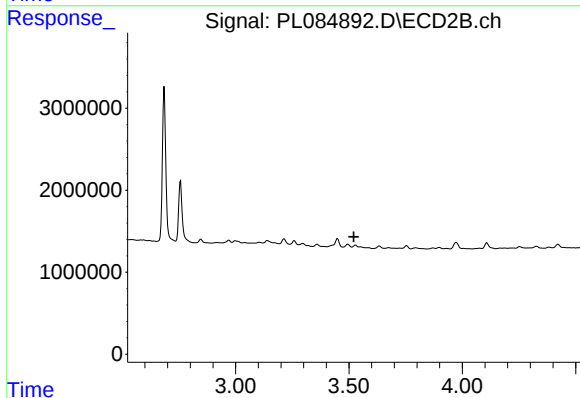


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.521 min
Response: 0
Conc: N.D.

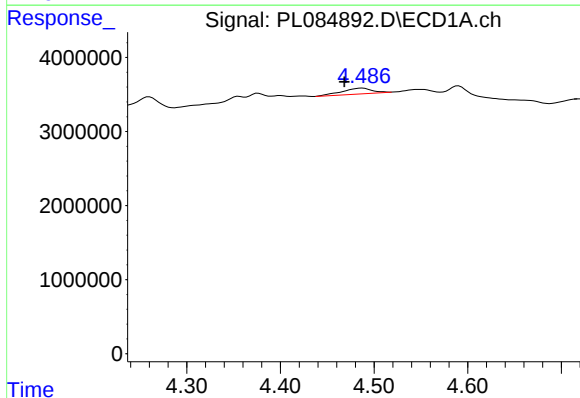


#6 beta-BHC

R.T.: 4.488 min
Delta R.T.: 0.019 min
Response: 1719807
Conc: 0.97 ng/ml

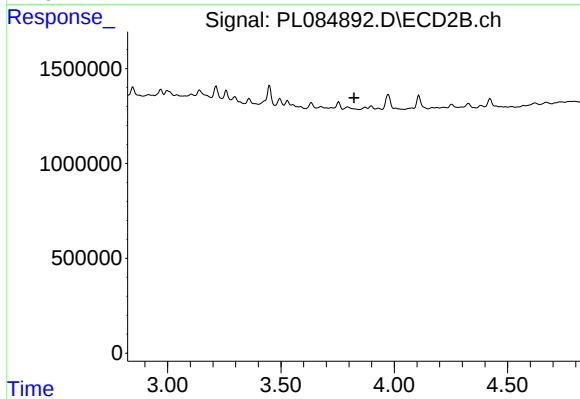

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.822 min
Response: 0
Conc: N.D.

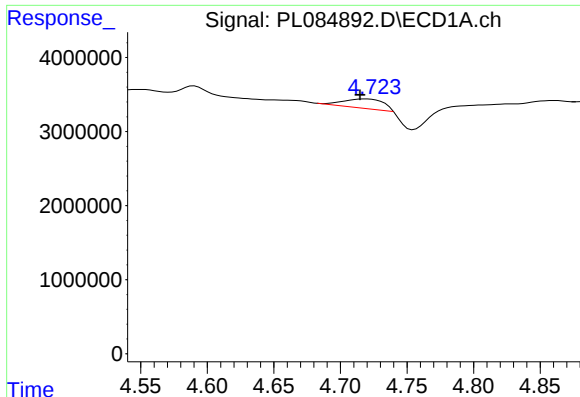

#7 delta-BHC


R.T.: 4.719 min
Delta R.T.: 0.005 min
Response: 2504077
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

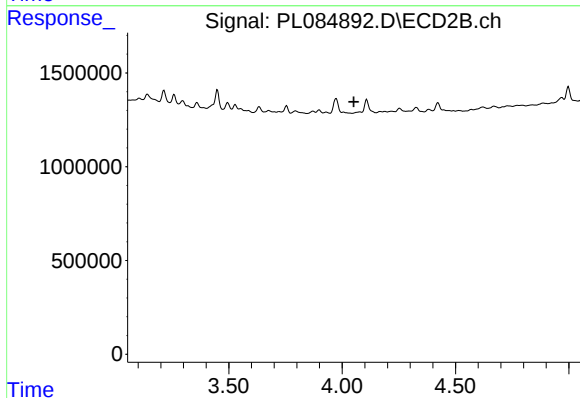


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.051 min
Response: 0
Conc: N.D.

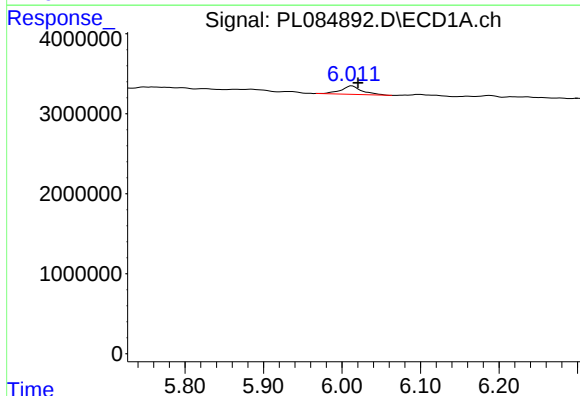


#9 Endosulfan I

R.T.: 6.013 min
Delta R.T.: -0.008 min
Response: 2011656
Conc: 0.71 ng/ml

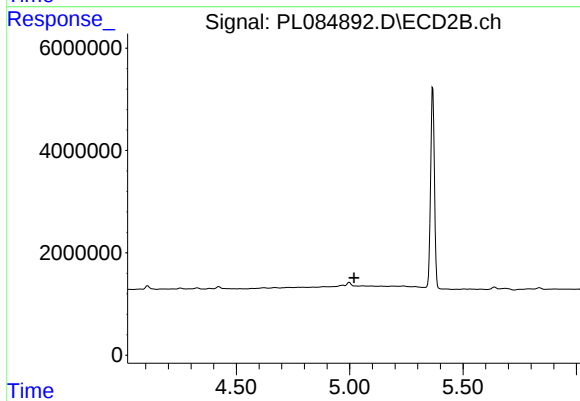

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.019 min
Response: 0
Conc: N.D.

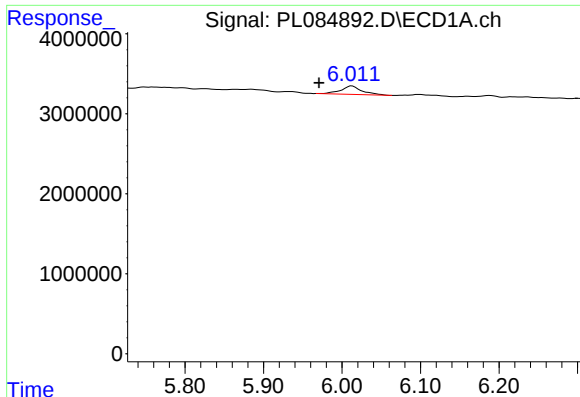

#11 cis-Chlordane


R.T.: 6.013 min
Delta R.T.: 0.042 min
Response: 2011656
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

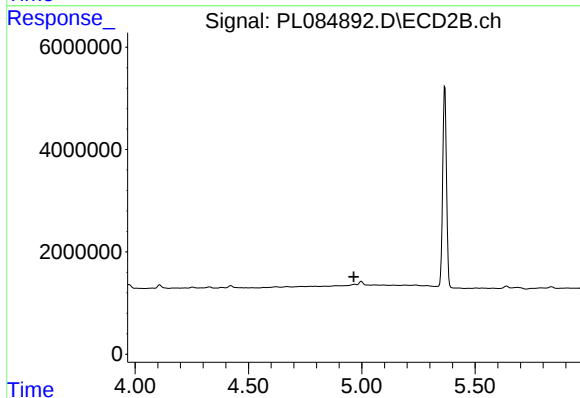


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

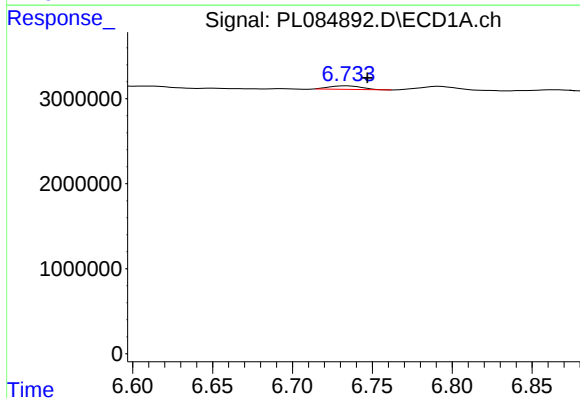


#15 Endosulfan II

R.T.: 6.734 min
Delta R.T.: -0.013 min
Response: 581541
Conc: 0.25 ng/ml

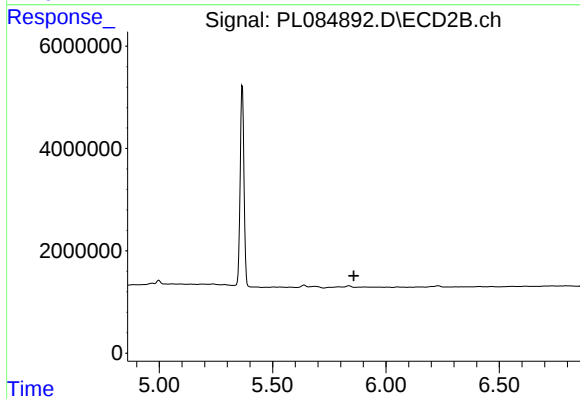

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.859 min
Response: 0
Conc: N.D.

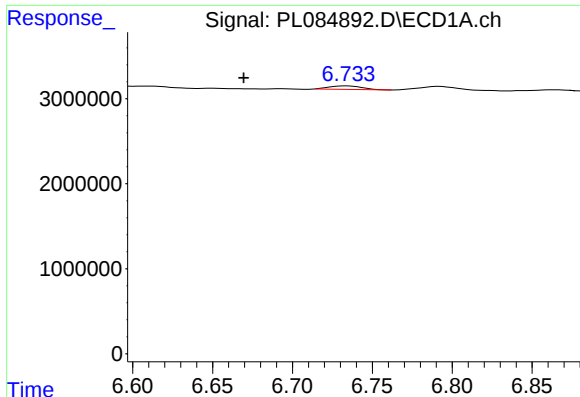

#16 4,4'-DDD


R.T.: 6.734 min
Delta R.T.: 0.065 min
Response: 581541
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

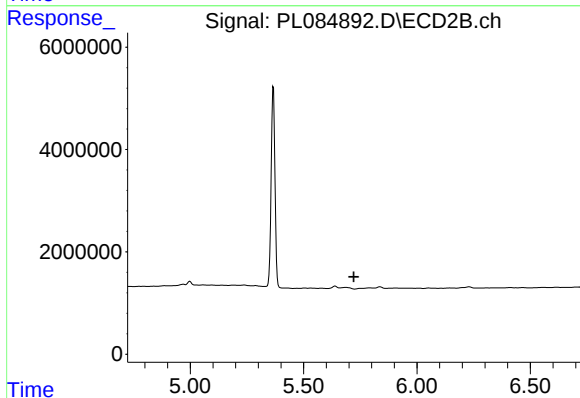


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.722 min
Response: 0
Conc: N.D.

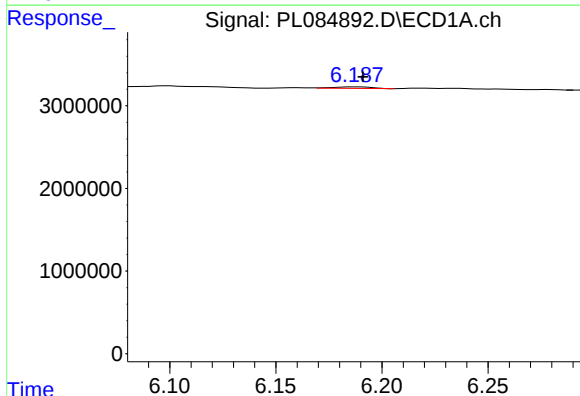


#22 Toxaphene-1

R.T.: 6.188 min
Delta R.T.: -0.003 min
Response: 237384
Conc: 11.54 ng/ml

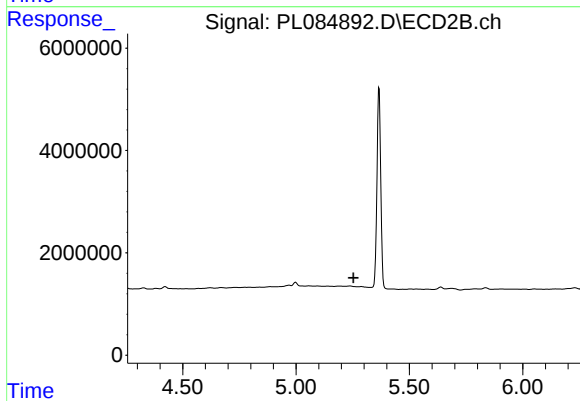

#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.254 min
Response: 0
Conc: N.D.

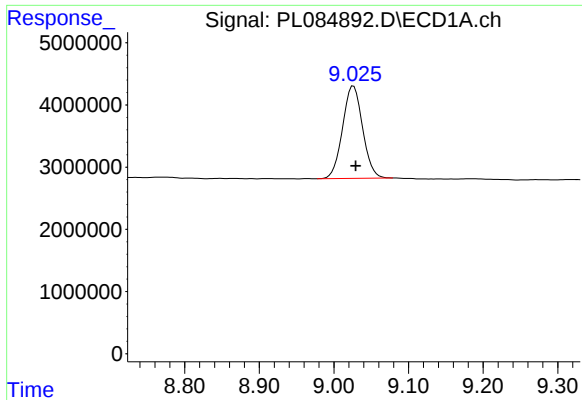

#27 Decachlorobiphenyl


R.T.: 9.026 min

Delta R.T.: -0.003 min

Response: 27696855

Conc: 16.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

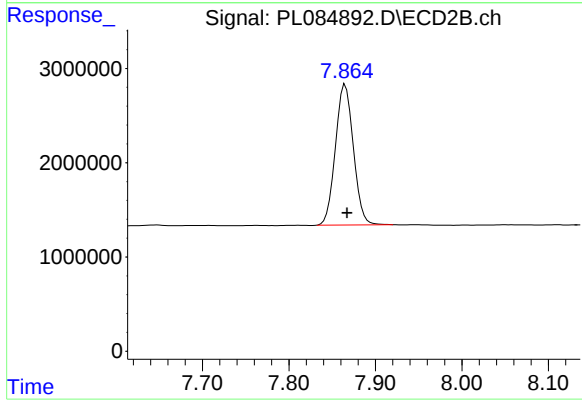

#27 Decachlorobiphenyl

R.T.: 7.865 min

Delta R.T.: -0.002 min

Response: 21442100

Conc: 15.83 ng/ml