

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
 Data File : PL084897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 18:39
 Operator : AR\AJ
 Sample : PIBLK217
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:39:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.685	55861059	26577127	22.283	22.513
27)	SA Decachlor...	9.027	7.865	89349800	71819446	52.137	53.027
Target Compounds							
3)	MA gamma-BHC...	4.222f	0.000	260437	0	<MDL	N.D. #
4)	MA Heptachlor	4.860	0.000	41497	0	<MDL	N.D. #
6)	B beta-BHC	4.487	0.000	477887	0	0.271	N.D. #
7)	B delta-BHC	4.715	0.000	5091856	0	1.395	N.D. #
8)	B Heptachlo...	5.635	0.000	439028	0	0.132	N.D. #
10)	B trans-Chl...	5.944f	0.000	1608363	0	0.510	N.D. #
11)	B cis-Chlor...	5.944	0.000	1608363	0	0.505	N.D. #
14)	MA Endrin	6.584f	0.000	415137	0	0.182	N.D. #
15)	B Endosulfa...	6.749	0.000	2023834	0	0.861	N.D. #
17)	MA 4,4'-DDT	6.953	0.000	392257	0	0.203	N.D. #
20)	A Methoxychlor	7.455	0.000	273437	0	0.282	N.D. #
23)	Toxaphene-2	6.953f	0.000	392257	0	5.902	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 18:39
Operator : AR\AJ
Sample : PIBLK217
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:39:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

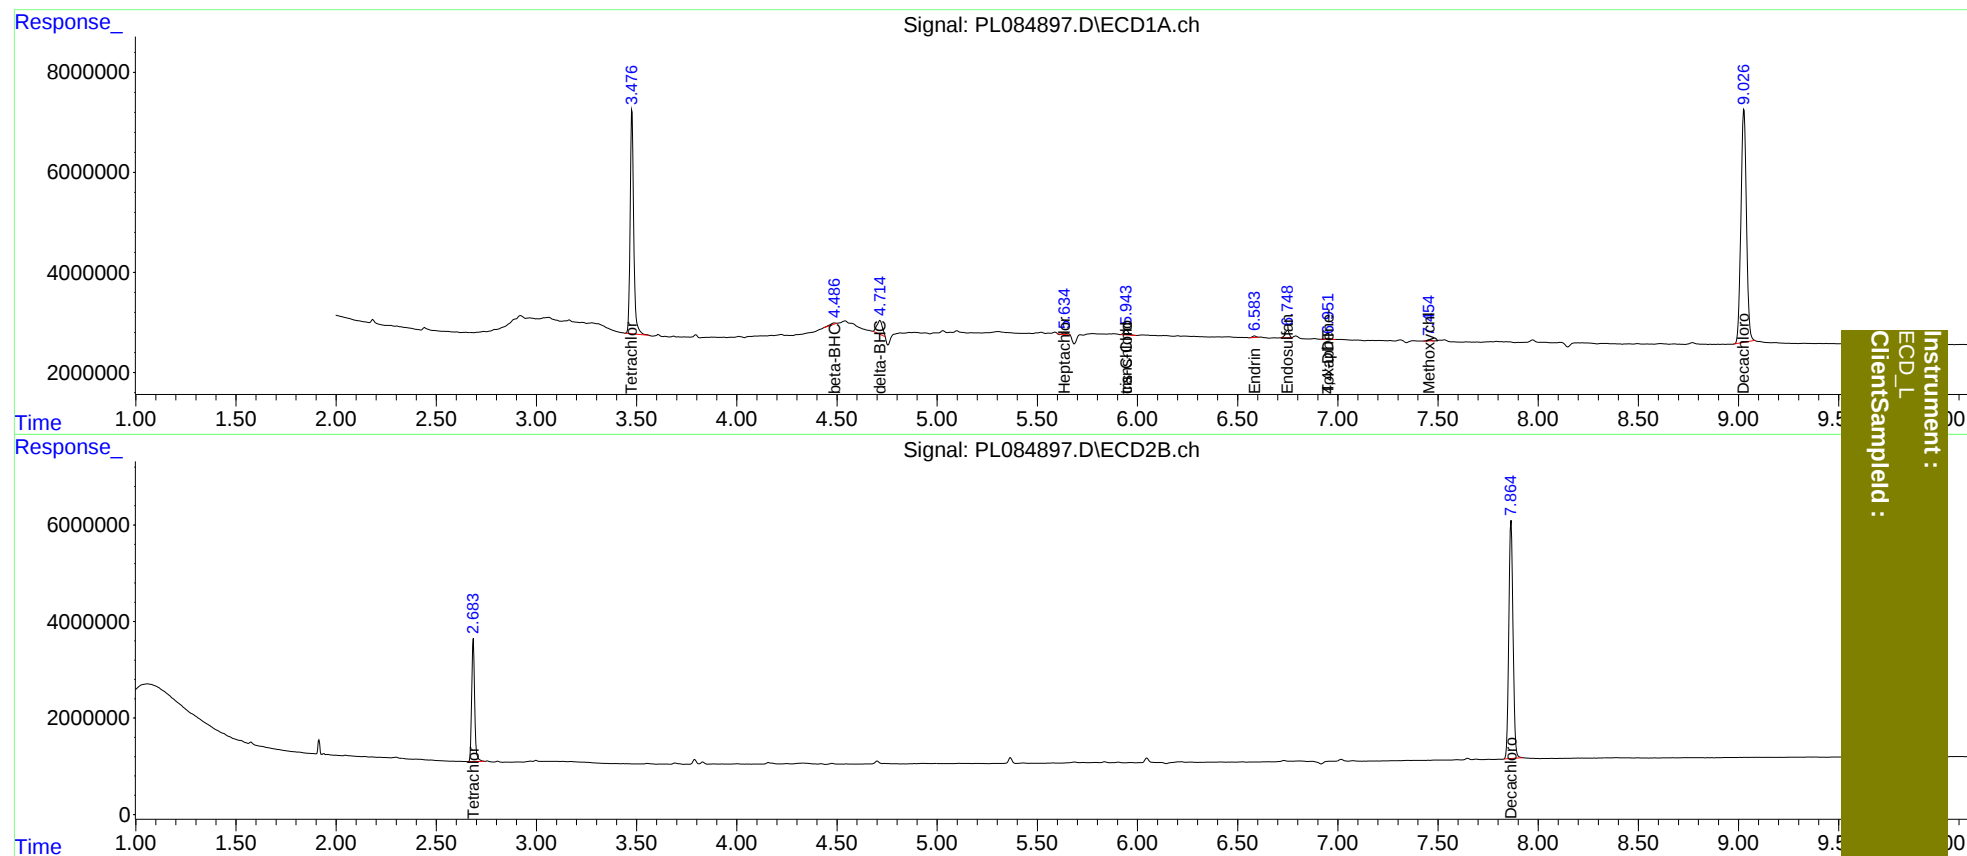


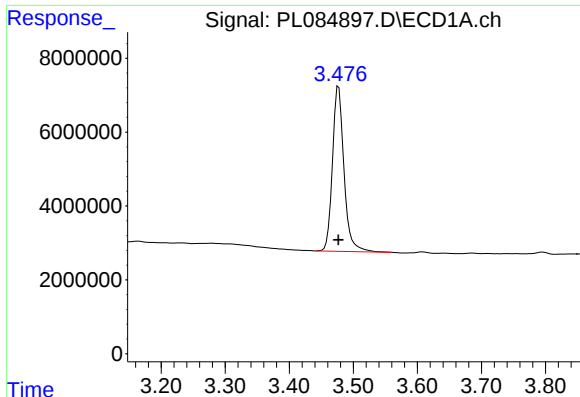

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 55861059
Conc: 22.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

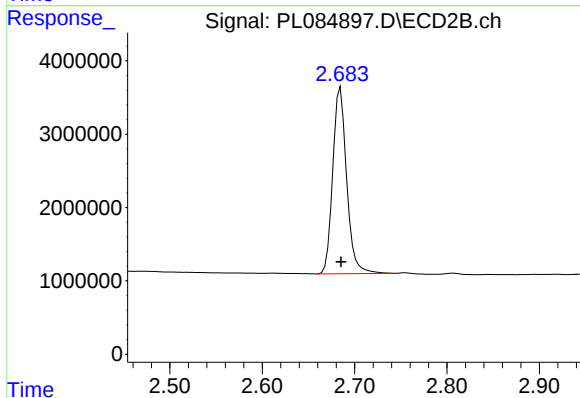


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: 0.000 min
Response: 26577127
Conc: 22.51 ng/ml

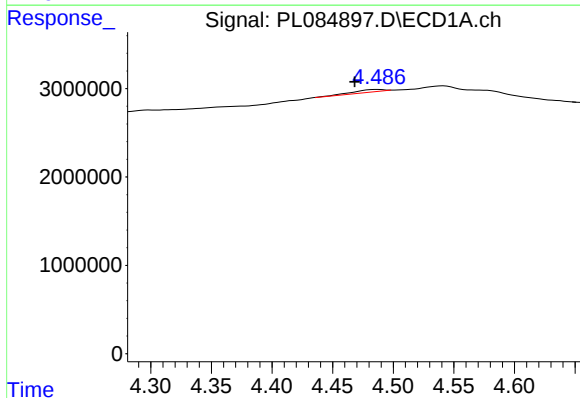


#6 beta-BHC

R.T.: 4.487 min
Delta R.T.: 0.019 min
Response: 477887
Conc: 0.27 ng/ml

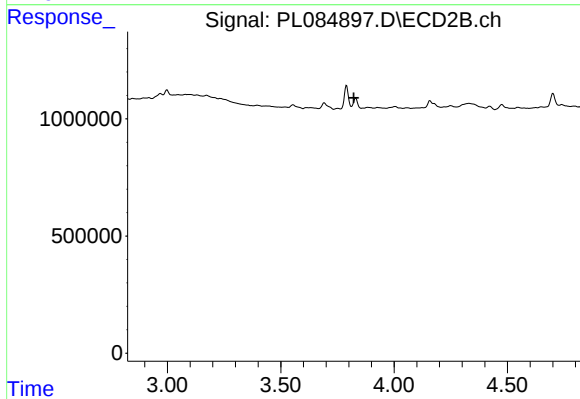

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 3.822 min
Response: 0
Conc: N.D.

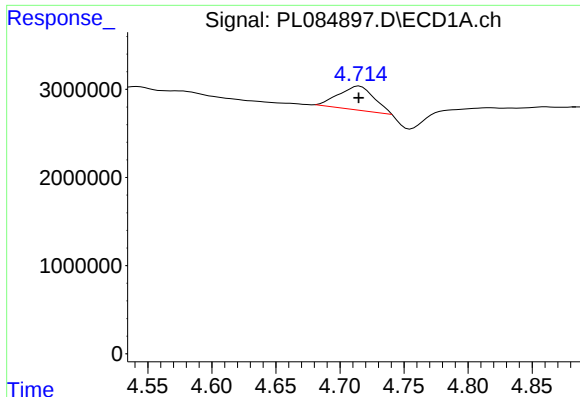

#7 delta-BHC


R.T.: 4.715 min
Delta R.T.: 0.000 min
Response: 5091856
Conc: 1.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

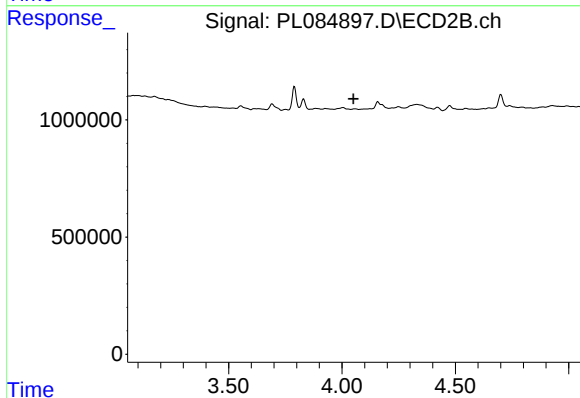


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.051 min
Response: 0
Conc: N.D.

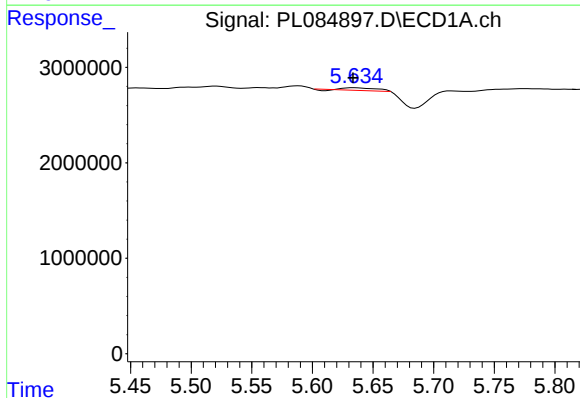


#8 Heptachlor epoxide

R.T.: 5.635 min
Delta R.T.: 0.001 min
Response: 439028
Conc: 0.13 ng/ml

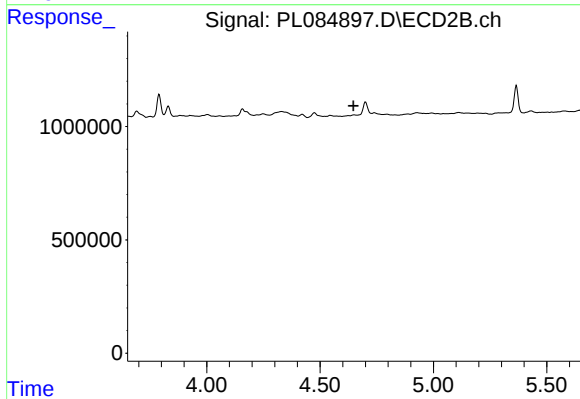

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.648 min
Response: 0
Conc: N.D.

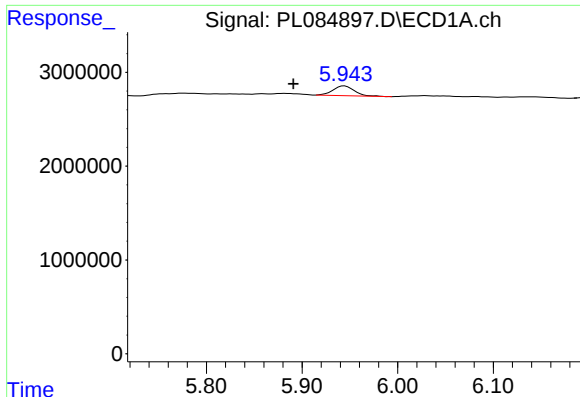

#10 trans-Chlordane


R.T.: 5.944 min
Delta R.T.: 0.053 min
Response: 1608363
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

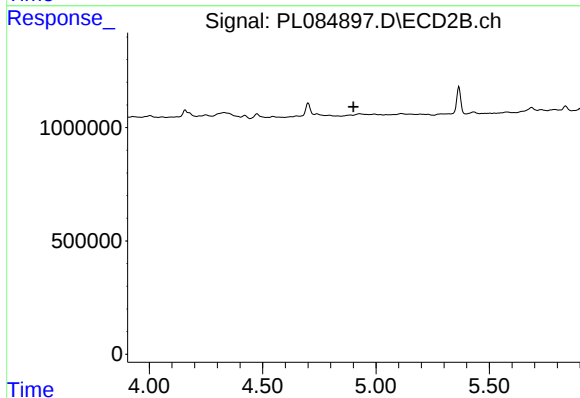


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.901 min
Response: 0
Conc: N.D.

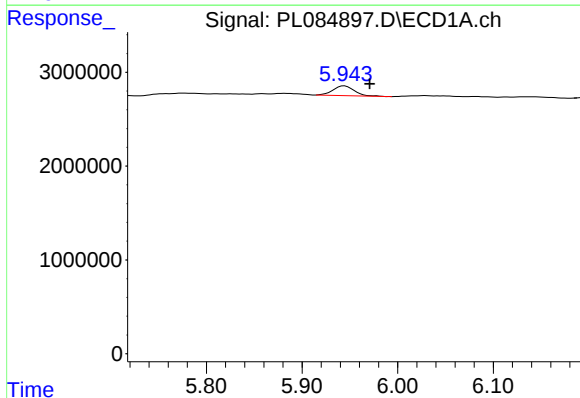


#11 cis-Chlordane

R.T.: 5.944 min
Delta R.T.: -0.027 min
Response: 1608363
Conc: 0.50 ng/ml

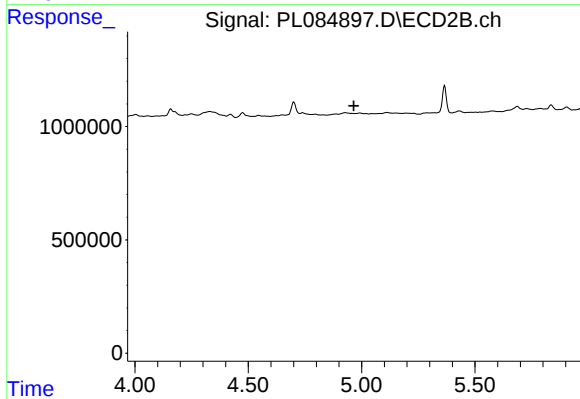

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

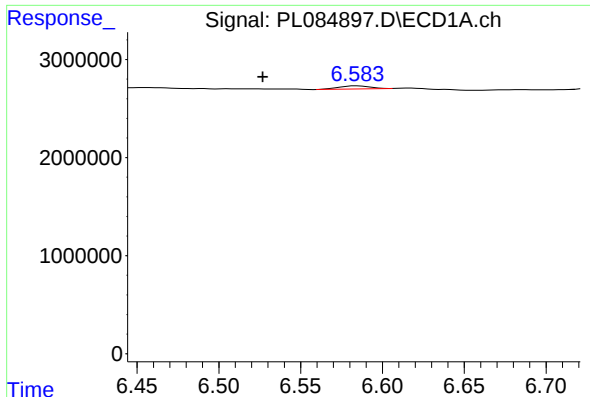

#14 Endrin


R.T.: 6.584 min
Delta R.T.: 0.058 min
Response: 415137
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

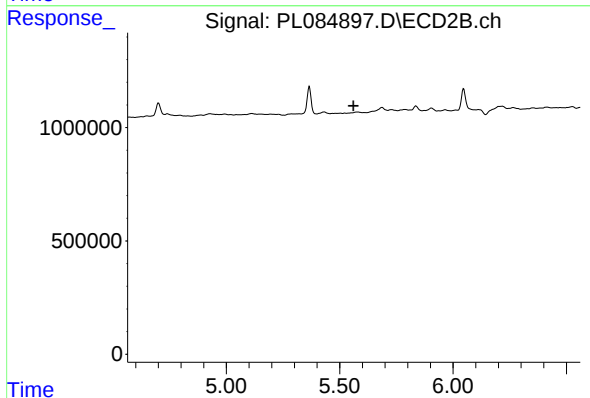


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.561 min
Response: 0
Conc: N.D.

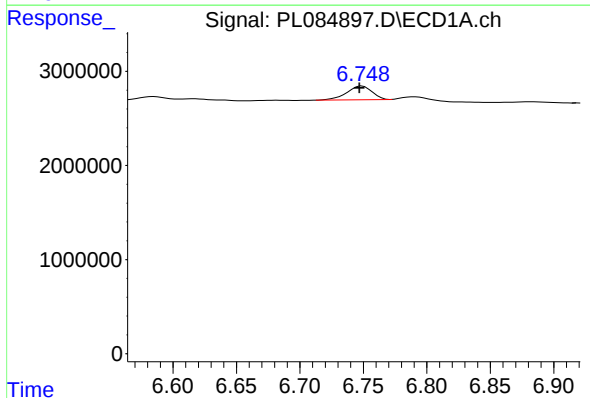


#15 Endosulfan II

R.T.: 6.749 min
Delta R.T.: 0.002 min
Response: 2023834
Conc: 0.86 ng/ml

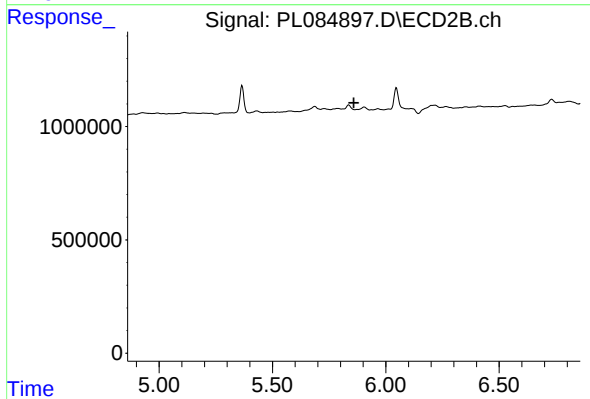

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.859 min
Response: 0
Conc: N.D.

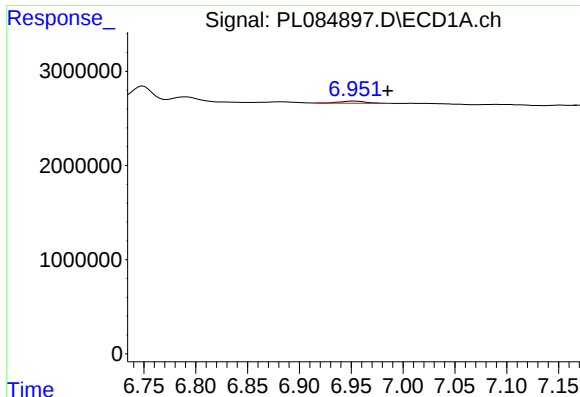

#17 4,4'-DDT


R.T.: 6.953 min
Delta R.T.: -0.033 min
Response: 392257
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

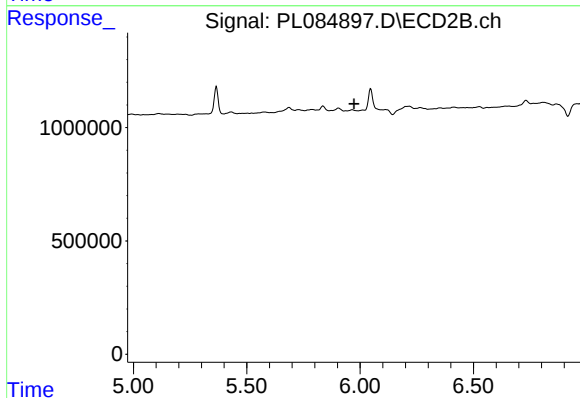


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 5.974 min
Response: 0
Conc: N.D.

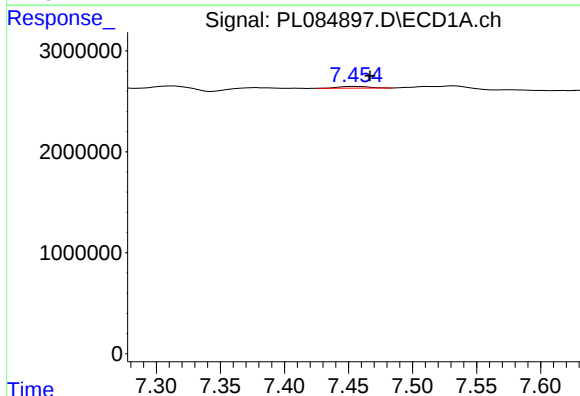


#20 Methoxychlor

R.T.: 7.455 min
Delta R.T.: -0.012 min
Response: 273437
Conc: 0.28 ng/ml

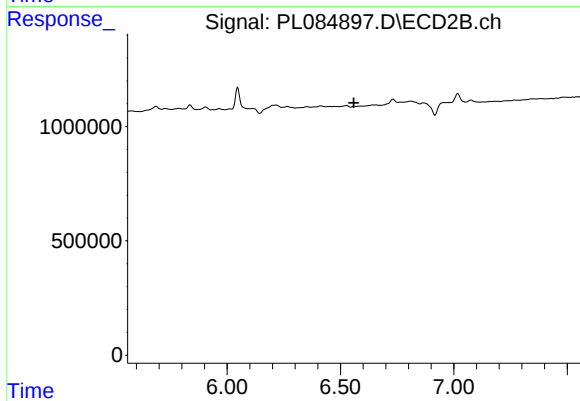

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.559 min
Response: 0
Conc: N.D.

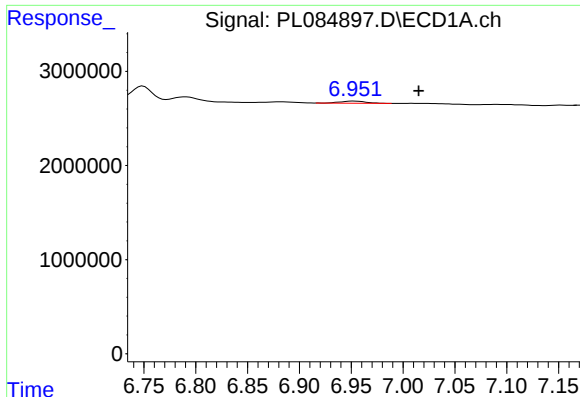

#23 Toxaphene-2


R.T.: 6.953 min
Delta R.T.: -0.063 min
Response: 392257
Conc: 5.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

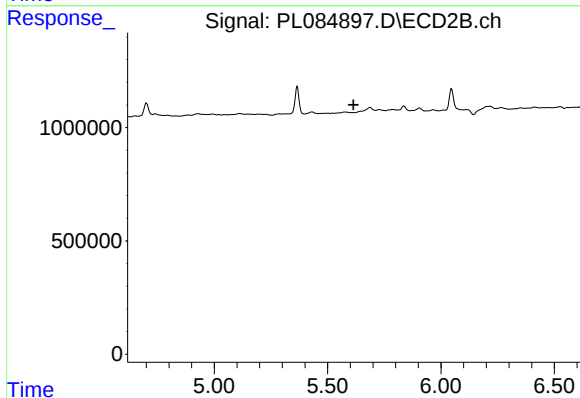


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.615 min
Response: 0
Conc: N.D.

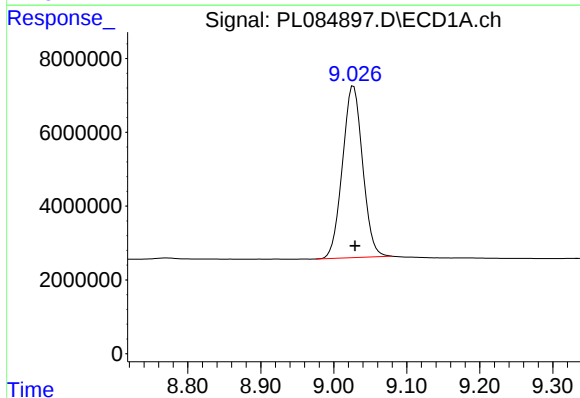

#27 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.002 min
Response: 89349800
Conc: 52.14 ng/ml

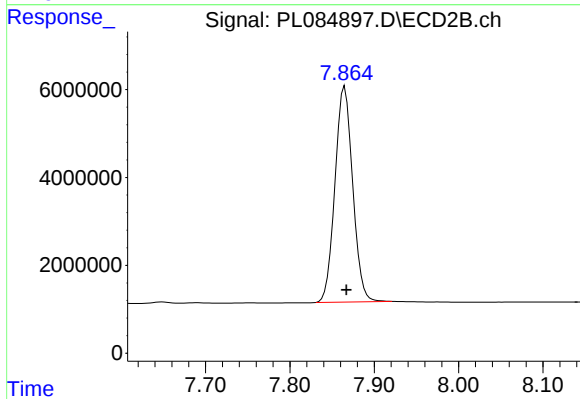

#27 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.002 min
Response: 71819446
Conc: 53.03 ng/ml