

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
 Data File : PL084868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 11:25
 Operator : AR\AJ
 Sample : 03573-01
 Misc : TOX MDL WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT3-2023-05

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/22/2023
 Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:28:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	2.687	44361460	21082603	17.695	17.859
27)	SA Decachlor...	9.036	7.869	58773451	46221386	34.295	34.127
Target Compounds							
22)	Toxaphene-1	6.198	5.255	1885383	701614	91.683	92.351m
23)	Toxaphene-2	7.021	5.616	7019225	715690	105.614m	80.160m
24)	Toxaphene-3	7.112	6.662	4757536	3822985	100.313	80.607
25)	Toxaphene-4	7.210	6.978	2790554	2603581	101.810	81.943
26)	Toxaphene-5	7.899	7.110	3324130	1457516	101.114	76.498m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:25
Operator : AR\AJ
Sample : 03573-01
Misc : TOX MDL WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

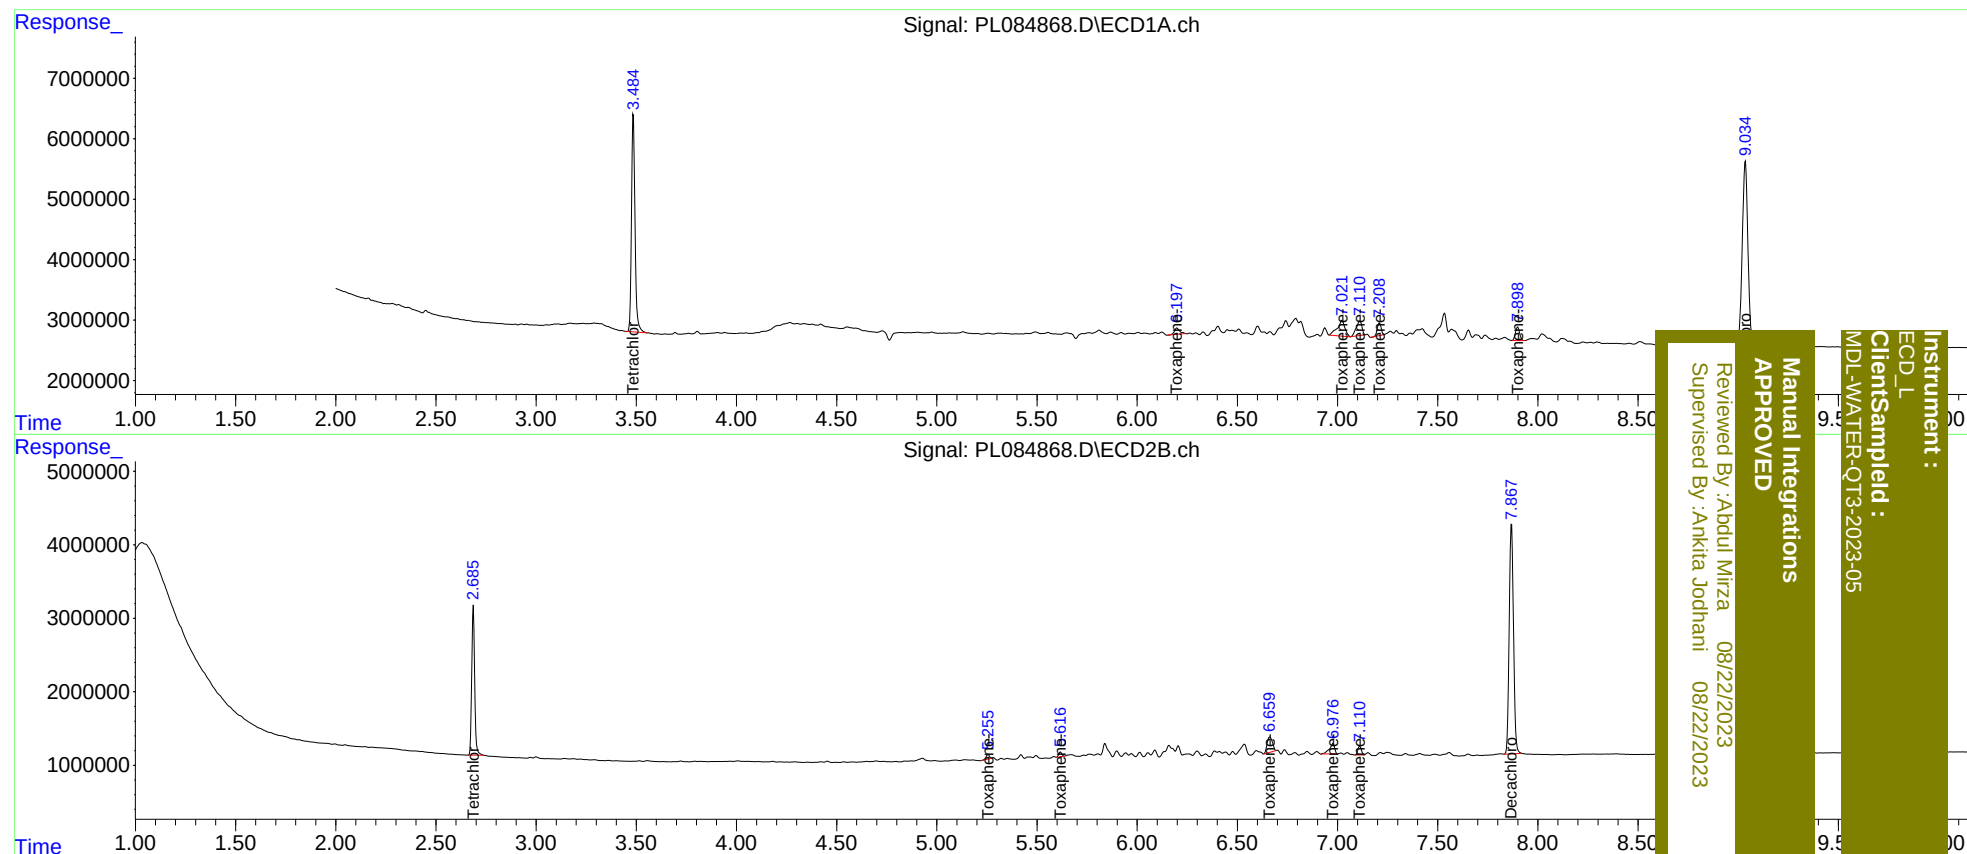

Reviewed By: Abdul Mirza 08/22/2023
Supervised By: Ankita Jodhani 08/22/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT3-2023-05