

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
 Data File : PL084896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2023 18:25
 Operator : AR\AJ
 Sample : 04049-16
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BH8T9

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/22/2023
 Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 21 22:38:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.685	48808619	23045294	19.469	19.522
27)	SA Decachlor...	9.026	7.865	53999676	42486260	31.510	31.369
Target Compounds							
8)	B Heptachlo...	5.618	4.645	10358046	721494	3.103m	0.477m#
13)	MA Dieldrin	6.296	5.285	111.8E6	61488015	39.080	39.669
14)	MA Endrin	6.525	5.569	906322	3234430	0.398	2.349 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 18:25
Operator : AR\AJ
Sample : 04049-16
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:38:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

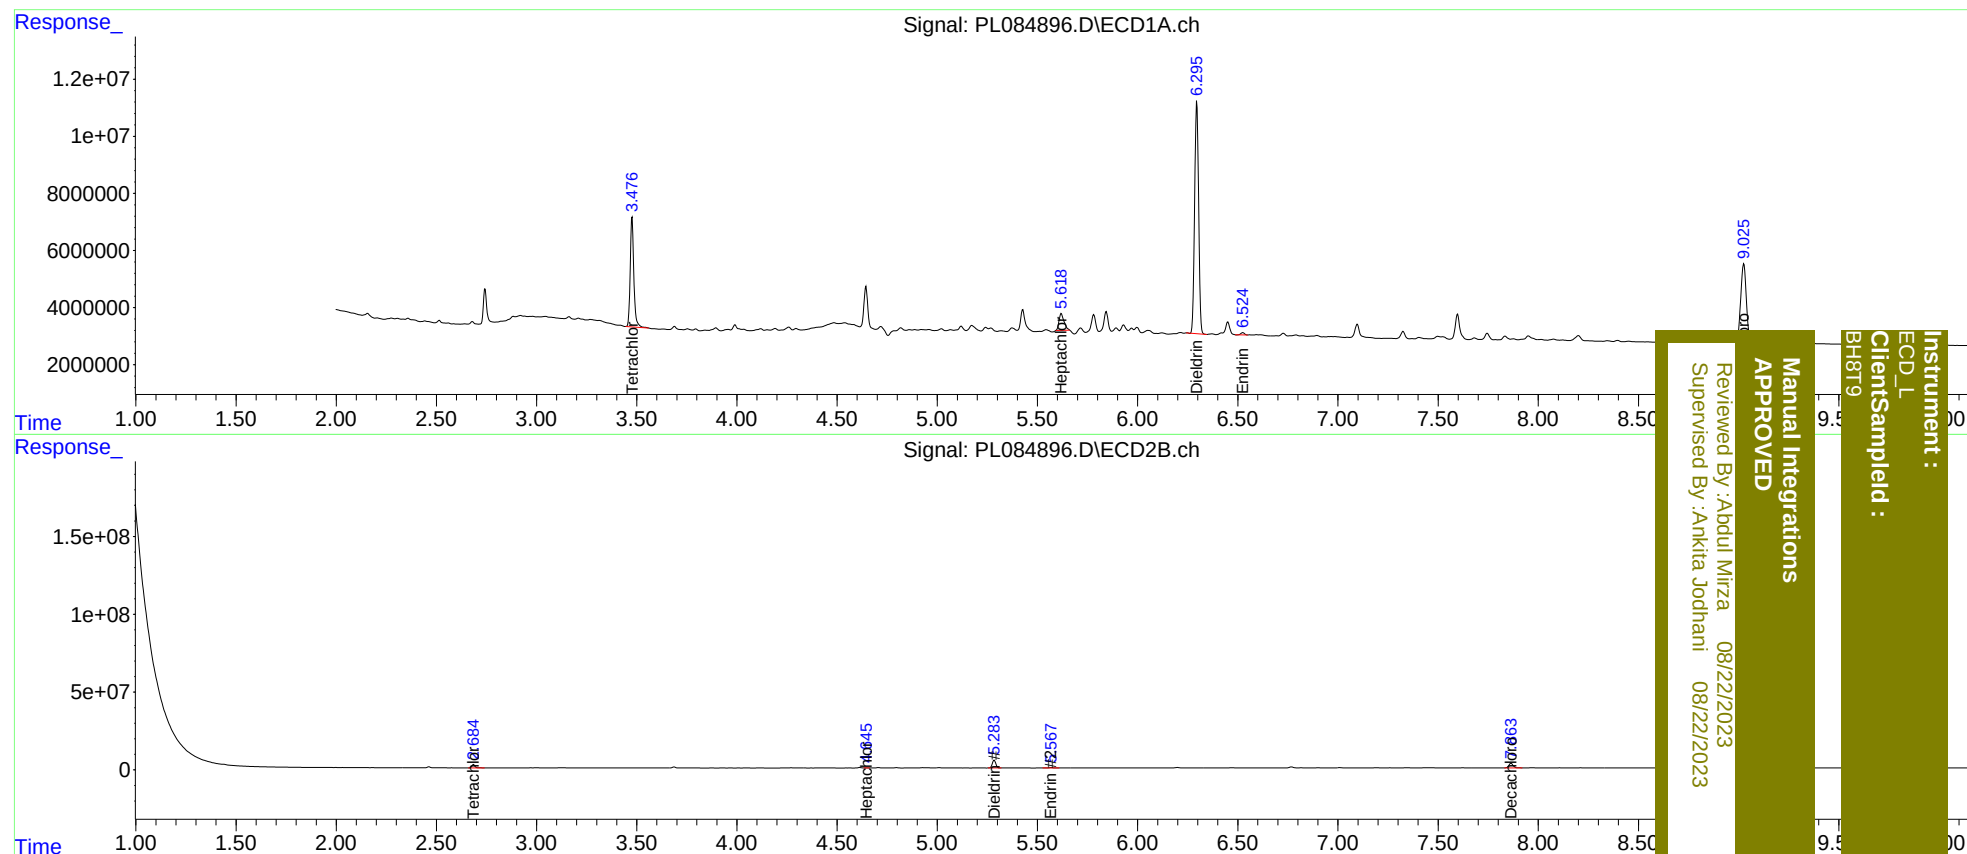

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/22/2023
Supervised By: Ankita Jodhani 08/22/2023

Instrument :
ECD_L
ClientSampled :
BH8T9