

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

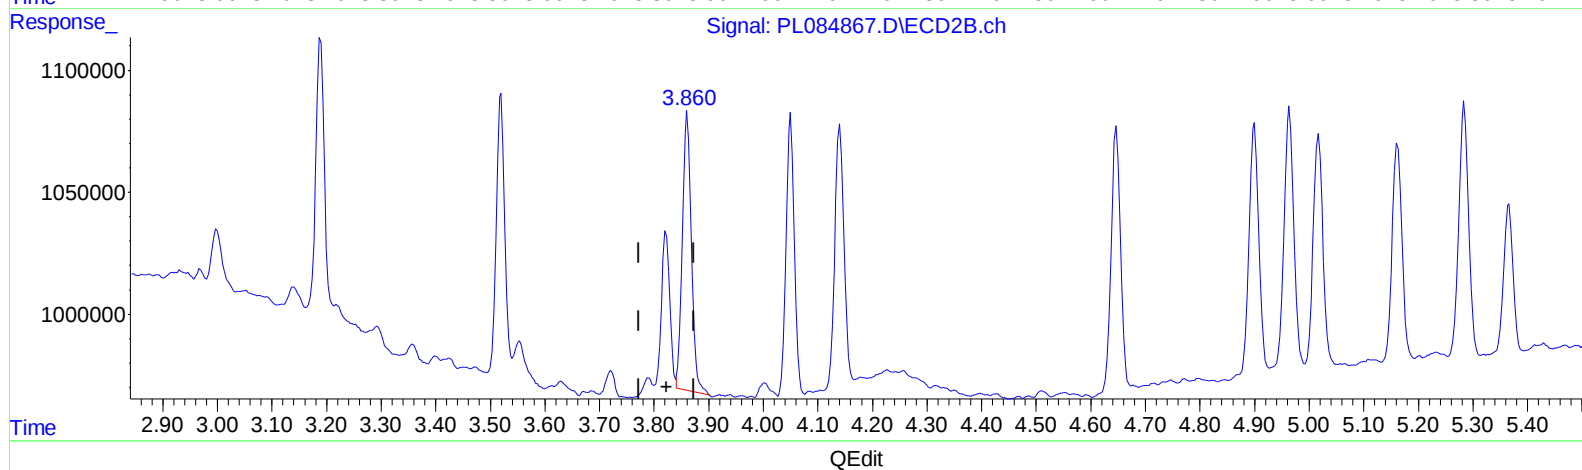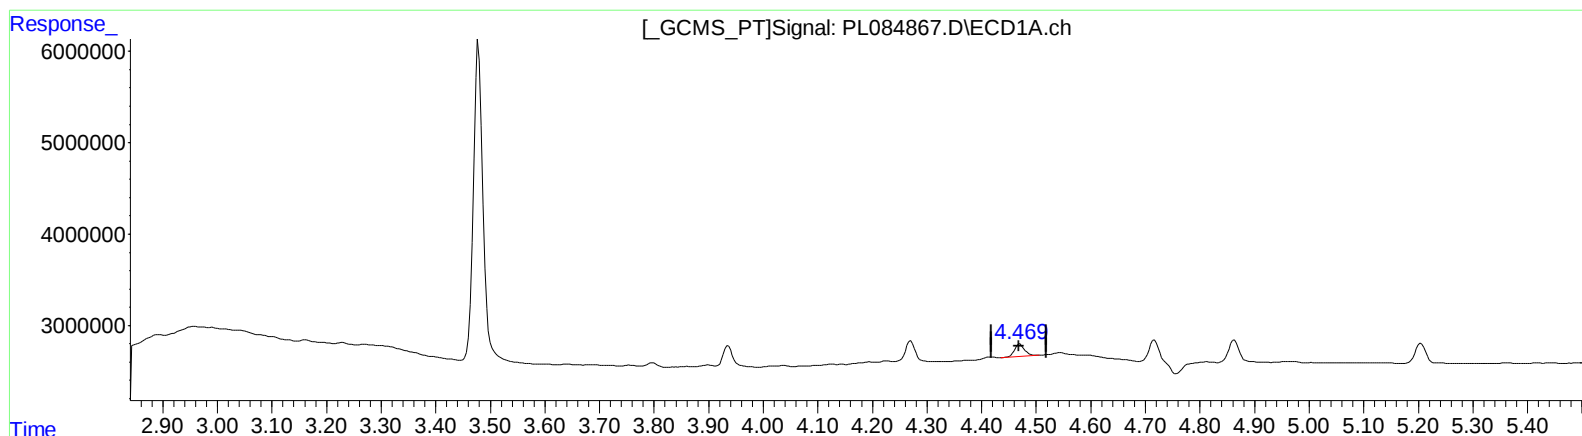

(6) beta-BHC (B)

4.470min 1.015 ng/ml

response 1792889

(6) beta-BHC #2 (B)

3.861min 1.612 ng/ml

response 1323961

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

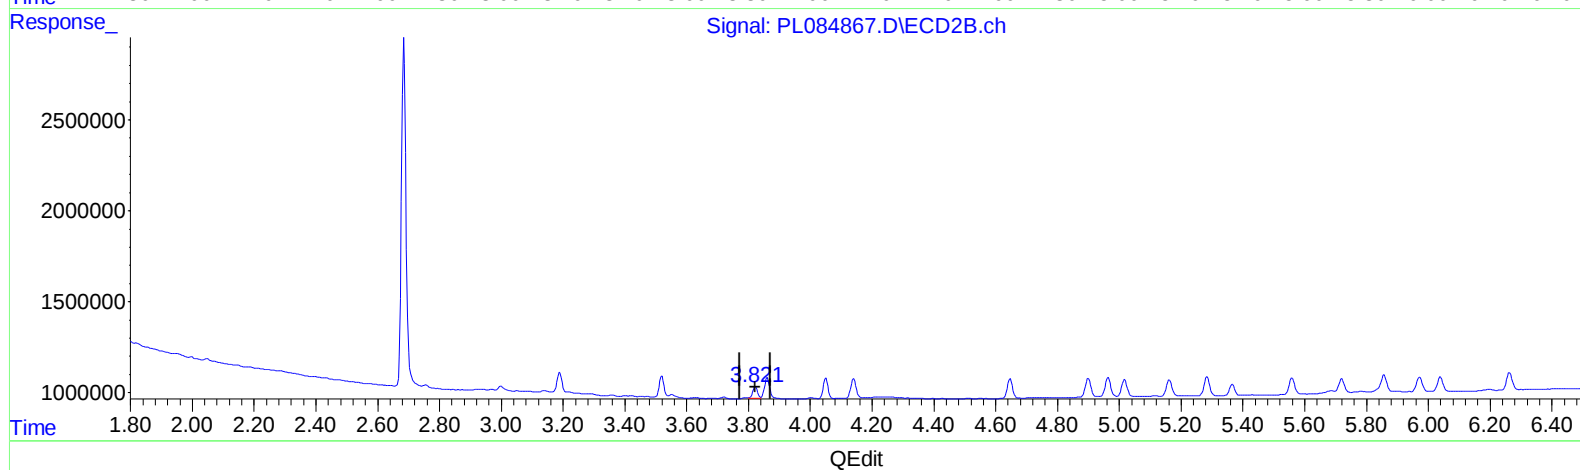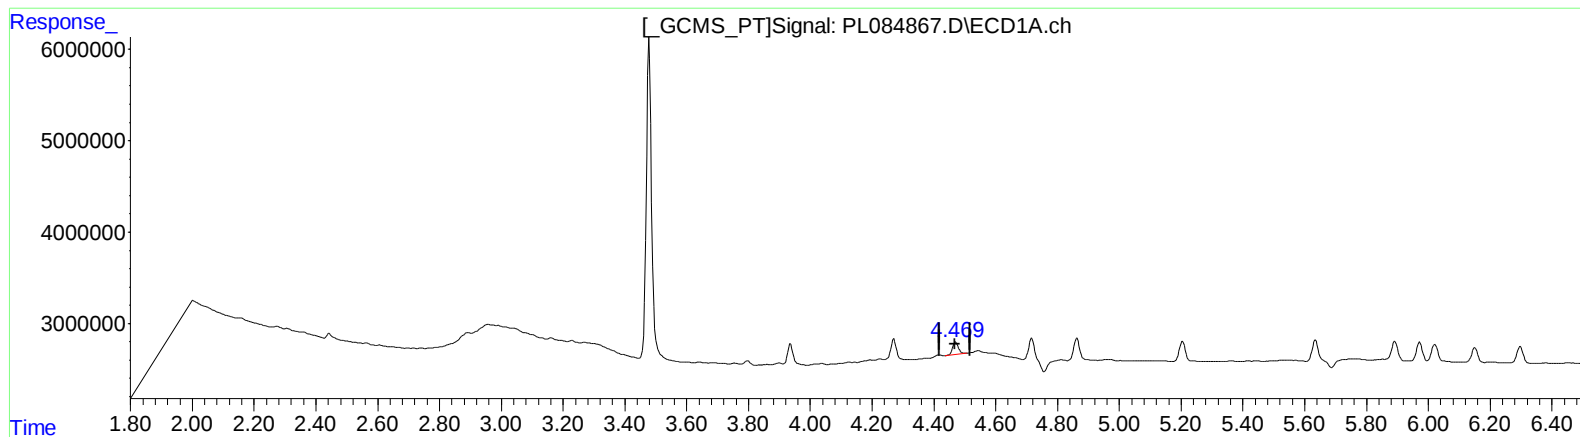

(6) beta-BHC (B)

4.470min 1.015 ng/ml

response 1792889

(6) beta-BHC #2 (B)

3.821min 0.802 ng/ml m

response 658618

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

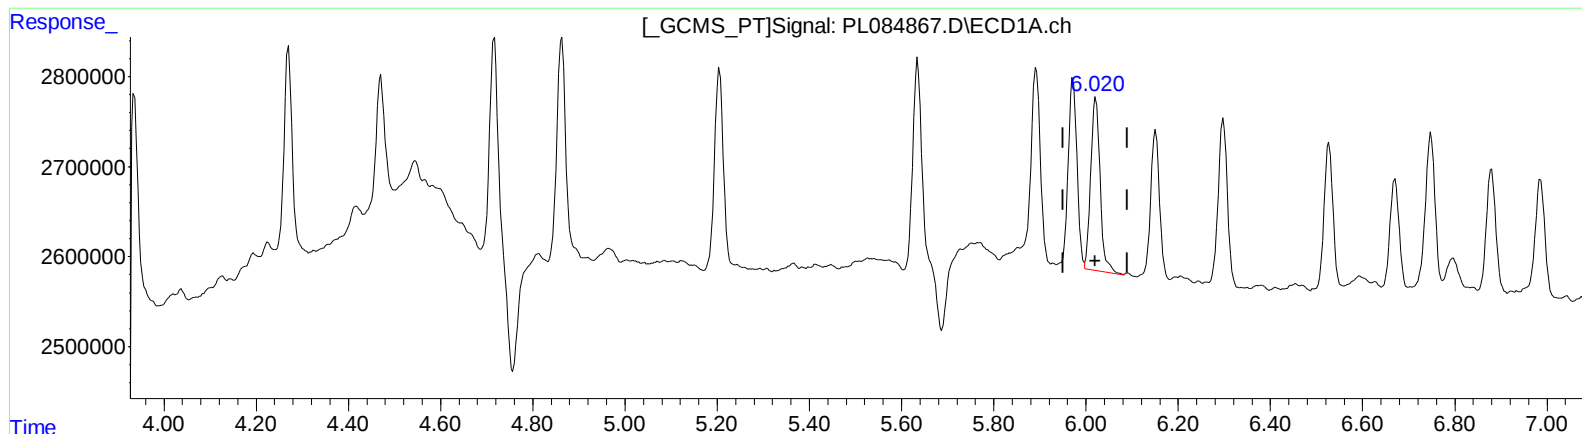

(9) Endosulfan I (A)
6.021min 0.964 ng/ml
response 2747210

(9) Endosulfan I #2 (A)
4.964min 0.963 ng/ml
response 1298203

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

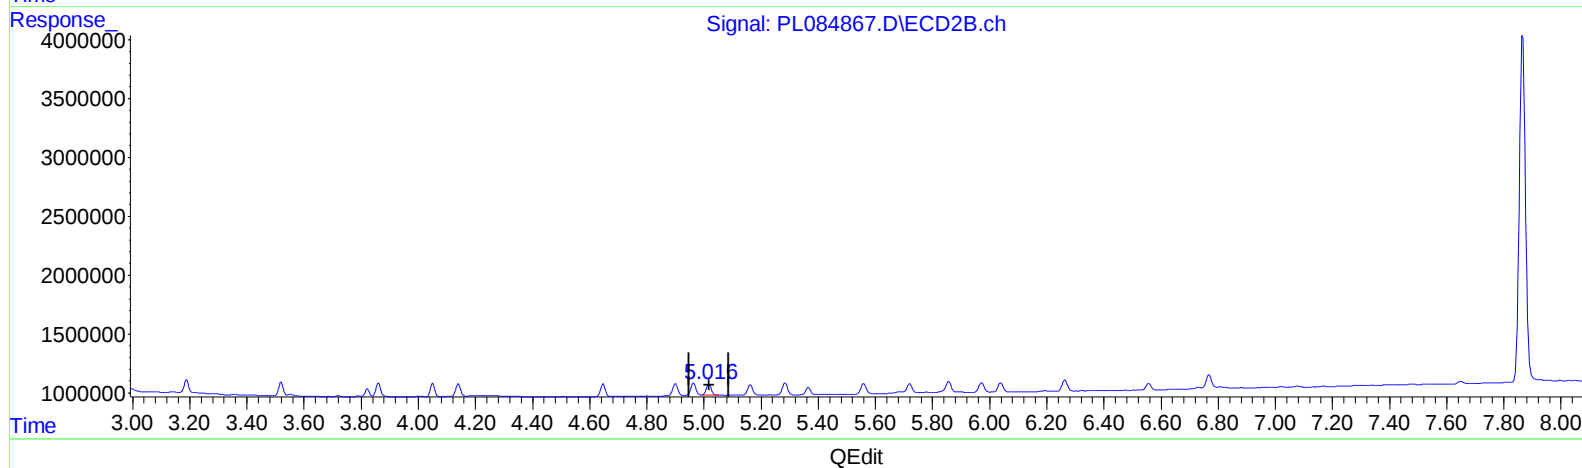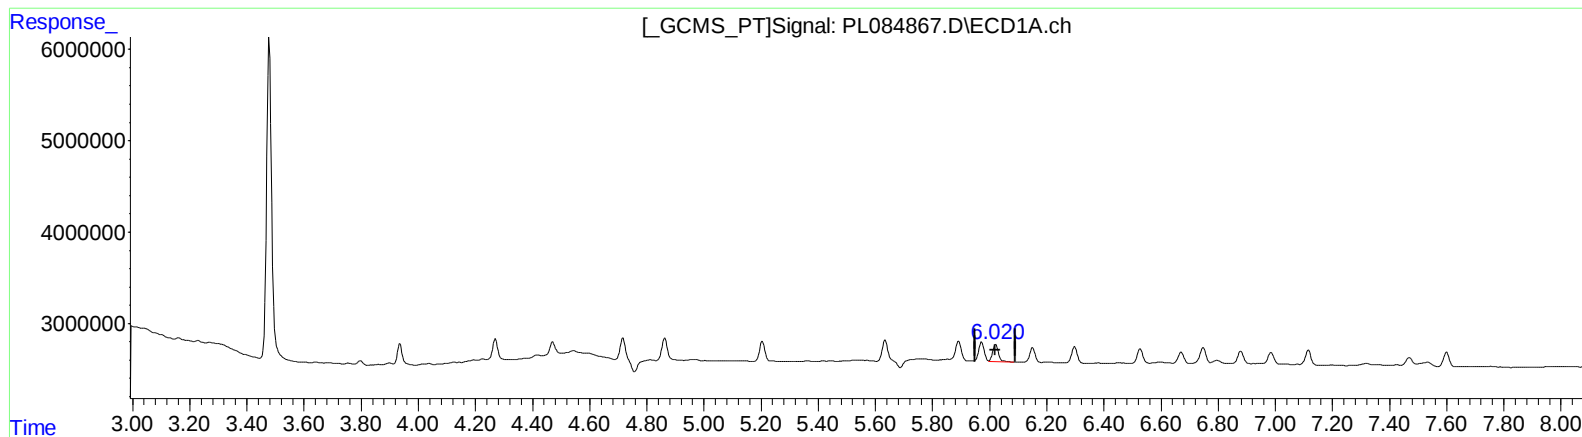

(9) Endosulfan I (A)
6.021min 0.964 ng/ml
response 2747210

(9) Endosulfan I #2 (A)
5.016min 0.853 ng/ml m
response 1150600

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

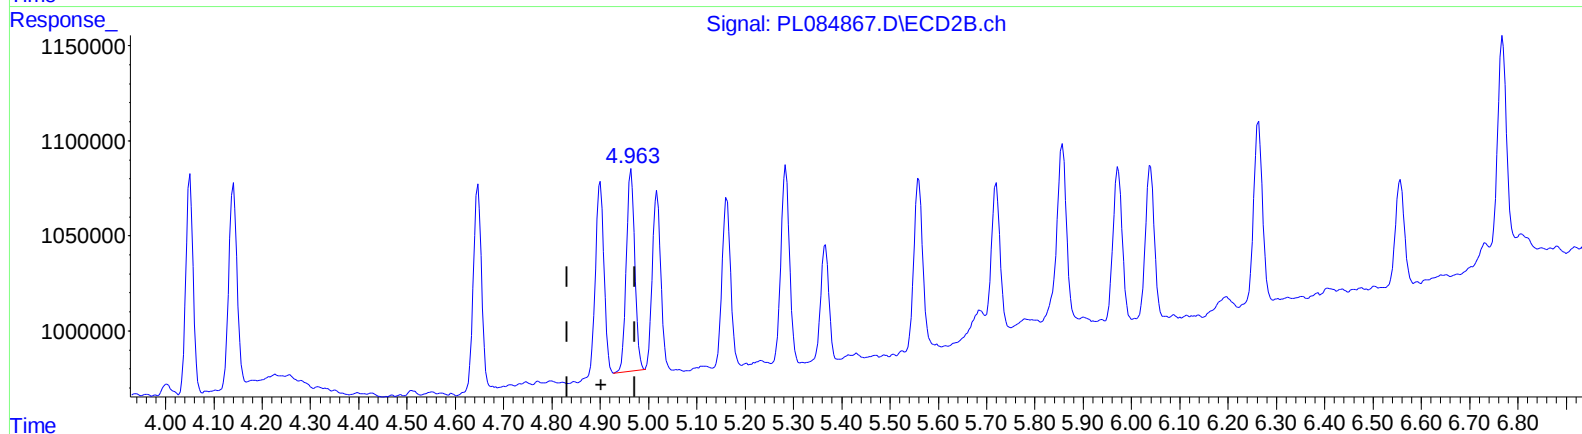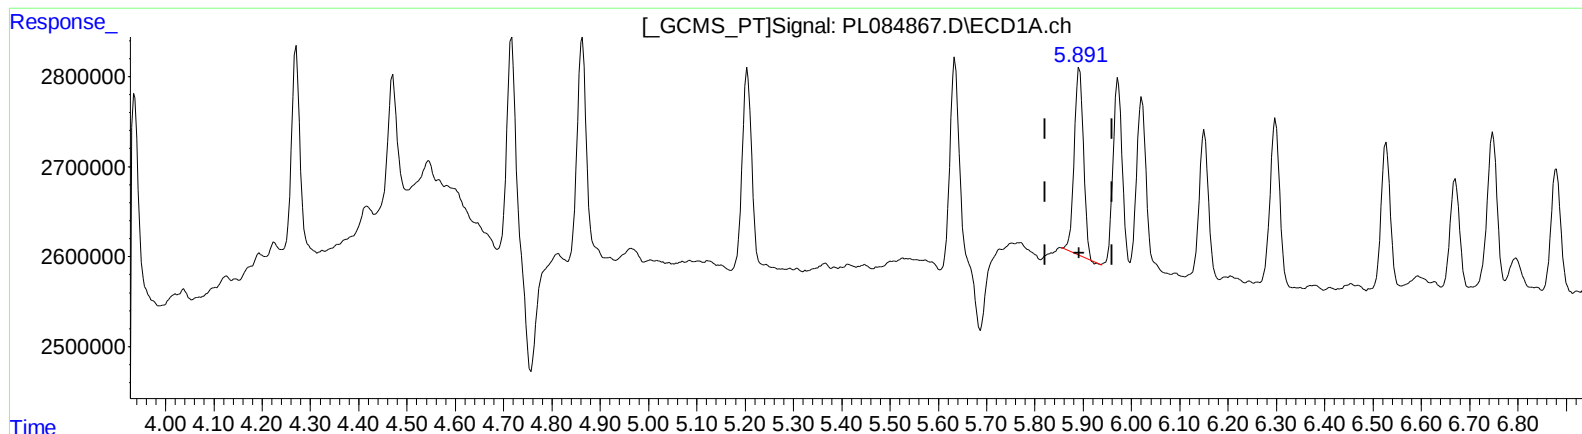

QEdit

(10) trans-Chlordane (B)

5.892min 0.890 ng/ml

response 2807156

(10) trans-Chlordane #2 (B)

4.964min 0.862 ng/ml

response 1298203

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

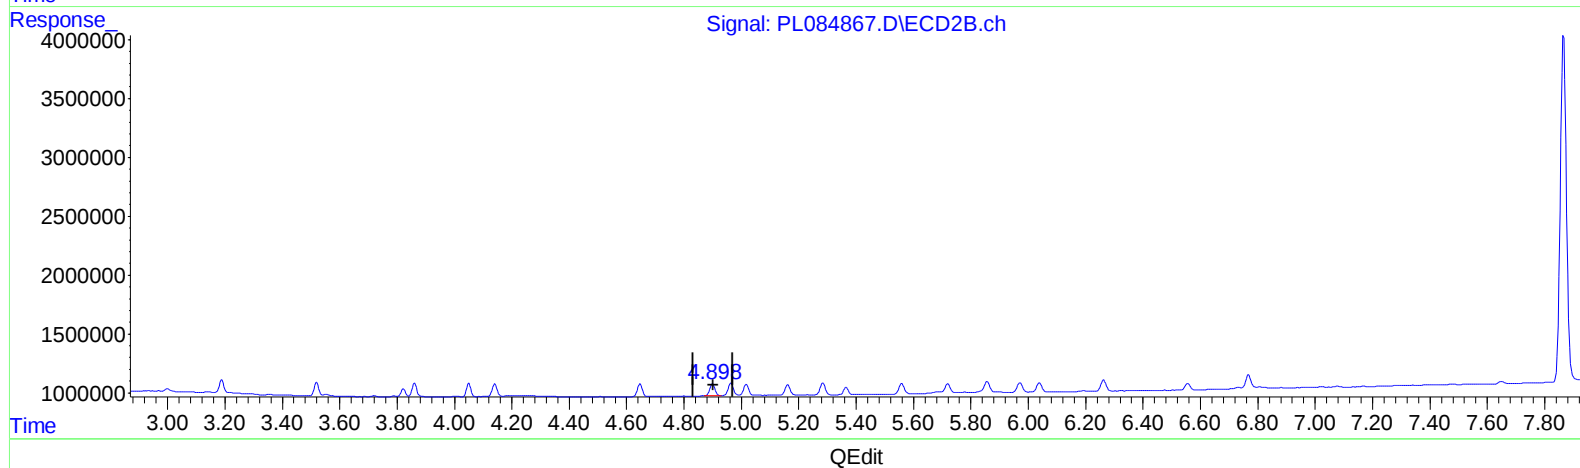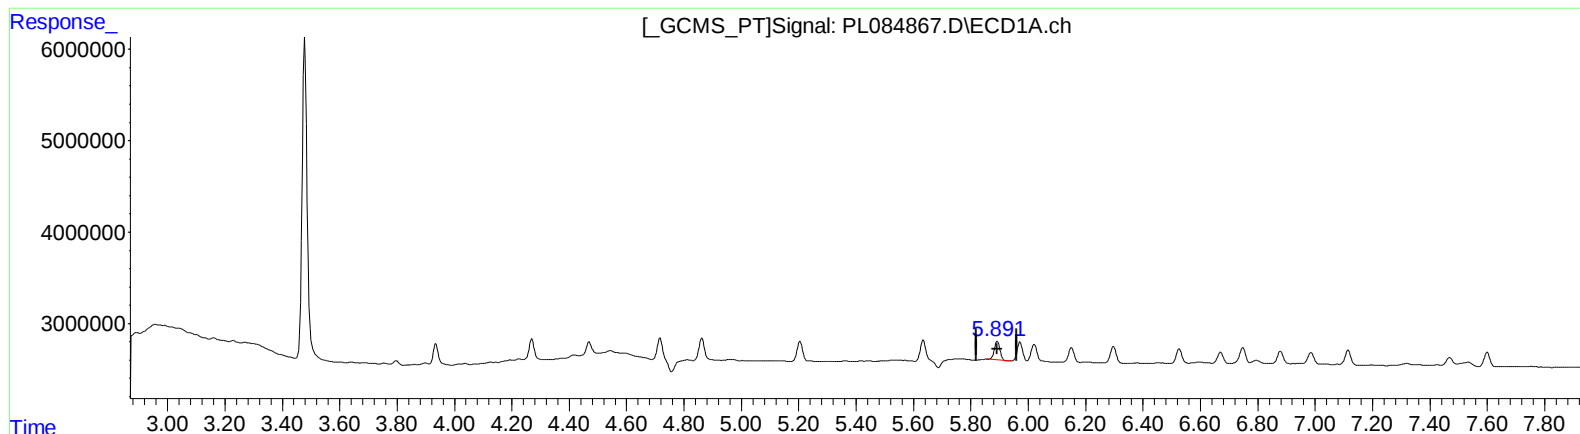

(10) trans-Chlordane (B)

5.892min 0.890 ng/ml

response 2807156

(10) trans-Chlordane #2 (B)

4.898min 0.829 ng/ml m

response 1249468

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

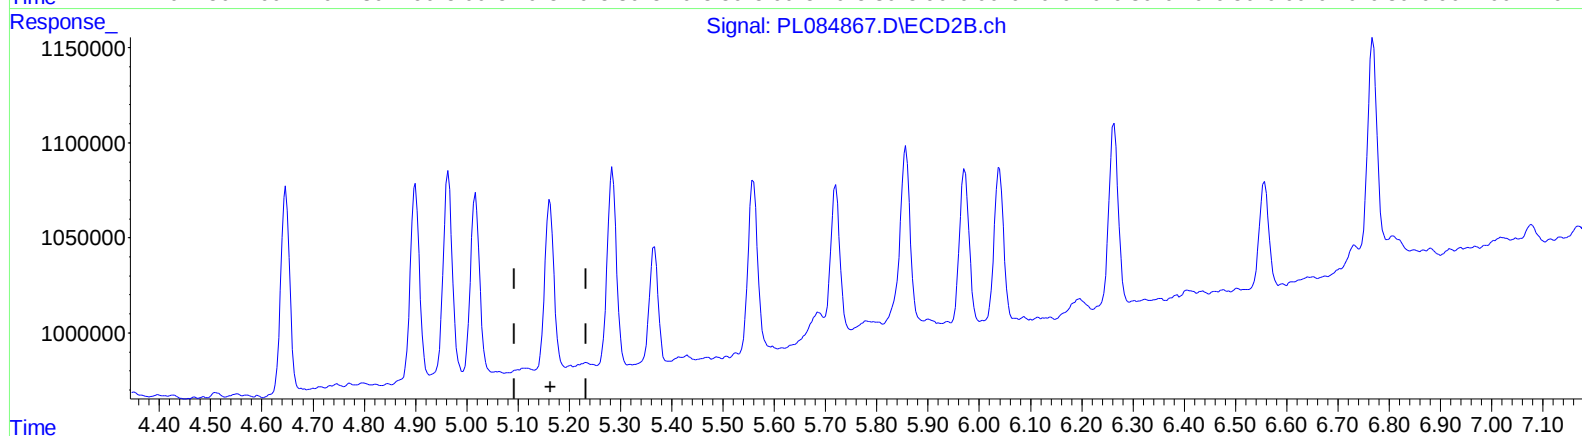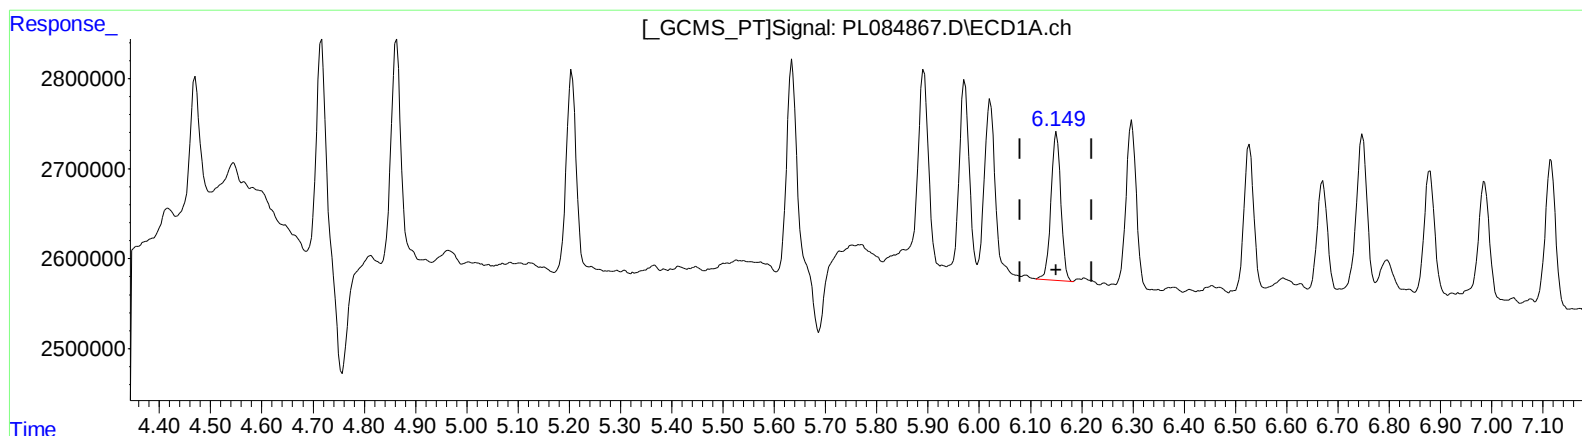

QEdit

(12) 4,4'-DDE (B)

6.151min 0.833 ng/ml

response 2203977

(12) 4,4'-DDE #2 (B)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

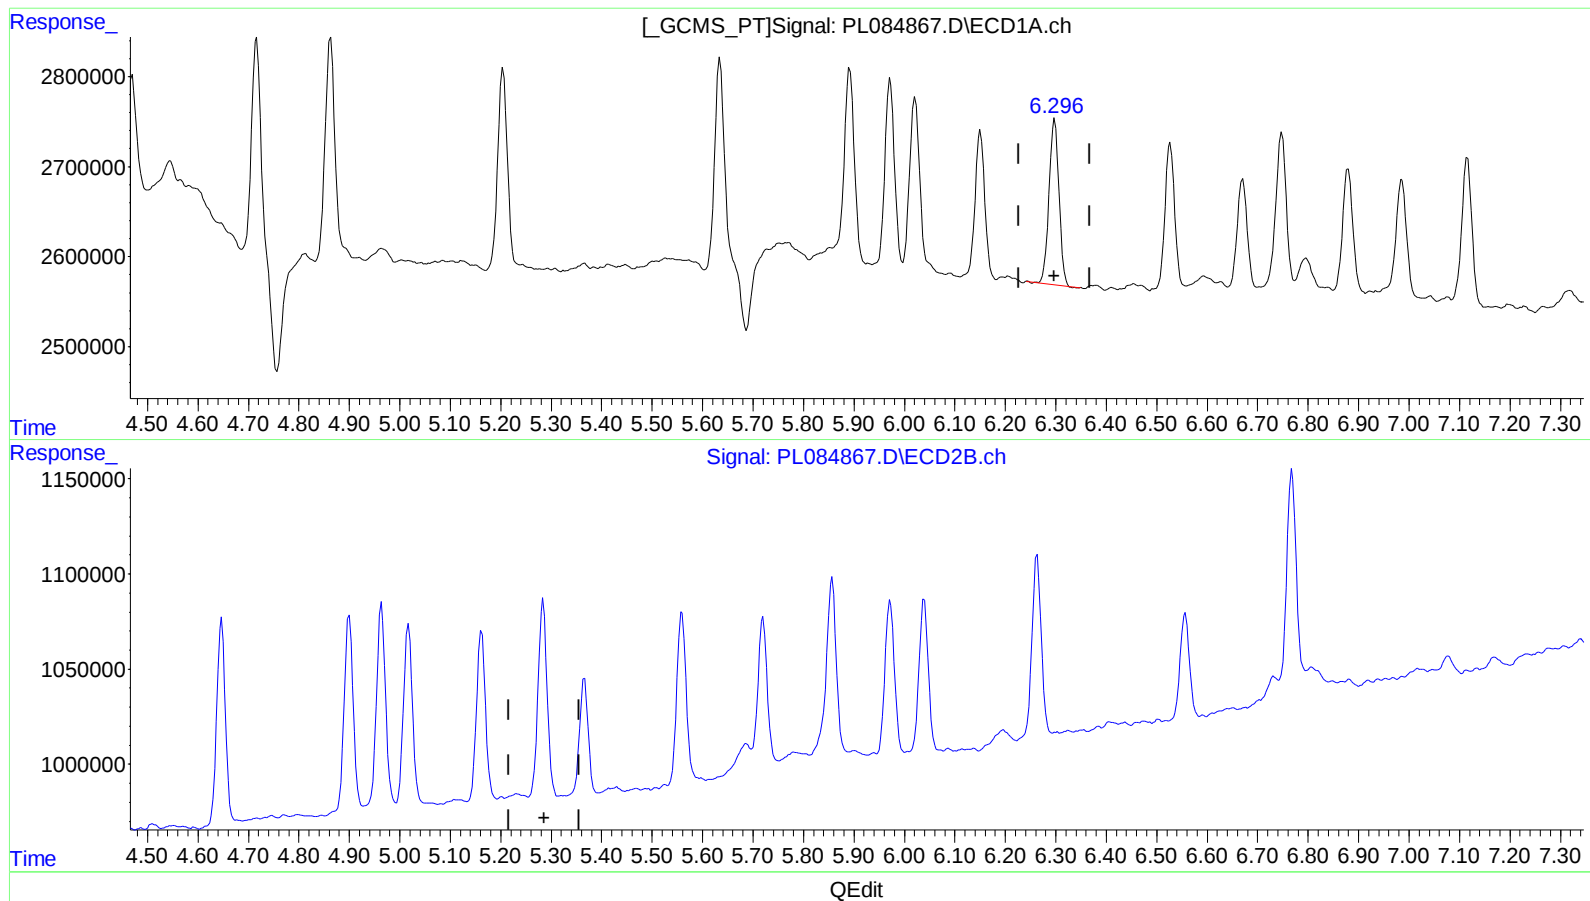

(13) Dieldrin (MA)
6.298min 0.881 ng/ml
response 2518433

(13) Dieldrin #2 (MA)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

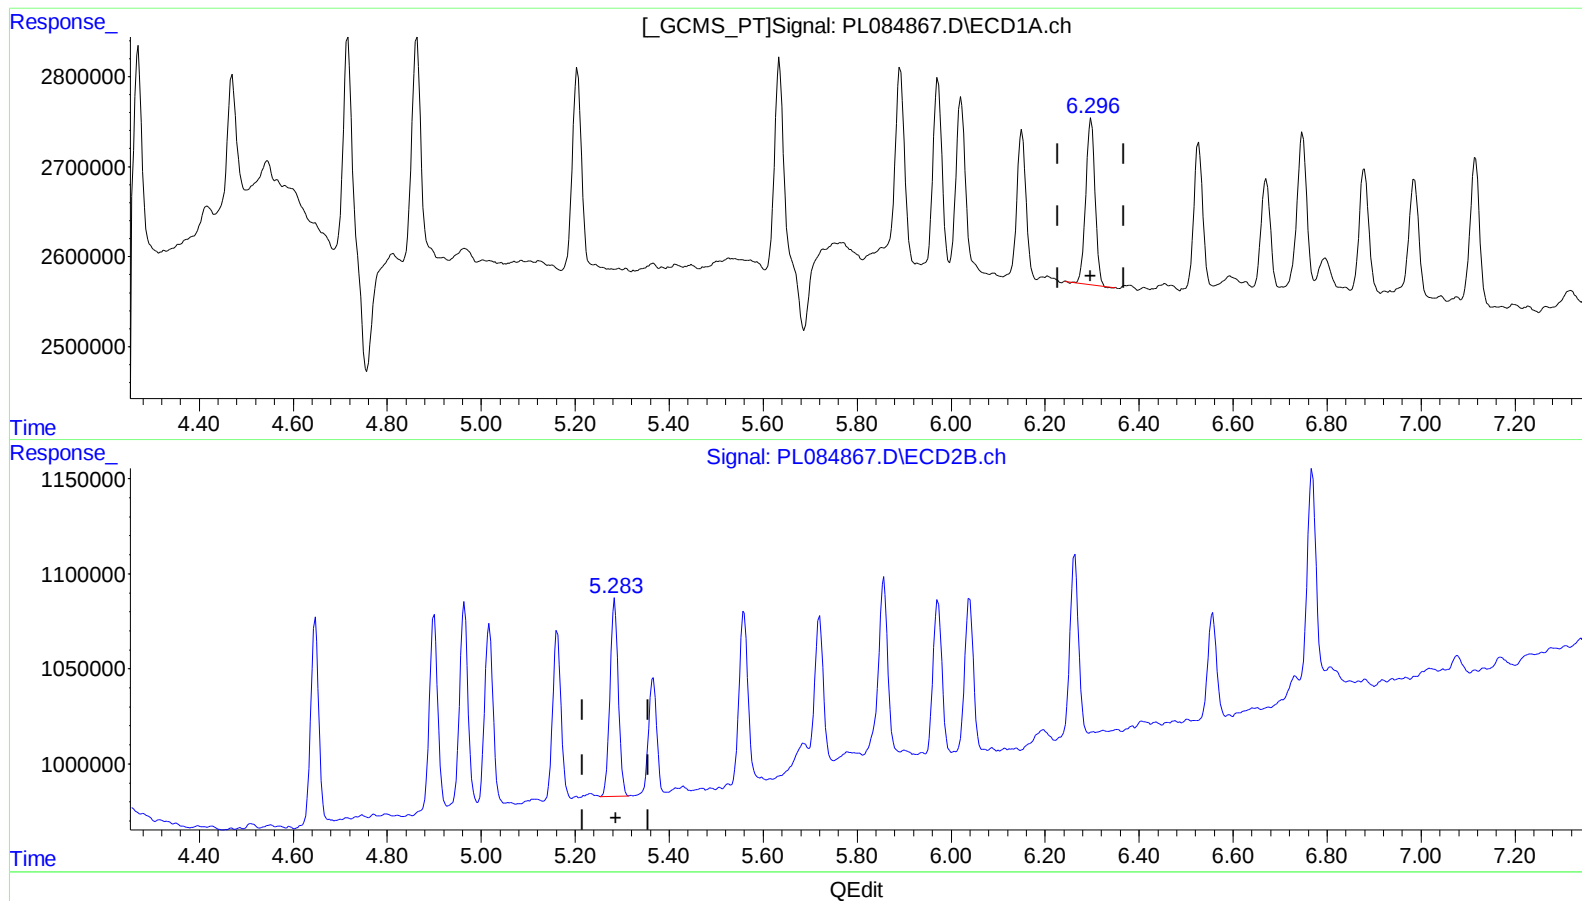

(13) Dieldrin (MA)
6.298min 0.881 ng/ml
response 2518433

(13) Dieldrin #2 (MA)
5.283min 0.835 ng/ml m
response 1294824

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

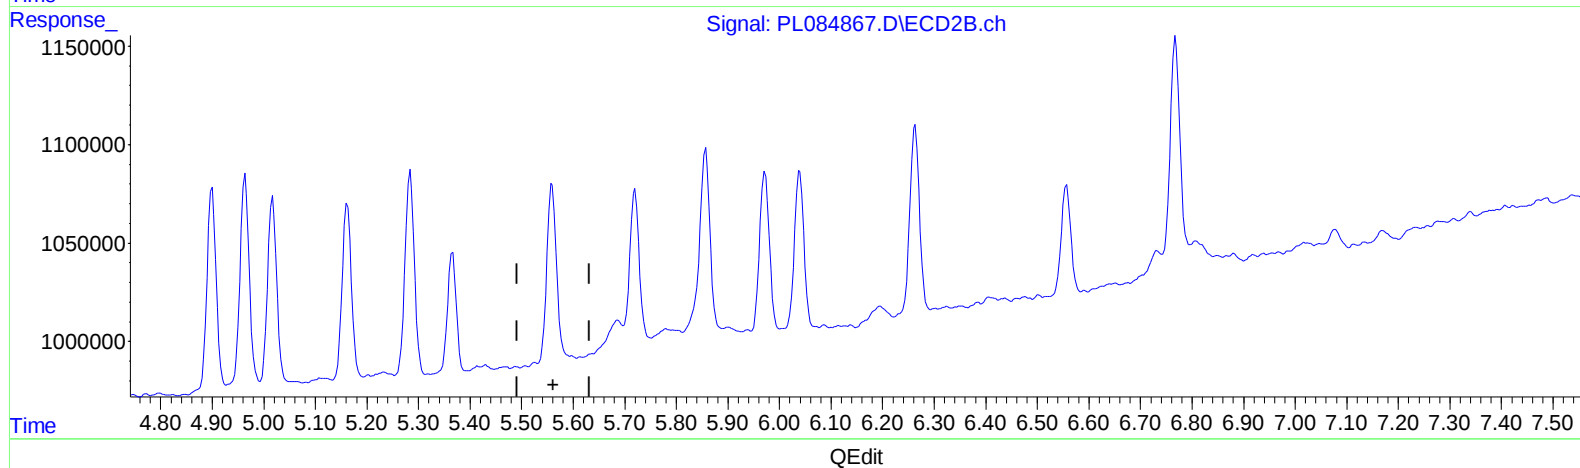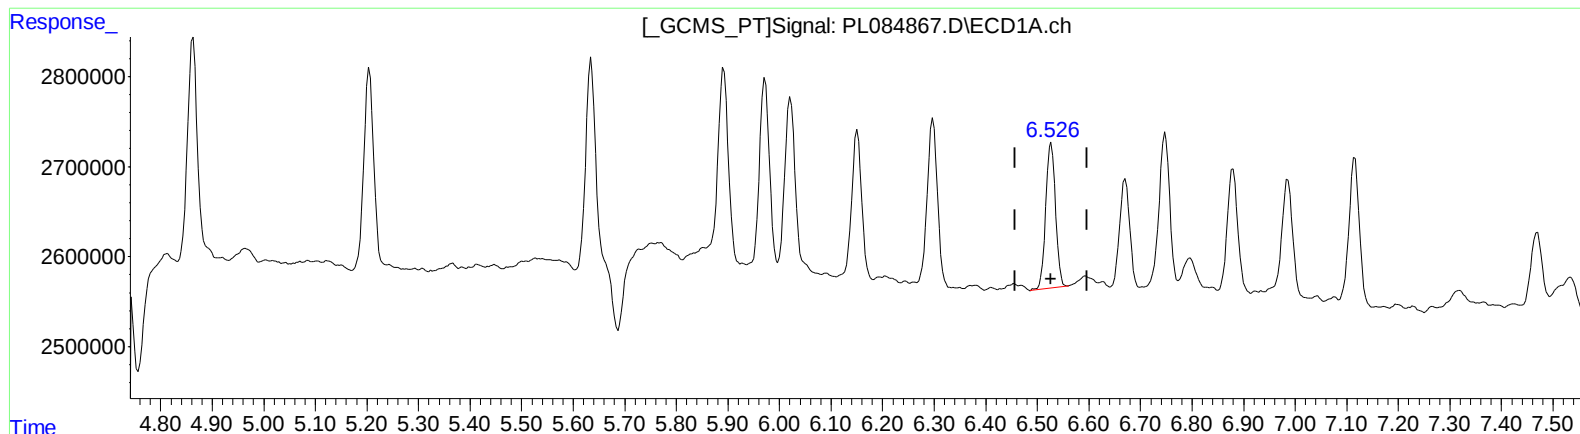

(14) Endrin (MA)
6.527min 0.936 ng/ml
response 2132343

(14) Endrin #2 (MA)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

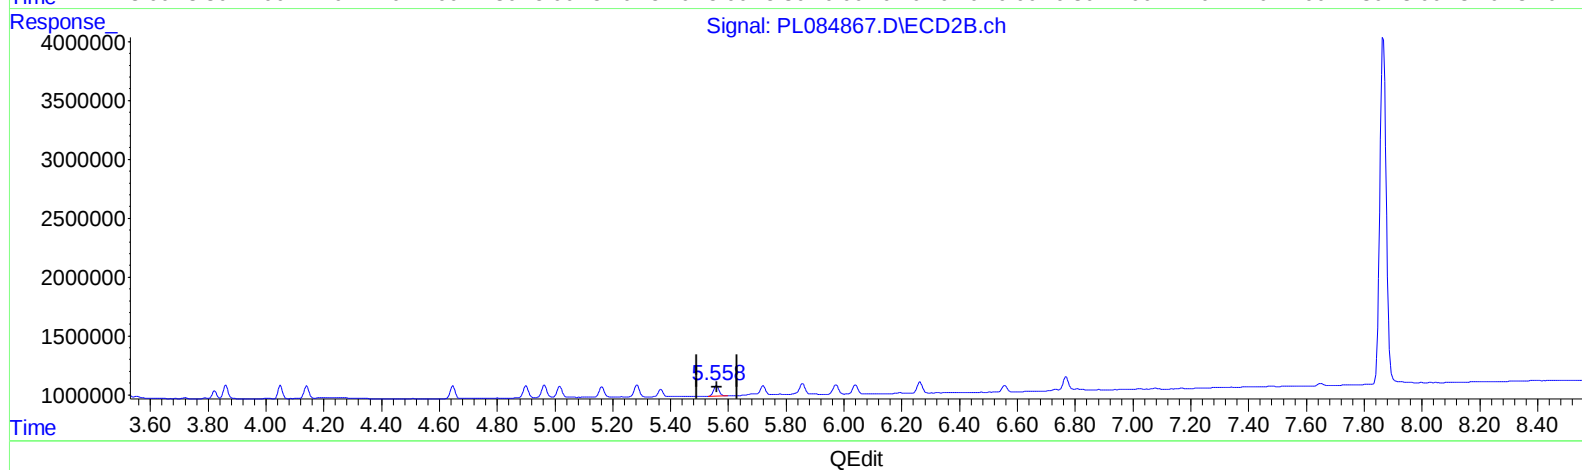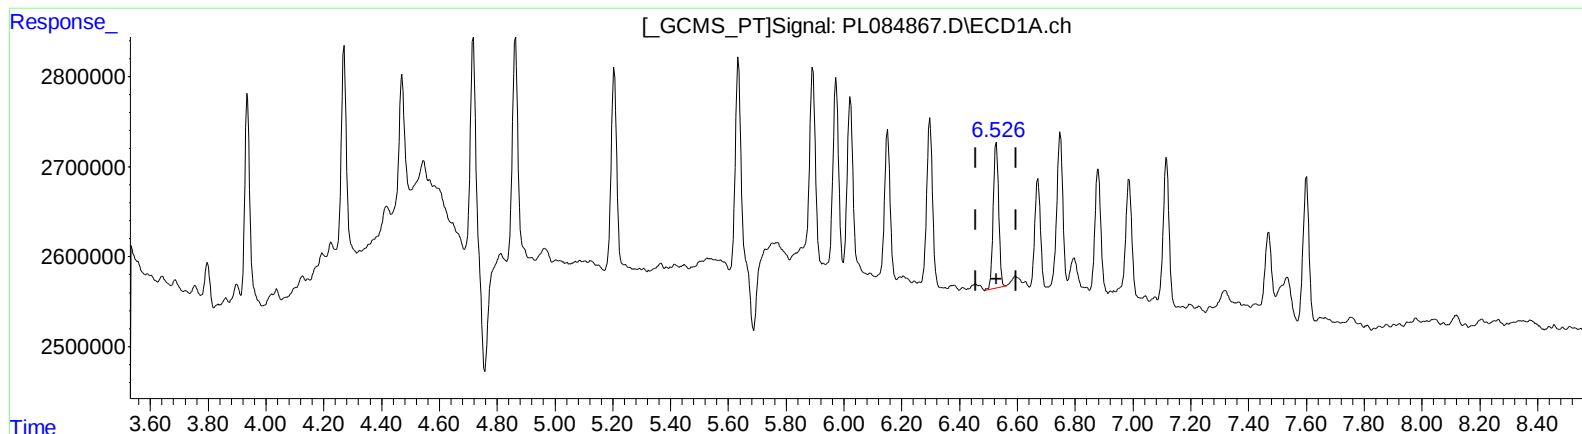

(14) Endrin (MA)

6.527min 0.936 ng/ml

response 2132343

(14) Endrin #2 (MA)

5.558min 0.833 ng/ml m

response 1147364

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

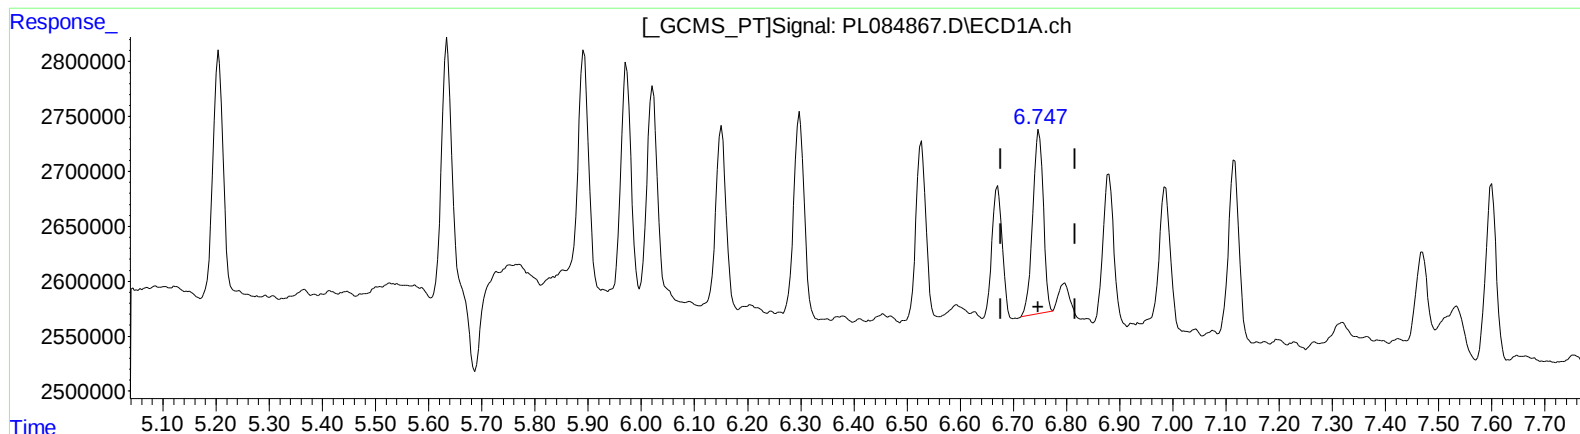

(15) Endosulfan II (B)
6.748min 0.991 ng/ml
response 2330483

(15) Endosulfan II #2 (B)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

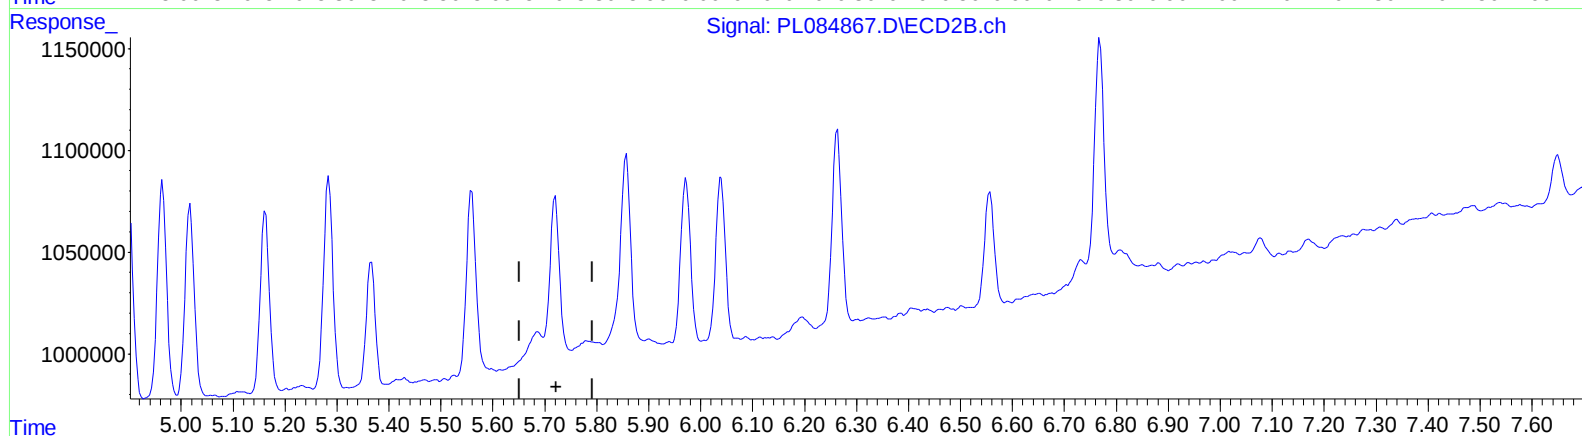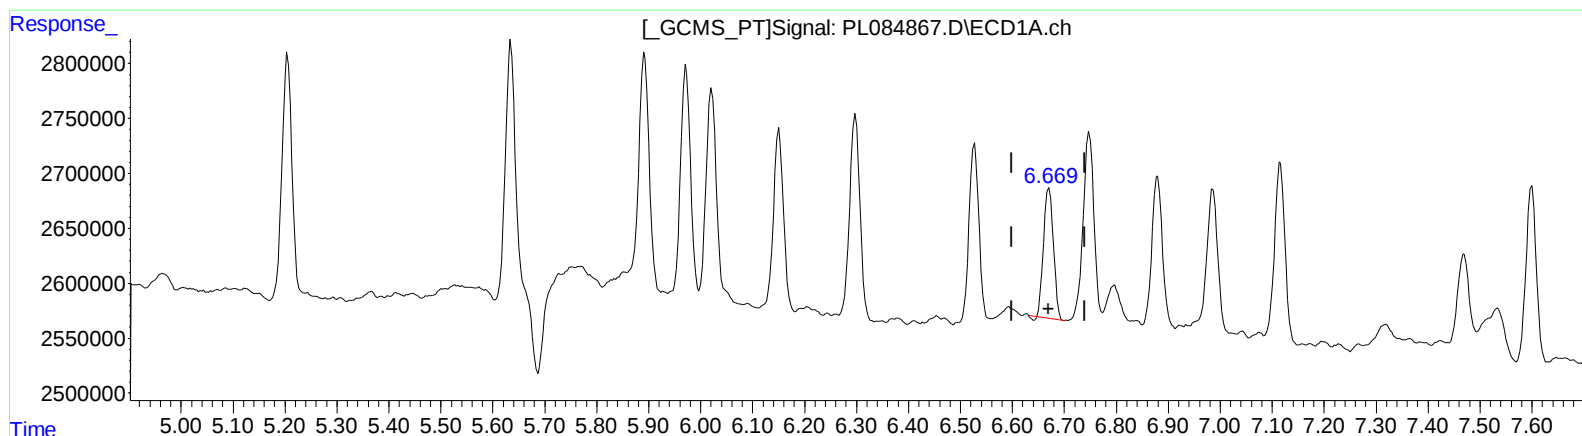

QEdit

(16) 4,4'-DDD (A)
6.670min 0.827 ng/ml
response 1563779

(16) 4,4'-DDD #2 (A)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

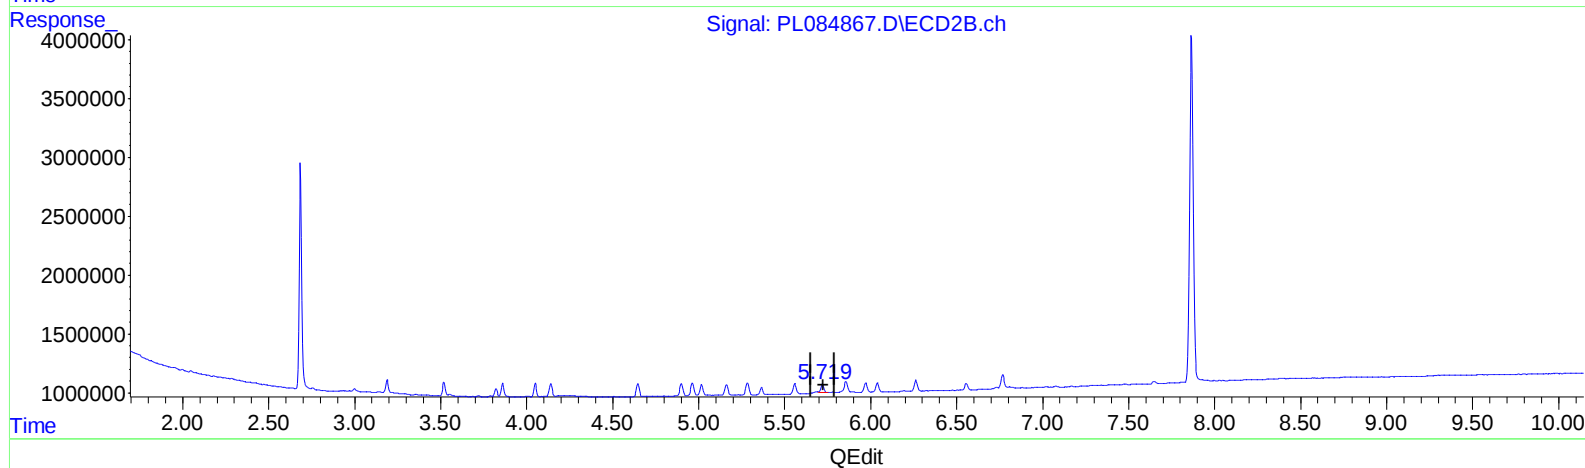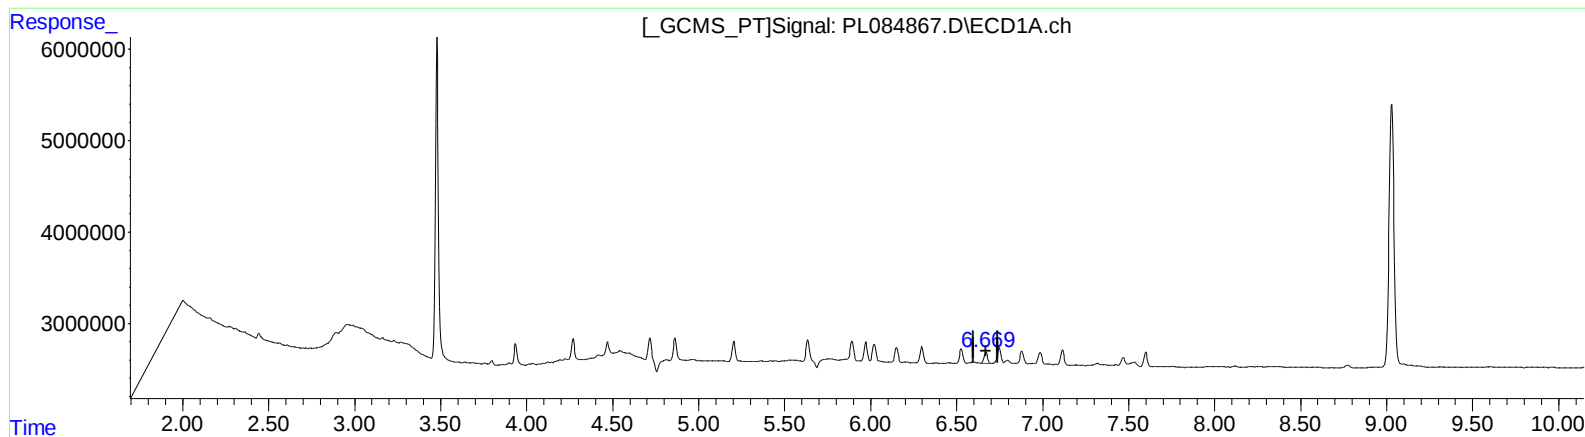

QEdit

(16) 4,4'-DDD (A)

6.669min 0.872 ng/ml m

response 1649640

(16) 4,4'-DDD #2 (A)

5.719min 0.794 ng/ml m

response 949223

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

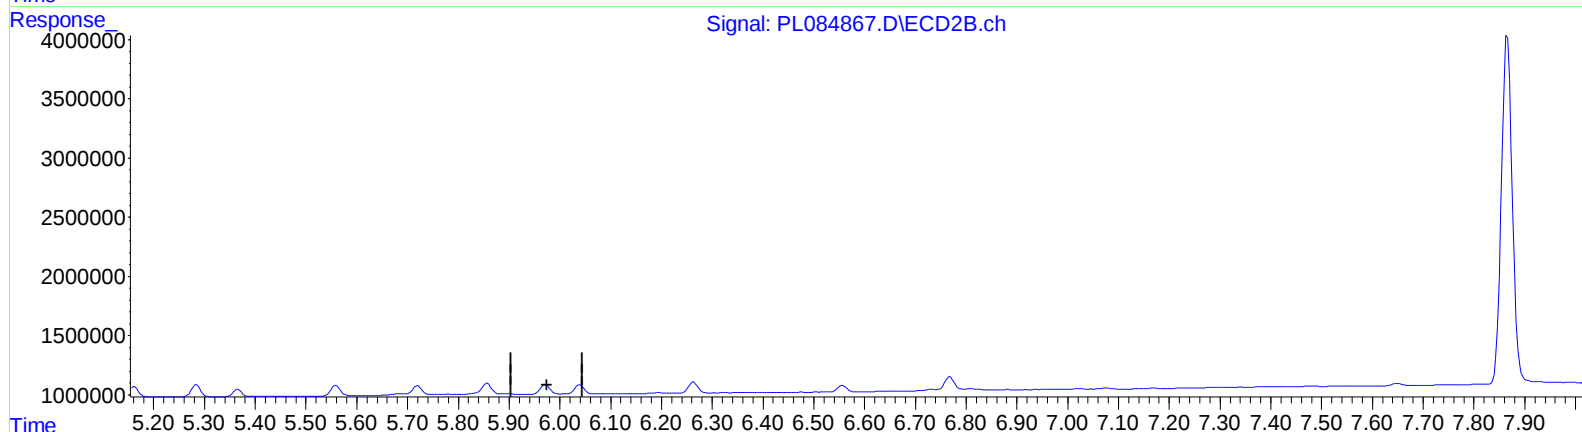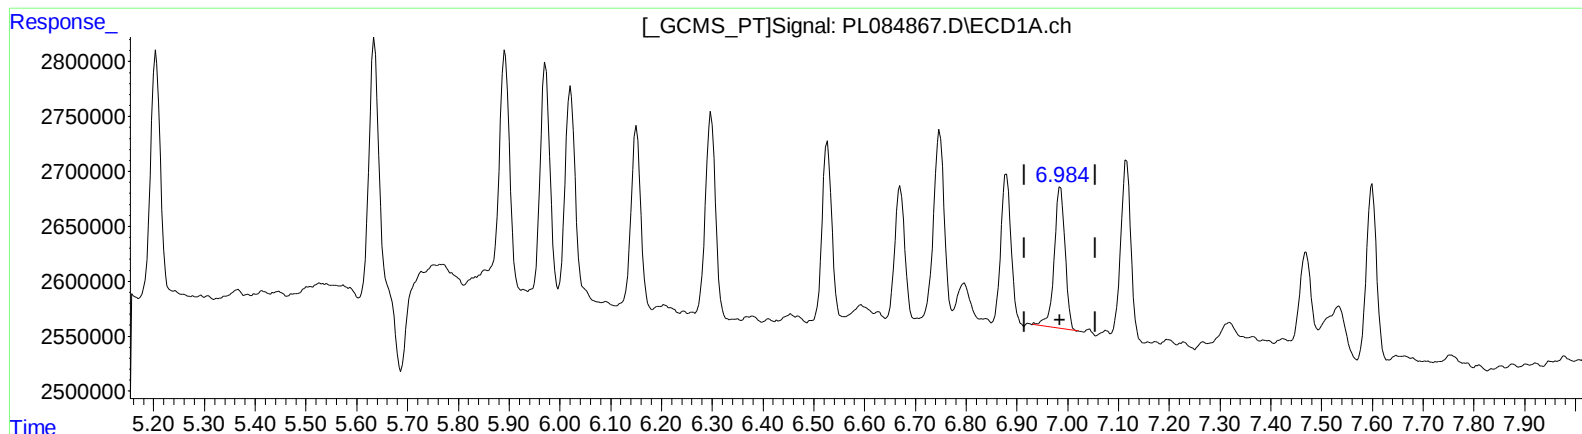

QEdit

(17) 4,4'-DDT (MA)
6.986min 0.995 ng/ml
response 1917908

(17) 4,4'-DDT #2 (MA)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

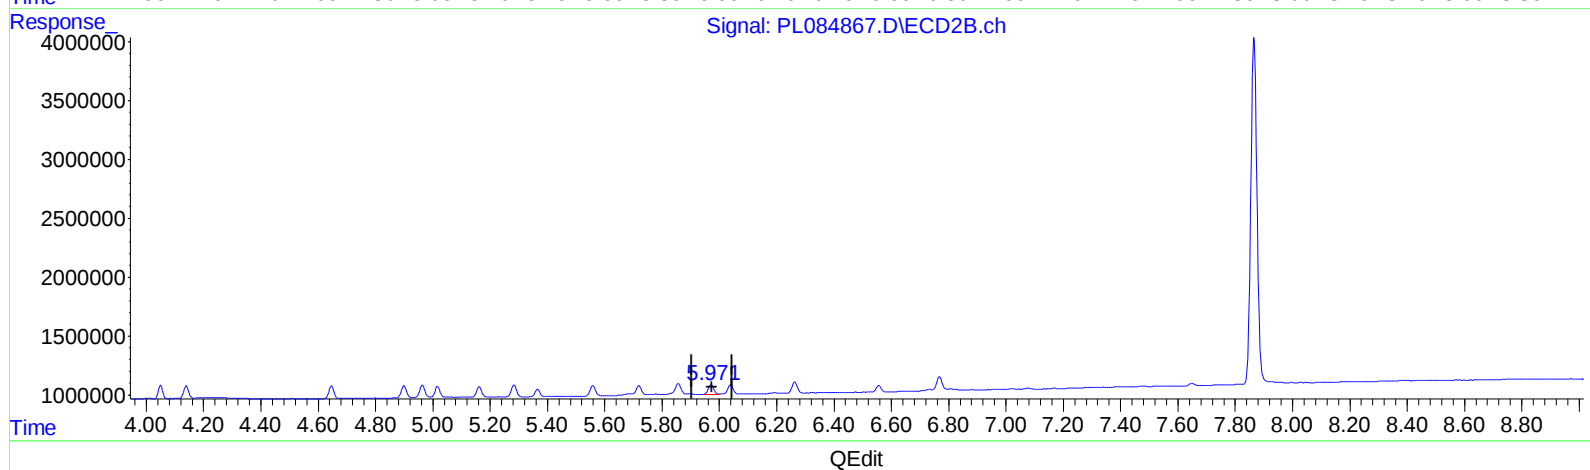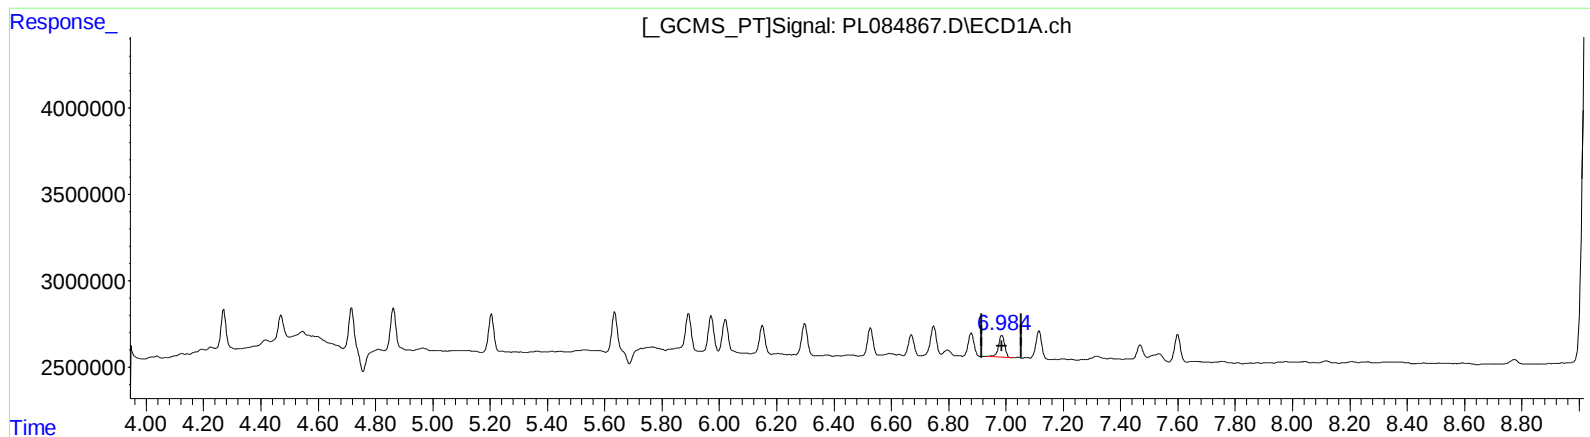

(17) 4,4'-DDT (MA)

6.986min 0.995 ng/ml

response 1917908

(17) 4,4'-DDT #2 (MA)

5.971min 0.844 ng/ml m

response 1094221

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

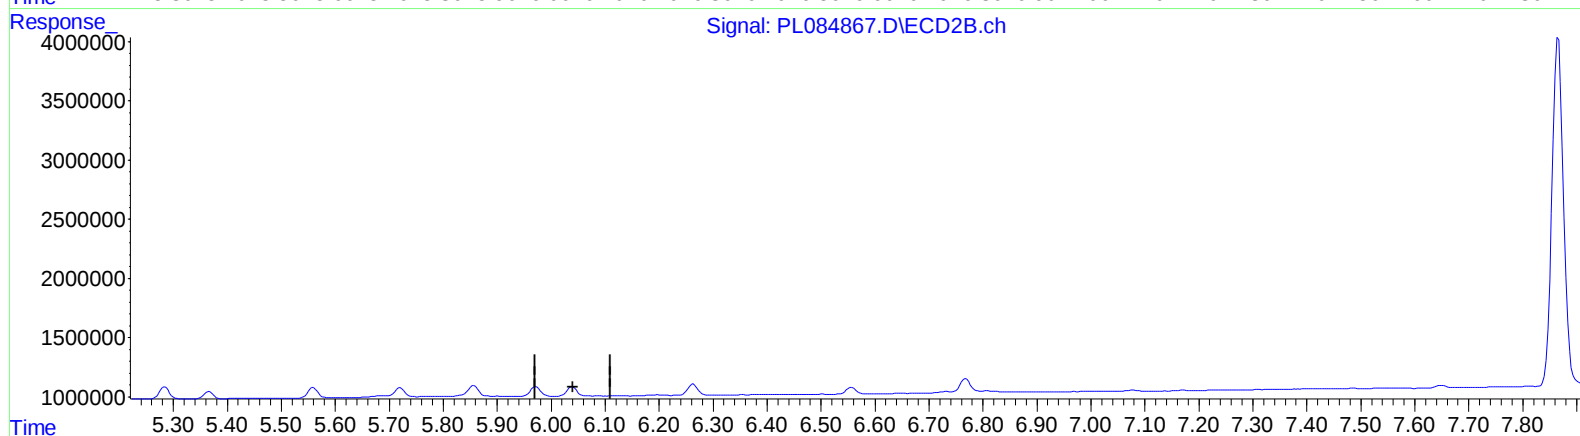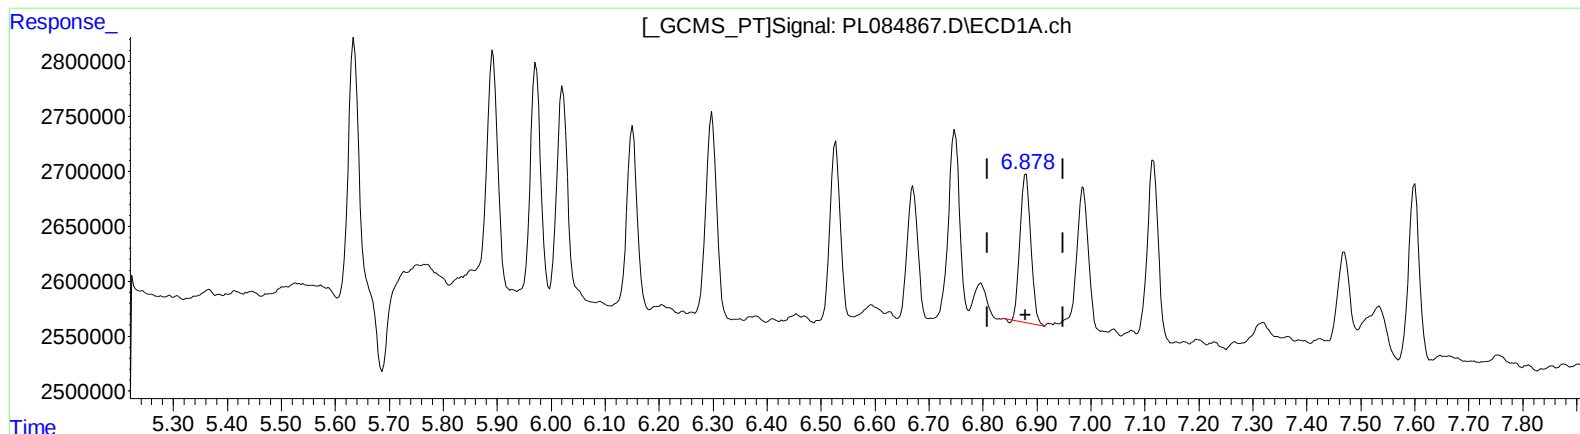

QEdit

(18) Endrin aldehyde (B)
6.880min 1.009 ng/ml
response 1877288

(18) Endrin aldehyde #2 (B)
0.000min 0.000 ng/ml
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

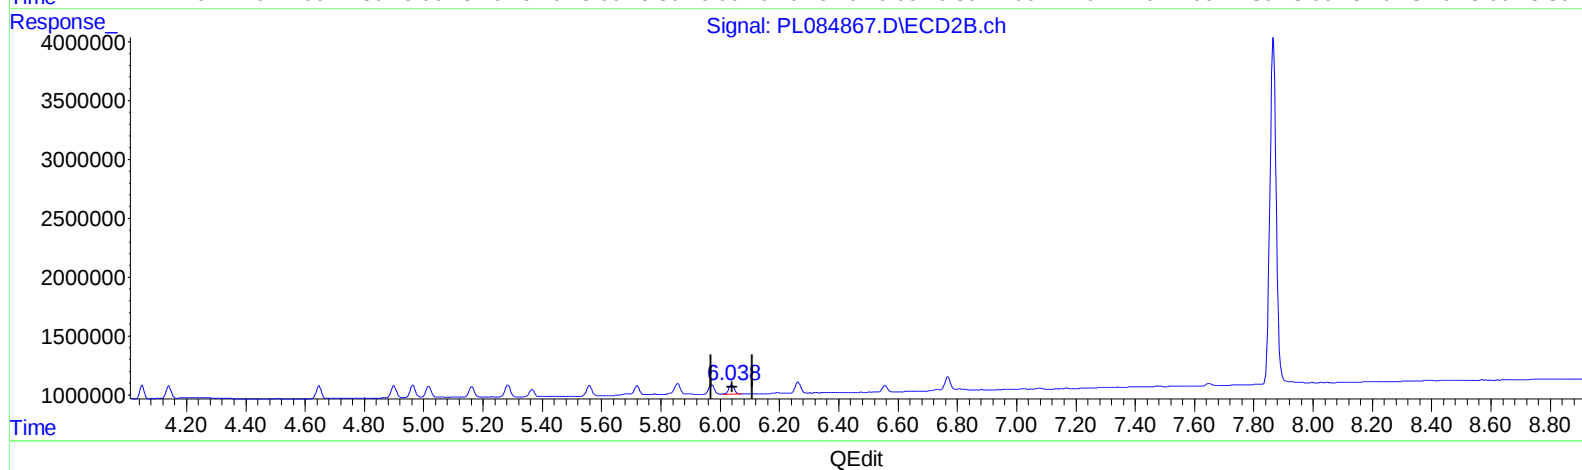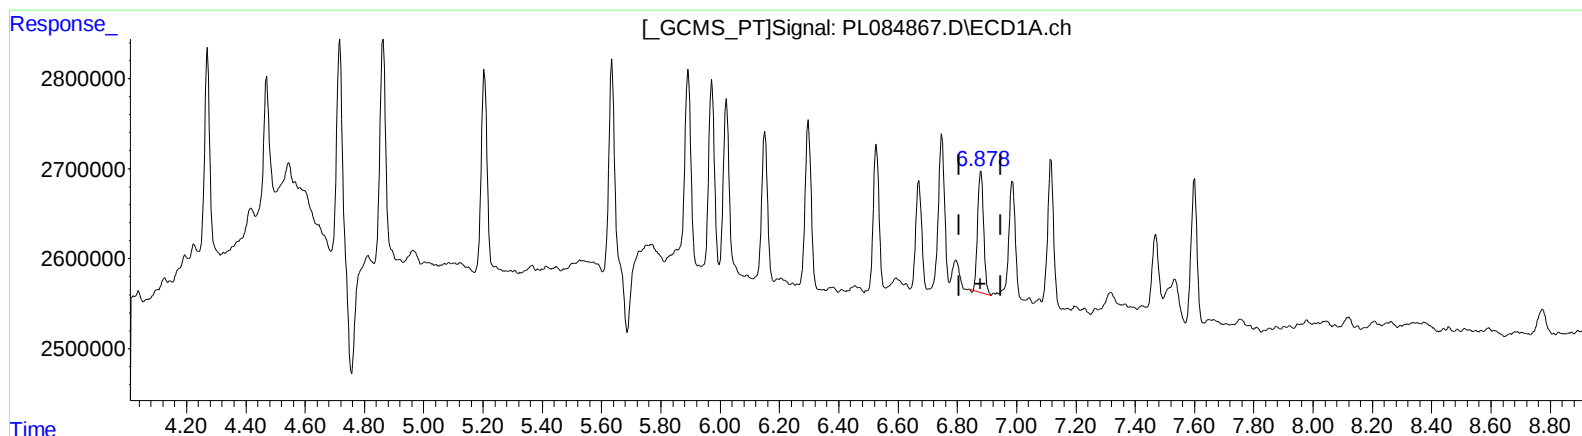

(18) Endrin aldehyde (B)

6.880min 1.009 ng/ml

response 1877288

(18) Endrin aldehyde #2 (B)

6.038min 0.894 ng/ml m

response 1016539

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

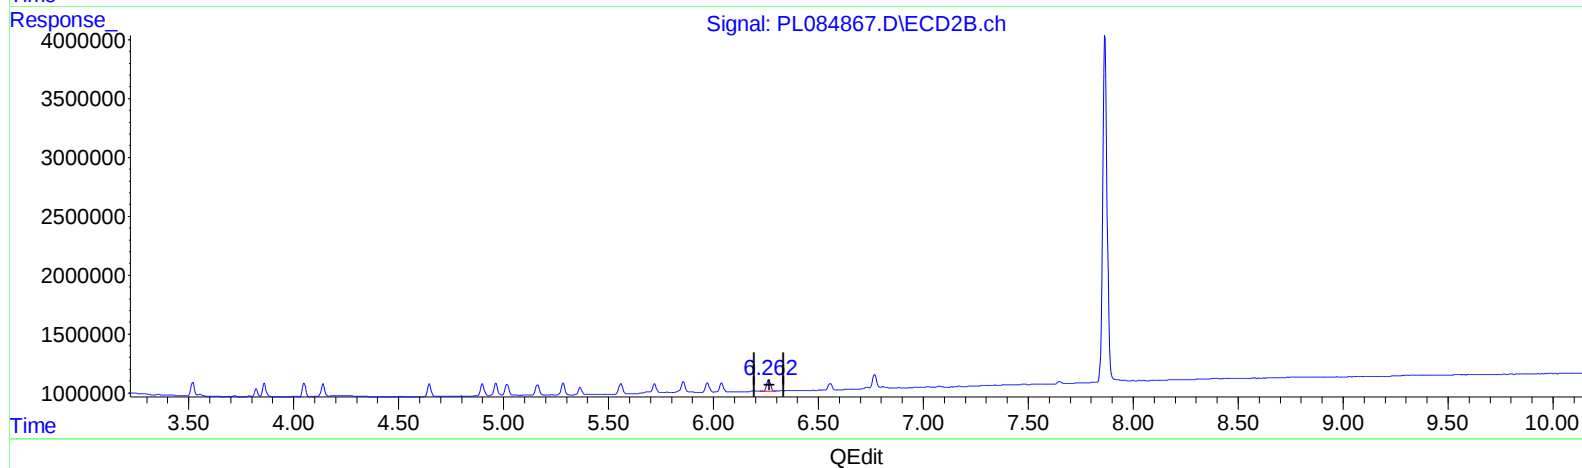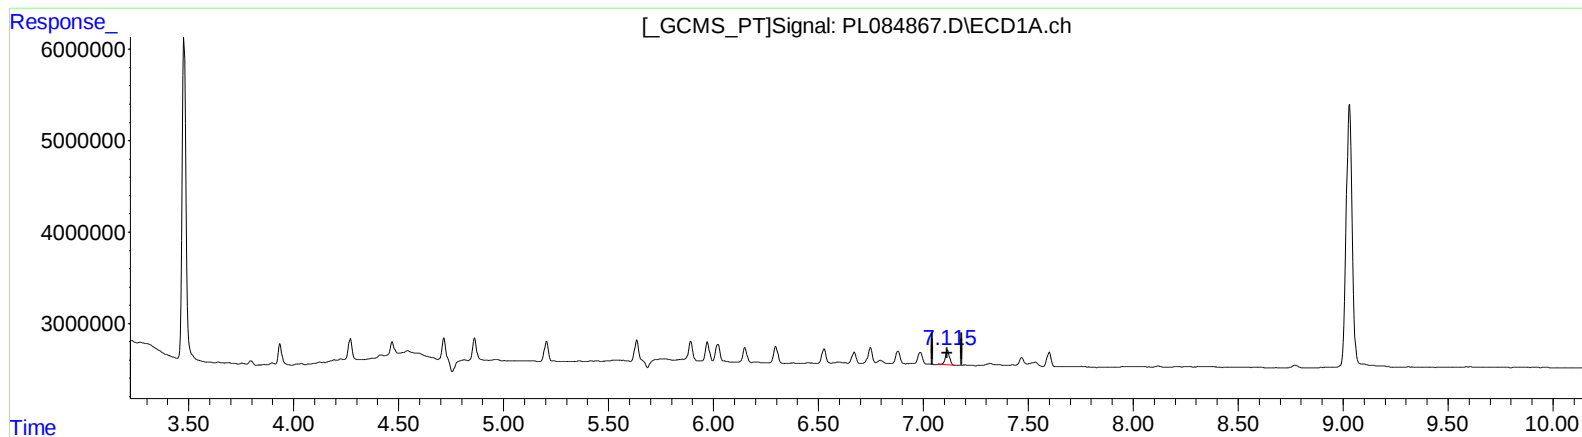

(19) Endosulfan Sulfate (B)

7.116min 1.010 ng/ml

response 2234411

(19) Endosulfan Sulfate #2 (B)

6.262min 0.900 ng/ml m

response 1229900

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

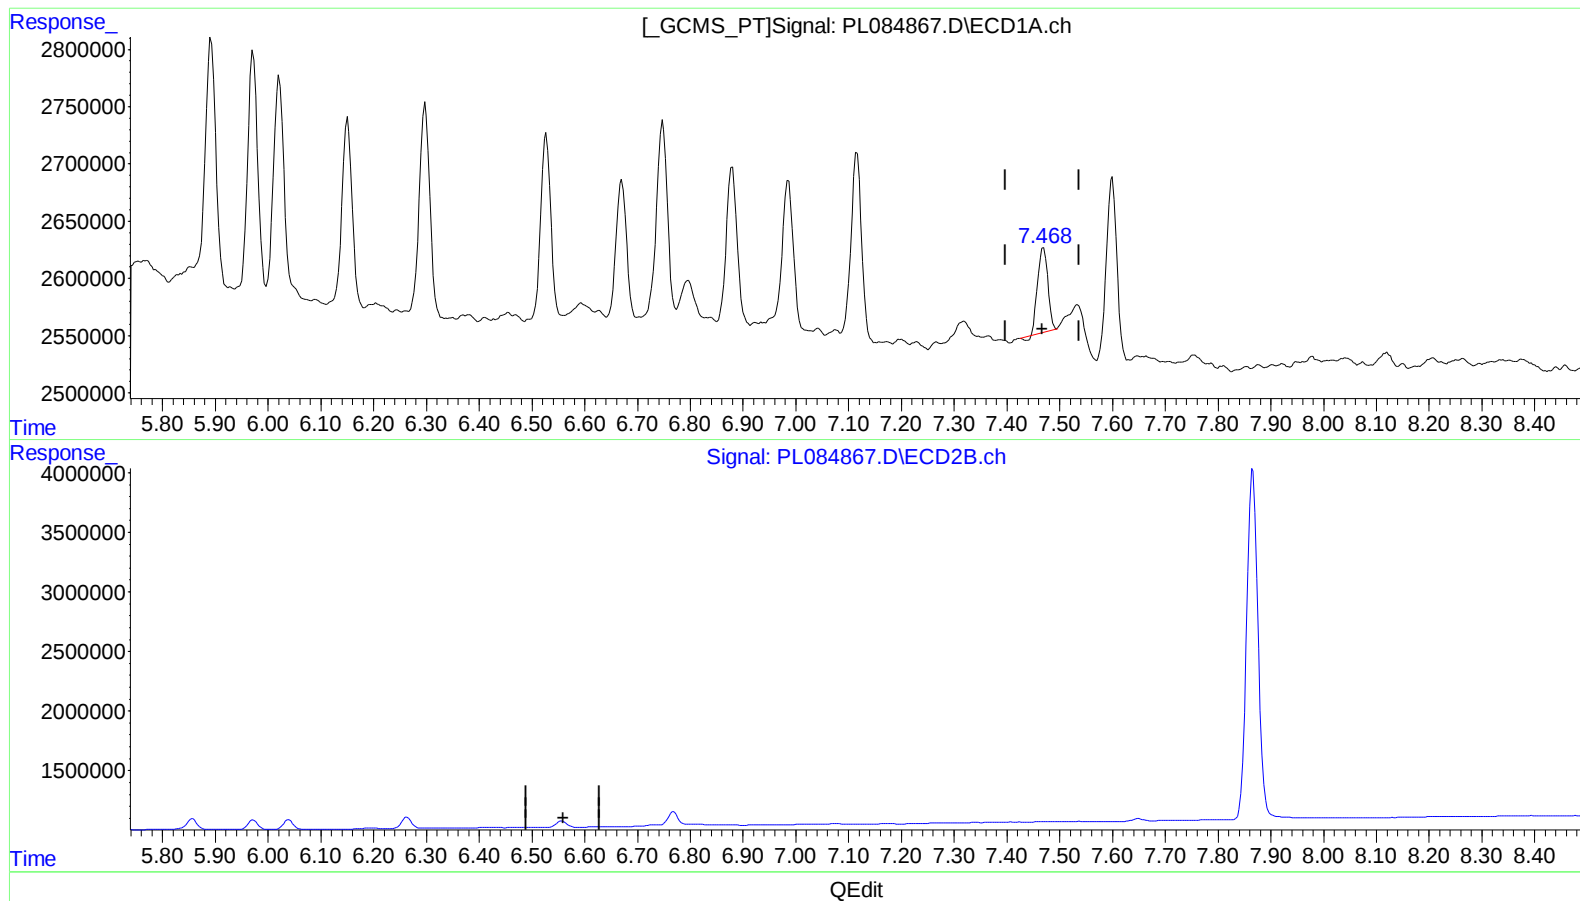

(20) Methoxychlor (A)

7.469min 1.013 ng/ml

response 983164

(20) Methoxychlor #2 (A)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082123\
Data File : PL084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2023 11:04
Operator : AR\AJ
Sample : 03573-01
Misc : PEST MDL WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
MDL-WATER-QT3-2023-05

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 21 22:28:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

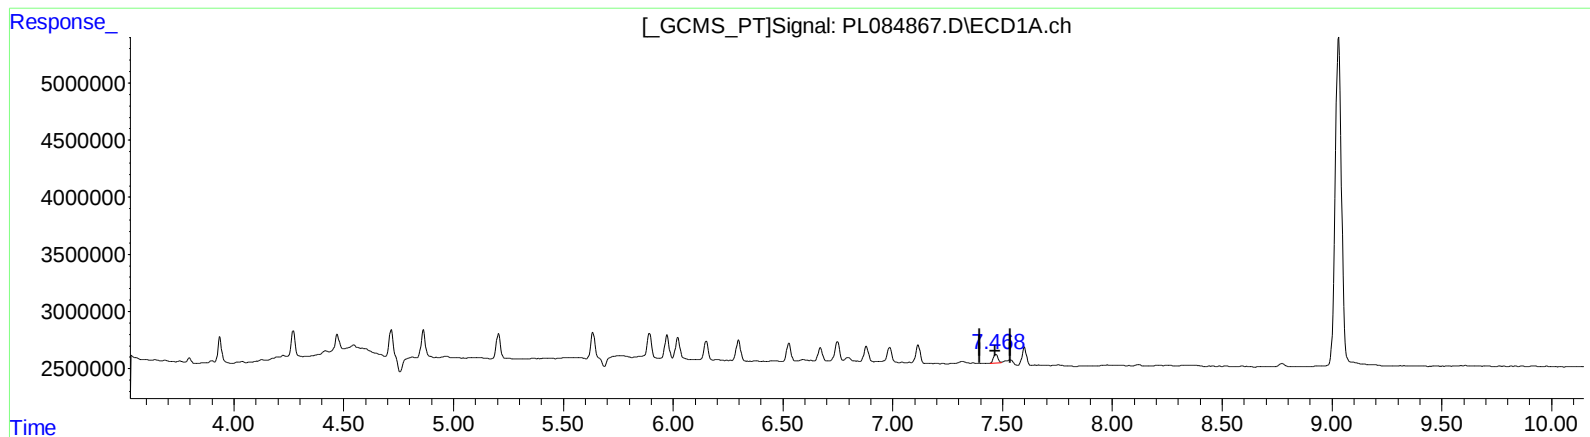

(20) Methoxychlor (A)
7.468min 1.118 ng/ml m
response 1085000

(20) Methoxychlor #2 (A)
6.555min 1.025 ng/ml m
response 725296