

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082124\
 Data File : PL091253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2024 04:02
 Operator : AR\AJ
 Sample : PIBLK246
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 05:27:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080824CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 10 07:10:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.784	53915949	51759399	26.626	29.493
27)	SA Decachlor...	9.056	7.924	39270032	51067692	25.224	29.756
Target Compounds							
6)	B beta-BHC	0.000	3.872f	0	1974474	N.D.	1.765
7)	B delta-BHC	4.762	0.000	2175409	0	0.777	N.D. #
8)	B Heptachlo...	5.683	0.000	9603017	0	3.687	N.D. #
9)	A Endosulfan I	6.105	0.000	954383	0	0.430	N.D. #
12)	B 4,4'-DDE	6.255f	5.196f	2341480	913096	1.172	0.488 #
14)	MA Endrin	6.519f	5.667	-84032	1280701	N.D.	0.669
15)	B Endosulfa...	6.797	0.000	2941106	0	1.531	N.D. #
20)	A Methoxychlor	7.495	0.000	1025910	0	1.230	N.D. #
22)	Toxaphene-1	5.851	0.000	1950325	0	260.158	N.D. #
23)	Toxaphene-2	0.000	5.667	0	1280701	N.D.	124.892


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082124\
Data File : PL091253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2024 04:02
Operator : AR\AJ
Sample : PIBLK246
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 05:27:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080824CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 10 07:10:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

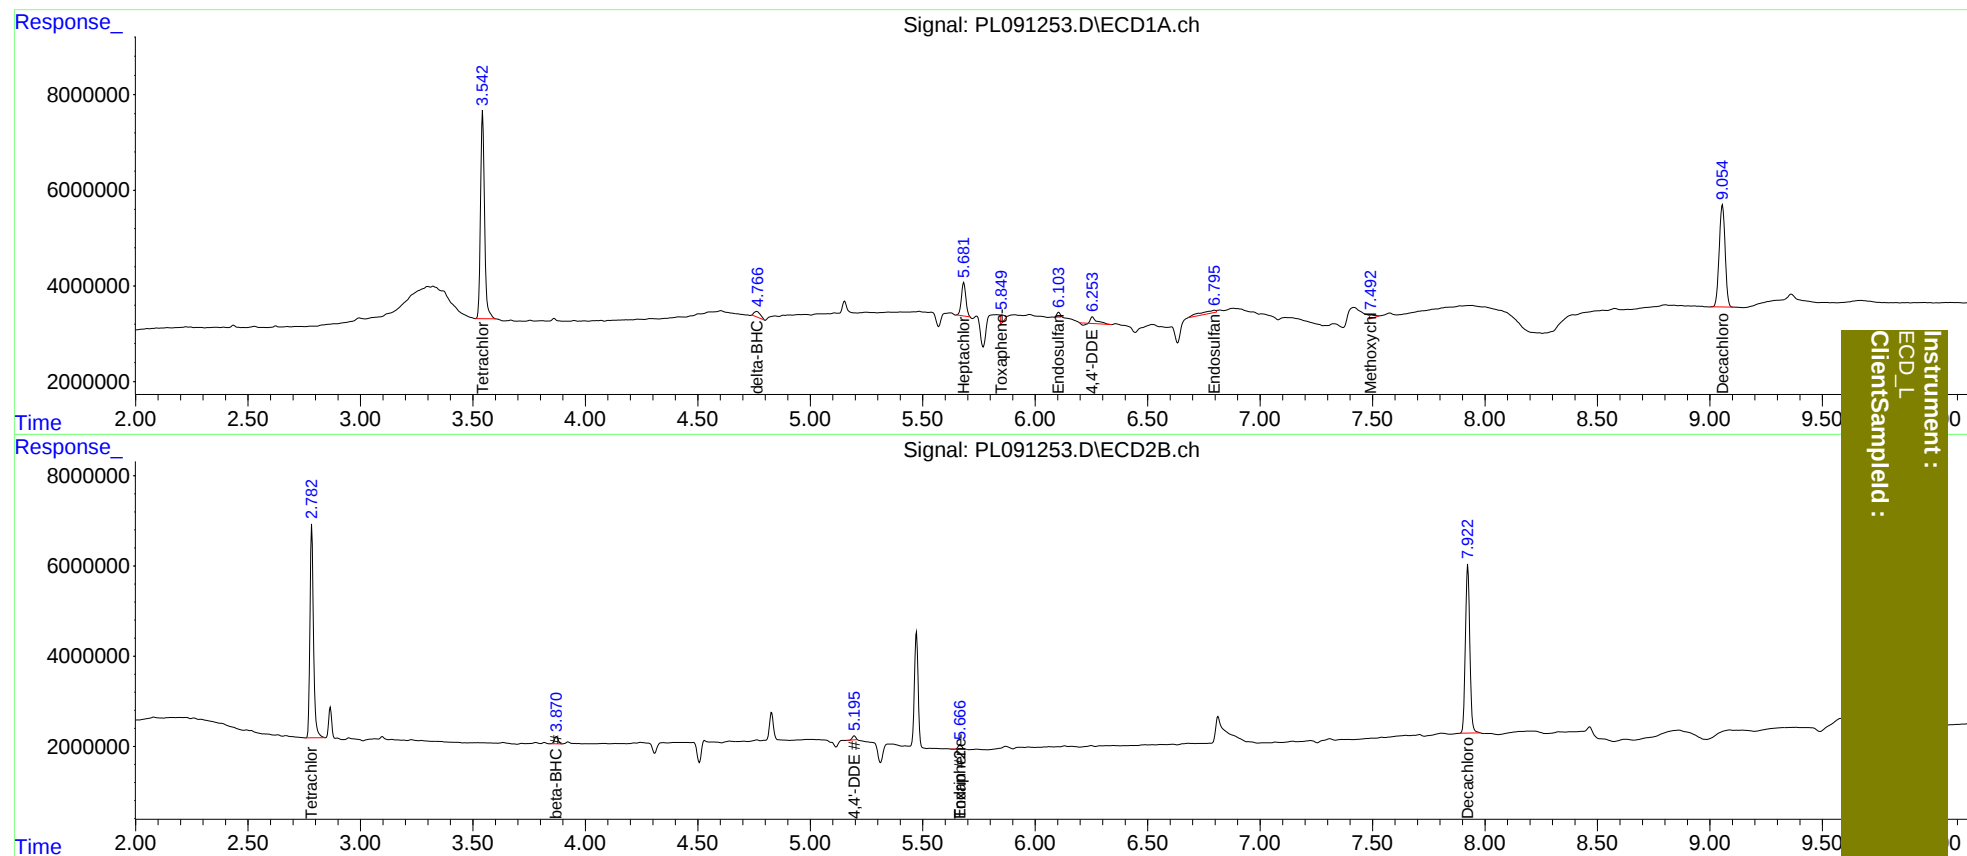


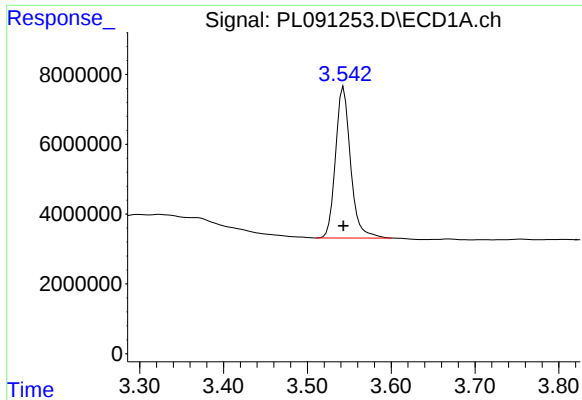

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 53915949
Conc: 26.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

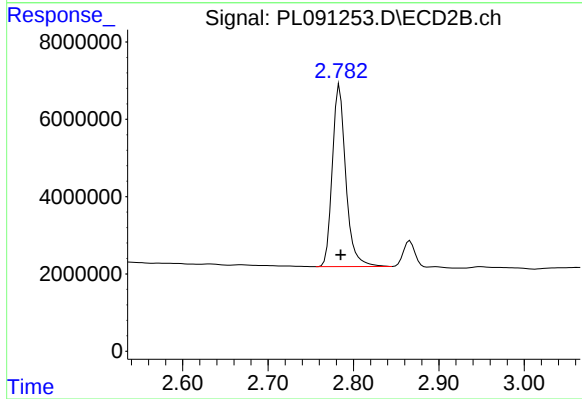


#1 Tetrachloro-m-xylene

R.T.: 2.784 min
Delta R.T.: -0.001 min
Response: 51759399
Conc: 29.49 ng/ml

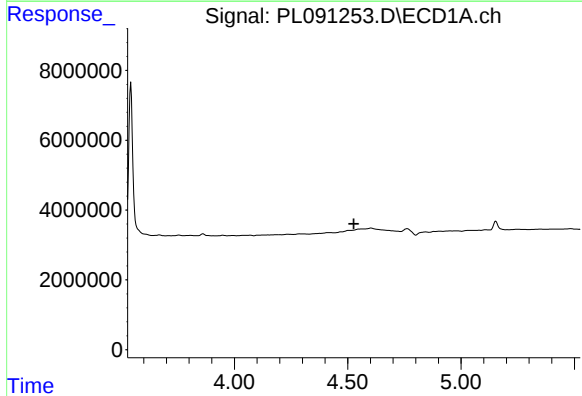


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.526 min
Response: 0
Conc: N.D.

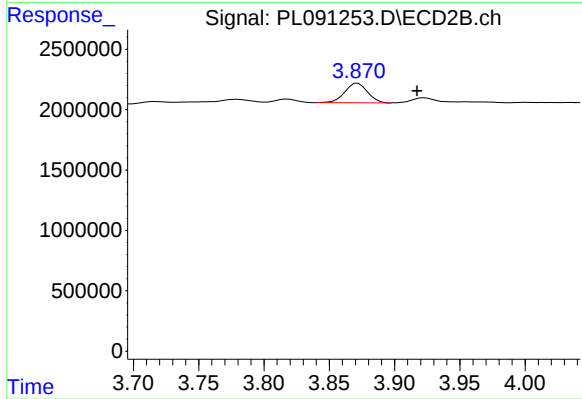

#6 beta-BHC


R.T.: 3.872 min
Delta R.T.: -0.045 min
Response: 1974474
Conc: 1.77 ng/ml

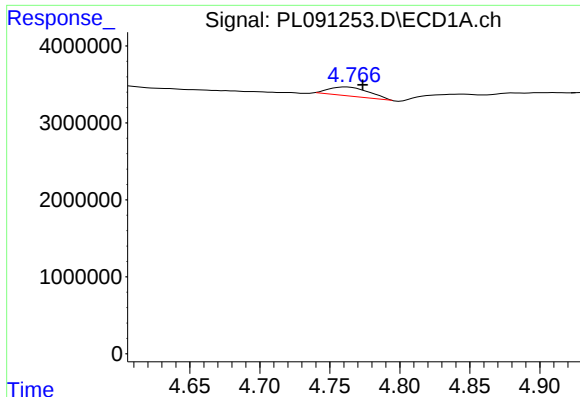

#7 delta-BHC


R.T.: 4.762 min
Delta R.T.: -0.011 min
Response: 2175409
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

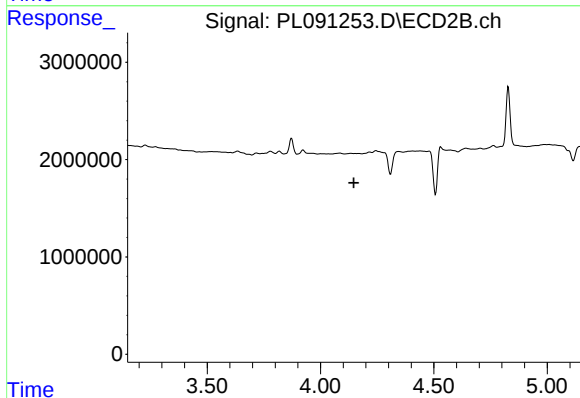


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.146 min
Response: 0
Conc: N.D.

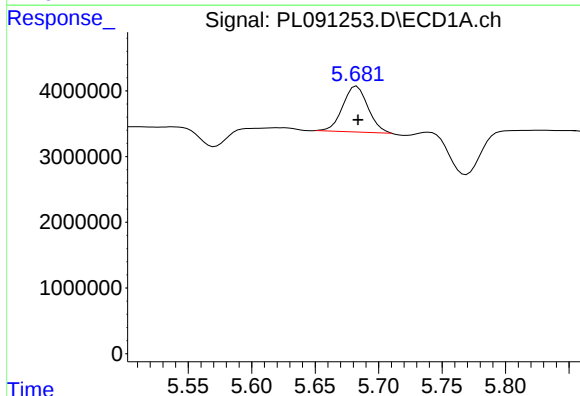


#8 Heptachlor epoxide

R.T.: 5.683 min
Delta R.T.: -0.001 min
Response: 9603017
Conc: 3.69 ng/ml

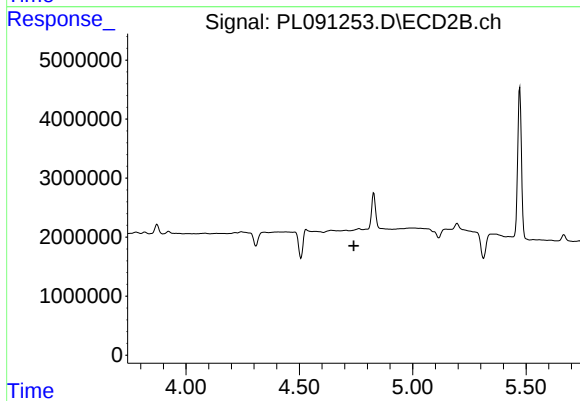

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.741 min
Response: 0
Conc: N.D.

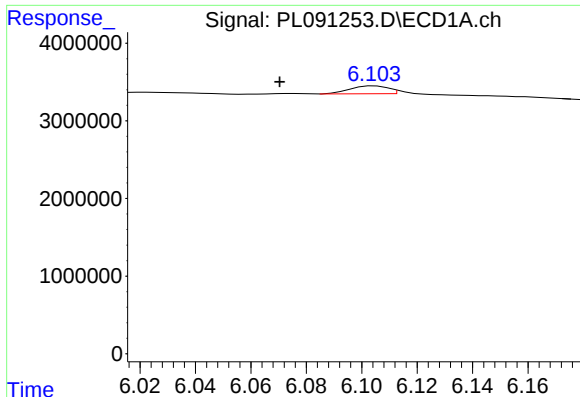

#9 Endosulfan I


R.T.: 6.105 min
Delta R.T.: 0.034 min
Response: 954383
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

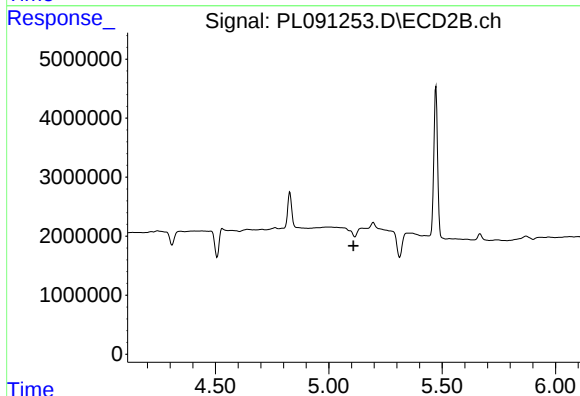


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

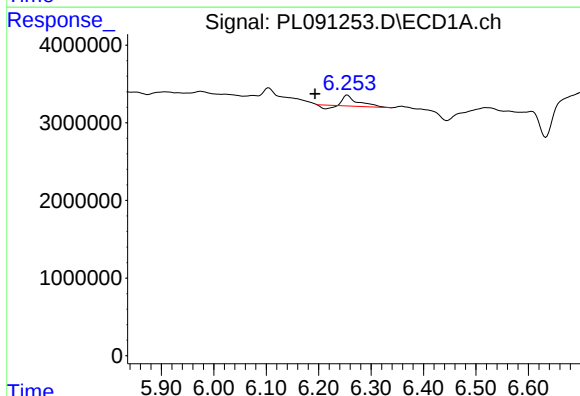


#12 4,4'-DDE

R.T.: 6.255 min
Delta R.T.: 0.062 min
Response: 2341480
Conc: 1.17 ng/ml

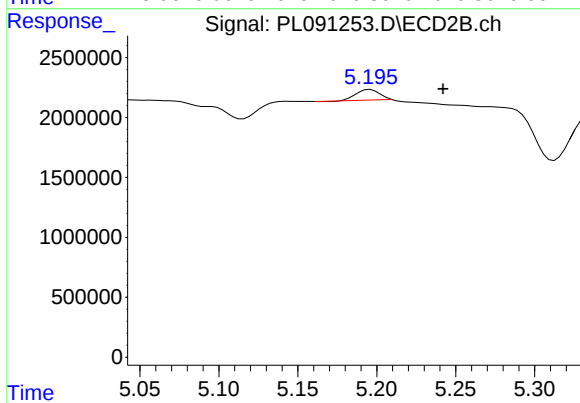

#12 4,4'-DDE


R.T.: 5.196 min
Delta R.T.: -0.046 min
Response: 913096
Conc: 0.49 ng/ml

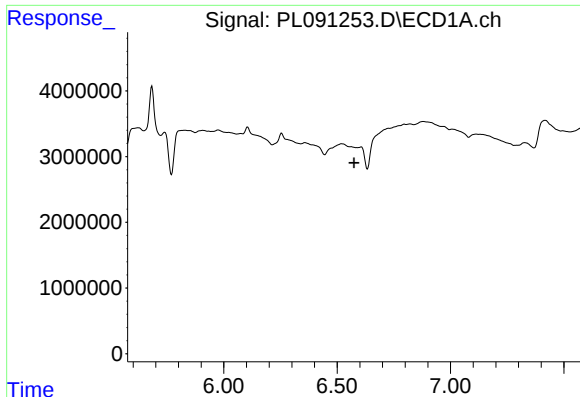

#14 Endrin


R.T.: 6.519 min
Delta R.T.: -0.055 min
Response: -84032
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

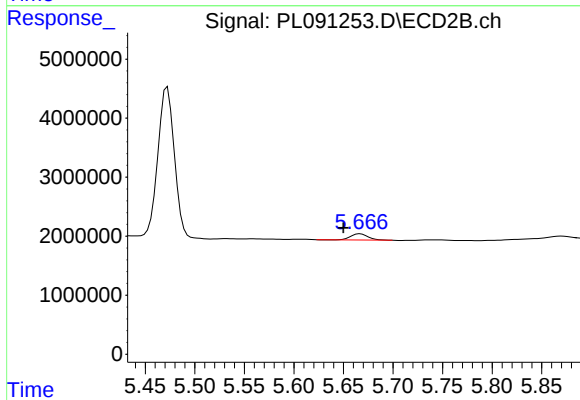


#14 Endrin

R.T.: 5.667 min
Delta R.T.: 0.017 min
Response: 1280701
Conc: 0.67 ng/ml

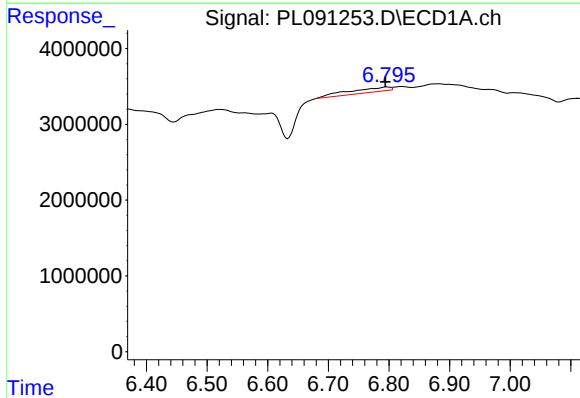


#15 Endosulfan II

R.T.: 6.797 min
Delta R.T.: 0.003 min
Response: 2941106
Conc: 1.53 ng/ml

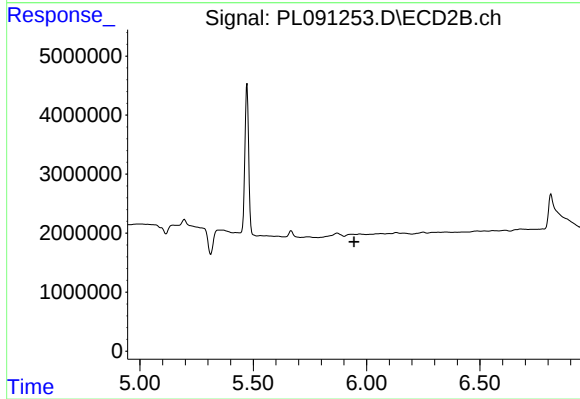

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.944 min
Response: 0
Conc: N.D.

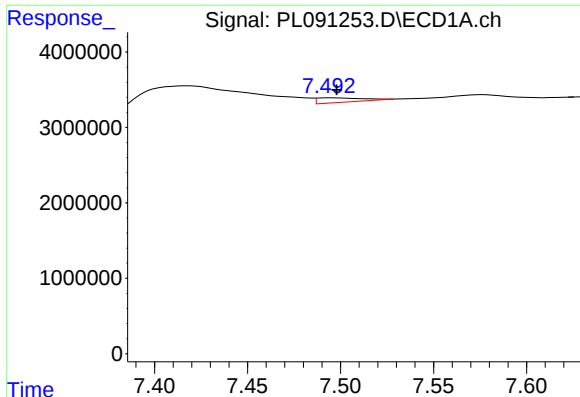

#20 Methoxychlor


R.T.: 7.495 min
Delta R.T.: -0.003 min
Response: 1025910
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

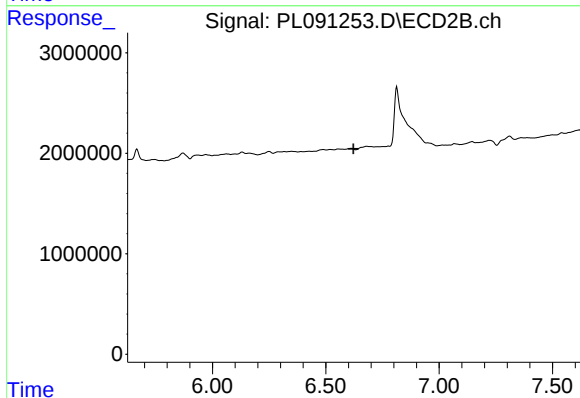


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.623 min
Response: 0
Conc: N.D.

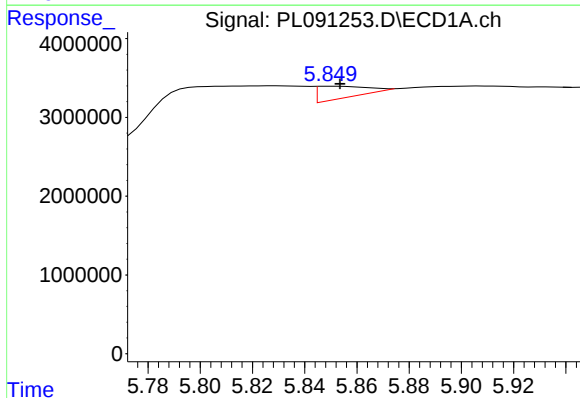


#22 Toxaphene-1

R.T.: 5.851 min
Delta R.T.: -0.003 min
Response: 1950325
Conc: 260.16 ng/ml

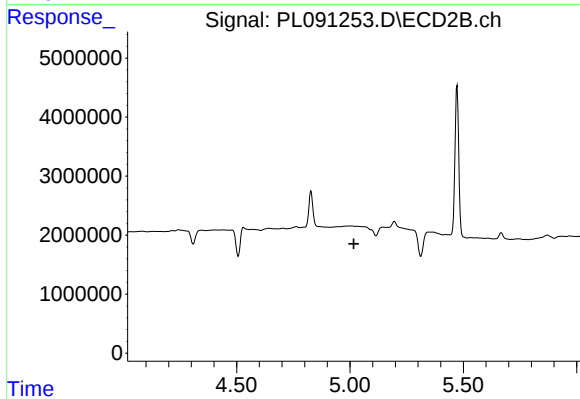

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T. : 5.017 min
Response: 0
Conc: N.D.

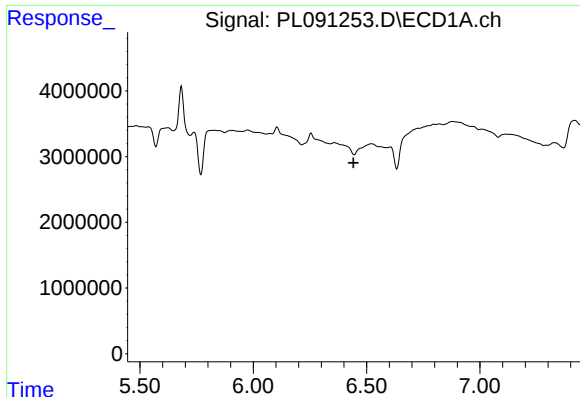

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.442 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

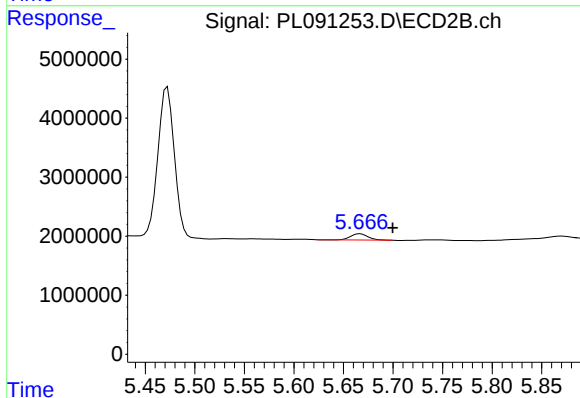


#23 Toxaphene-2

R.T.: 5.667 min
Delta R.T.: -0.033 min
Response: 1280701
Conc: 124.89 ng/ml

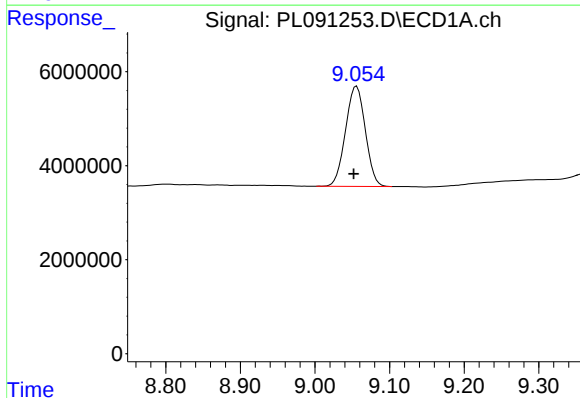

#27 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.004 min
Response: 39270032
Conc: 25.22 ng/ml

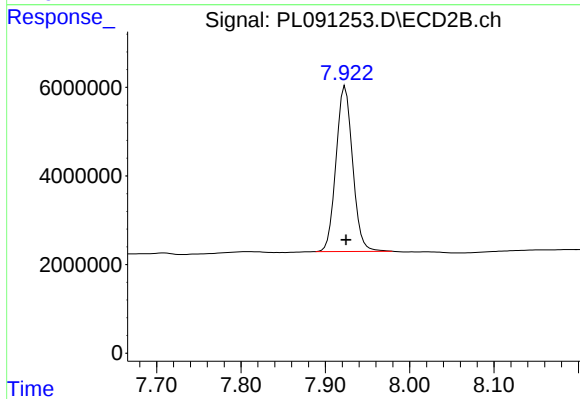

#27 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: 0.000 min
Response: 51067692
Conc: 29.76 ng/ml