

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082124\
 Data File : PL091235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Aug 2024 23:55
 Operator : AR\AJ
 Sample : P3504-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DCYD7

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/22/2024
 Supervised By : Ankita Jodhani 08/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 22 01:51:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080824CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 10 07:10:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.783	21991018	23776924	10.860	13.548m
2) SA Decachlor...	9.054	7.925	17011482	28270295	10.927	16.472 #
Target Compounds						
7) B delta-BHC	4.761	4.138	1456006	862162	0.520m	0.369 #
14) MA Endrin	6.565	5.647	2819480	3342435	1.546m	1.745m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082124\
Data File : PL091235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Aug 2024 23:55
Operator : AR\AJ
Sample : P3504-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 22 01:51:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080824CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 10 07:10:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

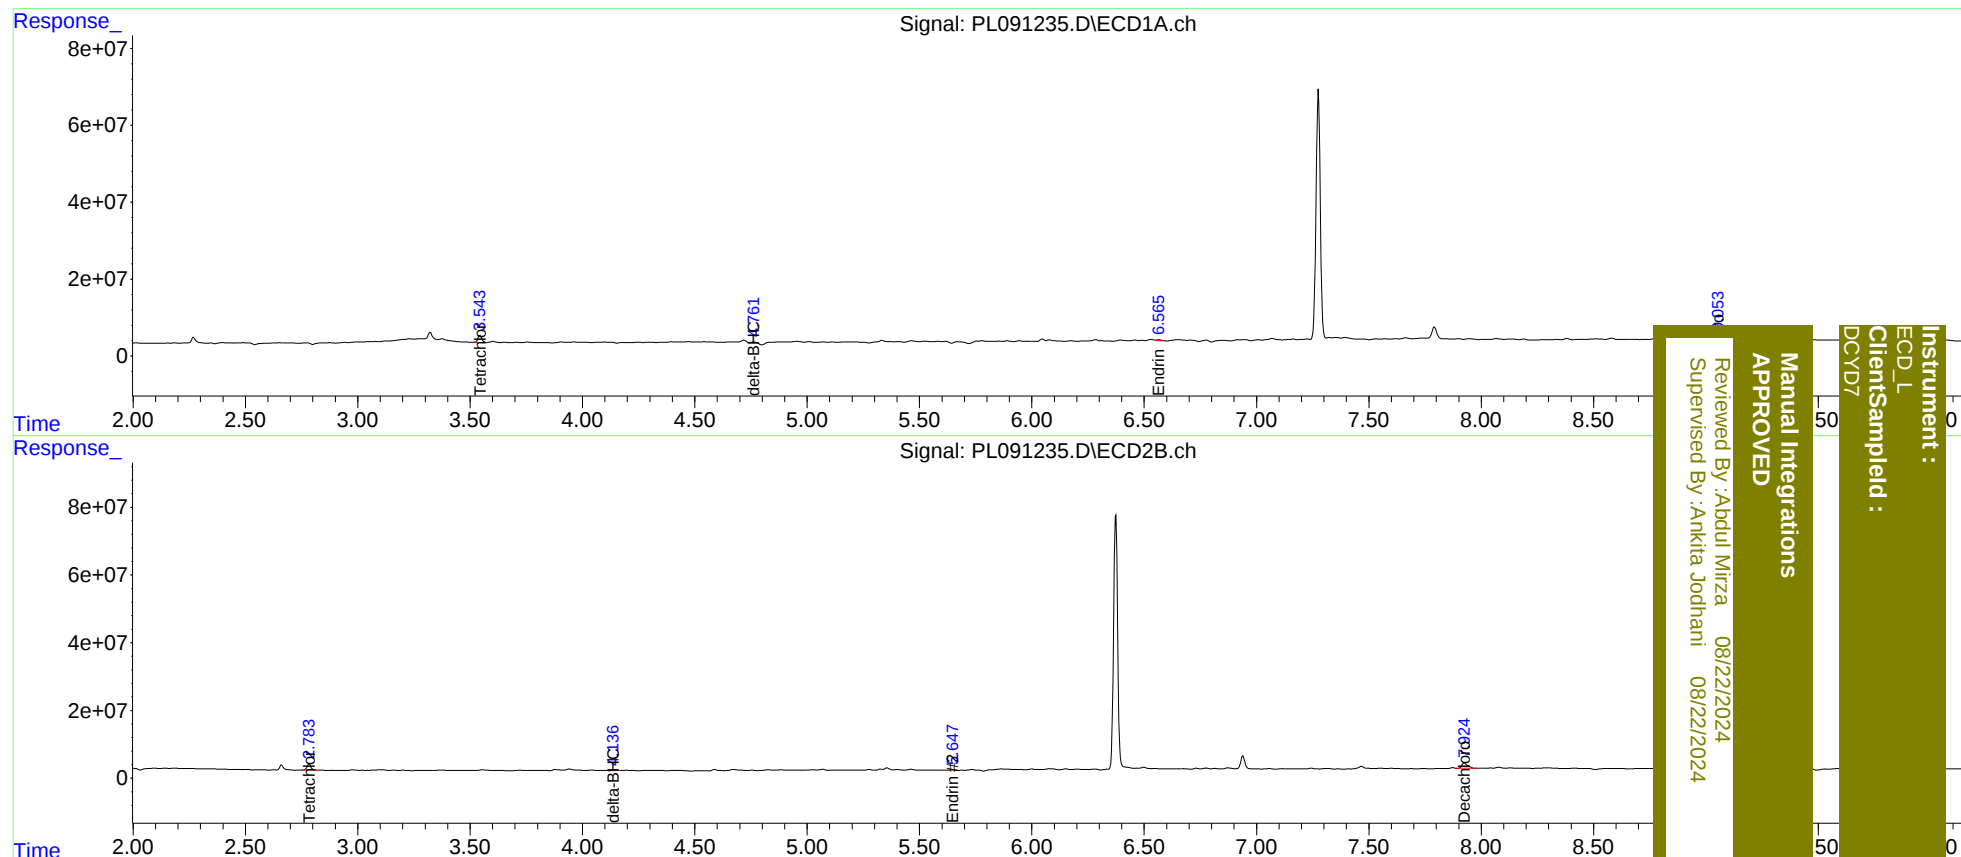

Reviewed By: Abdul Mirza 08/22/2024
Supervised By: Ankita Jodhani 08/22/2024

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
DCYD7