

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082221\
 Data File : PL069354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2021 02:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 07:40:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 21 02:23:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.570	11485103	32924898	24.893	22.984
28)	SA Decachlor...	10.403	11.493	15184308	25437236	22.497	20.755
Target Compounds							
4)	MA Heptachlor	6.150f	0.000	704236	0	1.017	N.D. #
7)	B delta-BHC	0.000	7.038f	0	4048485	N.D.	2.192 #
8)	B Heptachlo...	0.000	8.038	0	666415	N.D.	0.443 #
10)	B gamma-Chl...	0.000	8.290	0	661910	N.D.	0.430 #
14)	MA Endrin	8.078f	0.000	810589	0	1.404	N.D. #
25)	Chlordane-3	0.000	8.290	0	661910	N.D.	3.091 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082221\
Data File : PL069354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2021 02:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 07:40:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082021.M
Quant Title : GC Extractables
QLast Update : Sat Aug 21 02:23:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

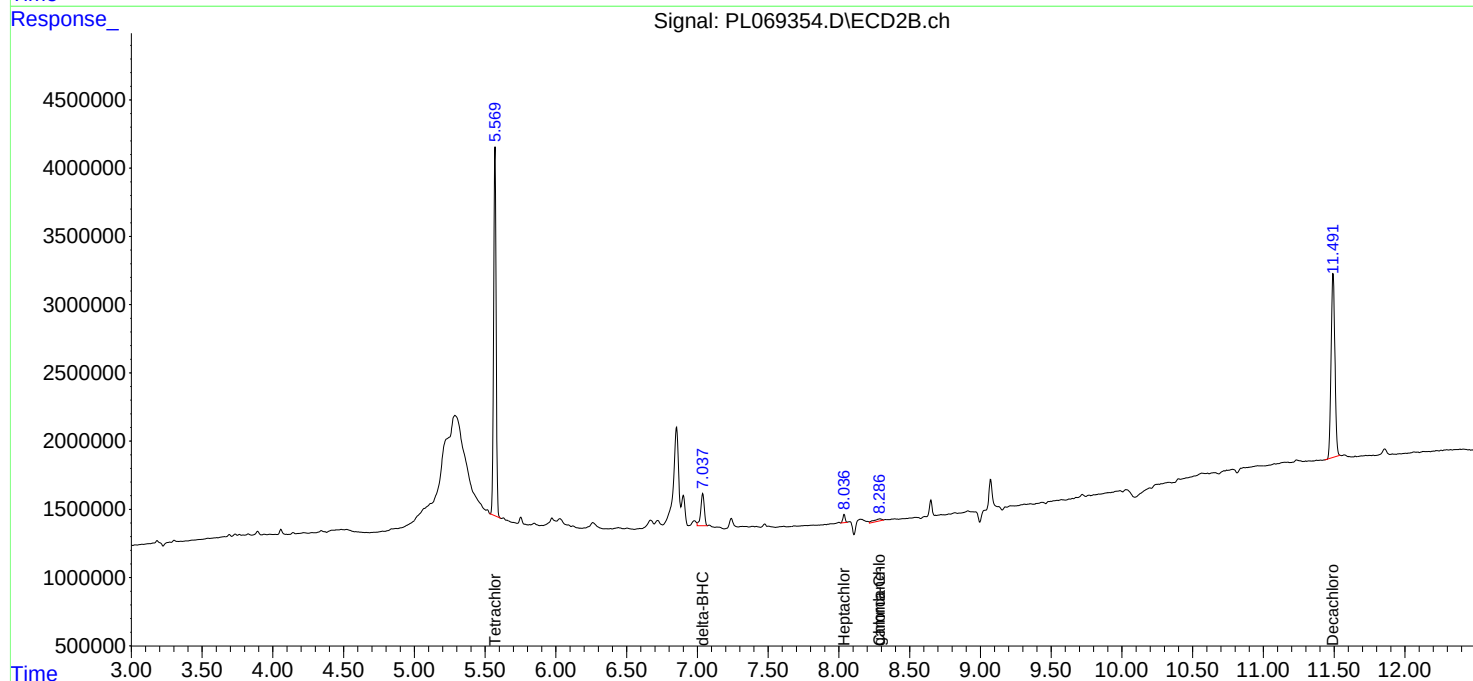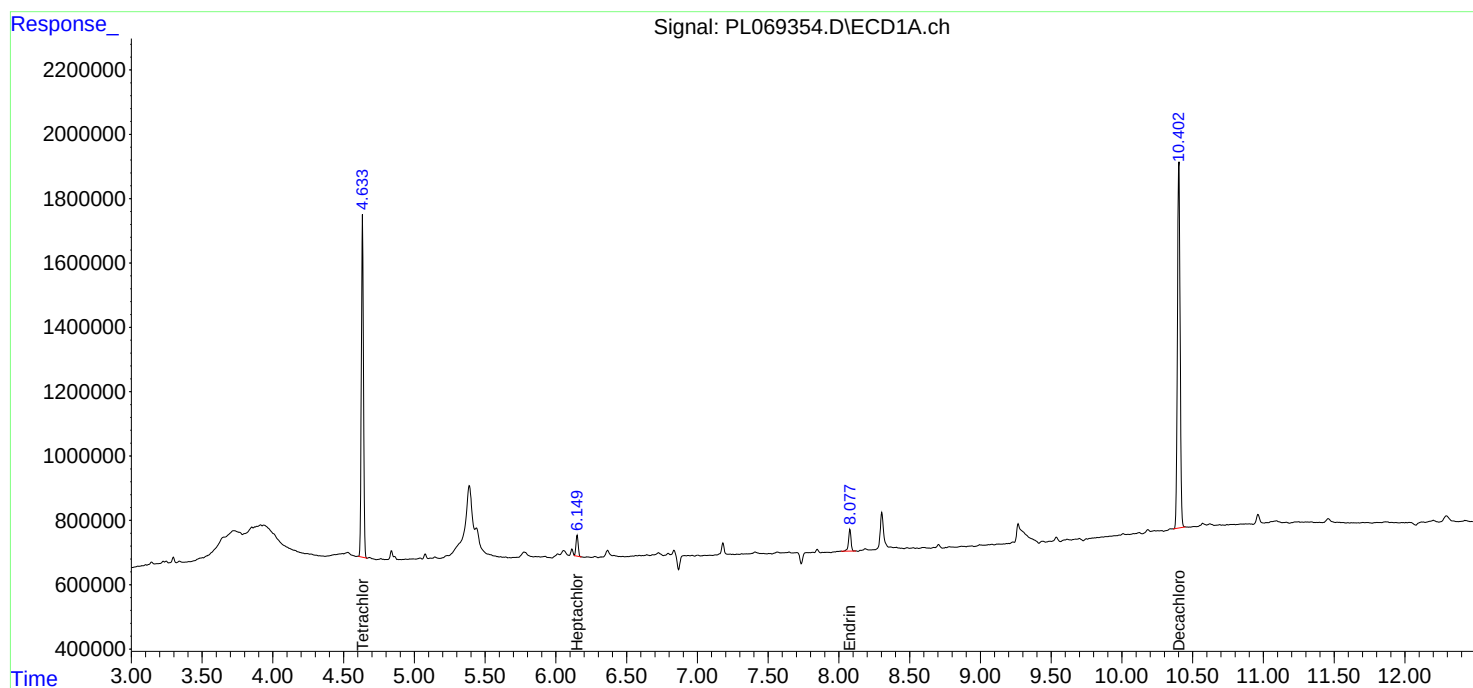


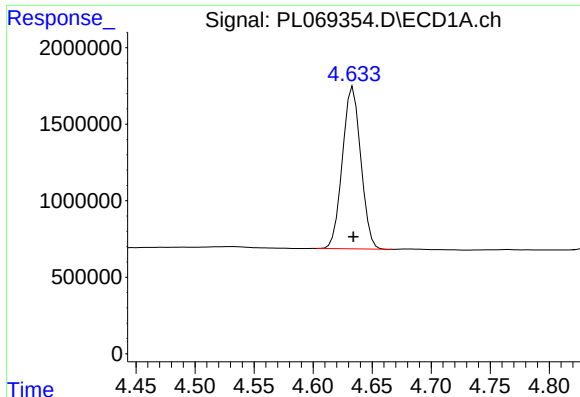

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 11485103
Conc: 24.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

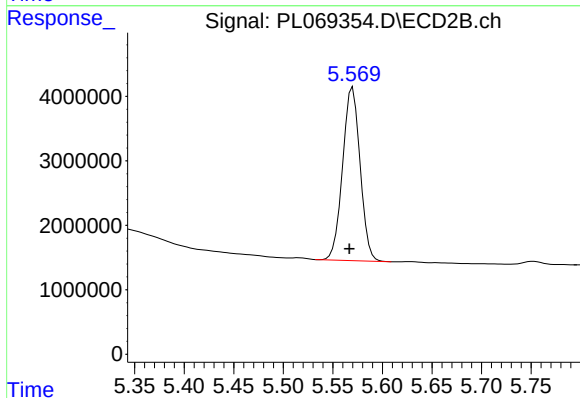


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.003 min
Response: 32924898
Conc: 22.98 ng/ml

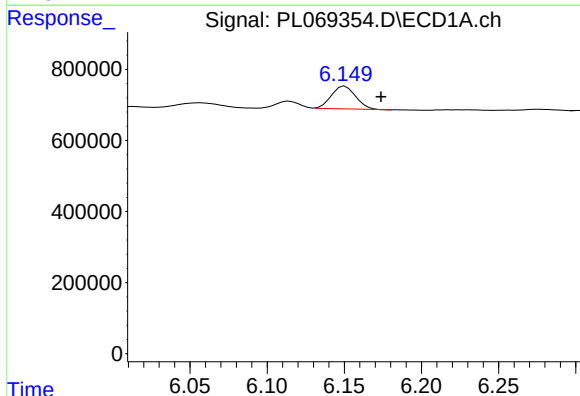


#4 Heptachlor

R.T.: 6.150 min
Delta R.T.: -0.023 min
Response: 704236
Conc: 1.02 ng/ml

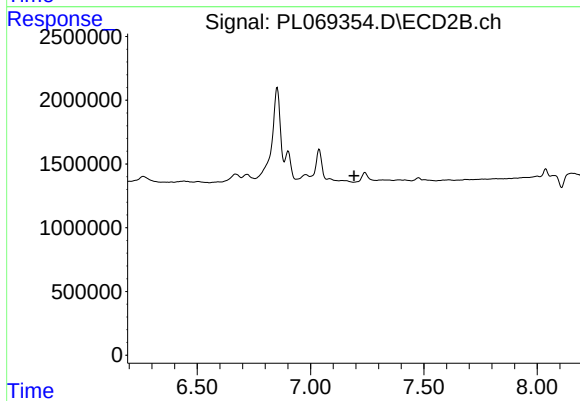

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.193 min
Response: 0
Conc: N.D.

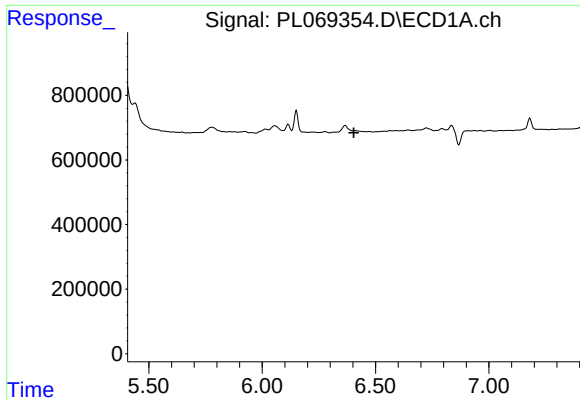

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

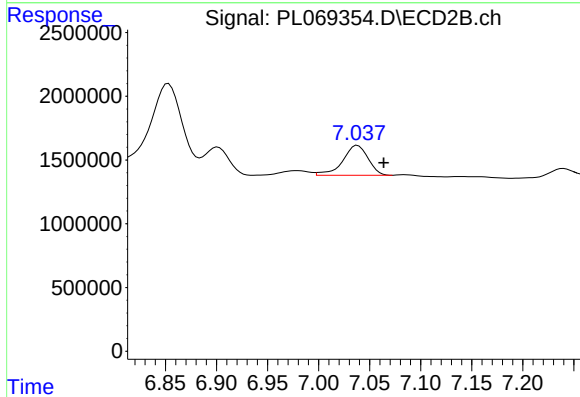


#7 delta-BHC

R.T.: 7.038 min
Delta R.T.: -0.026 min
Response: 4048485
Conc: 2.19 ng/ml

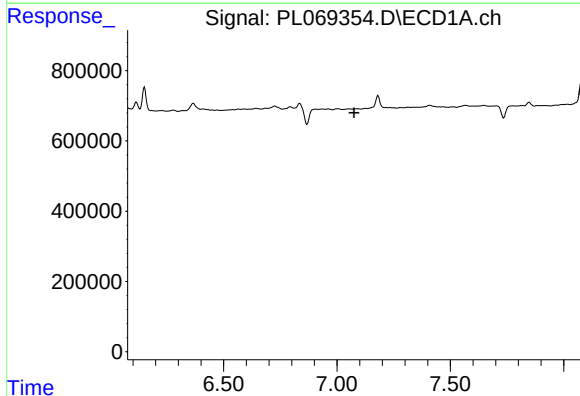


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.075 min
Response: 0
Conc: N.D.

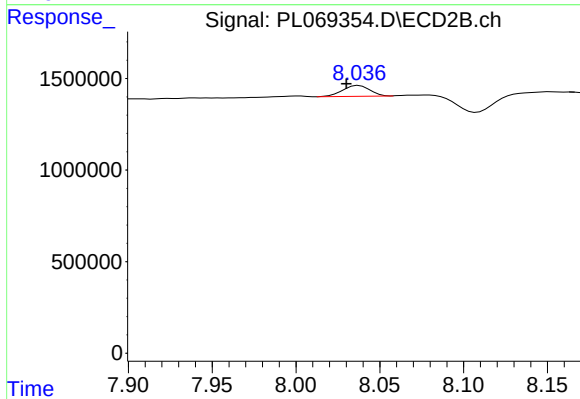

#8 Heptachlor epoxide


R.T.: 8.038 min
Delta R.T.: 0.008 min
Response: 666415
Conc: 0.44 ng/ml

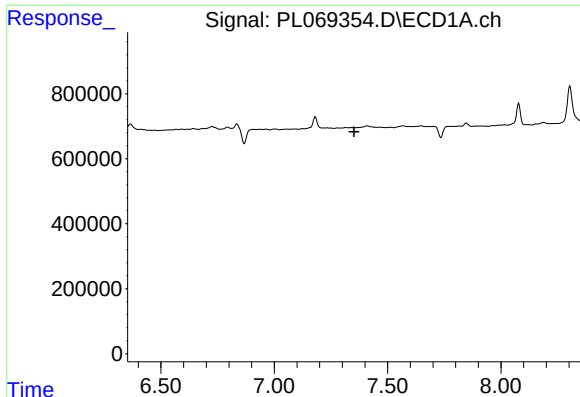

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

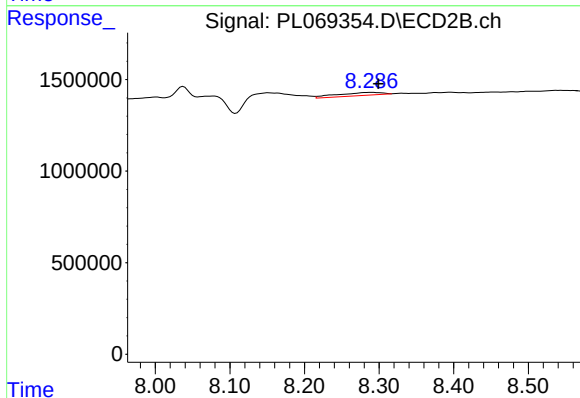


#10 gamma-Chlordane

R.T.: 8.290 min
Delta R.T.: -0.009 min
Response: 661910
Conc: 0.43 ng/ml

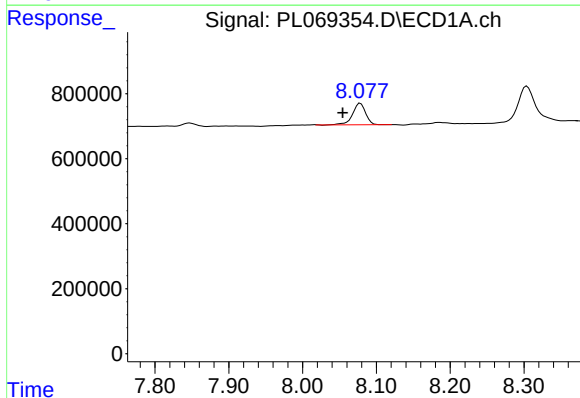


#14 Endrin

R.T.: 8.078 min
Delta R.T.: 0.024 min
Response: 810589
Conc: 1.40 ng/ml

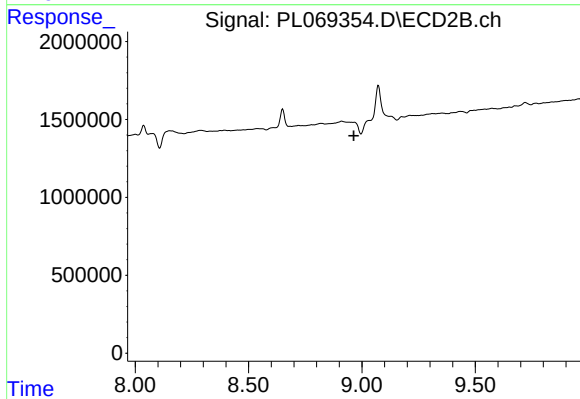

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.964 min
Response: 0
Conc: N.D.

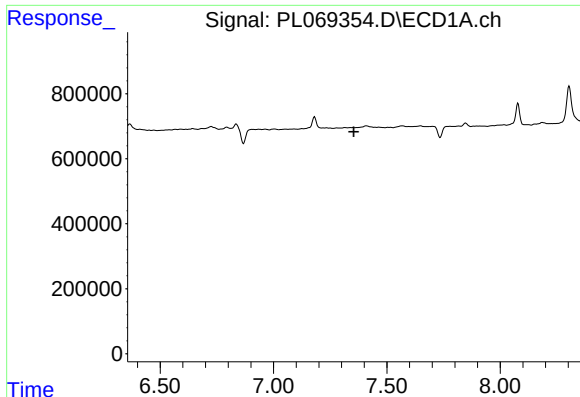

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

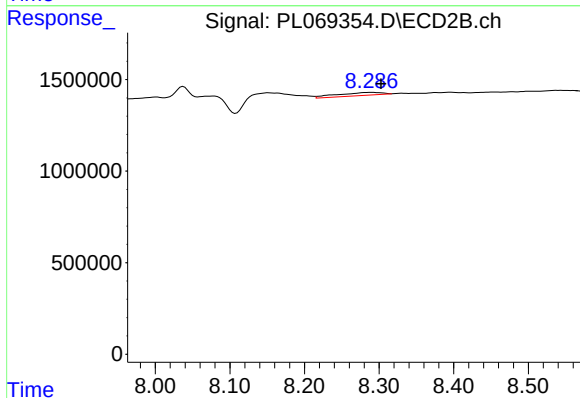


#25 Chlordane-3

R.T.: 8.290 min
Delta R.T.: -0.013 min
Response: 661910
Conc: 3.09 ng/ml

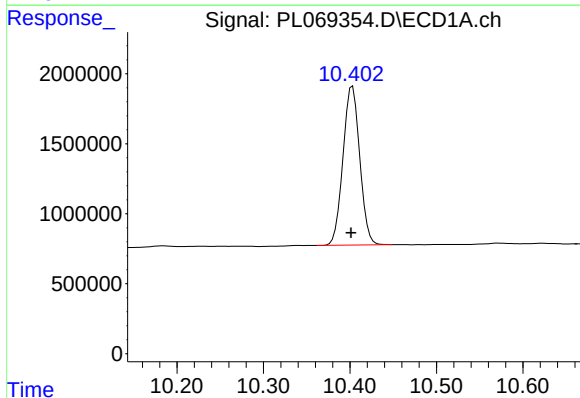

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: 0.002 min
Response: 15184308
Conc: 22.50 ng/ml

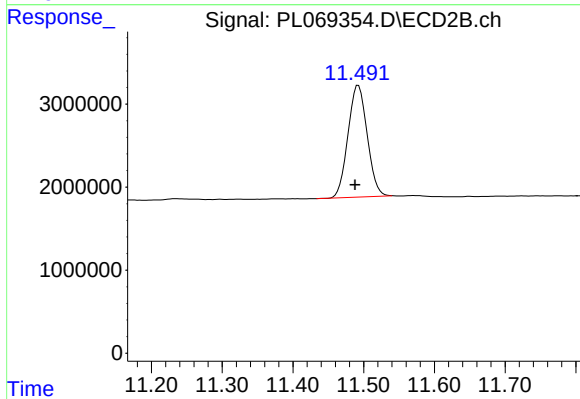

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.004 min
Response: 25437236
Conc: 20.76 ng/ml